


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100425\
Data File : BN037997.D
Acq On : 03 Oct 2025 14:09
Operator : RC/JU
Sample : DFTPP385
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP385

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Oct 03 16:35:17 2025

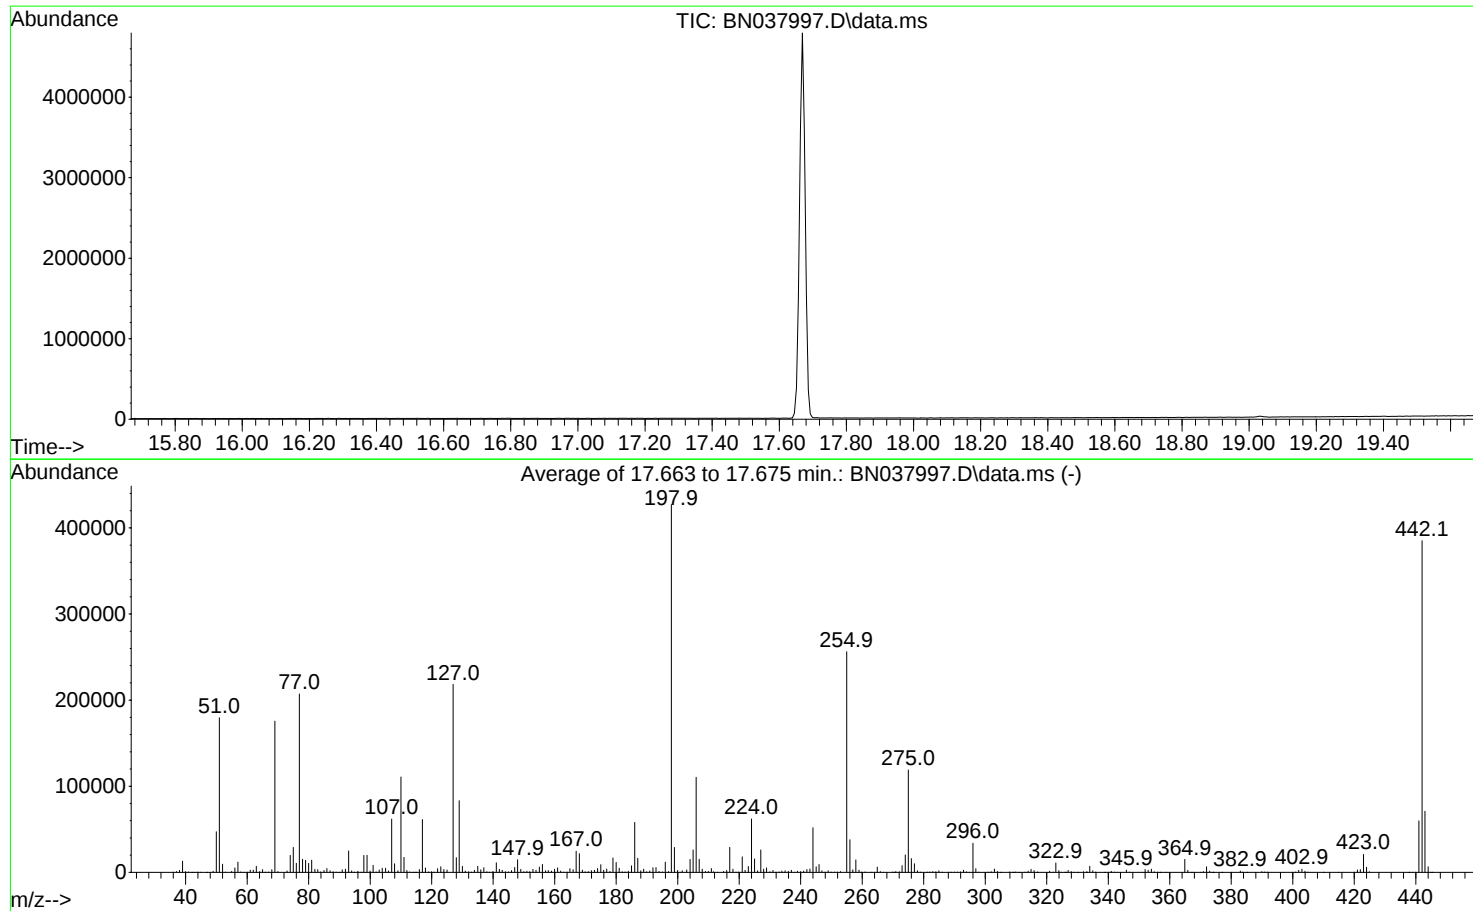

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	179510	PASS
68	69	0.00	2	1.8	3194	PASS
69	198	0.00	100	41.1	175637	PASS
70	69	0.00	2	0.5	852	PASS
127	198	10	80	51.1	218304	PASS
197	198	0.00	2	0.2	854	PASS
198	198	100	100	100.0	427179	PASS
199	198	5	9	6.8	29011	PASS
275	198	10	60	27.8	118883	PASS
365	198	1	100	3.5	15023	PASS
441	198	0.01	100	14.0	59755	PASS
442	198	50	100	90.2	385109	PASS
443	442	15	24	18.4	70973	PASS