


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100519\
 Data File : BN008022.D
 Acq On : 05 Oct 2019 12:53
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 03 18:39:49 2019

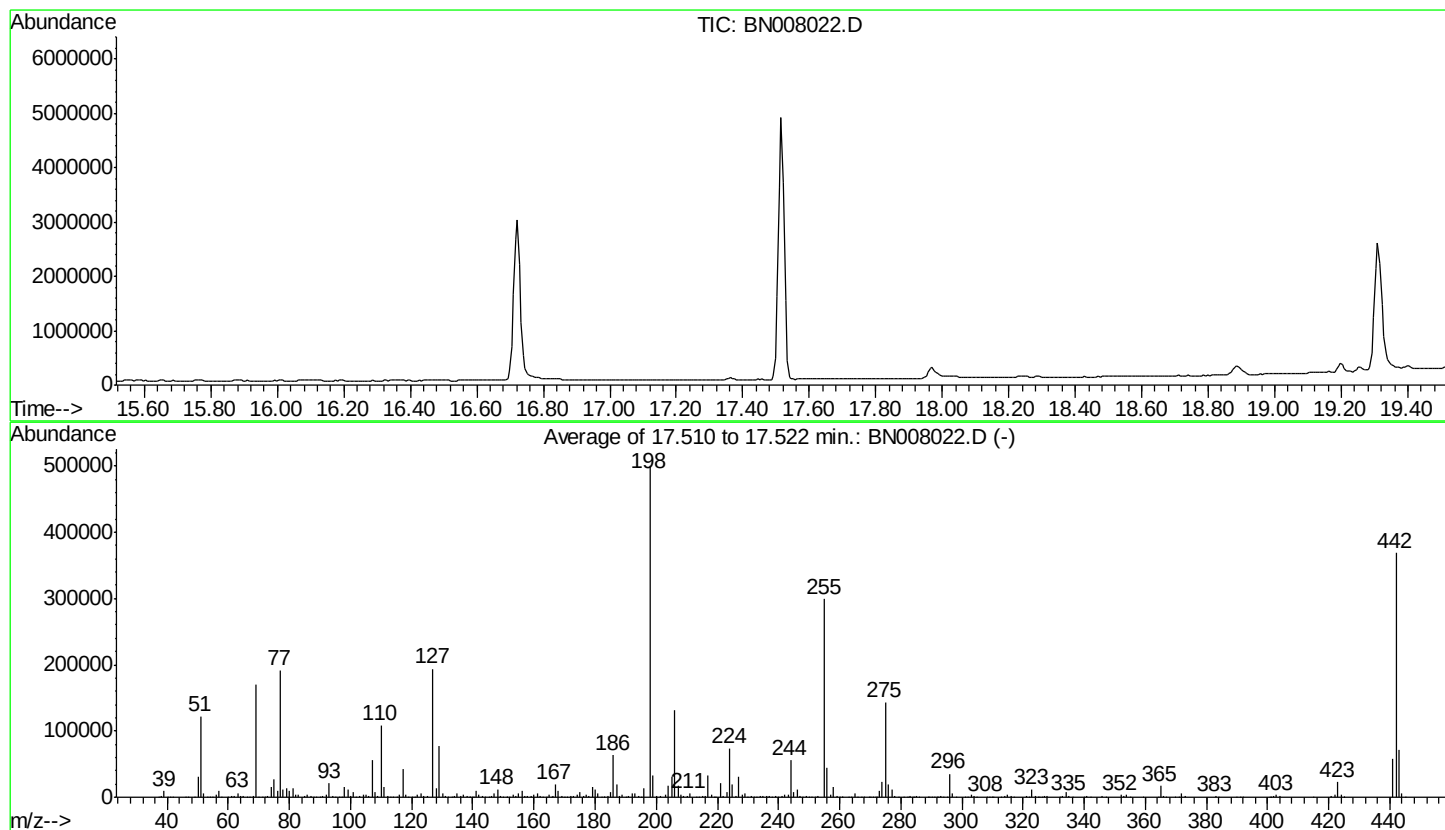

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	121238	PASS
68	69	0.00	2	1.7	2820	PASS
69	198	0.00	100	34.0	170214	PASS
70	69	0.00	2	0.3	471	PASS
127	198	10	80	38.7	193898	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	500586	PASS
199	198	5	9	6.7	33584	PASS
275	198	10	60	28.5	142722	PASS
365	198	1	100	3.3	16681	PASS
441	198	0.01	100	11.7	58450	PASS
442	198	50	100	73.6	368405	PASS
443	442	15	24	19.6	72170	PASS