


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100519\
 Data File : BN008041.D
 Acq On : 06 Oct 2019 00:49
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 03 18:39:49 2019

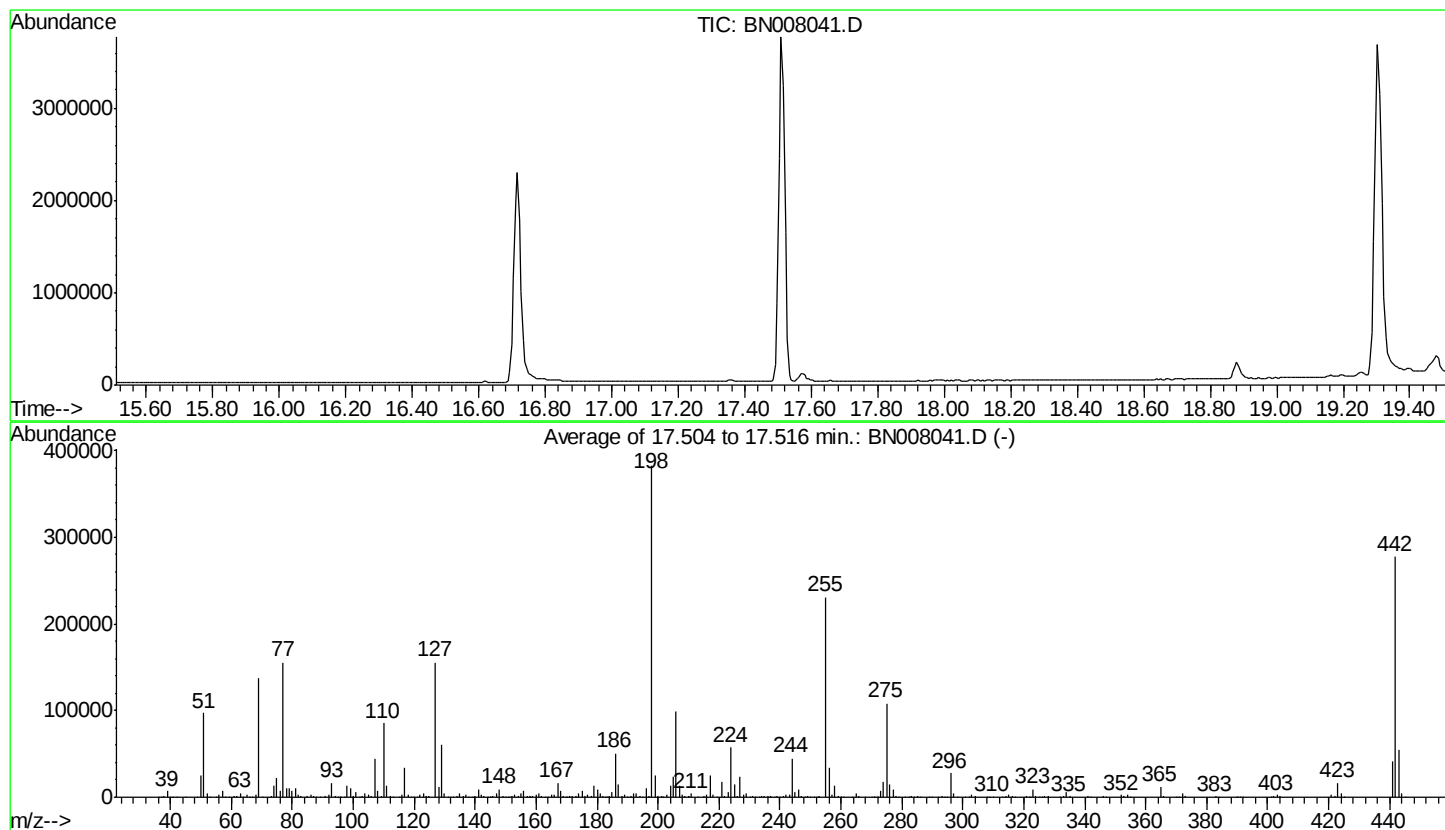

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	97169	PASS
68	69	0.00	2	1.8	2468	PASS
69	198	0.00	100	36.1	137984	PASS
70	69	0.00	2	0.5	696	PASS
127	198	10	80	40.6	155477	PASS
197	198	0.00	2	0.5	2100	PASS
198	198	100	100	100.0	382592	PASS
199	198	5	9	6.7	25562	PASS
275	198	10	60	28.3	108216	PASS
365	198	1	100	3.1	11893	PASS
441	198	0.01	100	11.0	41994	PASS
442	198	50	100	72.6	277589	PASS
443	442	15	24	19.6	54306	PASS