

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028055.D
 Acq On : 05 Oct 2023 19:04
 Operator : MA/JU
 Sample : 04607-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

Quant Time: Oct 06 01:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	5674	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.757	136	18473	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.578	164	9062	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.337	188	18151	0.400	ng/ul	-0.01
17) Chrysene-d12	21.524	240	15752	0.400	ng/ul	-0.01
23) Perylene-d12	23.985	264	18041	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.335	152	5955	0.200	ng/ul	-0.02
18) Fluoranthene-d10	19.362	212	12919	0.259	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.368	88	1353	0.179	ng/ul#	74
20) Pyrene	19.729	202	2179	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.825	252	4458	0.078	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028055.D
Acq On : 05 Oct 2023 19:04
Operator : MA/JU
Sample : 04607-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ35

Quant Time: Oct 06 01:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration




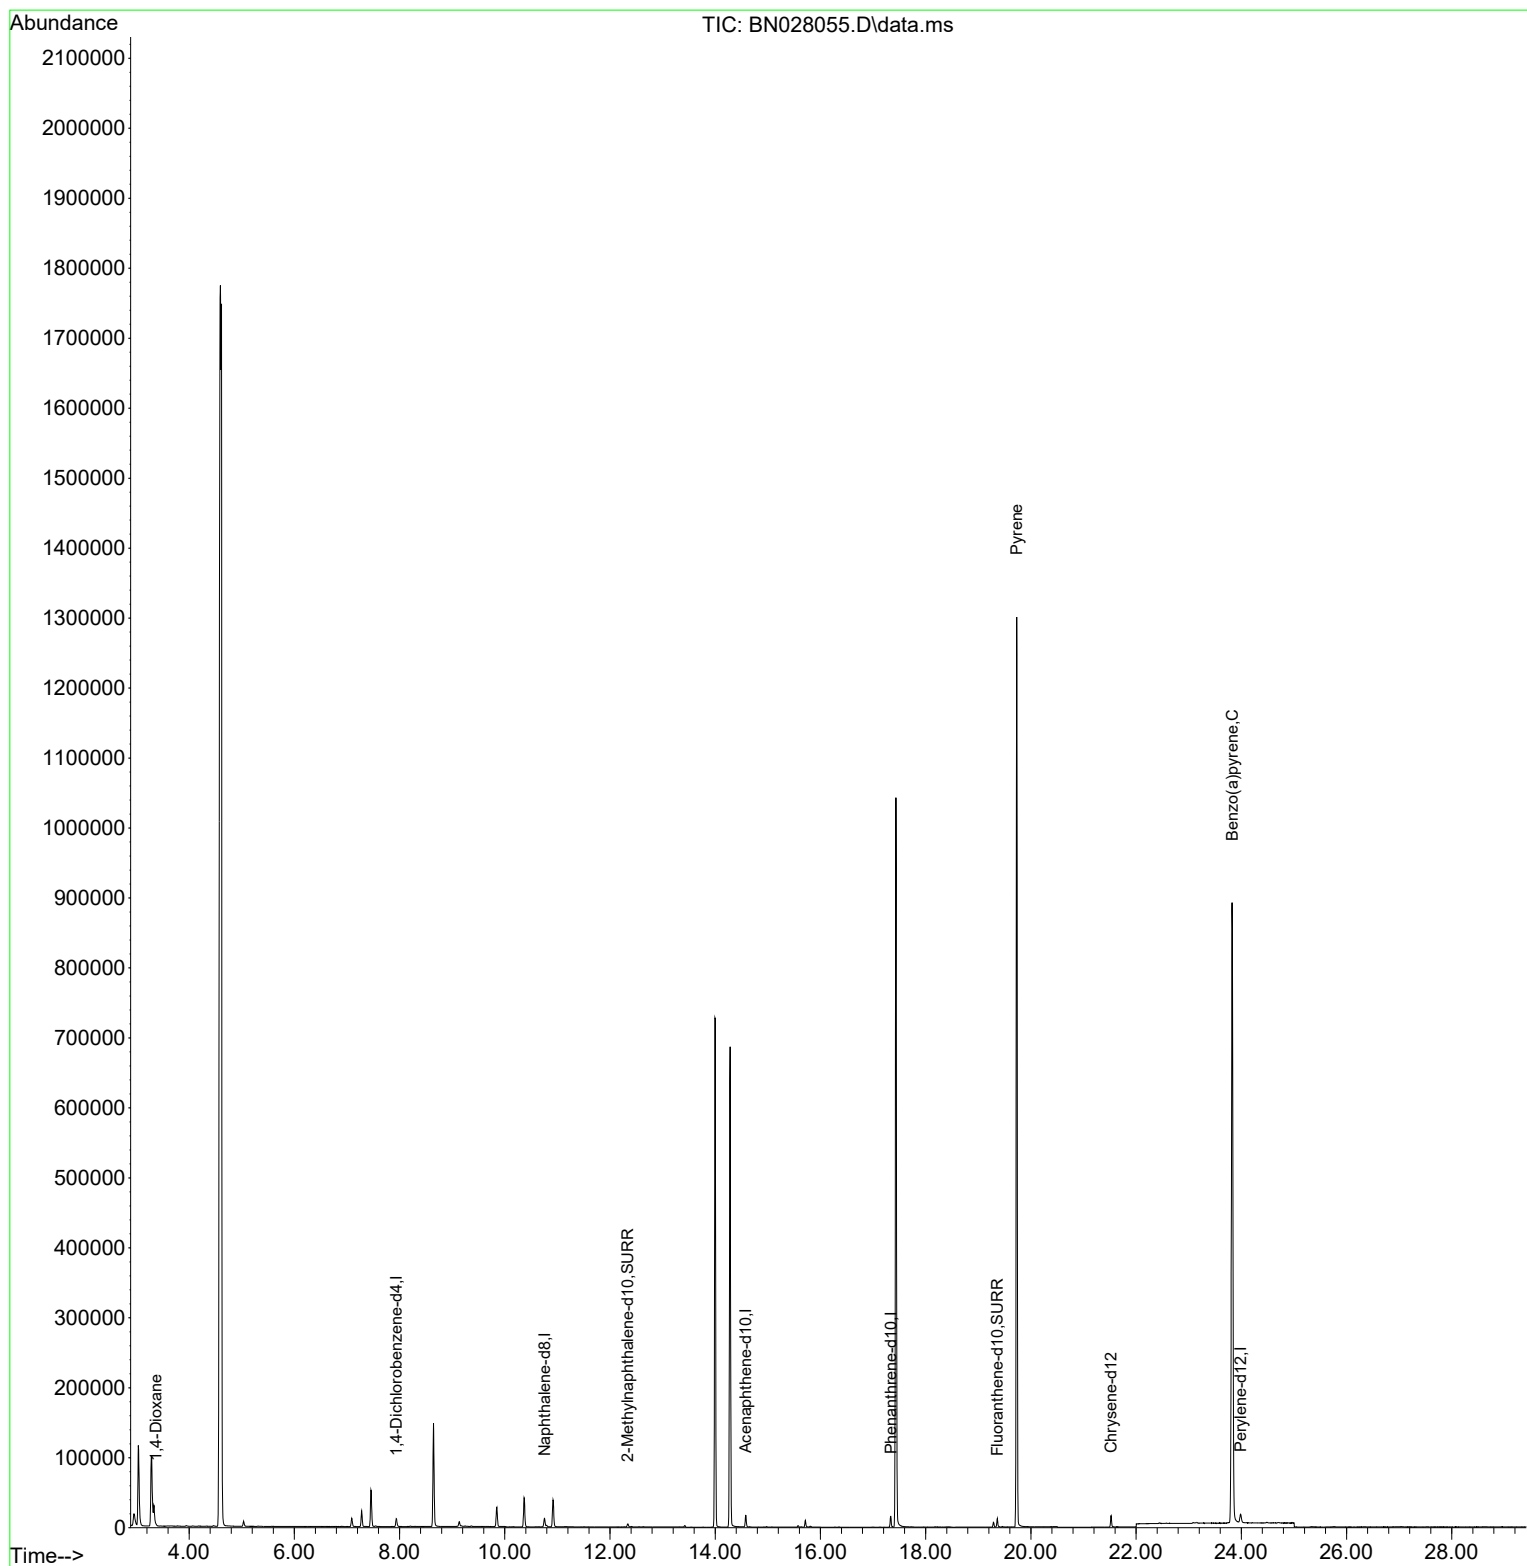


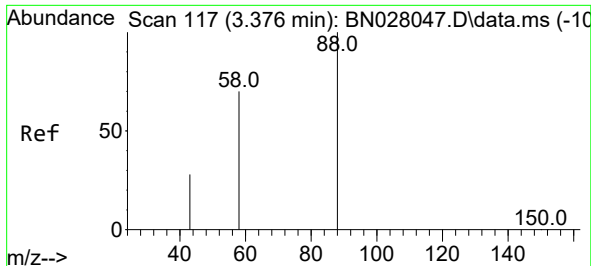

#2
1,4-Dioxane
Concen: 0.179 ng/ul
RT: 3.368 min Scan# 117
Delta R.T. 0.004 min
Lab File: BN028055.D
Acq: 05 Oct 2023 19:04




Instrument :
BNA_N
ClientSampleId :
BBJ35


Tgt Ion: 88 Resp: 1353
Ion Ratio Lower Upper
88 100
43 78.6 33.4 50.2#
58 56.0 45.7 68.5

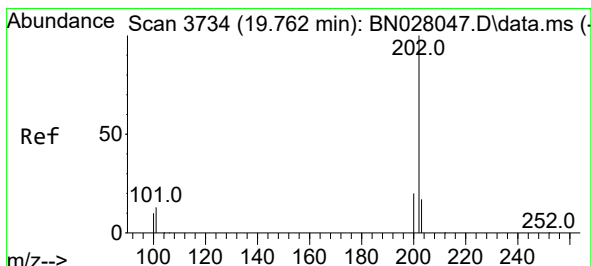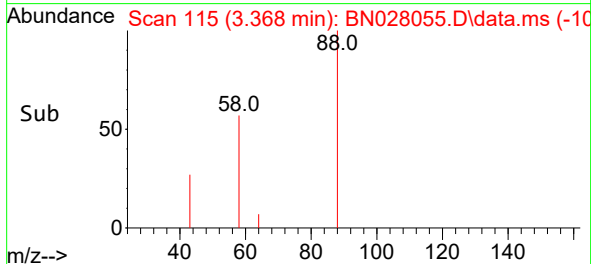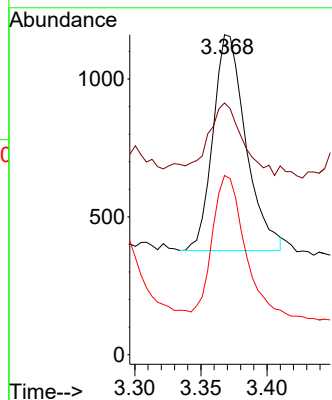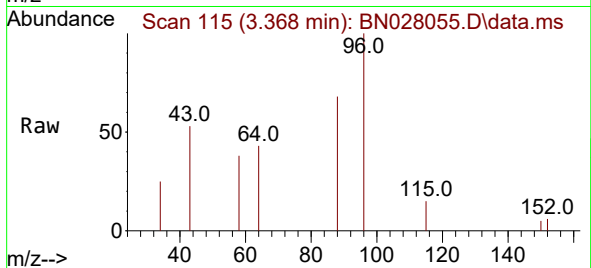

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.729 min Scan# 3727
Delta R.T. -0.042 min
Lab File: BN028055.D
Acq: 05 Oct 2023 19:04


Tgt Ion: 202 Resp: 2179
Ion Ratio Lower Upper
202 100
101 160.4 11.2 16.8#
100 1158.7 9.1 13.7#

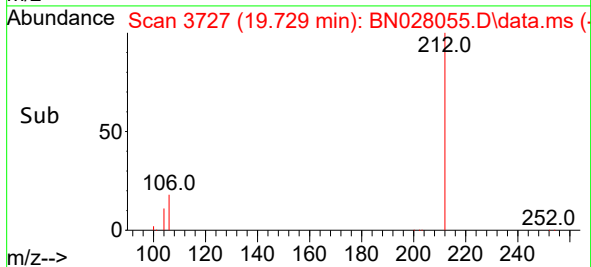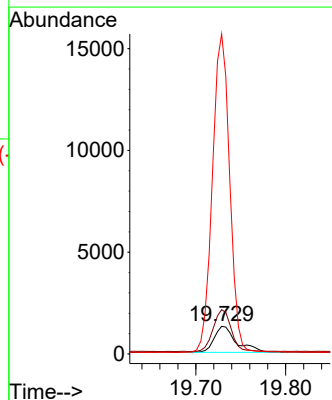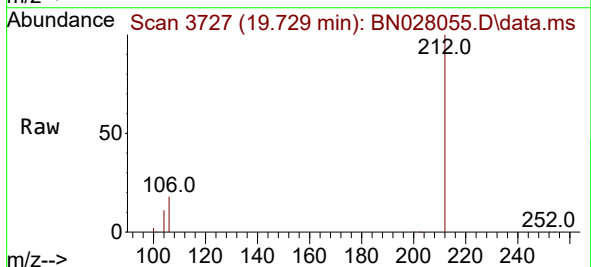

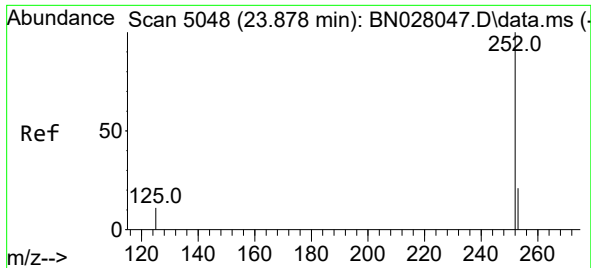

#26
 Benzo(a)pyrene
 Concen: 0.078 ng/ul
 RT: 23.825 min Scan# 50
 Delta R.T. -0.070 min
 Lab File: BN028055.D
 Acq: 05 Oct 2023 19:04

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

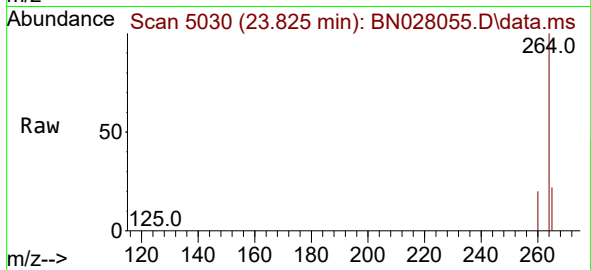

Tgt Ion:252 Resp: 4458
 Ion Ratio Lower Upper
 252 100
 253 61.4 23.4 35.2#
 125 48.6 15.3 22.9#

