

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028111.D
 Acq On : 07 Oct 2023 08:43
 Operator : MA/JU
 Sample : PB156035BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK035

Quant Time: Oct 08 00:50:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	5032	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	15406	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	8060	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.333	188	15863	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	13355	0.400	ng/ul	0.00
23) Perylene-d12	23.986	264	15534	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	46406	7.342	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	7644	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	14340	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.568	166	2300	0.071	ng/ul#	16
20) Pyrene	19.729	202	2023	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.825	252	4444	0.090	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028111.D
Acq On : 07 Oct 2023 08:43
Operator : MA/JU
Sample : PB156035BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK035

Quant Time: Oct 08 00:50:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




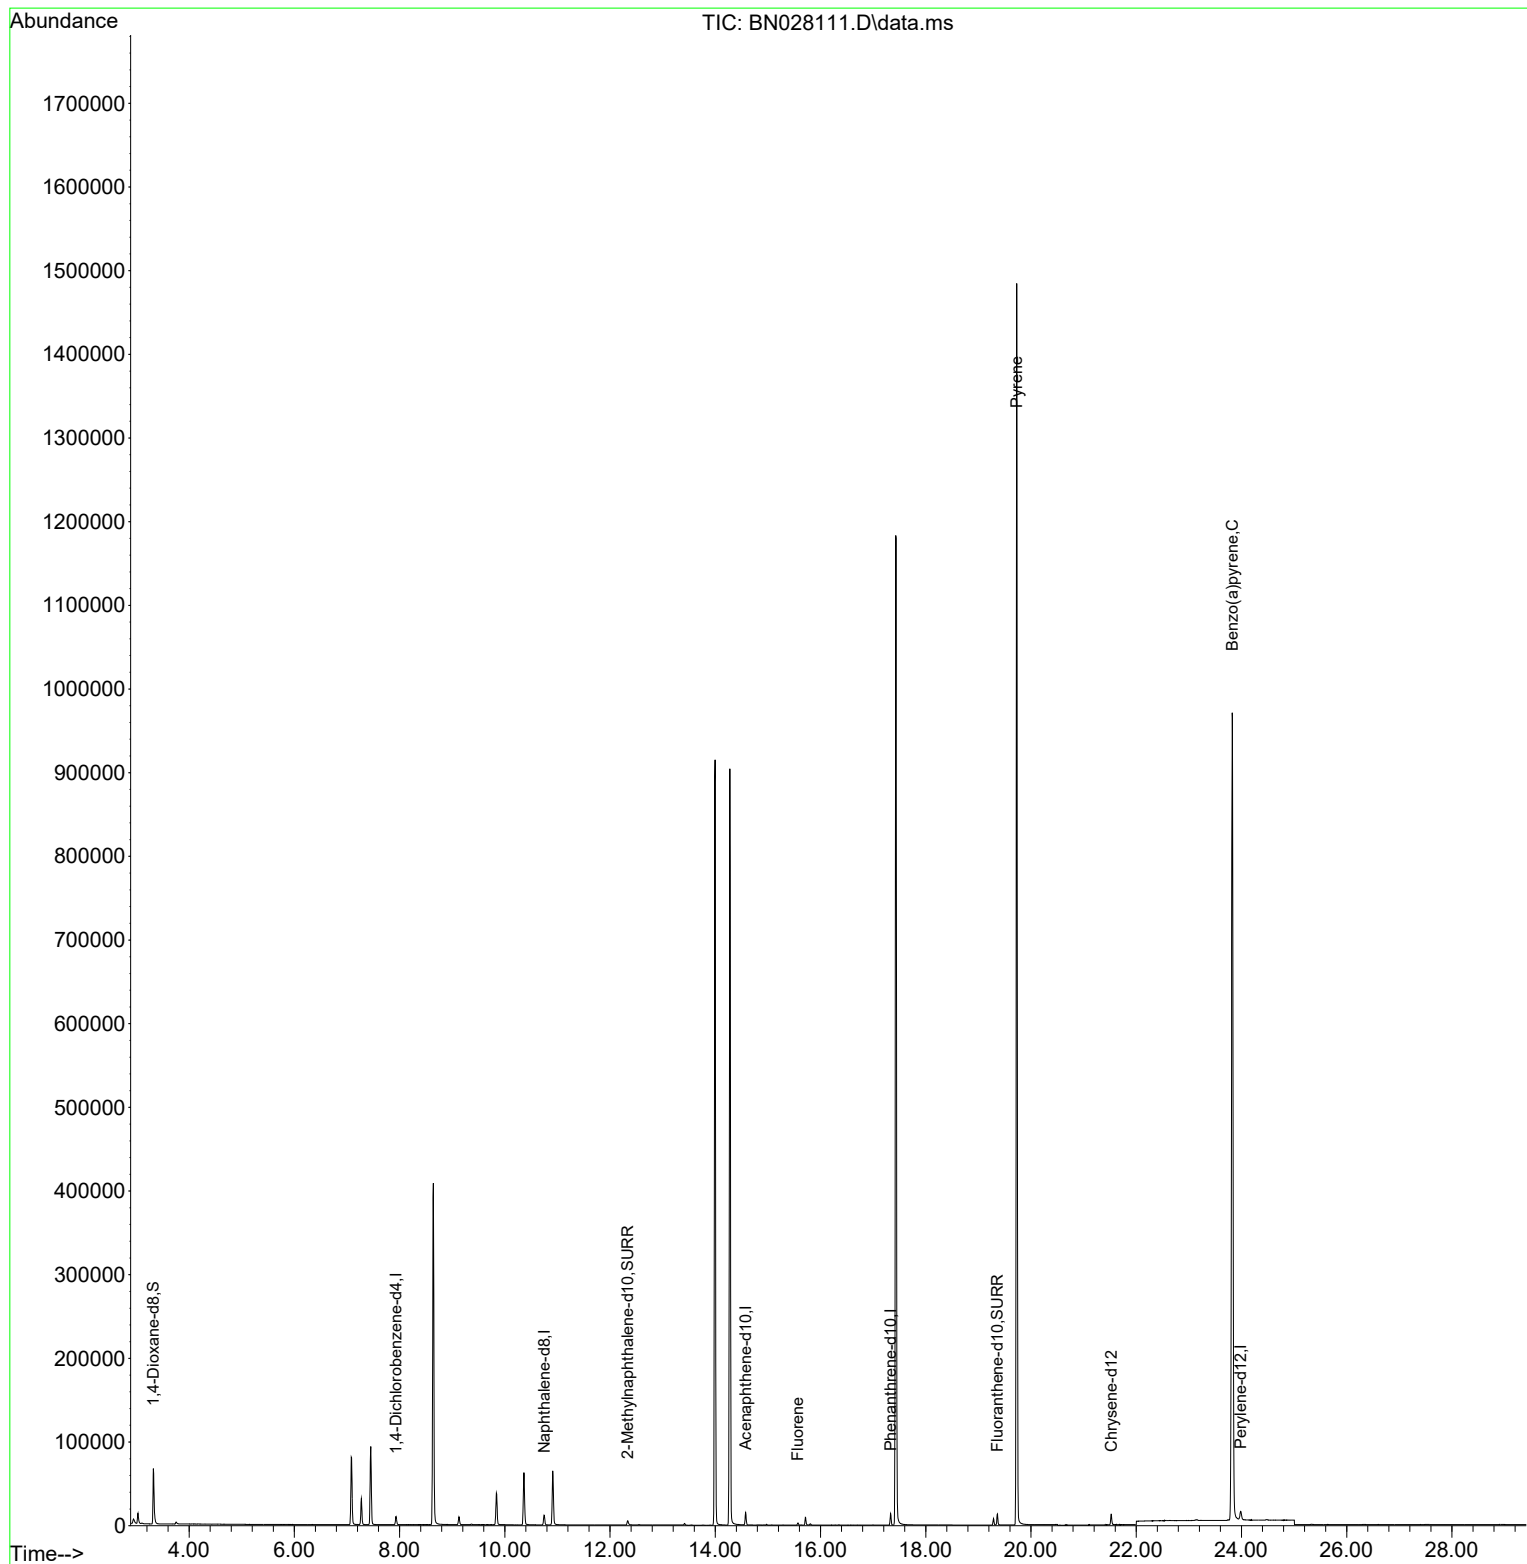


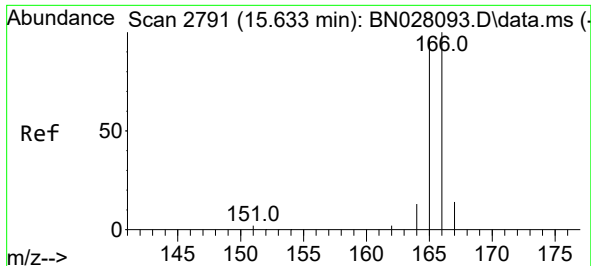

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.568 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN028111.D
Acq: 07 Oct 2023 08:43




Instrument :
BNA_N
ClientSampleId :
SBLK035


Tgt Ion:166 Resp: 2300
Ion Ratio Lower Upper
166 100
165 9.1 78.5 117.7#
167 31.5 11.2 16.8#

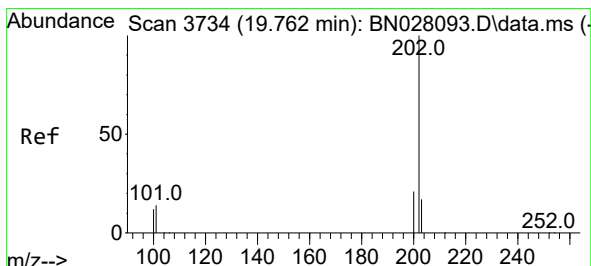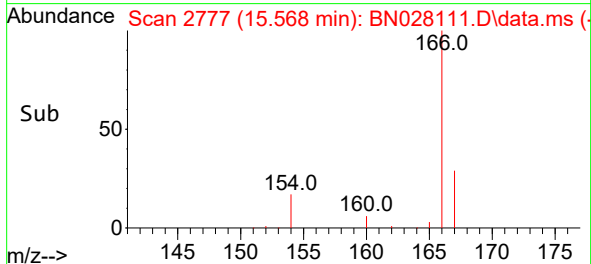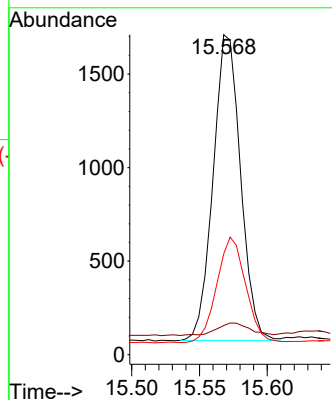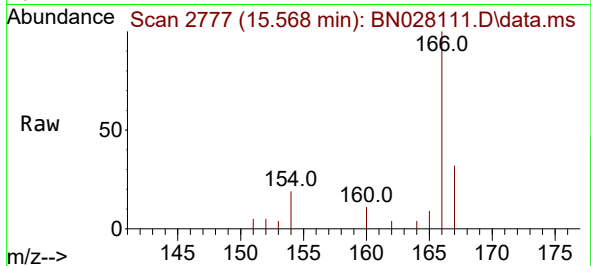

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.729 min Scan# 3727
Delta R.T. -0.028 min
Lab File: BN028111.D
Acq: 07 Oct 2023 08:43


Tgt Ion:202 Resp: 2023
Ion Ratio Lower Upper
202 100
101 160.4 11.2 16.8#
100 1120.7 9.1 13.7#

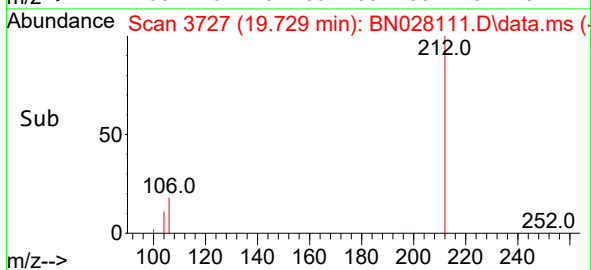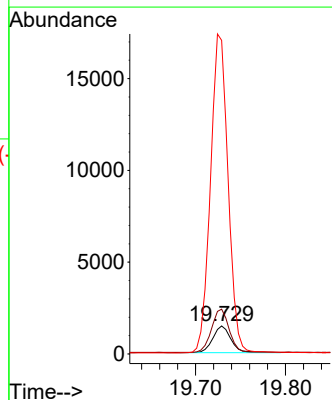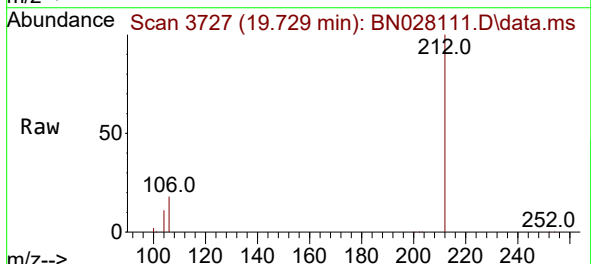

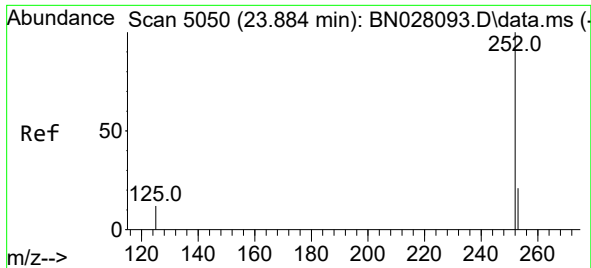

#26
 Benzo(a)pyrene
 Concen: 0.090 ng/ul
 RT: 23.825 min Scan# 50
 Delta R.T. -0.044 min
 Lab File: BN028111.D
 Acq: 07 Oct 2023 08:43

Instrument :
 BNA_N
 ClientSampleId :
 SBLK035

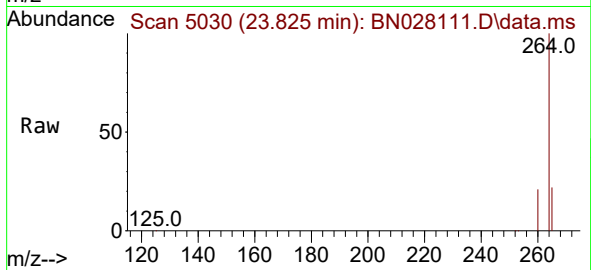

Tgt Ion:252 Resp: 4444
 Ion Ratio Lower Upper
 252 100
 253 57.3 23.4 35.2#
 125 47.3 15.3 22.9#

