

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028123.D
 Acq On : 07 Oct 2023 16:01
 Operator : MA/JU
 Sample : PB155976BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK976

Quant Time: Oct 08 00:51:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	5918	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	18047	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.573	164	9433	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	18447	0.400	ng/ul	0.00
17) Chrysene-d12	21.522	240	15371	0.400	ng/ul	0.00
23) Perylene-d12	23.983	264	17872	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	48254	6.492	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	7964	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	14382	0.295	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.568	166	2359	0.062	ng/ul#	15
20) Pyrene	19.724	202	2026	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.822	252	4680	0.083	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028123.D
Acq On : 07 Oct 2023 16:01
Operator : MA/JU
Sample : PB155976BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK976

Quant Time: Oct 08 00:51:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




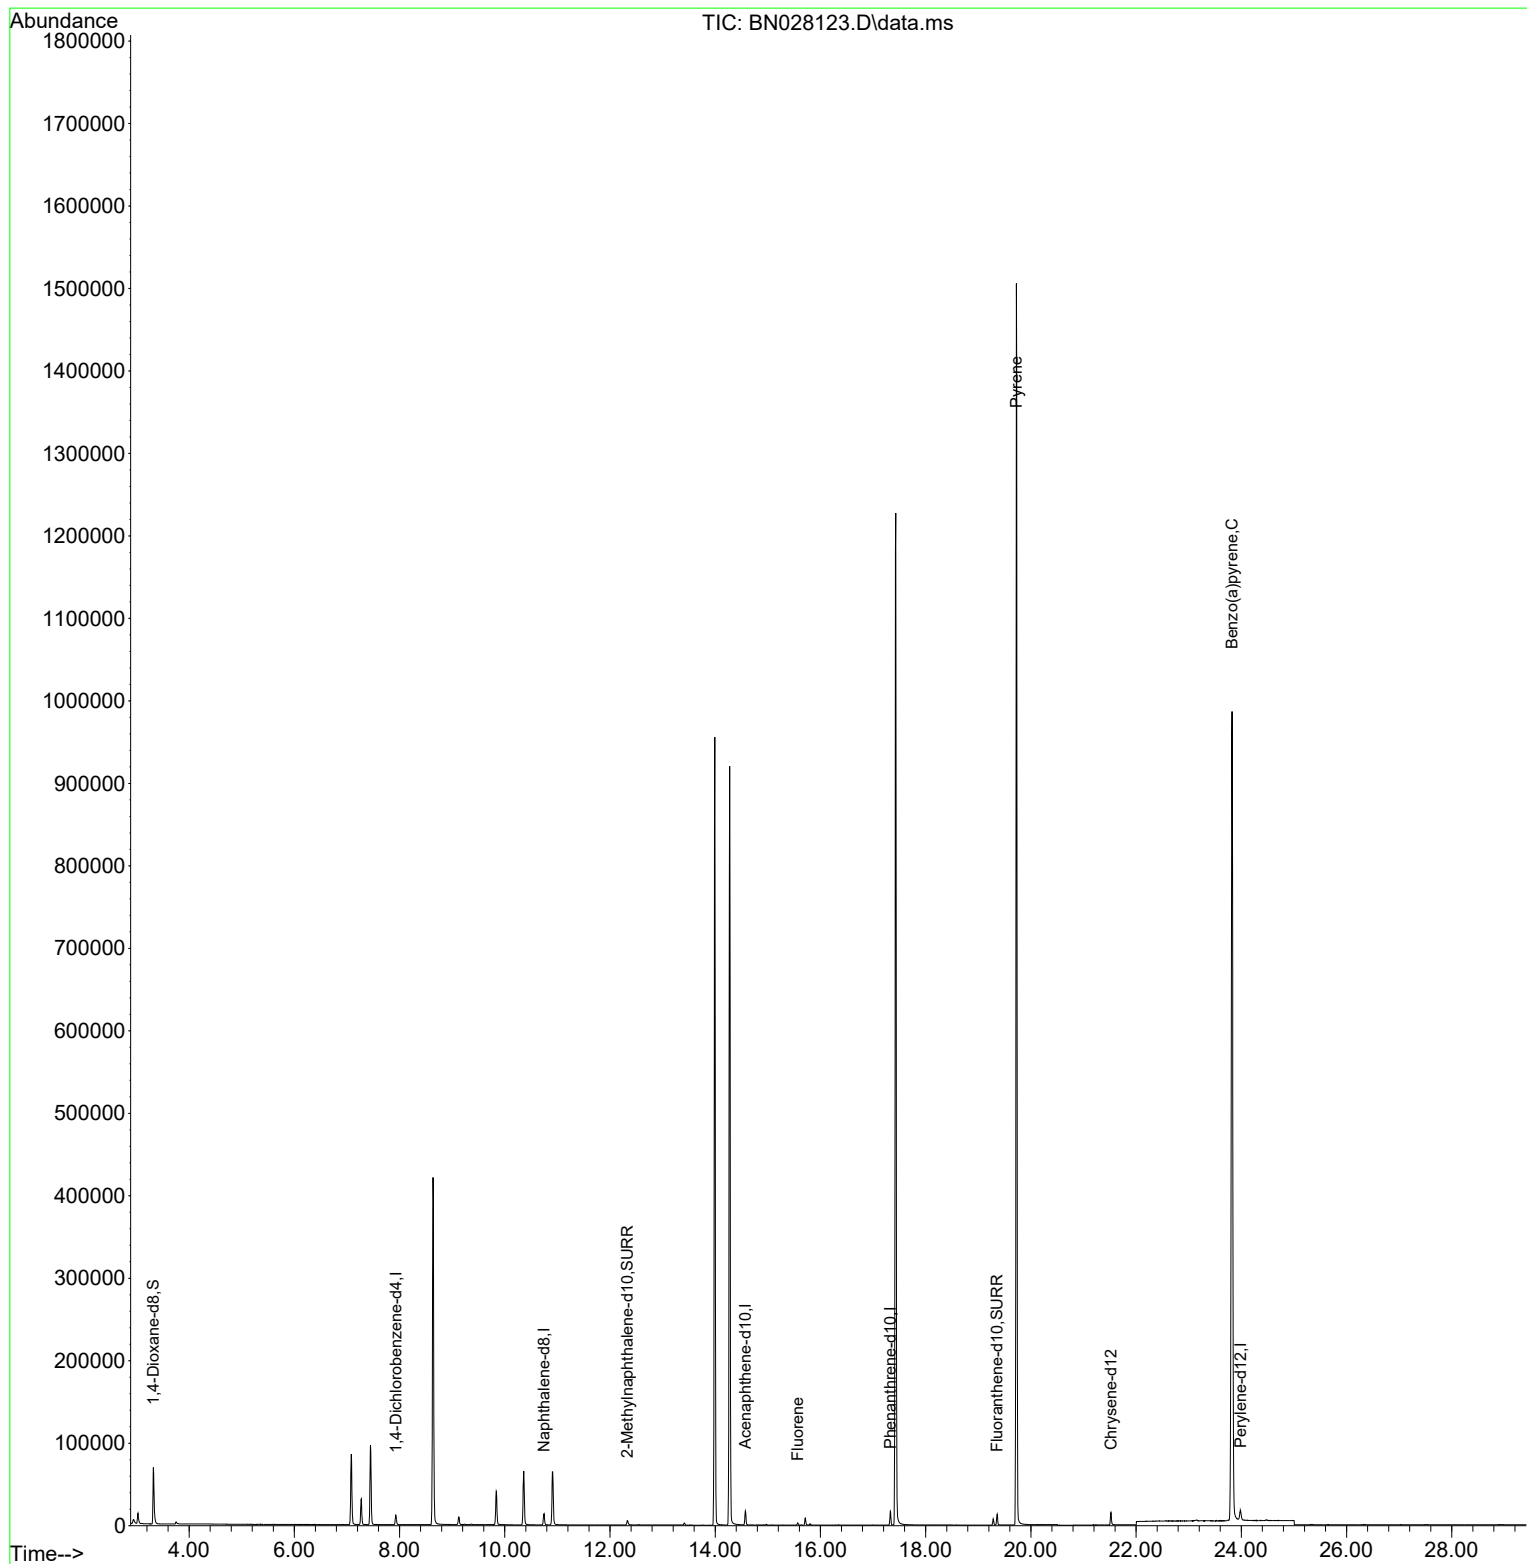


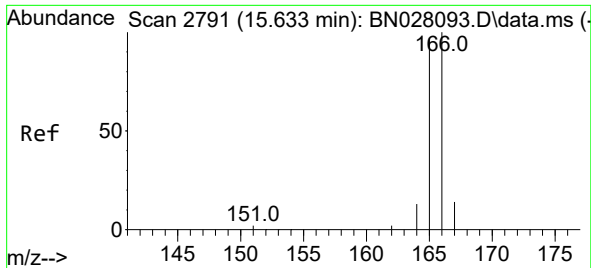

#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.568 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN028123.D
Acq: 07 Oct 2023 16:01




Instrument :
BNA_N
ClientSampleId :
SBLK976


Tgt Ion:166 Resp: 2359
Ion Ratio Lower Upper
166 100
165 9.4 78.5 117.7#
167 35.1 11.2 16.8#

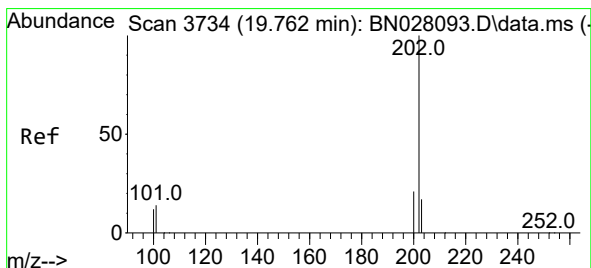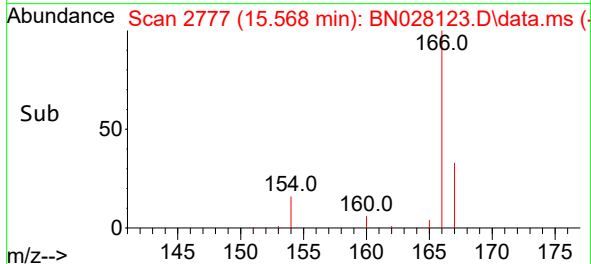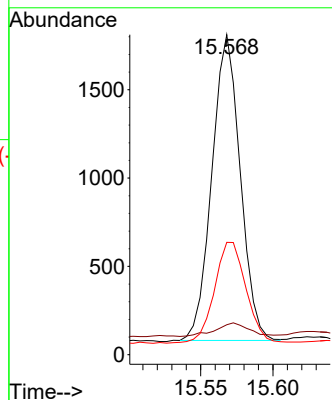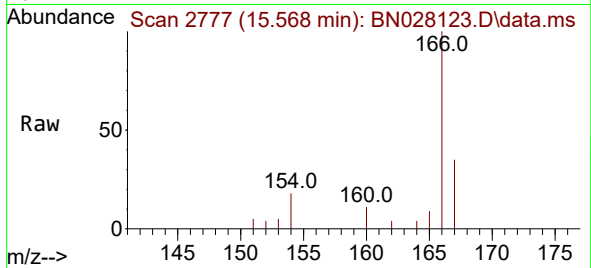

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.724 min Scan# 3726
Delta R.T. -0.033 min
Lab File: BN028123.D
Acq: 07 Oct 2023 16:01


Tgt Ion:202 Resp: 2026
Ion Ratio Lower Upper
202 100
101 165.0 11.2 16.8#
100 1190.7 9.1 13.7#

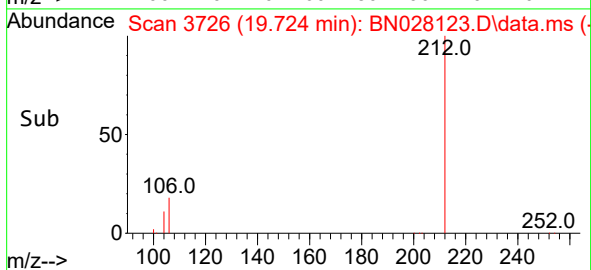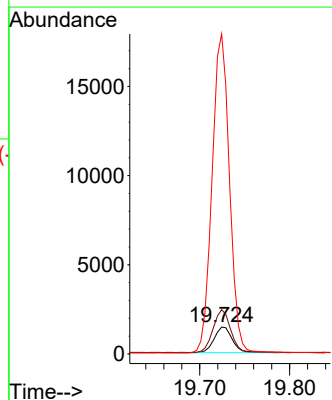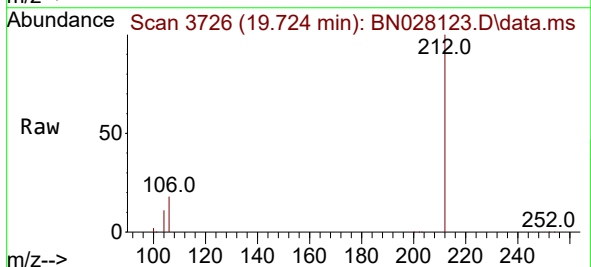

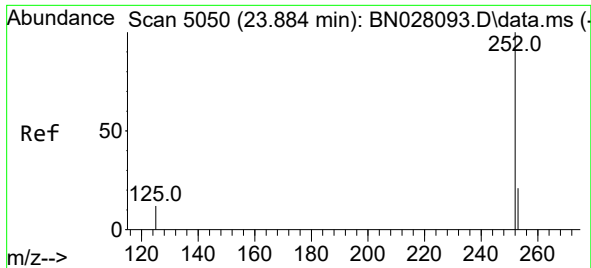

#26
 Benzo(a)pyrene
 Concen: 0.083 ng/ul
 RT: 23.822 min Scan# 50
 Delta R.T. -0.047 min
 Lab File: BN028123.D
 Acq: 07 Oct 2023 16:01

Instrument :
 BNA_N
 ClientSampleId :
 SBLK976

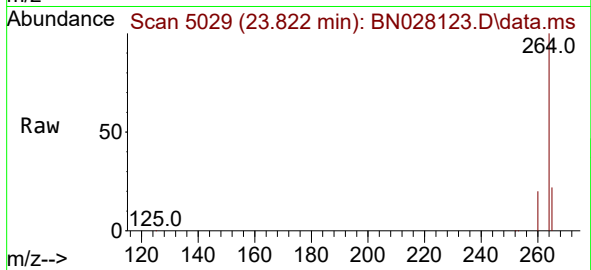

Tgt Ion:252 Resp: 4680
 Ion Ratio Lower Upper
 252 100
 253 56.5 23.4 35.2#
 125 47.2 15.3 22.9#

