

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028128.D
 Acq On : 07 Oct 2023 19:39
 Operator : MA/JU
 Sample : PB155974BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK974

Quant Time: Oct 08 00:52:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	5445	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	16511	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.573	164	8693	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	16774	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	13954	0.400	ng/ul	0.00
23) Perylene-d12	23.980	264	16328	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	49235	7.199	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.329	152	8116	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	14731	0.333	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.568	166	2469	0.071	ng/ul#	15
20) Pyrene	19.724	202	2127	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.819	252	5084	0.098	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028128.D
Acq On : 07 Oct 2023 19:39
Operator : MA/JU
Sample : PB155974BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK974

Quant Time: Oct 08 00:52:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




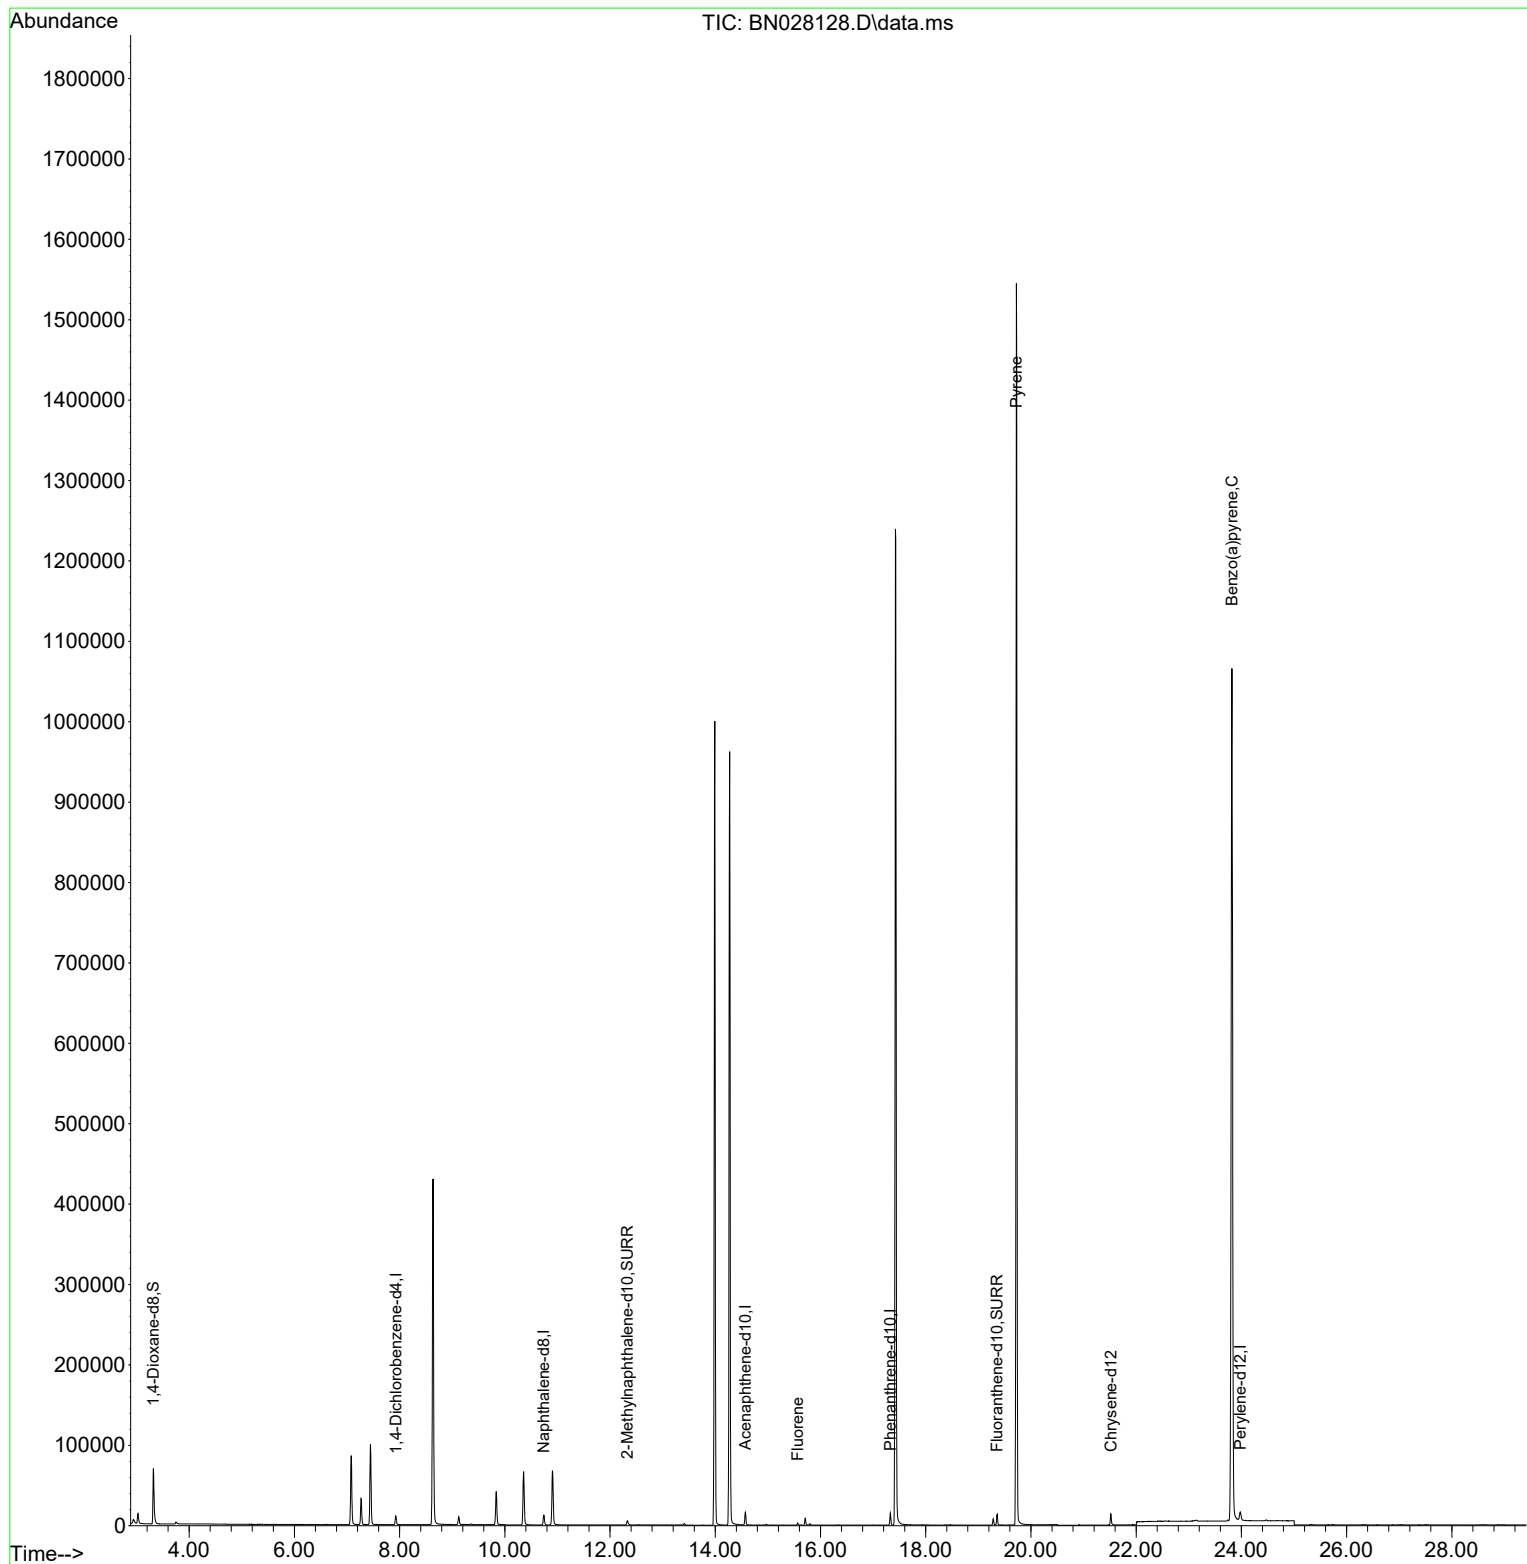


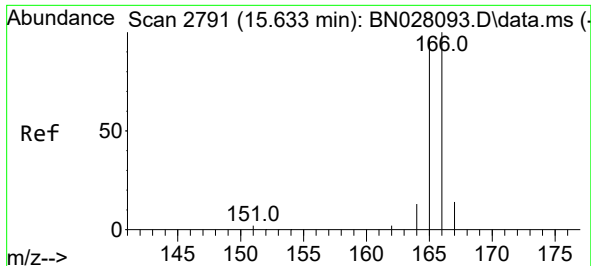

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.568 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN028128.D
Acq: 07 Oct 2023 19:39




Instrument :
BNA_N
ClientSampleId :
SBLK974


Tgt Ion:166 Resp: 2469
Ion Ratio Lower Upper
166 100
165 9.8 78.5 117.7#
167 35.8 11.2 16.8#

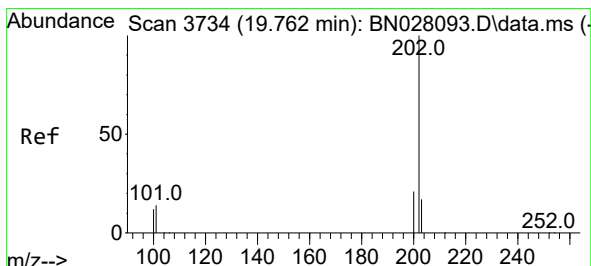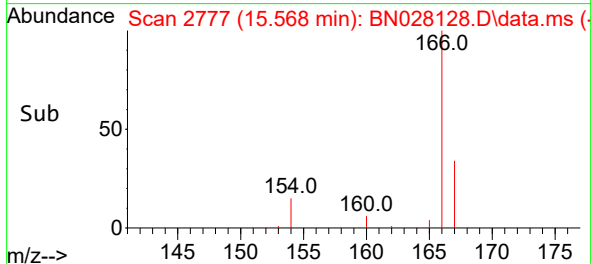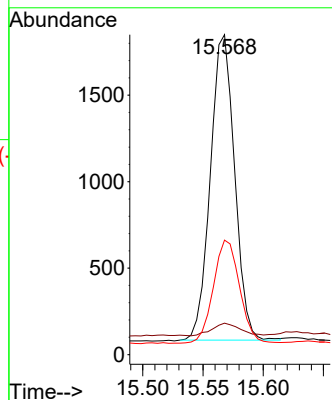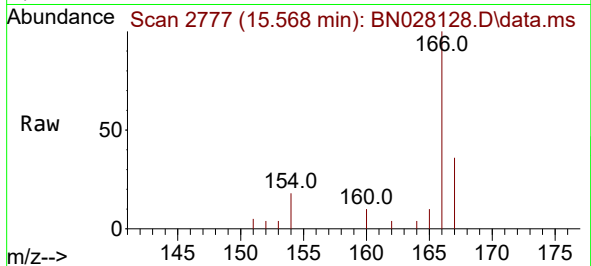

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.724 min Scan# 3726
Delta R.T. -0.033 min
Lab File: BN028128.D
Acq: 07 Oct 2023 19:39

Tgt Ion:202 Resp: 2127
Ion Ratio Lower Upper
202 100
101 169.1 11.2 16.8#
100 1239.4 9.1 13.7#

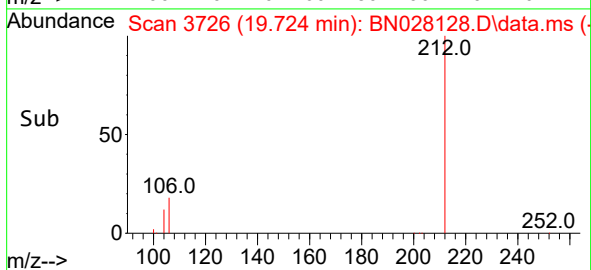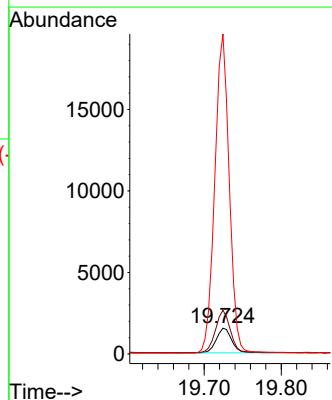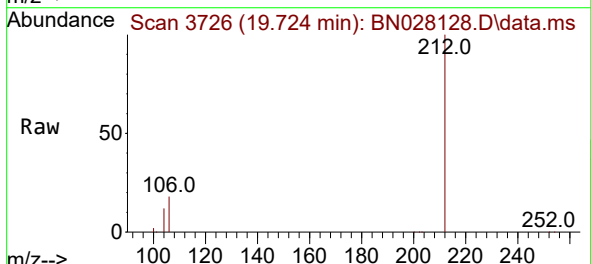

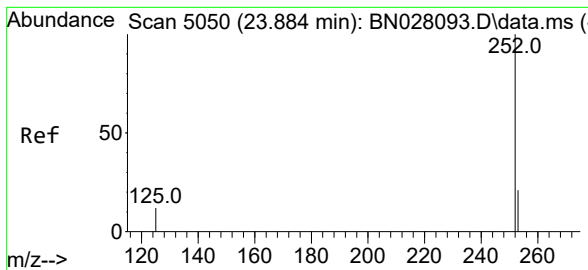

#26

Benzo(a)pyrene

Concen: 0.098 ng/ul

RT: 23.819 min Scan# 50

Delta R.T. -0.050 min

Lab File: BN028128.D


Acq: 07 Oct 2023 19:39

Instrument :

BNA_N

ClientSampleId :

SBLK974

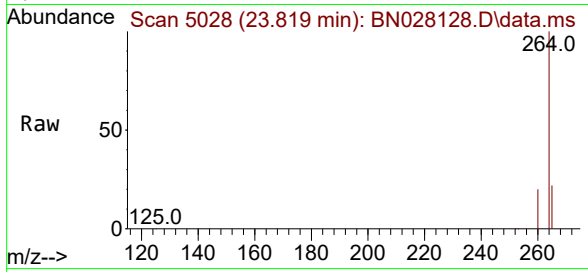

Tgt Ion:252 Resp: 5084

Ion Ratio Lower Upper

252 100

253 54.2 23.4 35.2#

125 43.3 15.3 22.9#

