

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028129.D
 Acq On : 07 Oct 2023 20:15
 Operator : MA/JU
 Sample : PB155978BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK978

Quant Time: Oct 08 00:52:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	5625	0.400	ng/ul	0.00
4) Naphthalene-d8	10.741	136	17020	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.573	164	9031	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	17406	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	14515	0.400	ng/ul	0.00
23) Perylene-d12	23.980	264	16642	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	55282	7.824	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	9349	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	17301	0.376	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.568	166	2807	0.077	ng/ul#	15
20) Pyrene	19.724	202	2455	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.819	252	6164	0.117	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028129.D
Acq On : 07 Oct 2023 20:15
Operator : MA/JU
Sample : PB155978BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Time: Oct 08 00:52:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




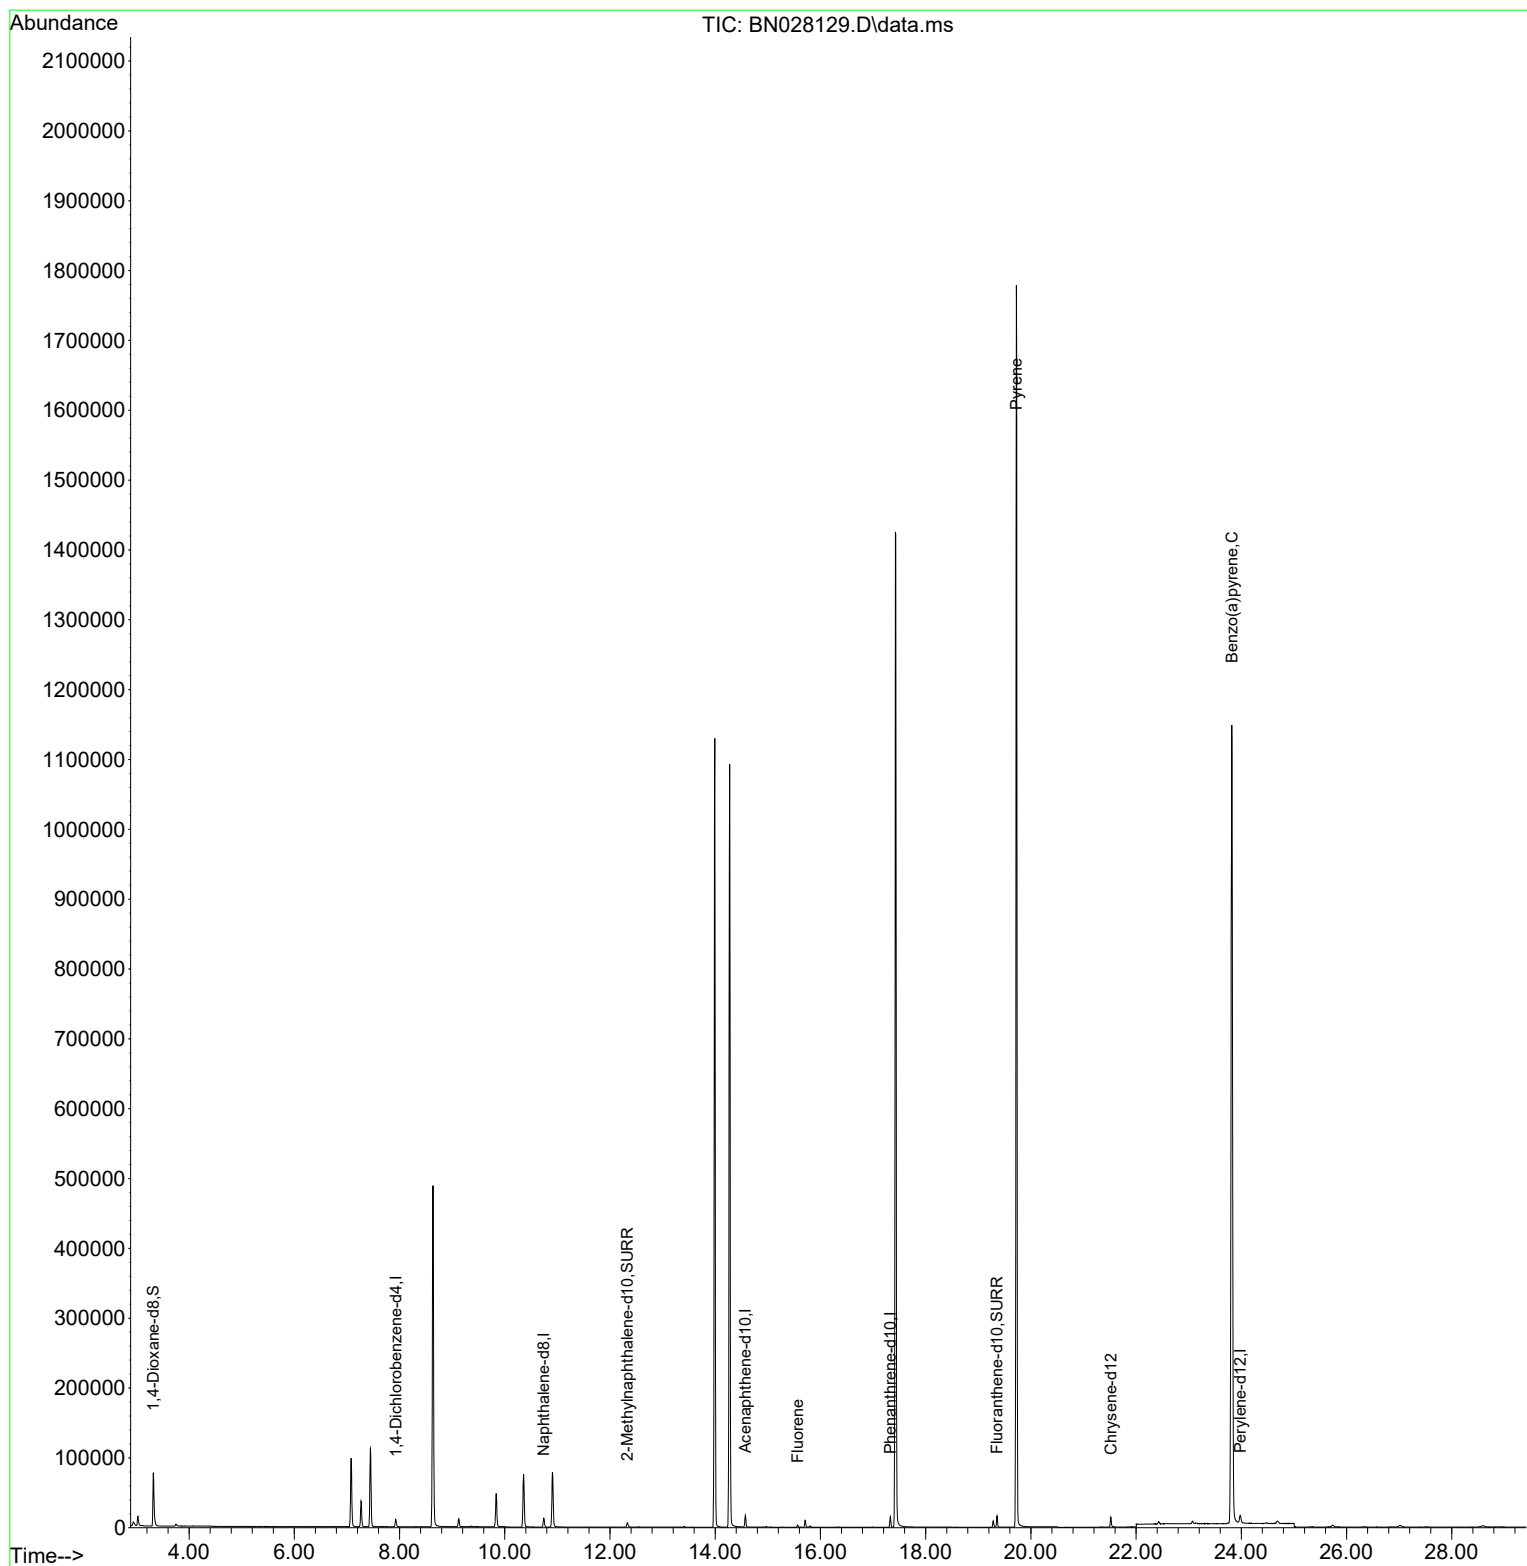


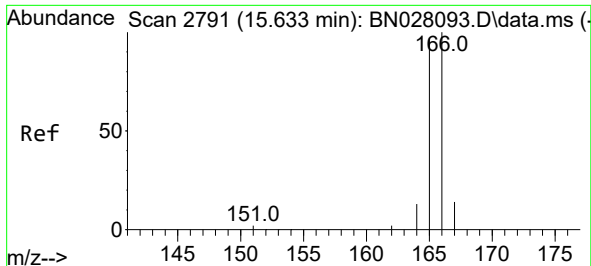

#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.568 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN028129.D
Acq: 07 Oct 2023 20:15




Instrument :
BNA_N
ClientSampleId :
SBLK978


Tgt Ion:166 Resp: 2807
Ion Ratio Lower Upper
166 100
165 9.5 78.5 117.7#
167 36.3 11.2 16.8#

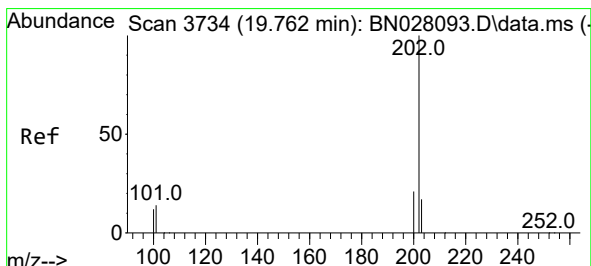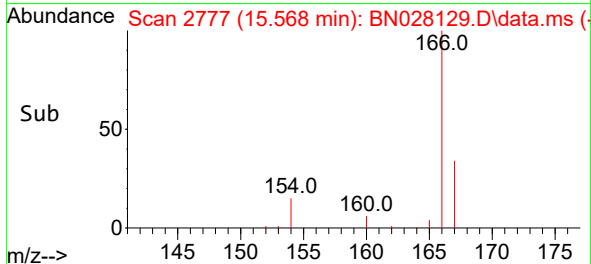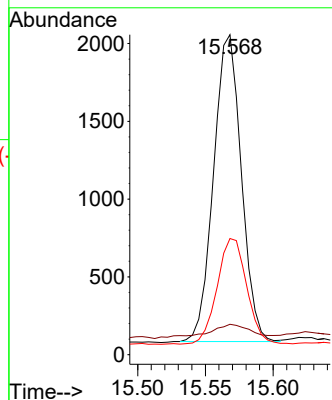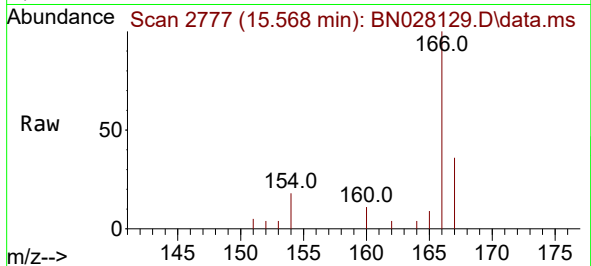

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.724 min Scan# 3726
Delta R.T. -0.033 min
Lab File: BN028129.D
Acq: 07 Oct 2023 20:15


Tgt Ion:202 Resp: 2455
Ion Ratio Lower Upper
202 100
101 166.9 11.2 16.8#
100 1224.4 9.1 13.7#

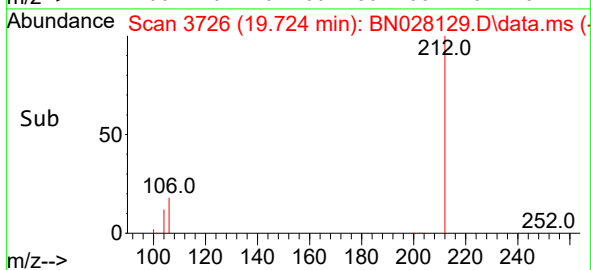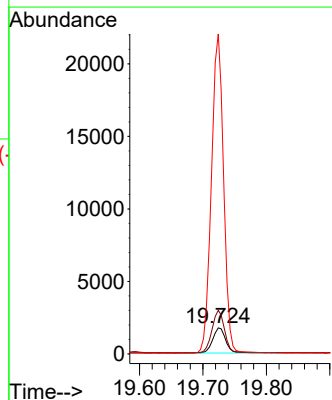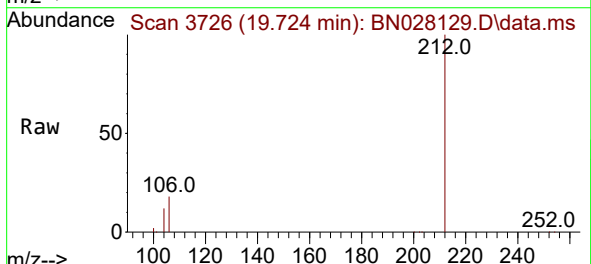

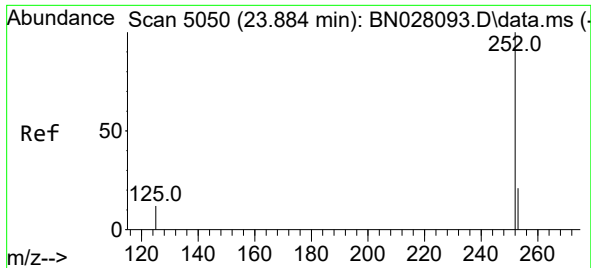

#26
Benzo(a)pyrene
Concen: 0.117 ng/ul
RT: 23.819 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN028129.D
Acq: 07 Oct 2023 20:15

Instrument :
BNA_N
ClientSampleId :
SBLK978

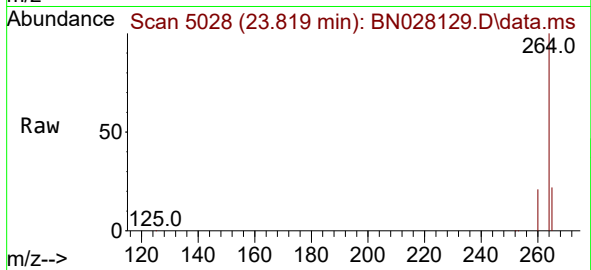

Tgt Ion:252 Resp: 6164
Ion Ratio Lower Upper
252 100
253 55.8 23.4 35.2#
125 41.0 15.3 22.9#

