

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028145.D
 Acq On : 08 Oct 2023 06:33
 Operator : MA/JU
 Sample : PB155980BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK980

Quant Time: Oct 09 00:46:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	5300	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	15728	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.569	164	8230	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.329	188	16058	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	13268	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264	15281	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	50190	7.539	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.330	152	8149	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	14860	0.353	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.563	166	2469	0.075	ng/ul#	15
20) Pyrene	19.724	202	2167	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.819	252	5178	0.107	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028145.D
Acq On : 08 Oct 2023 06:33
Operator : MA/JU
Sample : PB155980BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK980

Quant Time: Oct 09 00:46:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




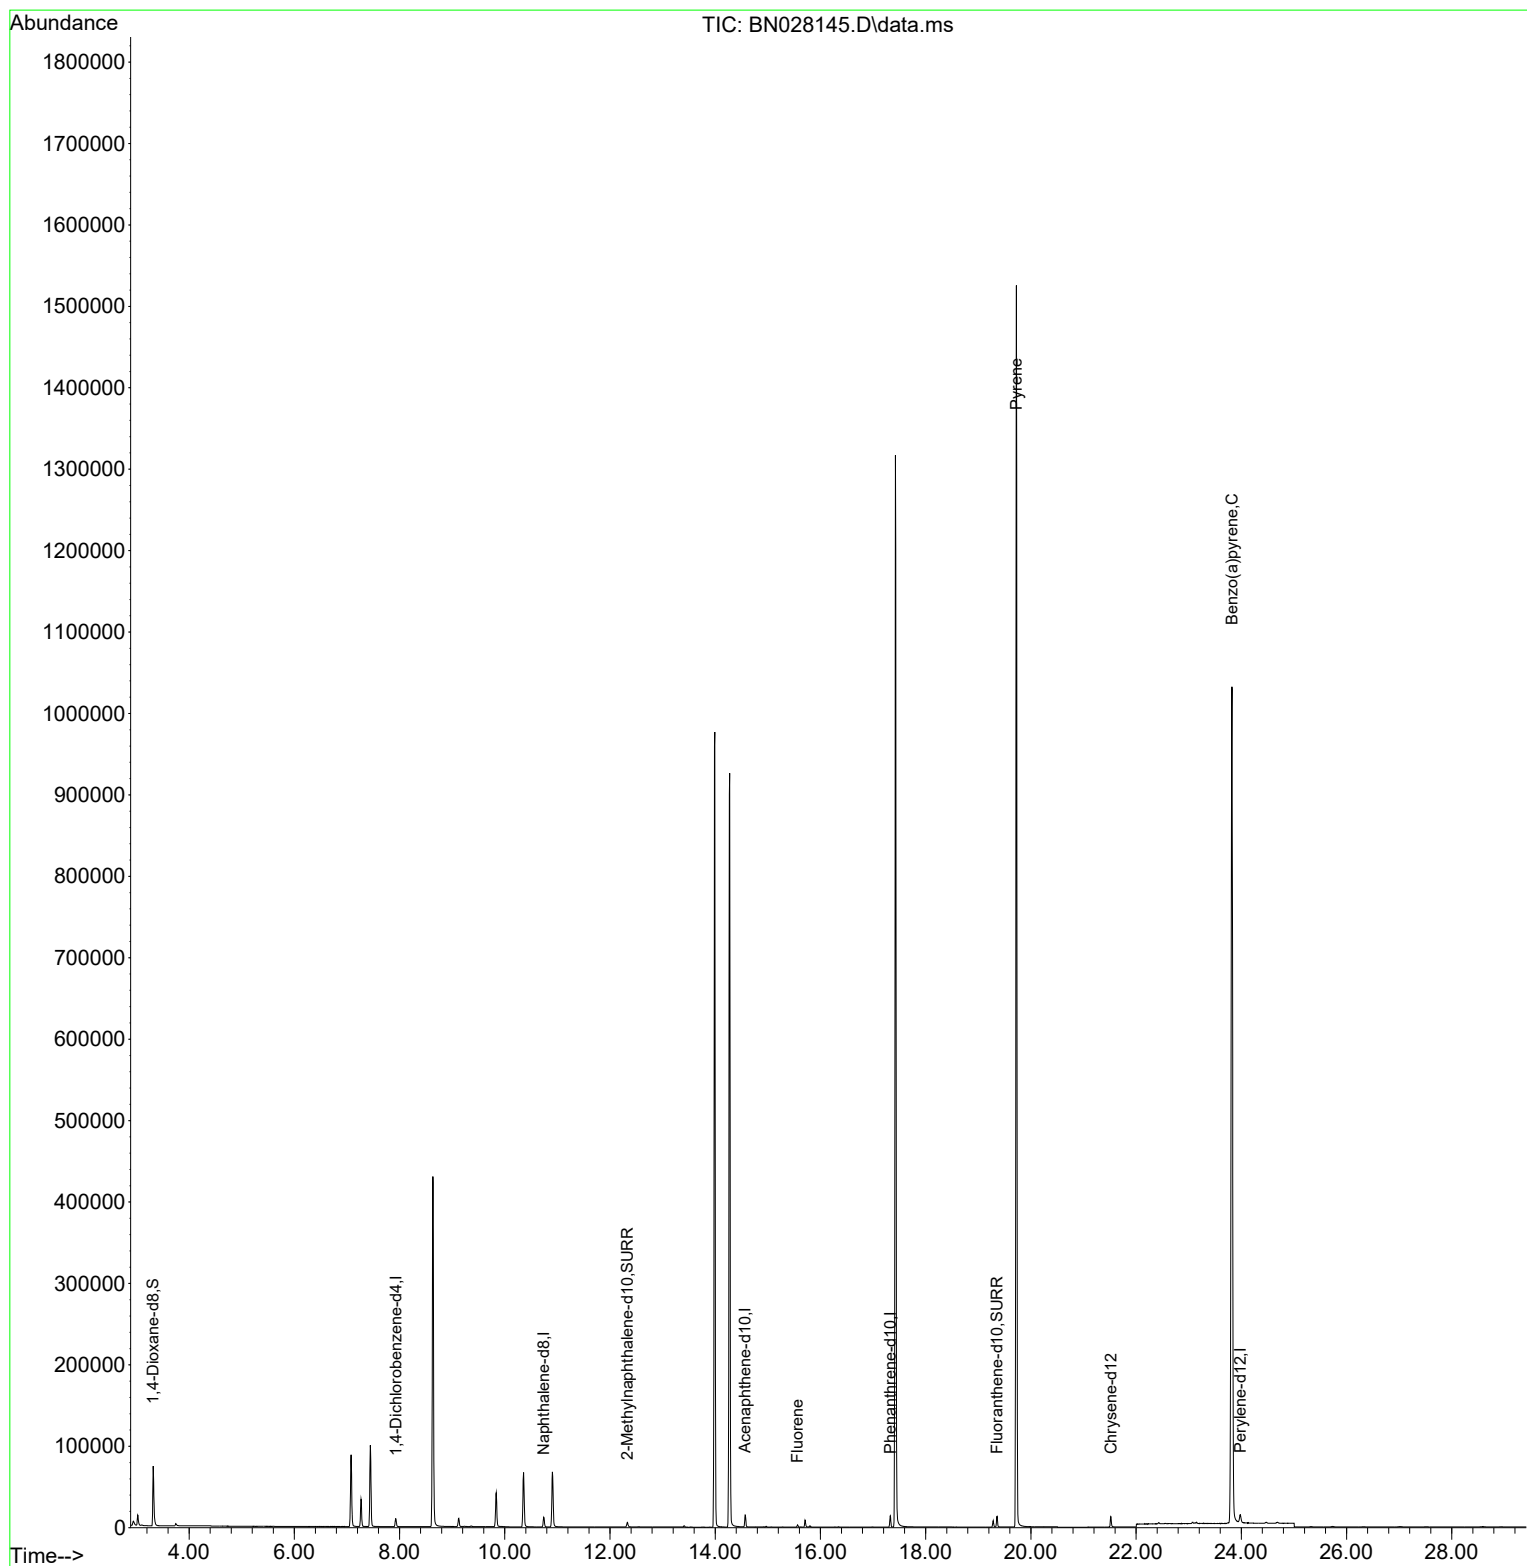


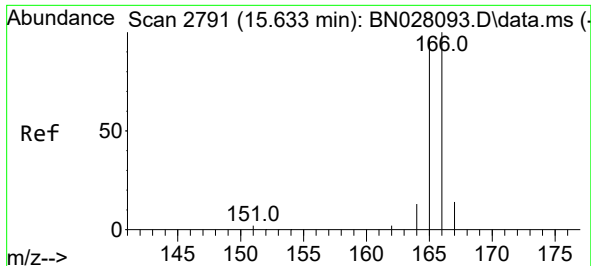

#12
Fluorene
Concen: 0.075 ng/ul
RT: 15.563 min Scan# 21
Delta R.T. -0.069 min
Lab File: BN028145.D
Acq: 08 Oct 2023 06:33




Instrument :
BNA_N
ClientSampleId :
SBLK980


Tgt Ion:166 Resp: 2469
Ion Ratio Lower Upper
166 100
165 9.4 78.5 117.7#
167 33.9 11.2 16.8#

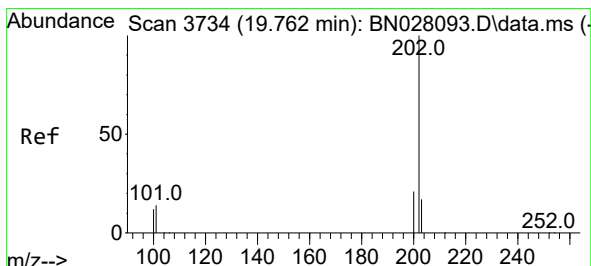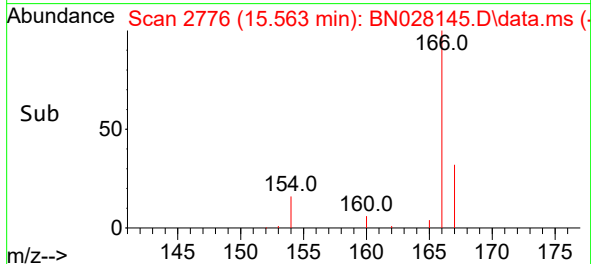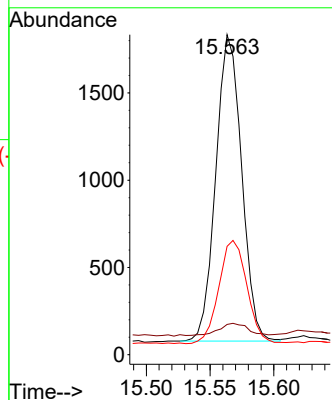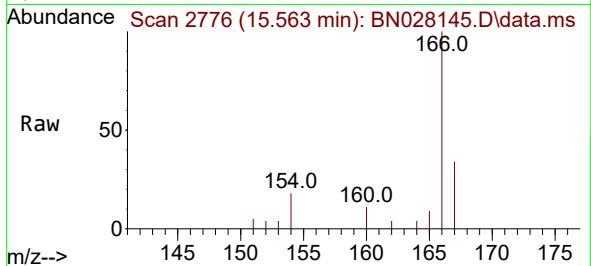

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.724 min Scan# 3726
Delta R.T. -0.033 min
Lab File: BN028145.D
Acq: 08 Oct 2023 06:33


Tgt Ion:202 Resp: 2167
Ion Ratio Lower Upper
202 100
101 166.9 11.2 16.8#
100 1186.8 9.1 13.7#

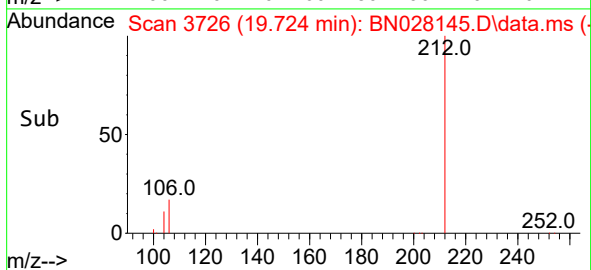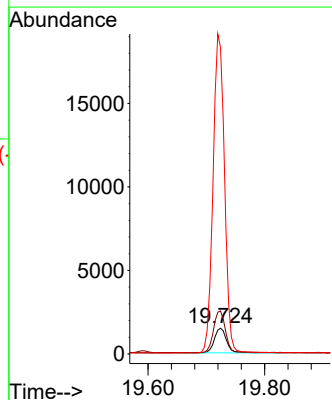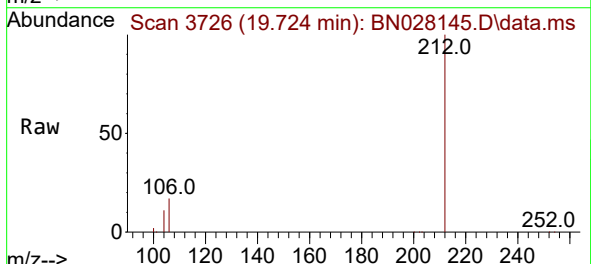

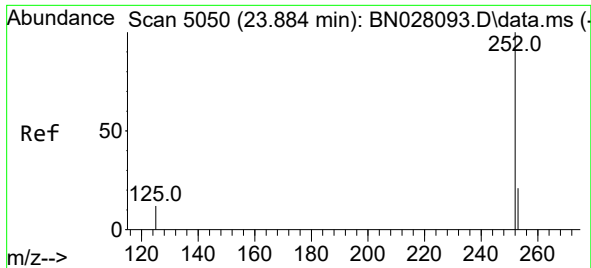

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.819 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN028145.D
Acq: 08 Oct 2023 06:33

Instrument :
BNA_N
ClientSampleId :
SBLK980

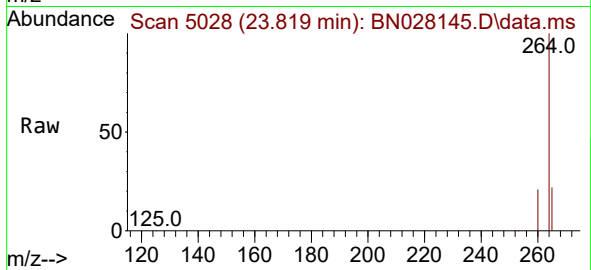

Tgt Ion:252 Resp: 5178
Ion Ratio Lower Upper
252 100
253 53.4 23.4 35.2#
125 42.5 15.3 22.9#

