

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028146.D
 Acq On : 08 Oct 2023 07:09
 Operator : MA/JU
 Sample : PB155982BL
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK982

Quant Time: Oct 09 00:46:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.924	152	4505	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.741	136	13704	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.569	164	7170	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.325	188	13983	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	11595	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264	13286	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	48836	8.631	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.330	152	7835	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	14480	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.564	166	2366	0.082	ng/ul#	16
20) Pyrene	19.725	202	2067	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.816	252	4973	0.118	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028146.D
Acq On : 08 Oct 2023 07:09
Operator : MA/JU
Sample : PB155982BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK982

Quant Time: Oct 09 00:46:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




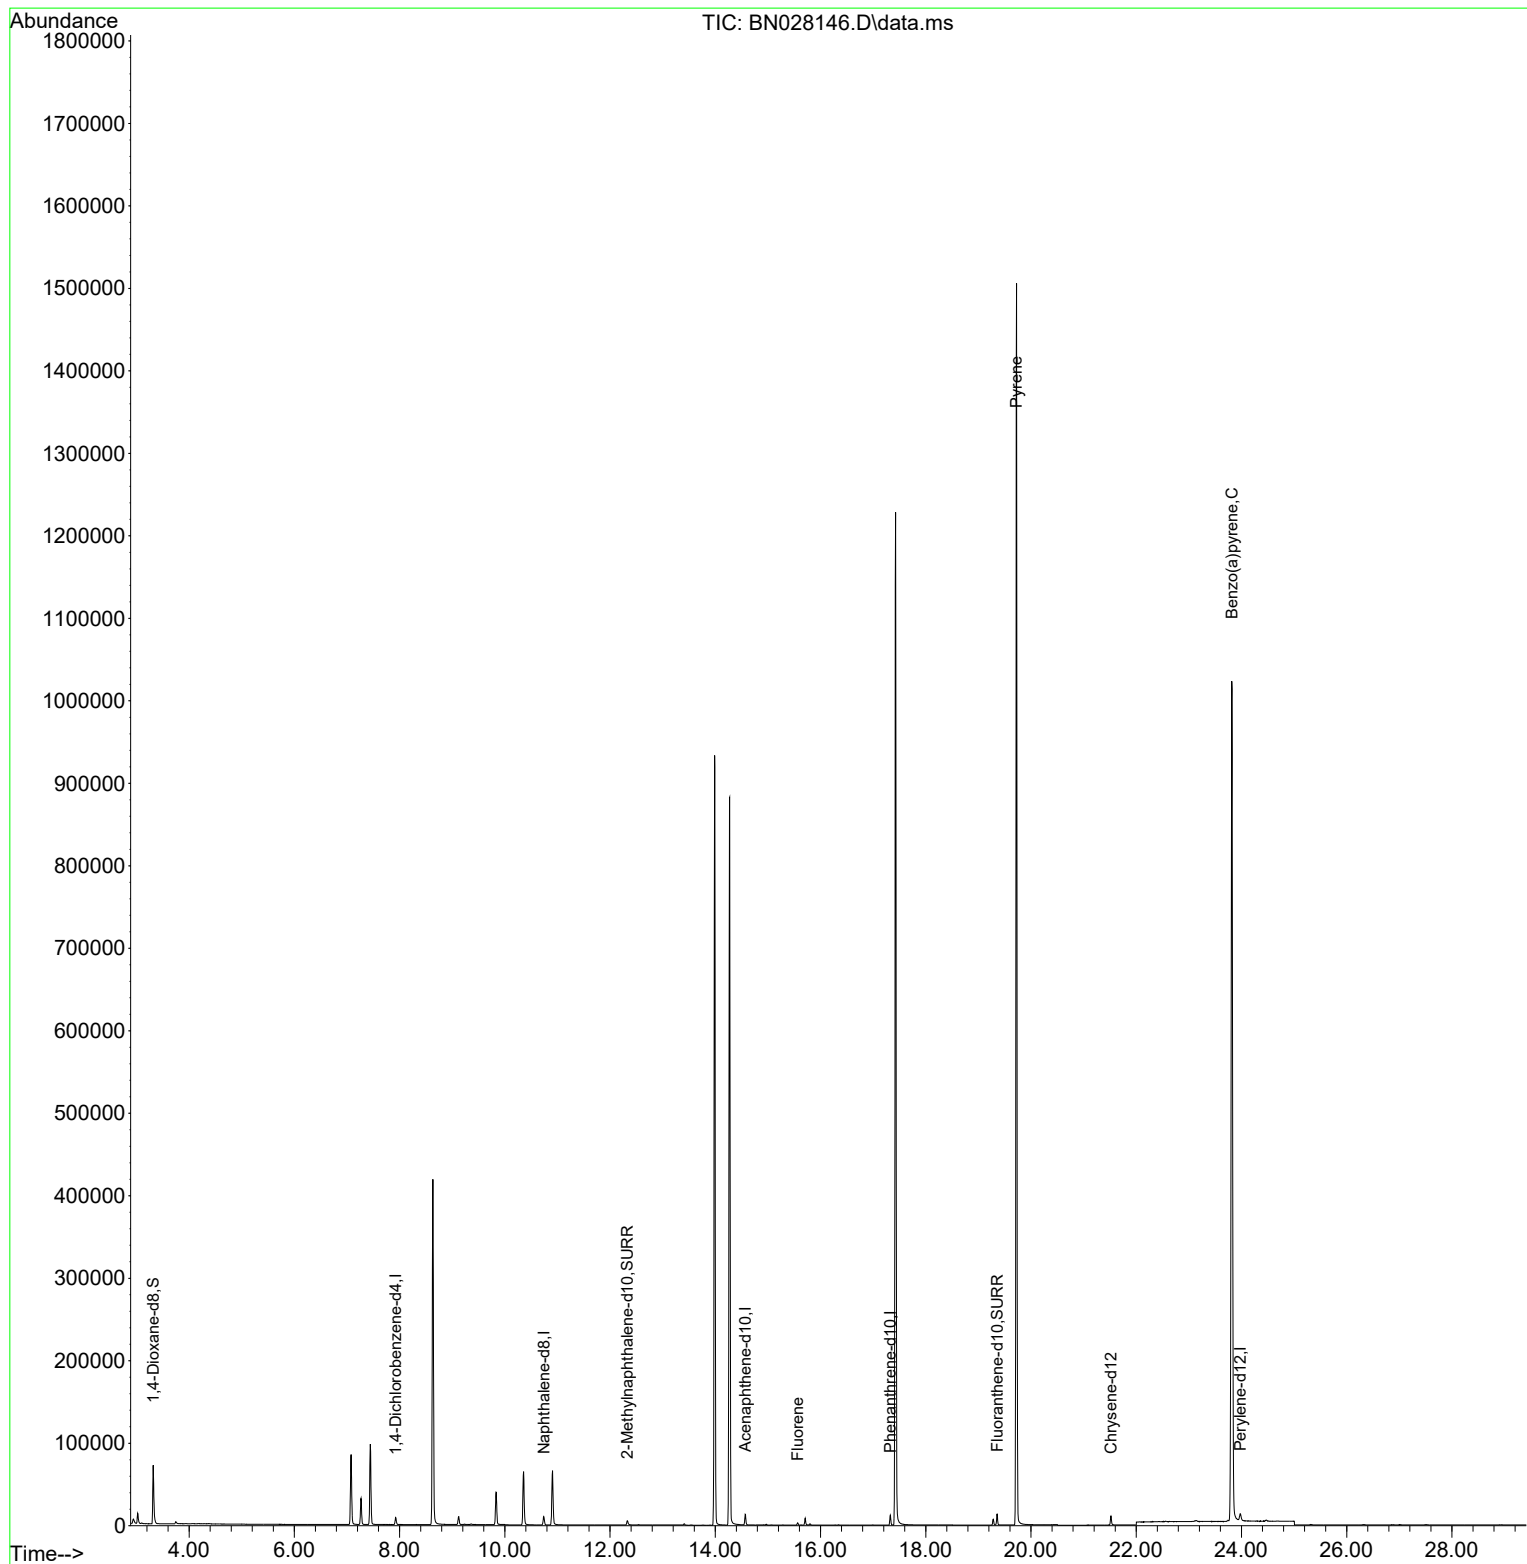


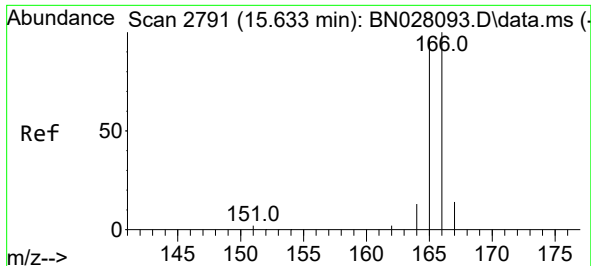

#12
Fluorene
Concen: 0.082 ng/ul
RT: 15.564 min Scan# 21
Delta R.T. -0.069 min
Lab File: BN028146.D
Acq: 08 Oct 2023 07:09




Instrument :
BNA_N
ClientSampleId :
SBLK982


Tgt Ion:166 Resp: 2366
Ion Ratio Lower Upper
166 100
165 9.6 78.5 117.7#
167 33.9 11.2 16.8#

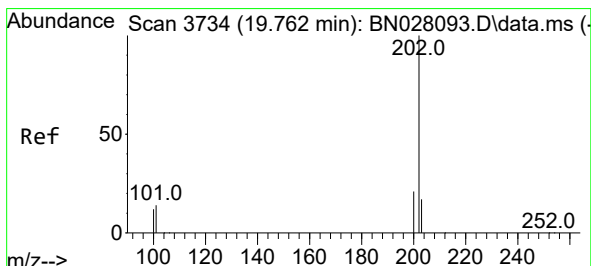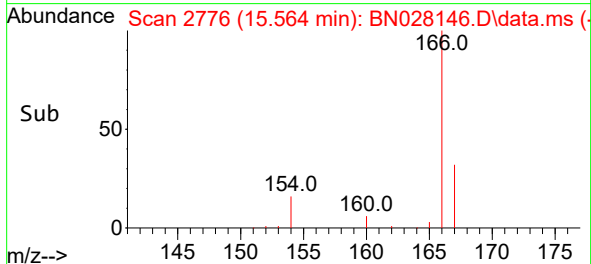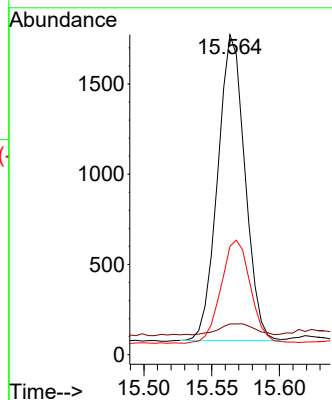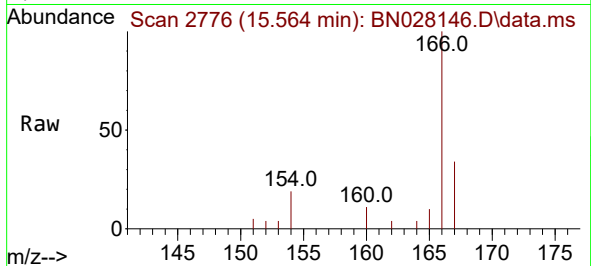

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.725 min Scan# 3726
Delta R.T. -0.032 min
Lab File: BN028146.D
Acq: 08 Oct 2023 07:09


Tgt Ion:202 Resp: 2067
Ion Ratio Lower Upper
202 100
101 157.5 11.2 16.8#
100 1123.6 9.1 13.7#

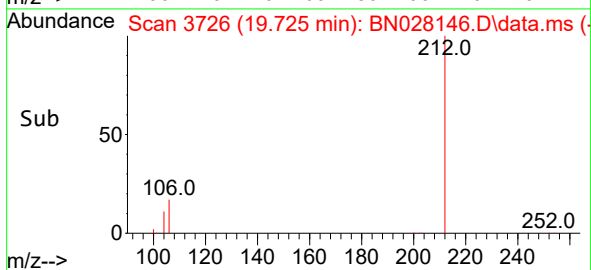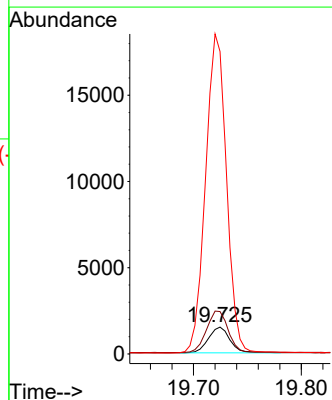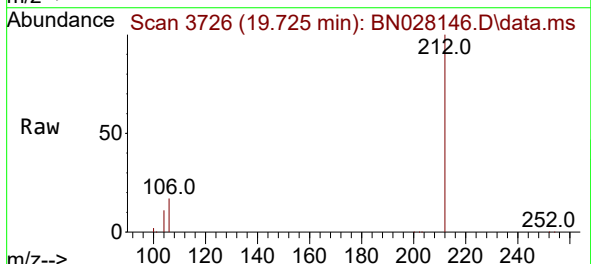

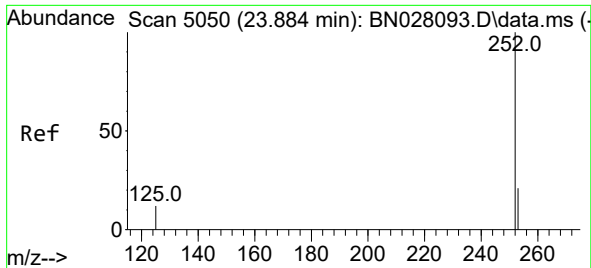

#26
 Benzo(a)pyrene
 Concen: 0.118 ng/ul
 RT: 23.816 min Scan# 50
 Delta R.T. -0.053 min
 Lab File: BN028146.D
 Acq: 08 Oct 2023 07:09

Instrument :
 BNA_N
 ClientSampleId :
 SBLK982

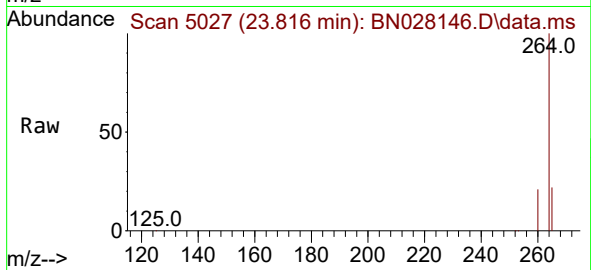

Tgt Ion:252 Resp: 4973
 Ion Ratio Lower Upper
 252 100
 253 52.7 23.4 35.2#
 125 42.0 15.3 22.9#

