




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028049.D
 Acq On : 05 Oct 2023 15:16
 Operator : MA/JU
 Sample : PB155824BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Manual IntegrationsAPPROVED

Quant Time: Oct 05 16:28:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

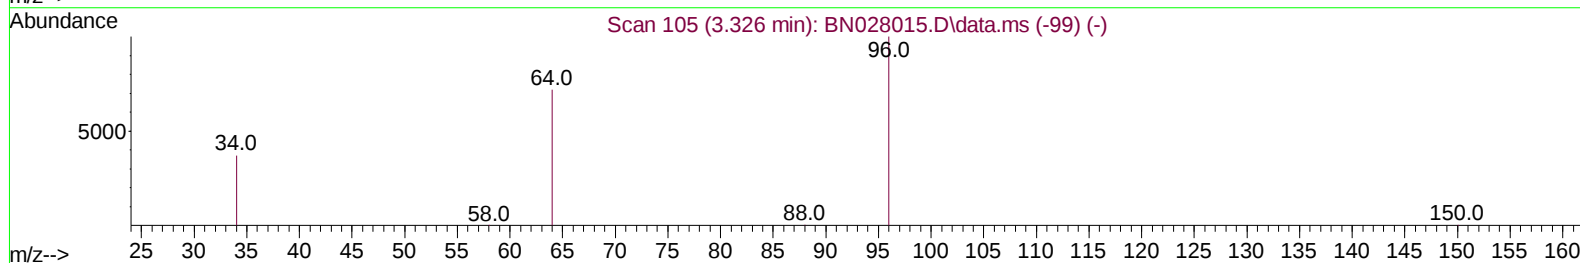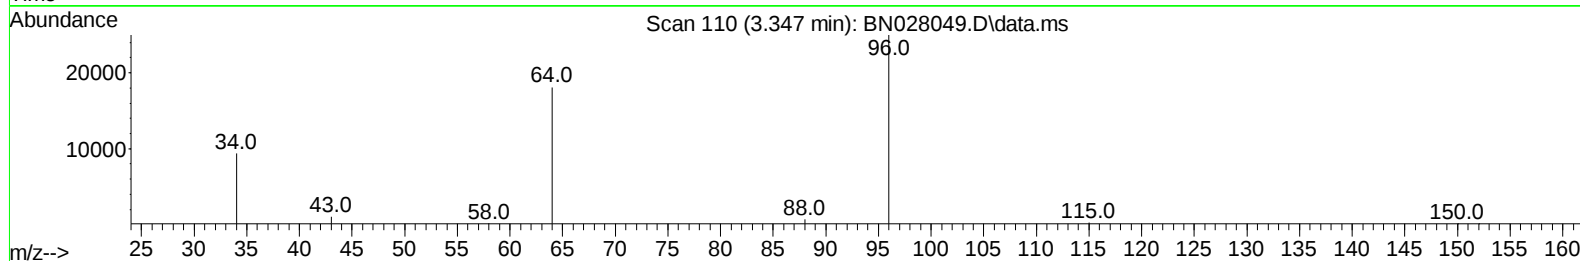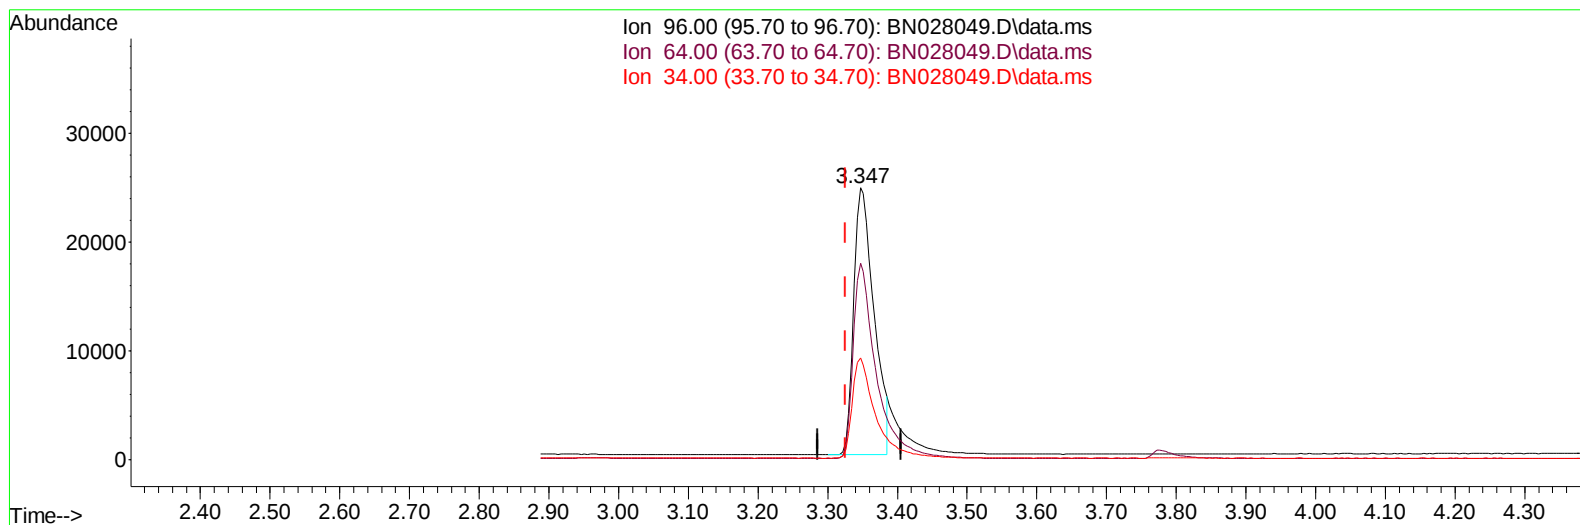

TIC: BN028049.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.347min (+ 0.021) 4.45 ng/u1

response 49500

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.70	72.37
34.00	37.00	37.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028049.D
 Acq On : 05 Oct 2023 15:16
 Operator : MA/JU
 Sample : PB155824BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Manual IntegrationsAPPROVED

Quant Time: Oct 05 16:28:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

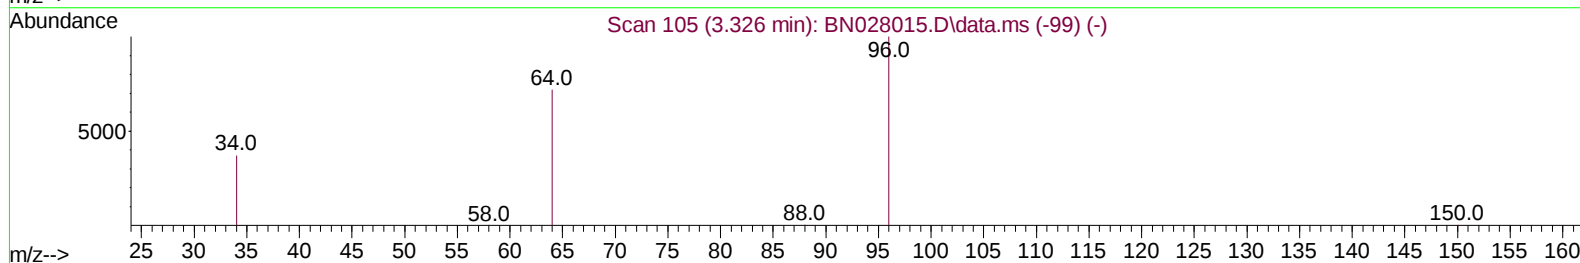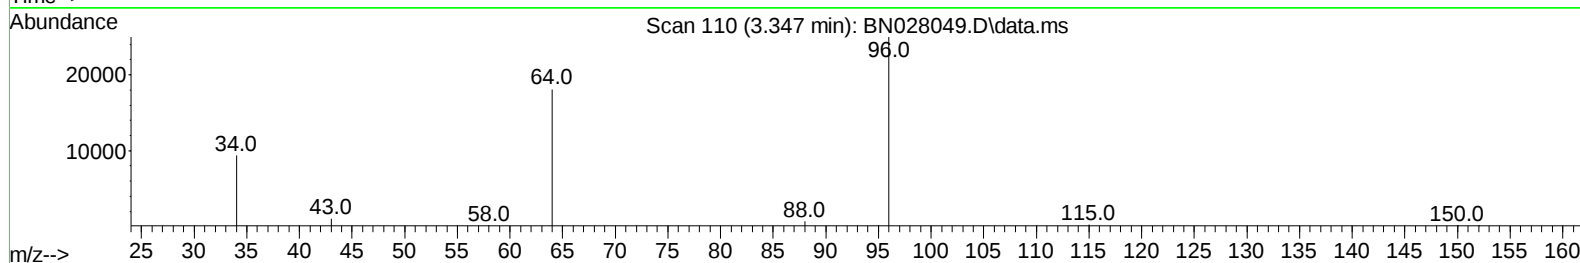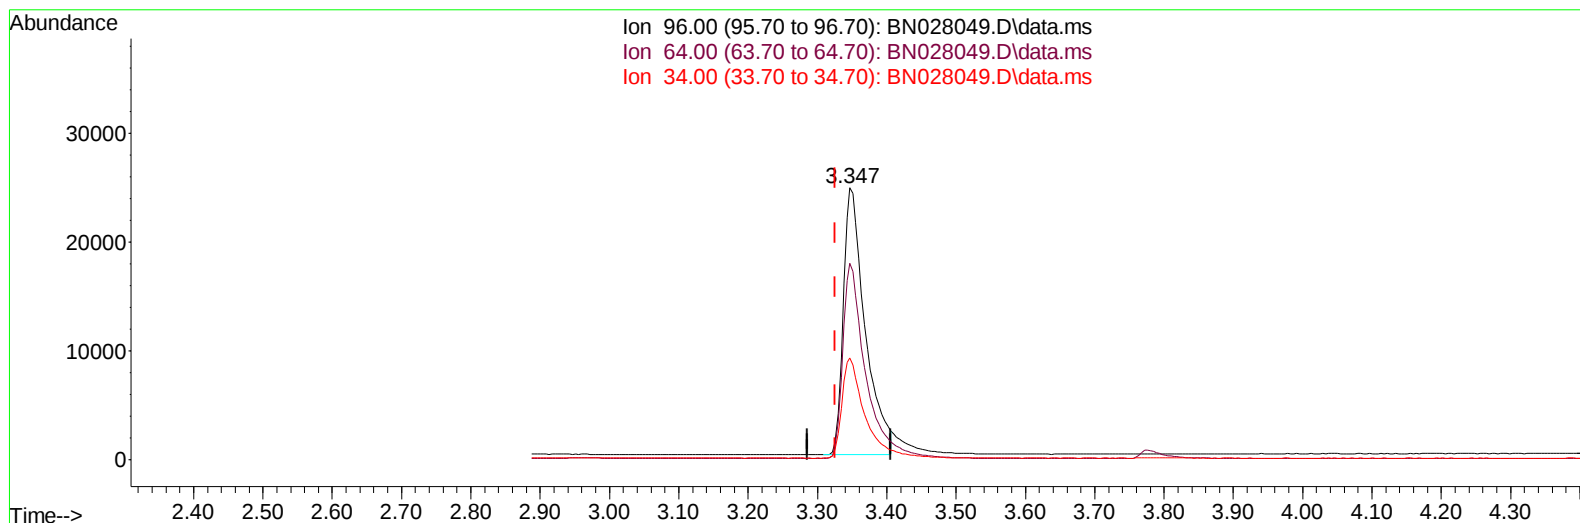

TIC: BN028049.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.347min (+ 0.021) 4.82 ng/ul m

response 53614

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.70	72.37
34.00	37.00	37.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028049.D
 Acq On : 05 Oct 2023 15:16
 Operator : MA/JU
 Sample : PB155824BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK824

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

Quant Time: Oct 05 16:28:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	8857	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	26503	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.578	164	14338	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.337	188	28411	0.400	ng/ul	-0.01
17) Chrysene-d12	21.524	240	24012	0.400	ng/ul	-0.01
23) Perylene-d12	23.988	264	27487	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.347	96	53614m	4.819	ng/ul	0.02
6) 2-Methylnaphthalene-d10	12.335	152	10643	0.249	ng/ul	-0.02
18) Fluoranthene-d10	19.362	212	19776	0.260	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028049.D
Acq On : 05 Oct 2023 15:16
Operator : MA/JU
Sample : PB155824BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK824

Manual IntegrationsAPPROVED

Quant Time: Oct 05 16:28:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :mohammad ahmed 10/06/2023

