




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028055.D
 Acq On : 05 Oct 2023 19:04
 Operator : MA/JU
 Sample : 04607-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

Manual IntegrationsAPPROVED

Quant Time: Oct 06 01:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

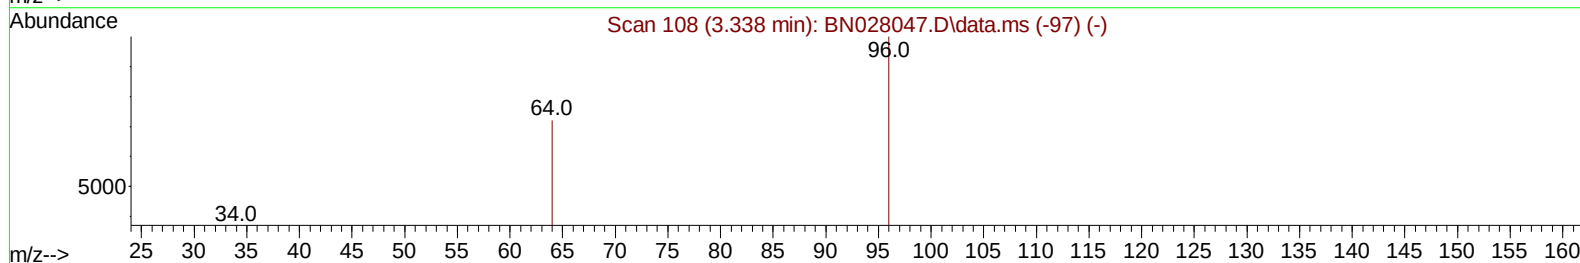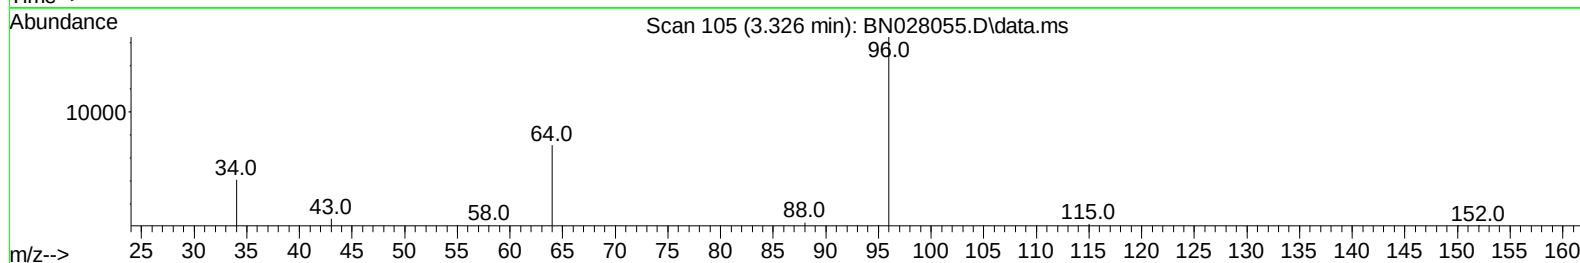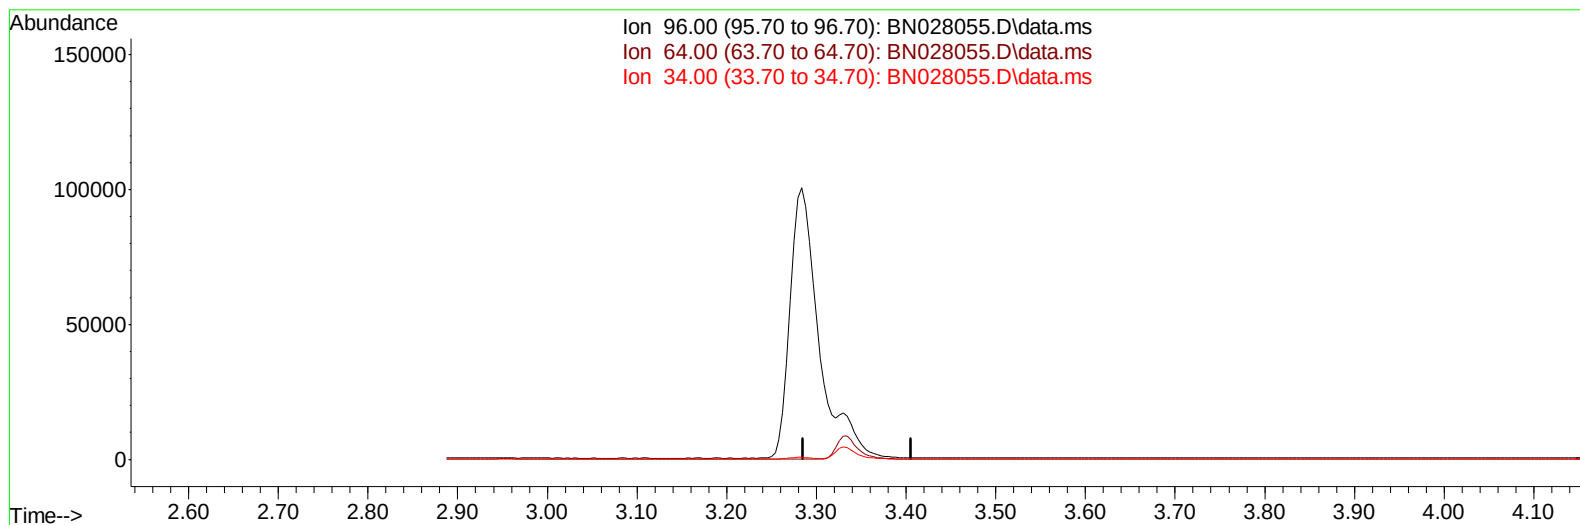

TIC: BN028055.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.326min (-3.326) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	62.70	0.00#
34.00	37.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028055.D
 Acq On : 05 Oct 2023 19:04
 Operator : MA/JU
 Sample : 04607-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

Manual IntegrationsAPPROVED

Quant Time: Oct 06 01:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

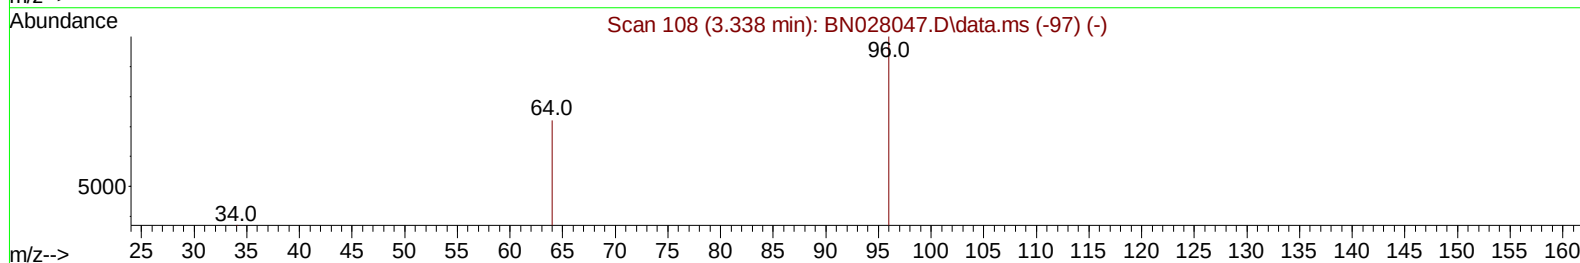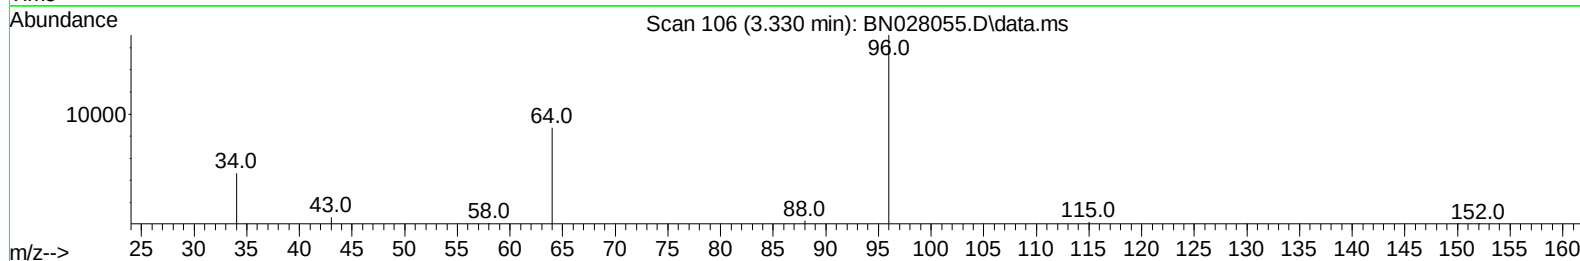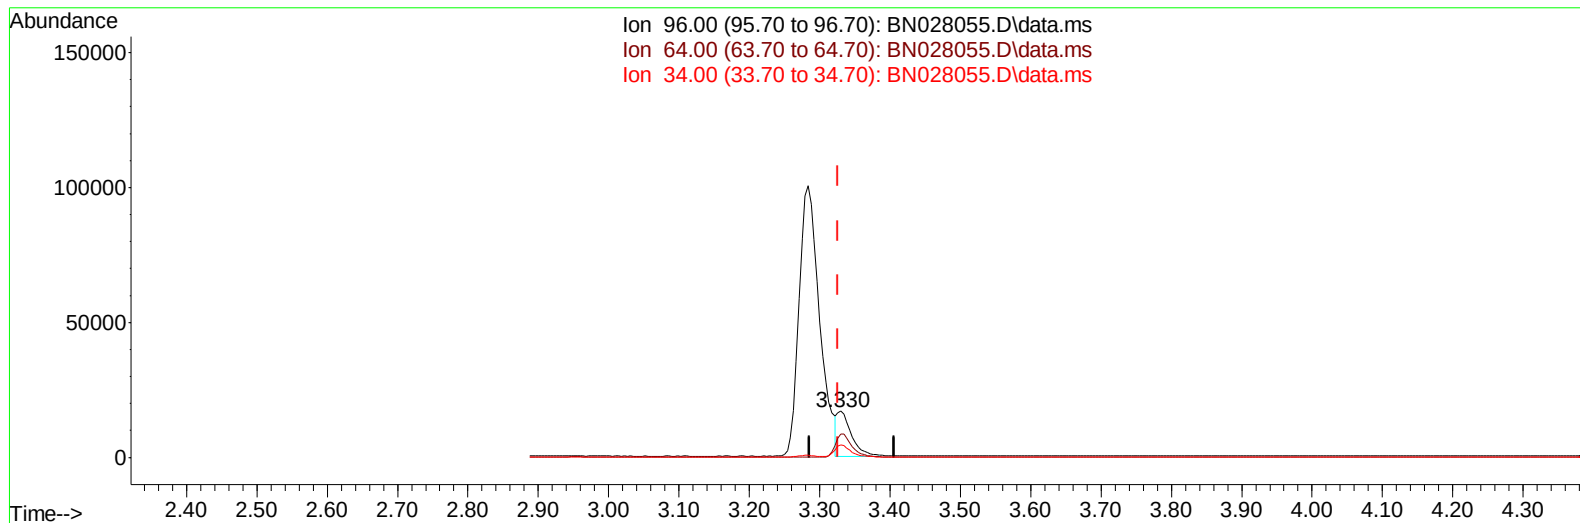

TIC: BN028055.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.330min (+ 0.004) 3.32 ng/ul m

response 23640

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.70	51.07
34.00	37.00	27.32#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028055.D
 Acq On : 05 Oct 2023 19:04
 Operator : MA/JU
 Sample : 04607-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

Quant Time: Oct 06 01:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.937	152		5674	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.757	136		18473	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.578	164		9062	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.337	188		18151	0.400	ng/ul	-0.01
17) Chrysene-d12	21.524	240		15752	0.400	ng/ul	-0.01
23) Perylene-d12	23.985	264		18041	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.330	96		23640m	3.317	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152		5955	0.200	ng/ul	-0.02
18) Fluoranthene-d10	19.362	212		12919	0.259	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.368	88		1353	0.179	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Oct 06 01:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration

