




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028114.D
 Acq On : 07 Oct 2023 10:32
 Operator : MA/JU
 Sample : 04624-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHA3

Manual IntegrationsAPPROVED

Quant Time: Oct 08 00:50:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

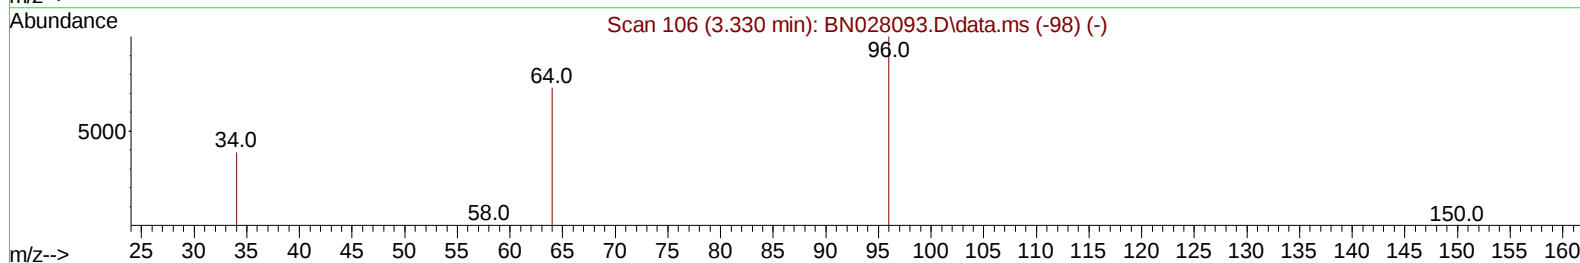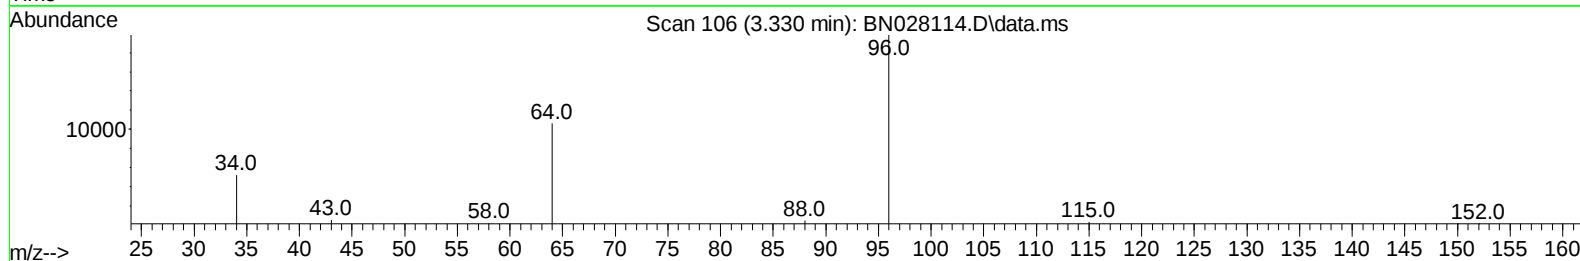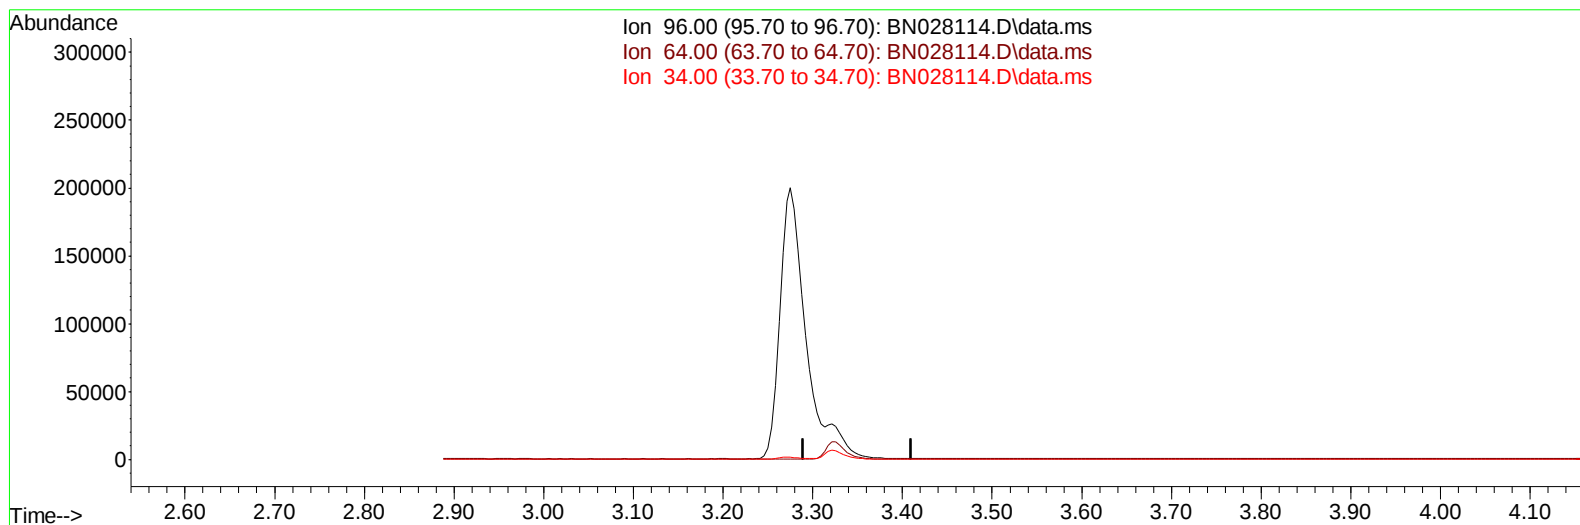

TIC: BN028114.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.330min (-3.330) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	62.70	0.00#
34.00	37.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028114.D
 Acq On : 07 Oct 2023 10:32
 Operator : MA/JU
 Sample : 04624-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHA3

Manual IntegrationsAPPROVED

Quant Time: Oct 08 00:50:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

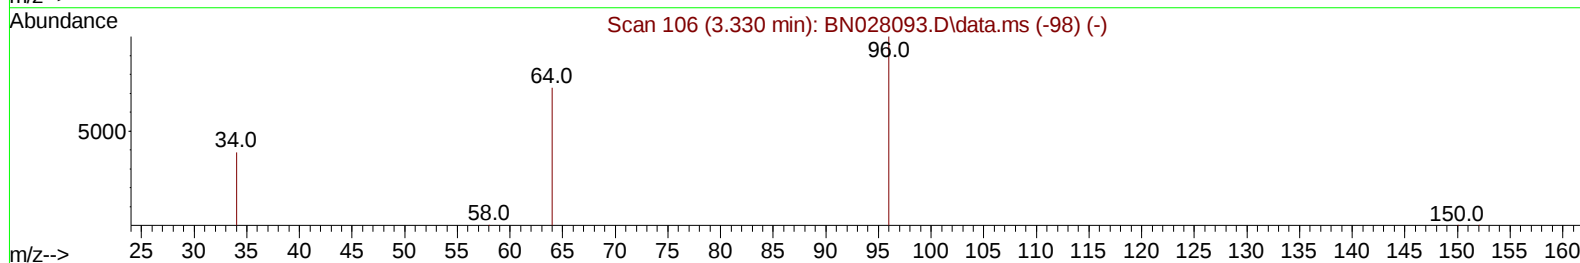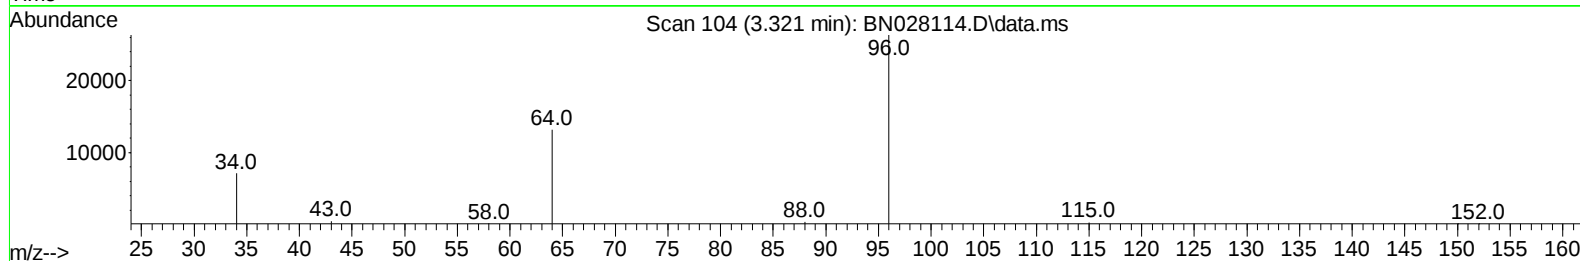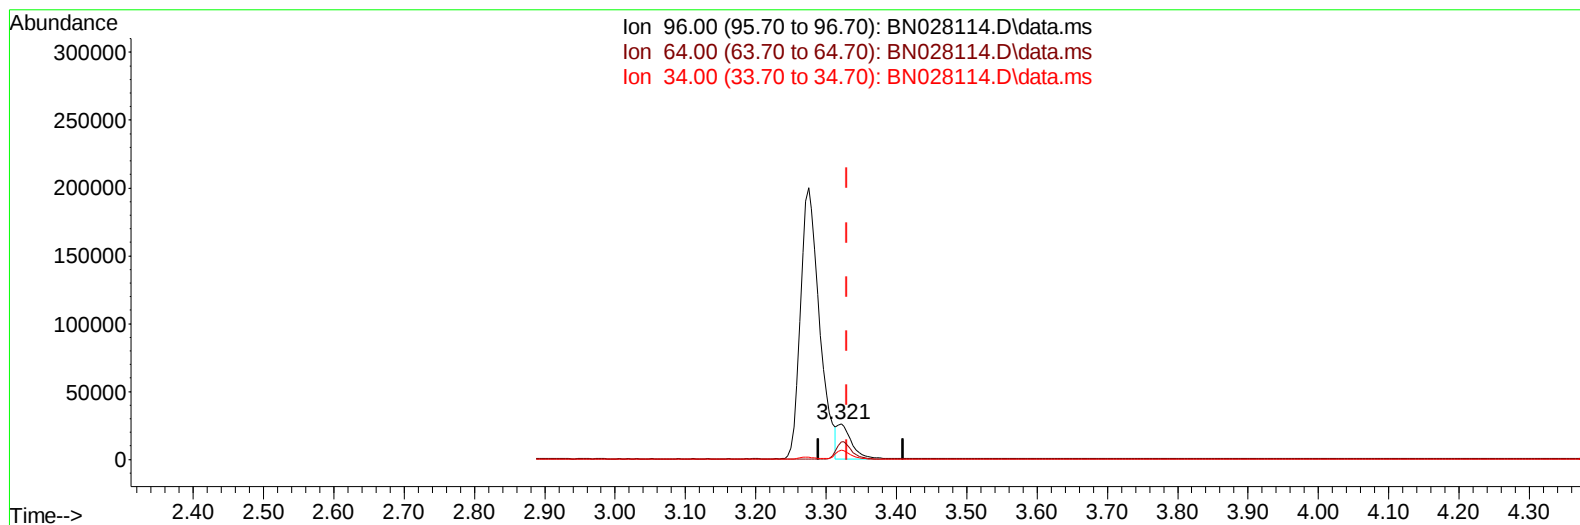

TIC: BN028114.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.321min (-0.008) 5.33 ng/ul m

response 35194

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.70	49.95#
34.00	37.00	27.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028114.D
 Acq On : 07 Oct 2023 10:32
 Operator : MA/JU
 Sample : 04624-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHA3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/08/2023
 Supervised By :mohammad ahmed 10/08/2023

Quant Time: Oct 08 00:50:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.933	152		5260	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136		16014	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.573	164		8620	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.333	188		17221	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240		14411	0.400	ng/ul	0.00
23) Perylene-d12	23.983	264		16399	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.321	96		35194m	5.327	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152		7001	0.271	ng/ul	0.00
18) Fluoranthene-d10	19.362	212		16463	0.360	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.359	88		27817	3.977	ng/ul#	83
19) Fluoranthene	19.390	202		1229	0.022	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028114.D
Acq On : 07 Oct 2023 10:32
Operator : MA/JU
Sample : 04624-15
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHA3

Manual IntegrationsAPPROVED

Quant Time: Oct 08 00:50:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/08/2023
Supervised By :mohammad ahmed 10/08/2023

