

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028055.D
 Acq On : 05 Oct 2023 19:04
 Operator : MA/JU
 Sample : 04607-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ35

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :mohammad ahmed 10/06/2023

Quant Time: Oct 06 01:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 03 15:50:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	5674	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.757	136	18473	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.578	164	9062	0.400	ng/u1	-0.01
13) Phenanthrene-d10	17.337	188	18151	0.400	ng/u1	-0.01
17) Chrysene-d12	21.524	240	15752	0.400	ng/u1	-0.01
23) Perylene-d12	23.985	264	18041	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.330	96	23640m	3.317	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.335	152	5955	0.200	ng/u1	-0.02
18) Fluoranthene-d10	19.362	212	12919	0.259	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.368	88	1353	0.179	ng/u1#	Qvalue 74

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028055.D
Acq On : 05 Oct 2023 19:04
Operator : MA/JU
Sample : 04607-02
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BBJ35

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :mohammad ahmed 10/06/2023


Quant Time: Oct 06 01:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 03 15:50:04 2023
Response via : Initial Calibration

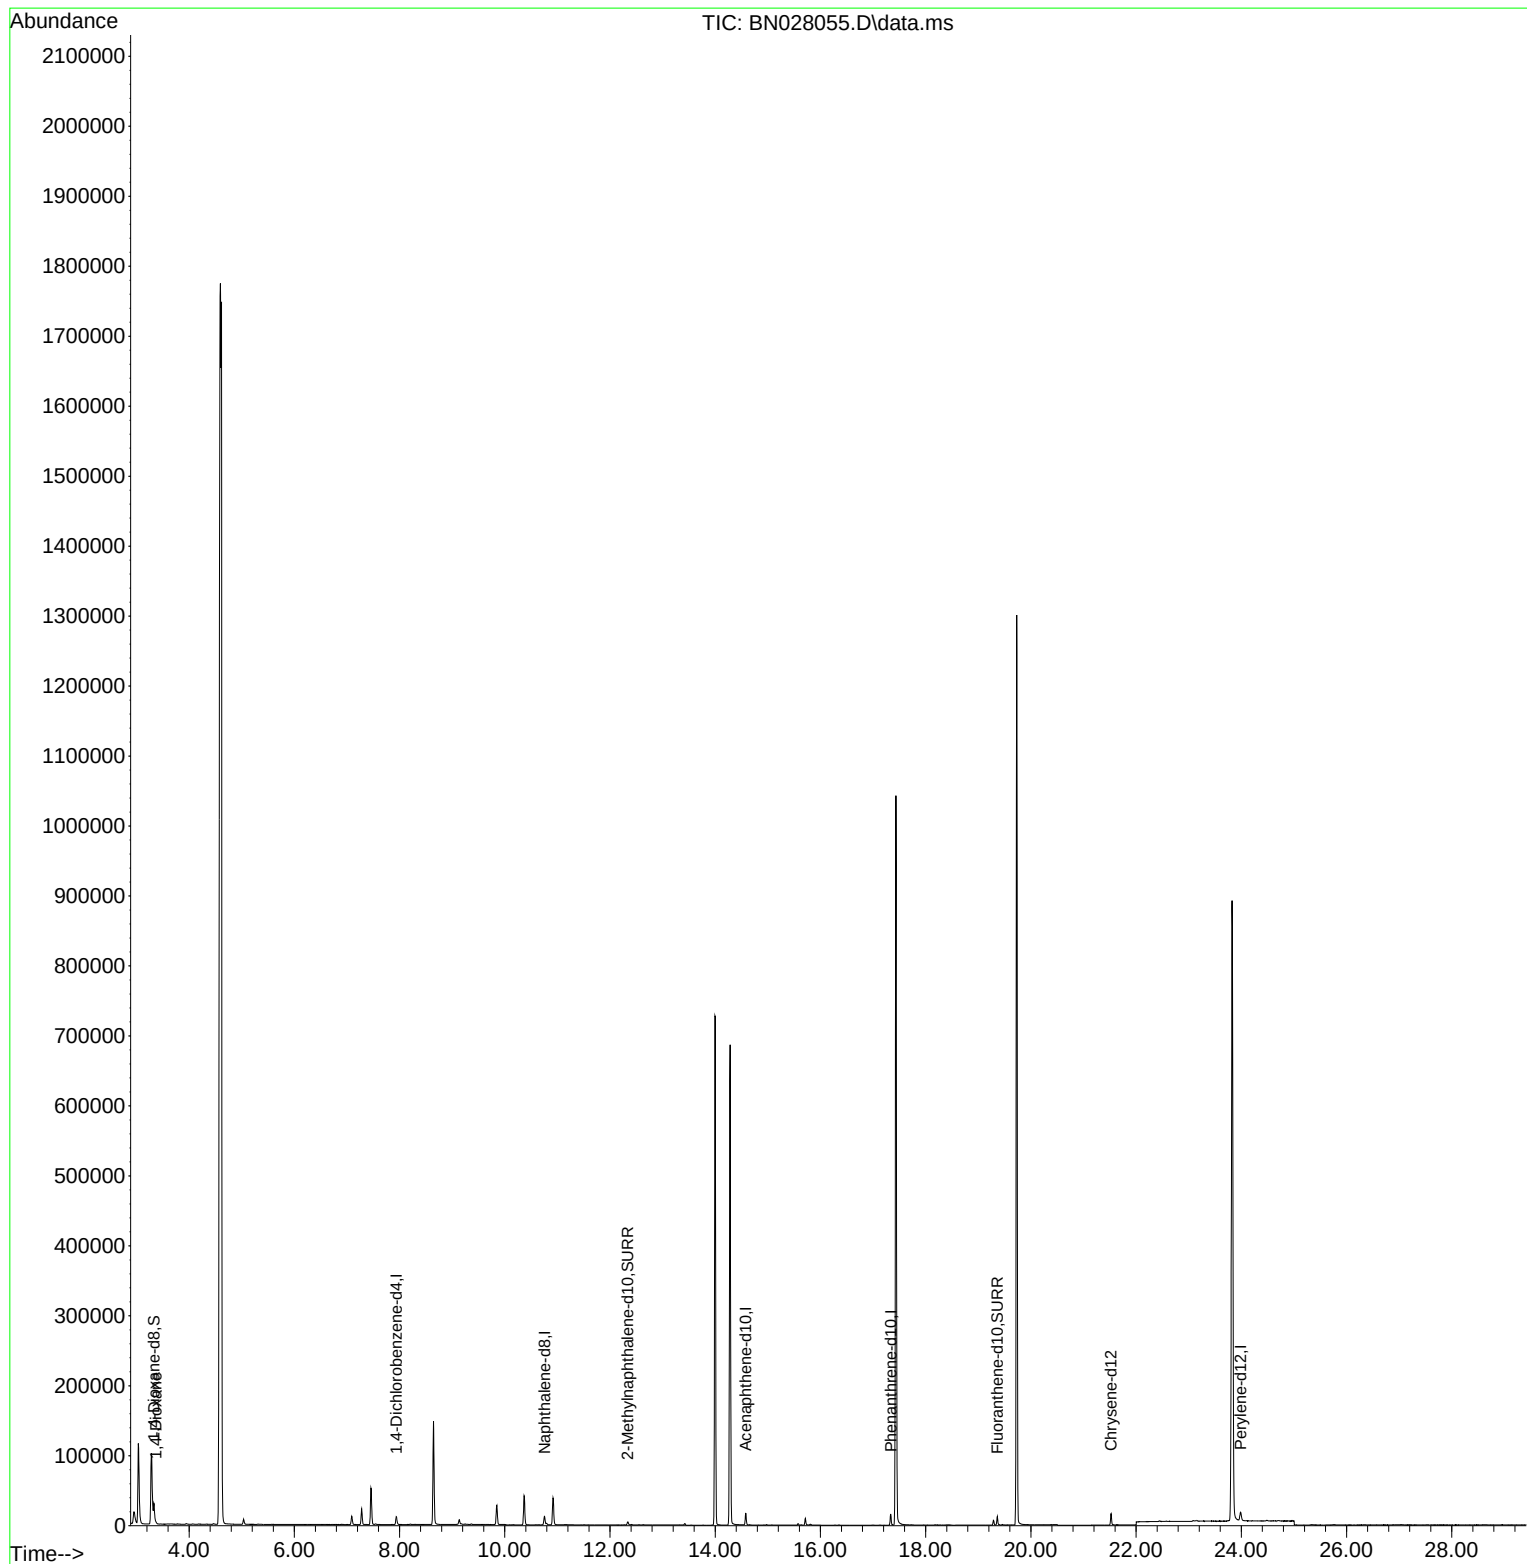

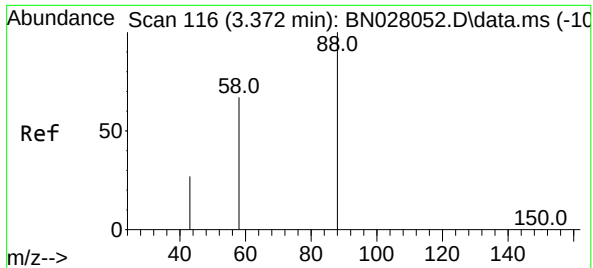

#2
1,4-Dioxane
Concen: 0.179 ng/ul
RT: 3.368 min Scan# 11
Delta R.T. 0.004 min
Lab File: BN028055.D
Acq: 05 Oct 2023 19:04

Instrument :
BNA_N
ClientSampleId :
BBJ35

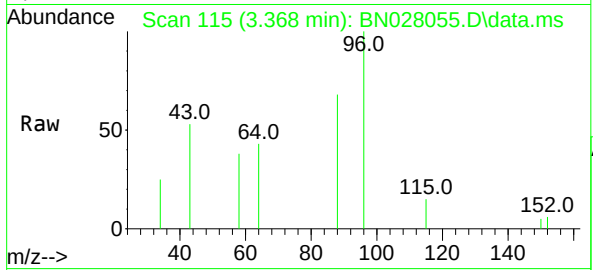

Tgt Ion: 88 Resp: 135
Ion Ratio Lower Upper
88 100
43 78.6 33.4 50.2
58 56.0 45.7 68.5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :mohammad ahmed 10/06/2023

