

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028096.D
 Acq On : 06 Oct 2023 22:49
 Operator : MA/JU
 Sample : 04624-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBK85

Quant Time: Oct 07 01:30:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	4983	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	15341	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	8181	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	15844	0.400	ng/ul	0.00
17) Chrysene-d12	21.525	240	13615	0.400	ng/ul	# 0.00
23) Perylene-d12	23.992	264	15300	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	25963	4.148	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	6403	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	13057	0.302	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.363	88	1101	0.166	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028096.D
Acq On : 06 Oct 2023 22:49
Operator : MA/JU
Sample : 04624-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBK85


Quant Time: Oct 07 01:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

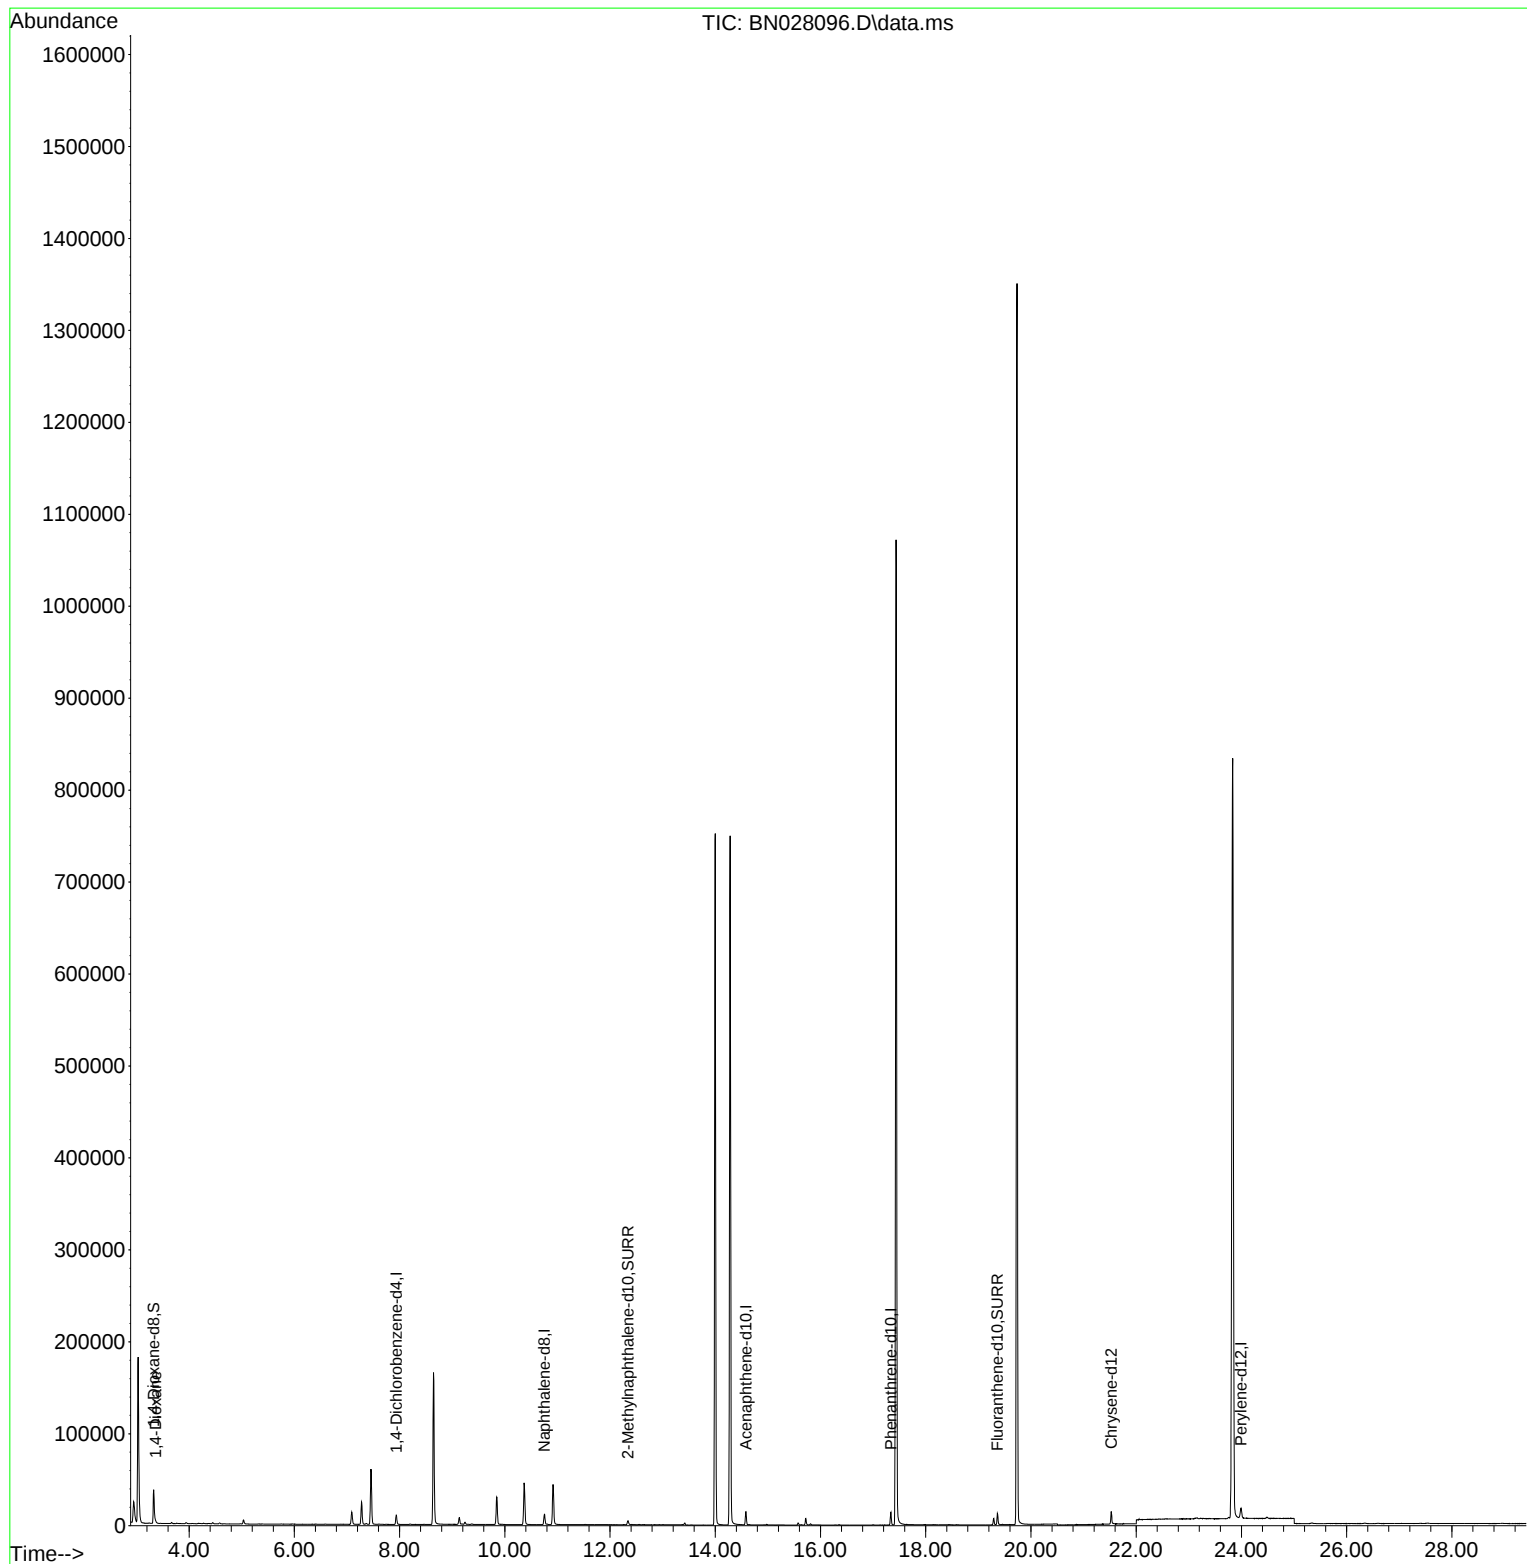

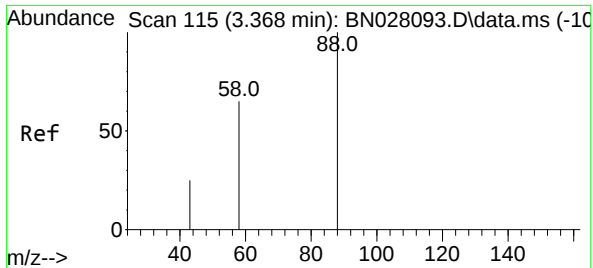

#2
 1,4-Dioxane
 Concen: 0.166 ng/ul
 RT: 3.363 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028096.D
 Acq: 06 Oct 2023 22:49

Instrument :
 BNA_N
 ClientSampleId :
 BBK85

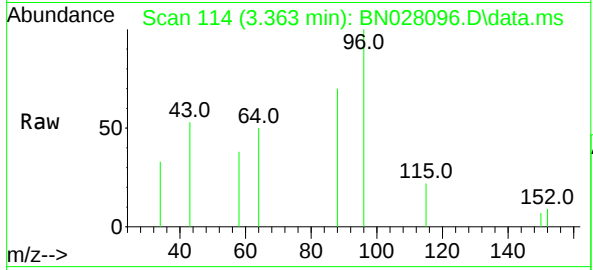

Tgt Ion: 88 Resp: 1101

Ion	Ratio	Lower	Upper
88	100		
43	75.9	33.4	50.2#
58	54.0	45.7	68.5

