

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028099.D
 Acq On : 07 Oct 2023 00:43
 Operator : MA/JU
 Sample : 04624-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHA1

Quant Time: Oct 07 01:38:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	4608	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	14378	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	7523	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	14934	0.400	ng/ul	0.00
17) Chrysene-d12	21.525	240	12844	0.400	ng/ul	# 0.00
23) Perylene-d12	23.989	264	14803	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	26480	4.575	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	6401	0.276	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	14291	0.351	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.363	88	958	0.156	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028099.D
Acq On : 07 Oct 2023 00:43
Operator : MA/JU
Sample : 04624-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHA1


Quant Time: Oct 07 01:38:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

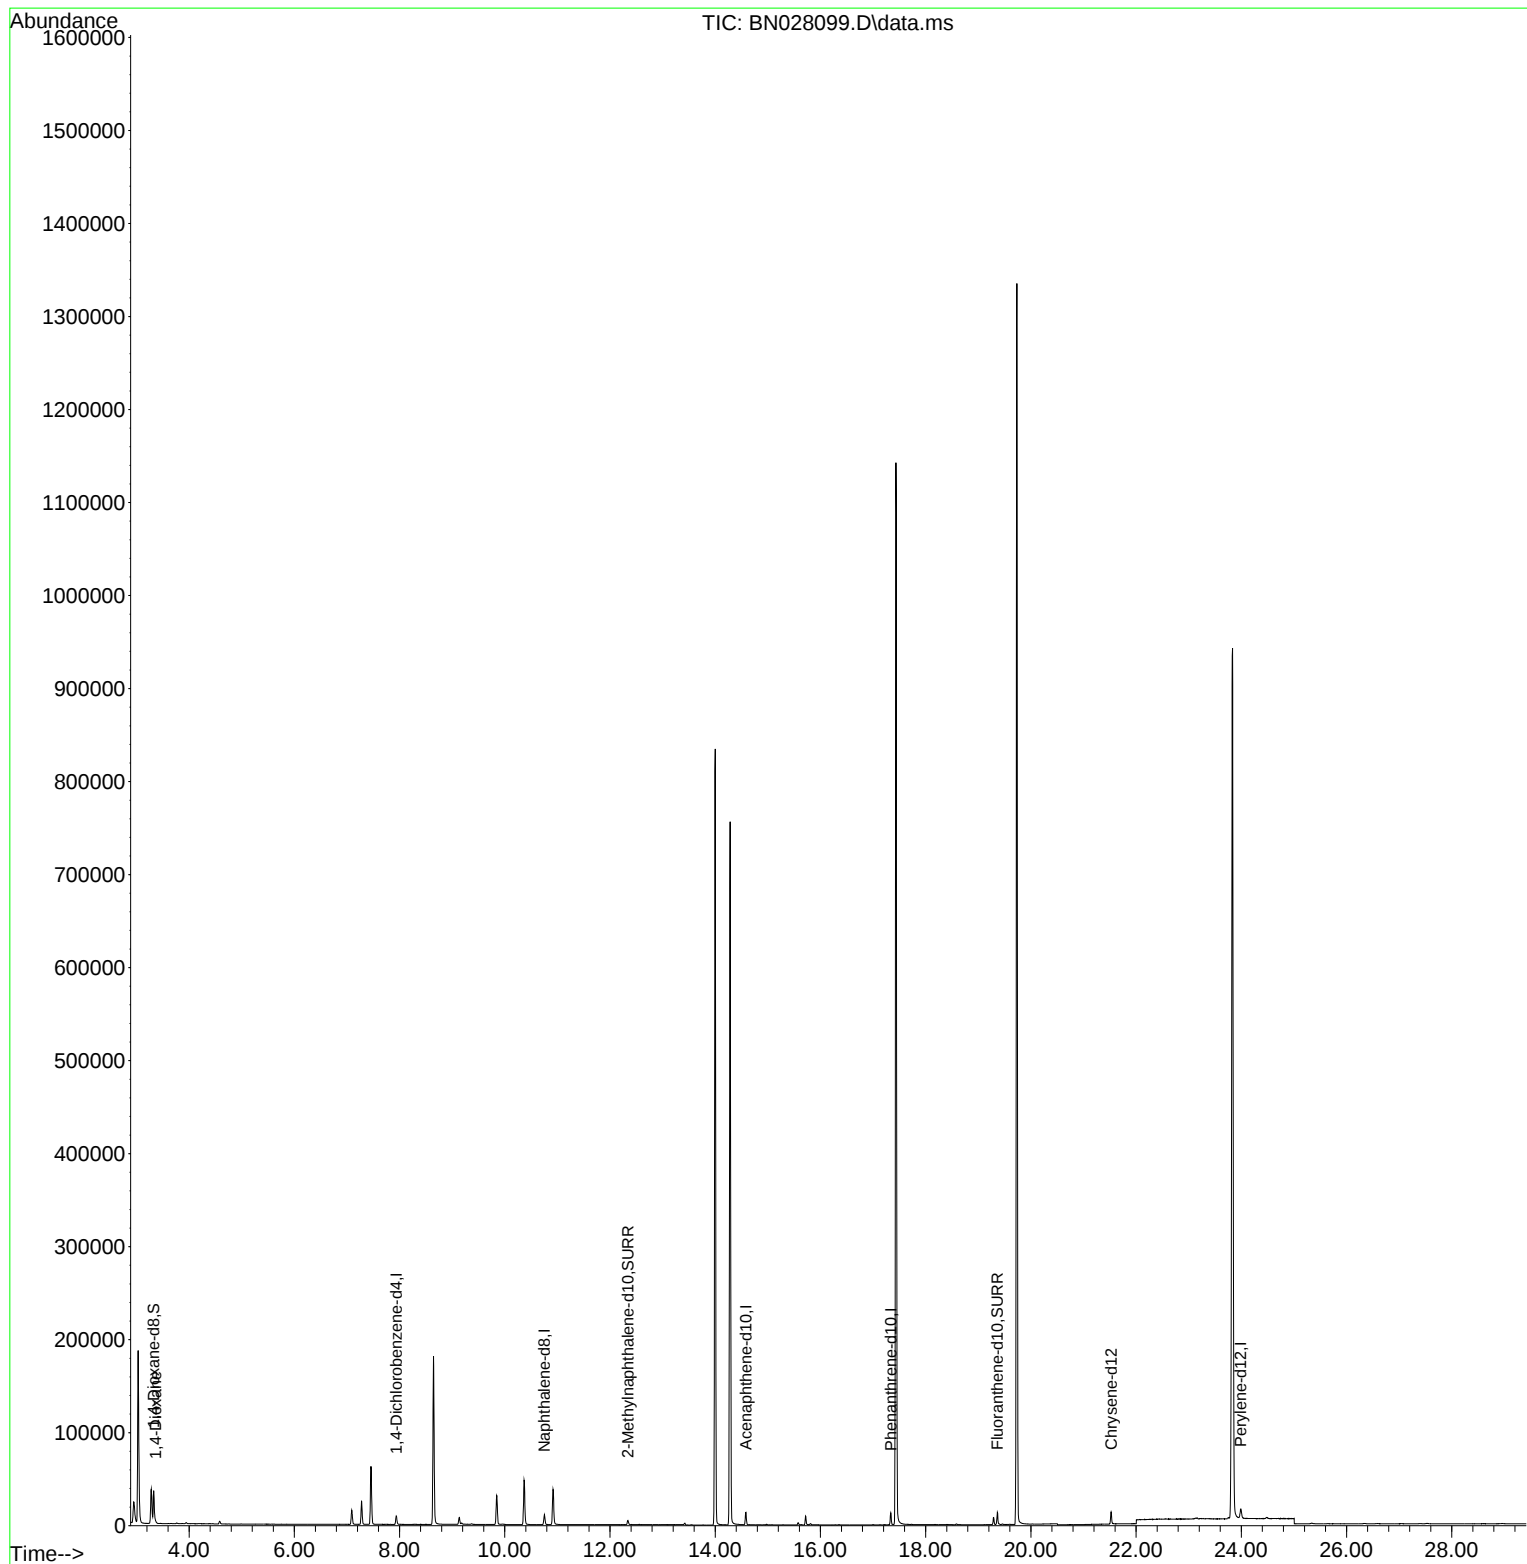

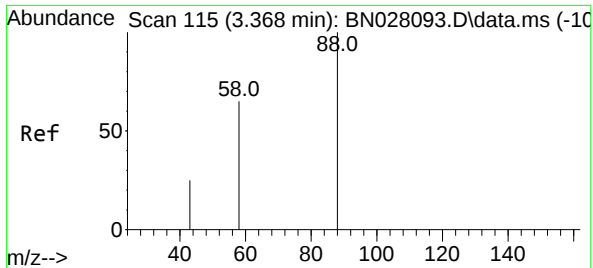

#2
 1,4-Dioxane
 Concen: 0.156 ng/ul
 RT: 3.363 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028099.D
 Acq: 07 Oct 2023 00:43

Instrument :
 BNA_N
 ClientSampleId :
 BBHA1

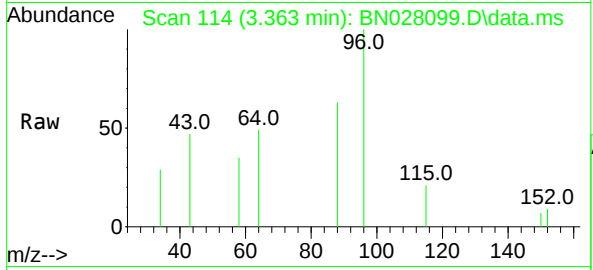

Tgt Ion: 88 Resp: 958

Ion	Ratio	Lower	Upper
88	100		
43	75.3	33.4	50.2#
58	55.6	45.7	68.5

