

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028103.D
 Acq On : 07 Oct 2023 03:12
 Operator : MA/JU
 Sample : 04624-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHB3

Quant Time: Oct 07 04:19:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	5709	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	17752	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	9612	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.333	188	18952	0.400	ng/ul	0.00
17) Chrysene-d12	21.522	240	16507	0.400	ng/ul	# 0.00
23) Perylene-d12	23.986	264	18808	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	29862	4.164	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	8699	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	19159	0.366	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	2690	0.354	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028103.D
Acq On : 07 Oct 2023 03:12
Operator : MA/JU
Sample : 04624-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHB3

Quant Time: Oct 07 04:19:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

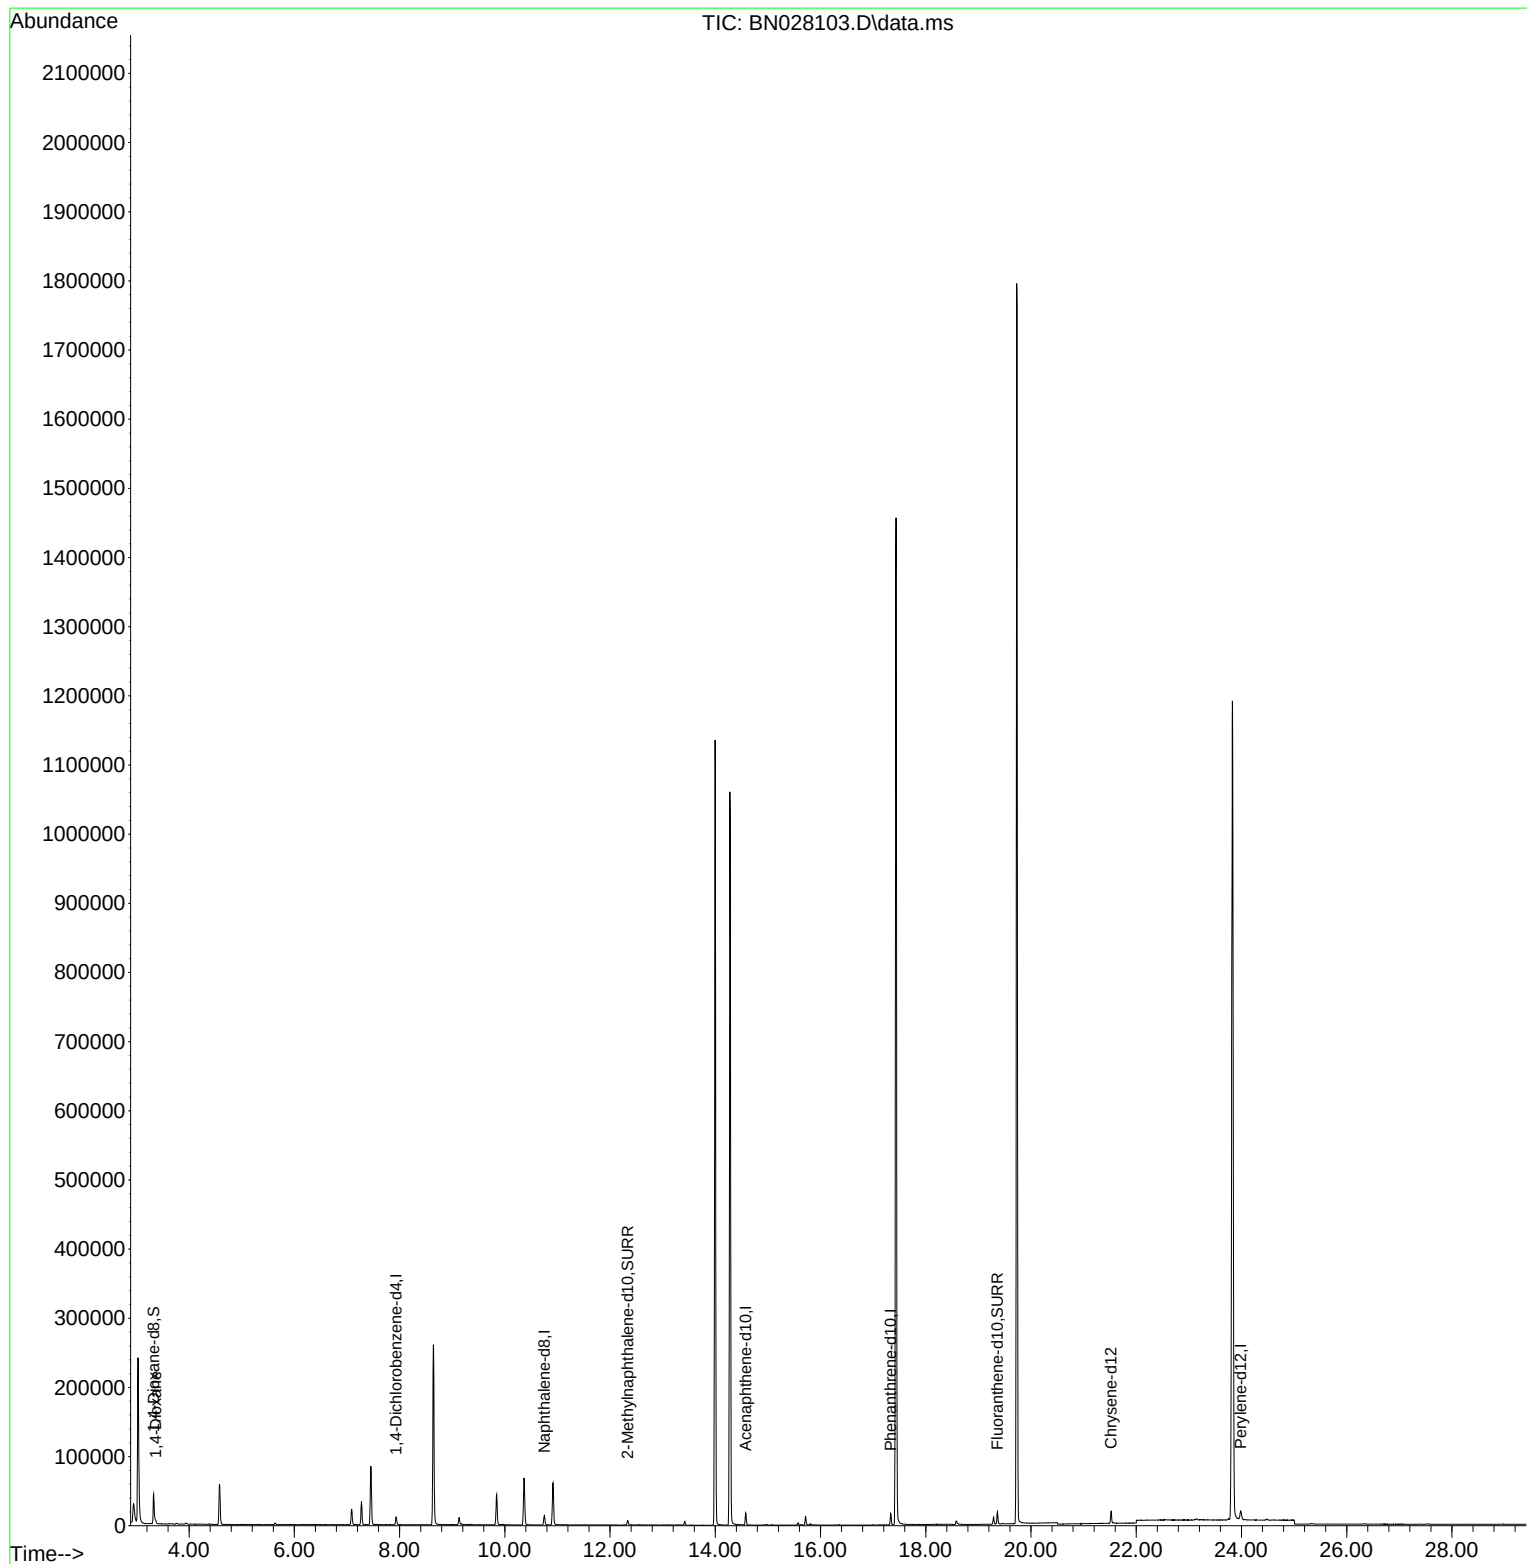

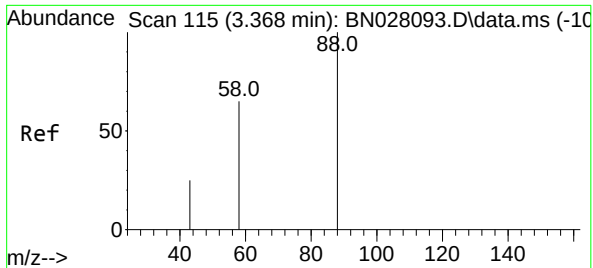

#2
 1,4-Dioxane
 Concen: 0.354 ng/ul
 RT: 3.364 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028103.D
 Acq: 07 Oct 2023 03:12

Instrument :
 BNA_N
 ClientSampleId :
 BBHB3

Tgt Ion:	88	Resp:	2690
Ion	Ratio	Lower	Upper
88	100		
43	41.8	33.4	50.2
58	51.5	45.7	68.5

