

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028106.D
 Acq On : 07 Oct 2023 05:03
 Operator : MA/JU
 Sample : 04624-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJS0

Quant Time: Oct 07 05:55:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	4876	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	14953	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.578	164	8088	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.333	188	15899	0.400	ng/ul	0.00
17) Chrysene-d12	21.522	240	13663	0.400	ng/ul	# 0.00
23) Perylene-d12	23.986	264	15697	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	26140	4.268	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	7533	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	16719	0.386	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.364	88	4598	0.709	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028106.D
Acq On : 07 Oct 2023 05:03
Operator : MA/JU
Sample : 04624-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJS0


Quant Time: Oct 07 05:55:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

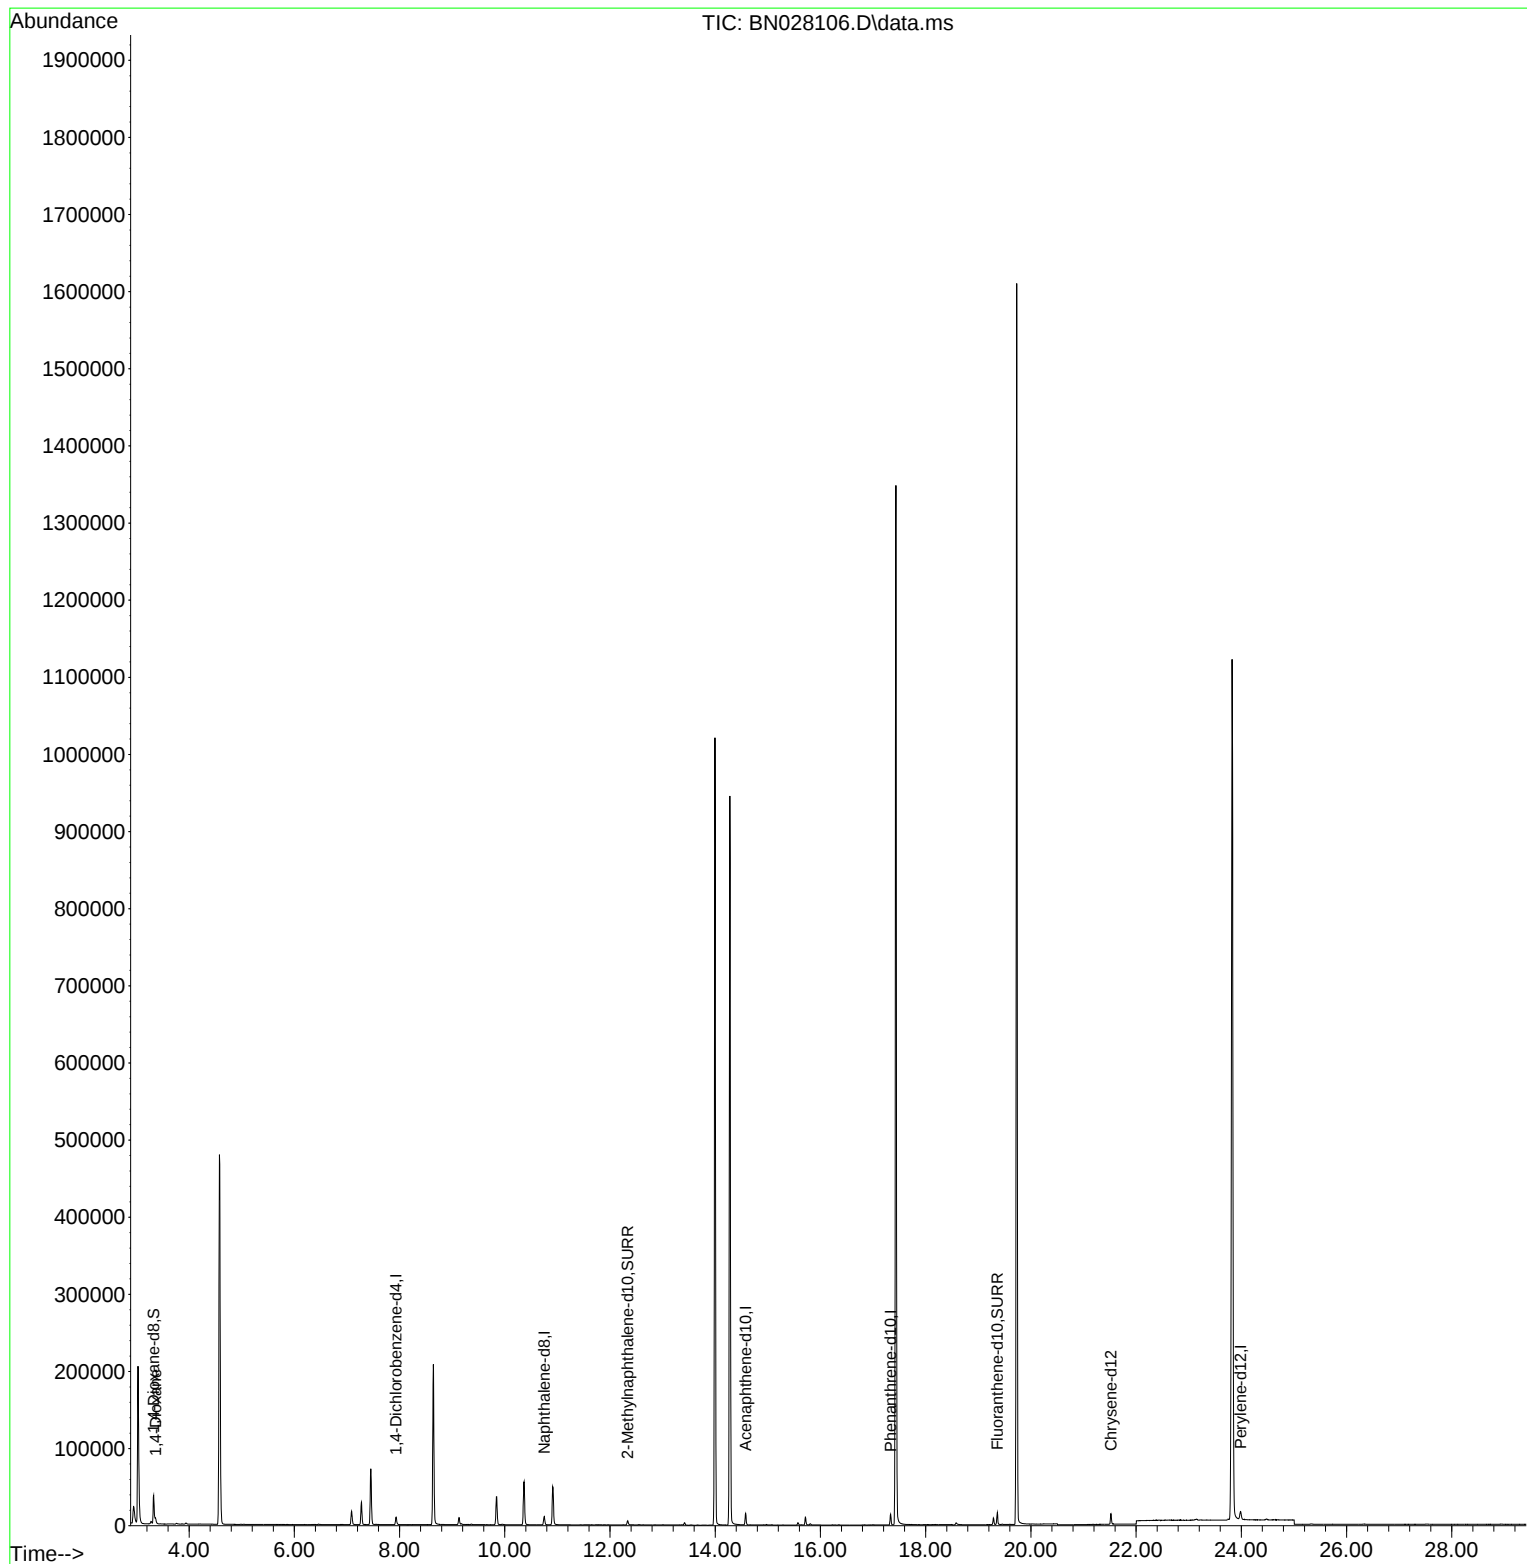


Abundance Scan 115 (3.368 min): BN028093.D\data.ms (-10

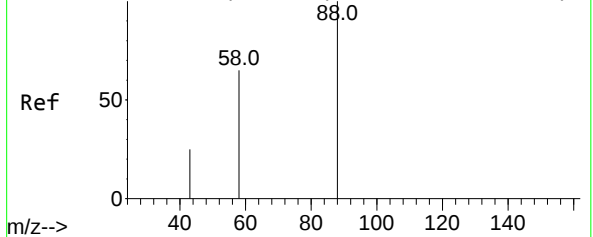

Abundance Scan 114 (3.364 min): BN028106.D\data.ms

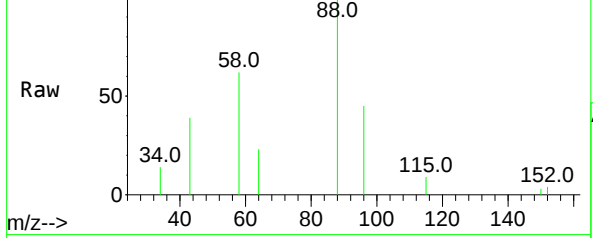

Abundance Scan 114 (3.364 min): BN028106.D\data.ms (-10

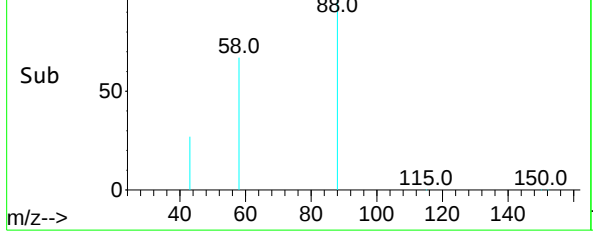

#2
1,4-Dioxane
Concen: 0.709 ng/ul
RT: 3.364 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN028106.D
Acq: 07 Oct 2023 05:03

Instrument :
BNA_N
ClientSampleId :
BBJS0

Tgt Ion:	88	Resp:	4598
Ion	Ratio	Lower	Upper
88	100		
43	39.1	33.4	50.2
58	62.4	45.7	68.5

