

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028122.D
 Acq On : 07 Oct 2023 15:24
 Operator : MA/JU
 Sample : 04607-08
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKB2

Quant Time: Oct 08 00:51:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4957	0.400	ng/ul	0.00
4) Naphthalene-d8	10.746	136	16430	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.573	164	8409	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	16414	0.400	ng/ul	0.00
17) Chrysene-d12	21.522	240	13927	0.400	ng/ul	0.00
23) Perylene-d12	23.980	264	16137	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	29485	4.736	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	8700	0.329	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	19835	0.449	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.359	88	952	0.144	ng/ul#	72
5) Naphthalene	10.795	128	1289	0.028	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028122.D
Acq On : 07 Oct 2023 15:24
Operator : MA/JU
Sample : 04607-08
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKB2

Quant Time: Oct 08 00:51:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration




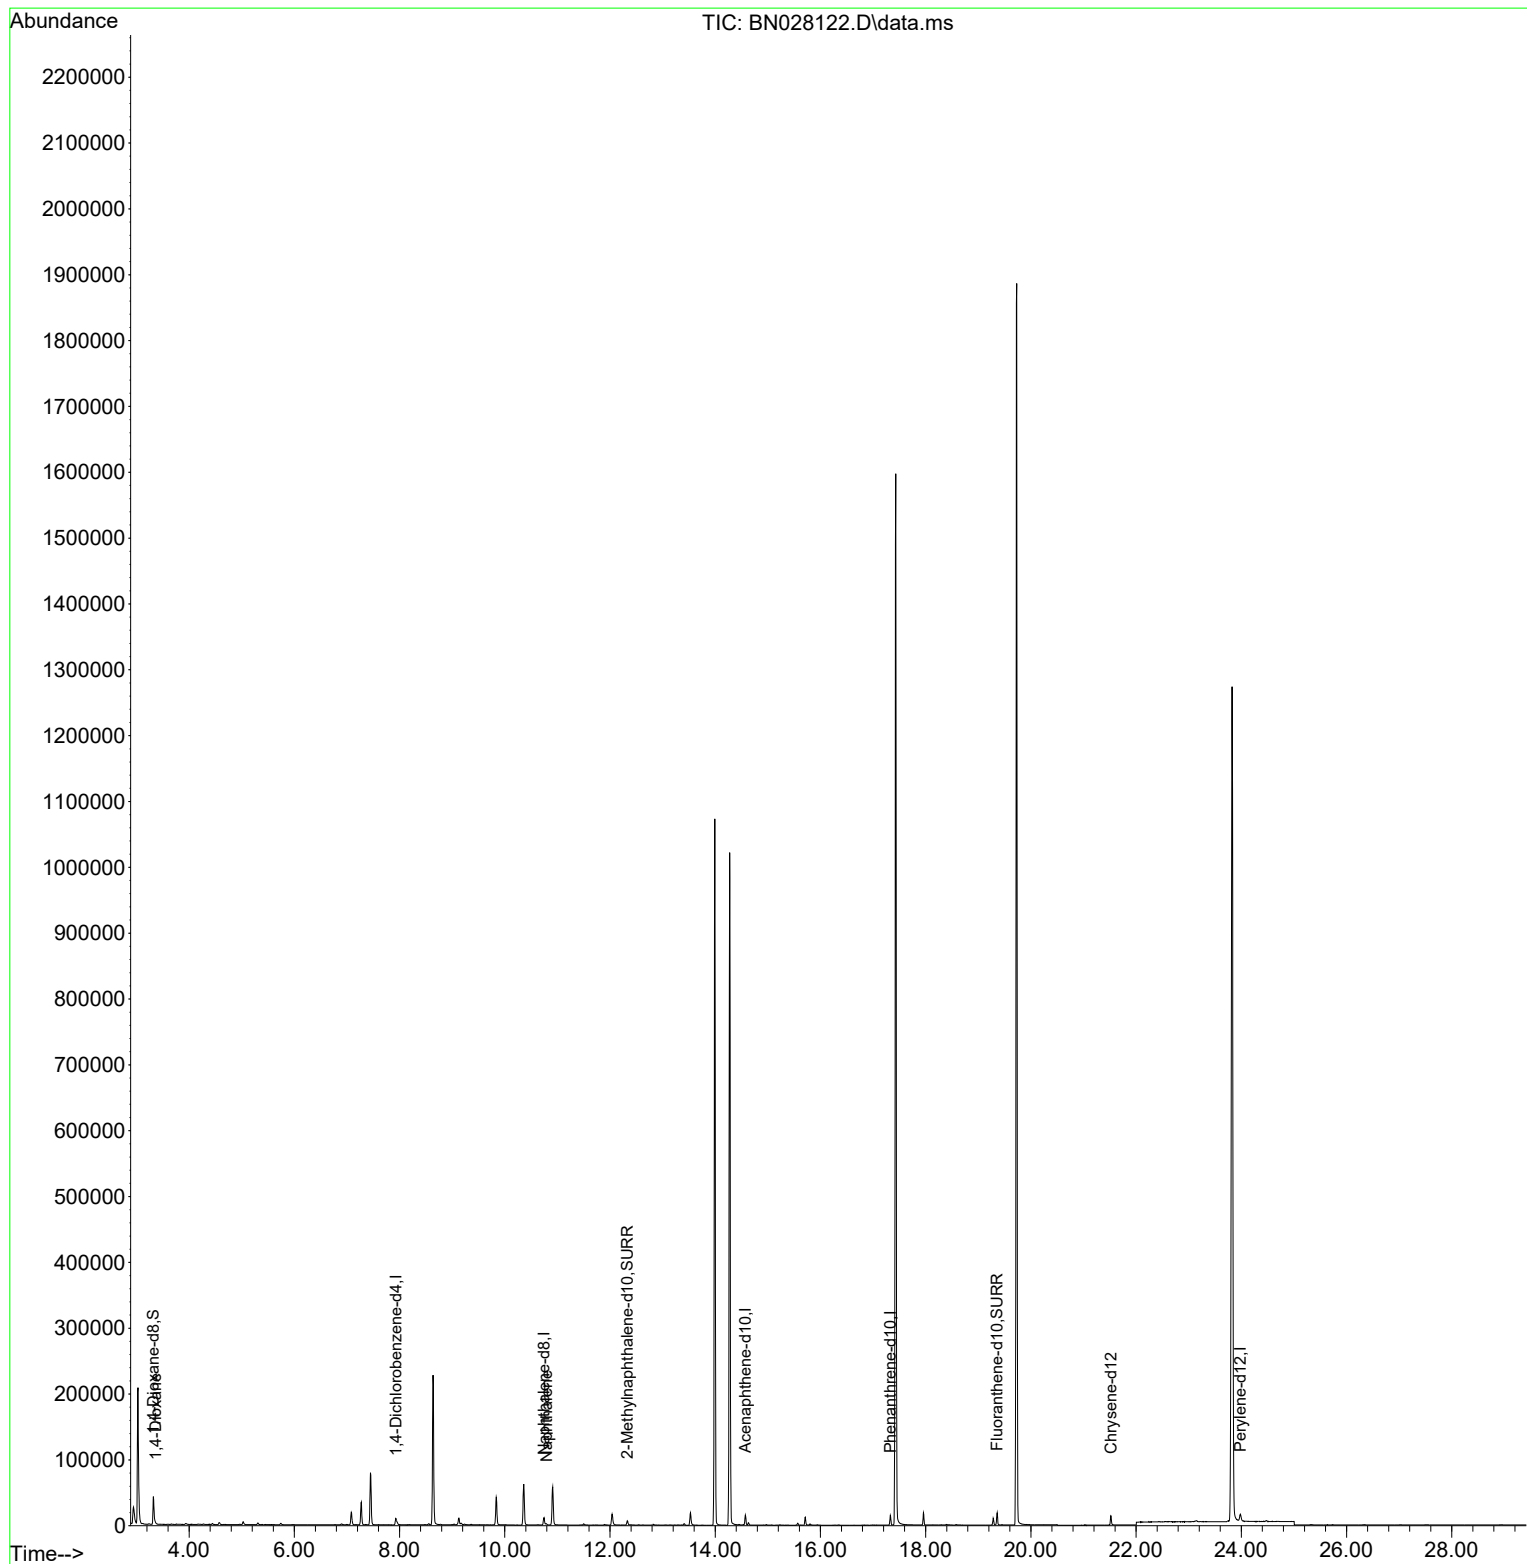


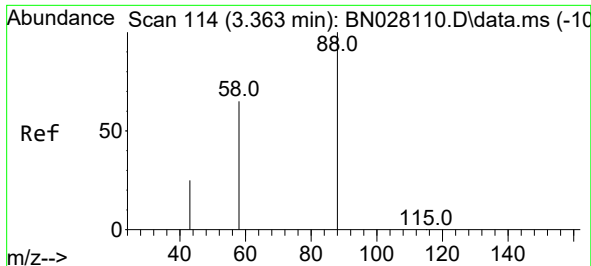

#2
1,4-Dioxane
Concen: 0.144 ng/ul
RT: 3.359 min Scan# 114
Delta R.T. -0.004 min
Lab File: BN028122.D
Acq: 07 Oct 2023 15:24

Instrument :
BNA_N
ClientSampleId :
BBKB2

Tgt Ion: 88 Resp: 952
Ion Ratio Lower Upper
88 100
43 78.0 33.4 50.2#
58 52.9 45.7 68.5

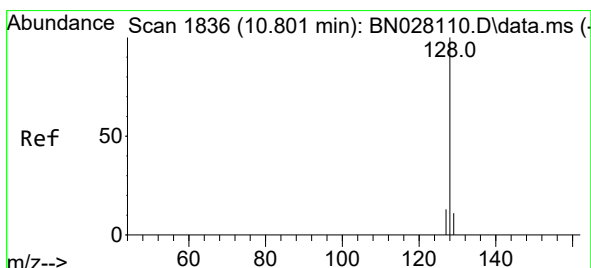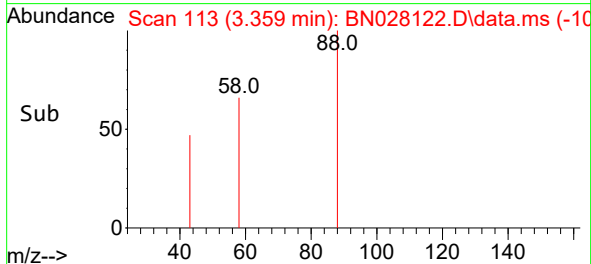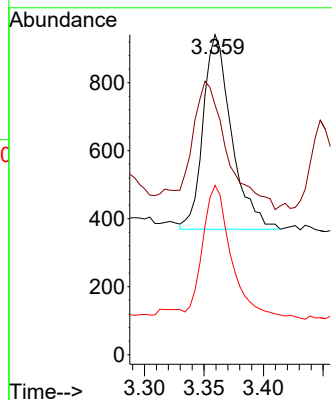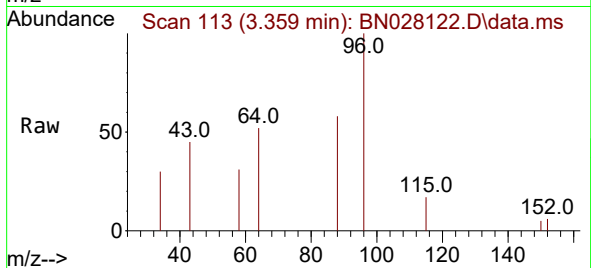

#5
Naphthalene
Concen: 0.028 ng/ul
RT: 10.795 min Scan# 1835
Delta R.T. -0.011 min
Lab File: BN028122.D
Acq: 07 Oct 2023 15:24

Tgt Ion:128 Resp: 1289
Ion Ratio Lower Upper
128 100
129 20.5 9.4 14.0#
127 20.5 11.0 16.4#

