

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028133.D
 Acq On : 07 Oct 2023 22:39
 Operator : MA/JU
 Sample : 04607-15
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHC1

Quant Time: Oct 08 00:53:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4745	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	14430	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.573	164	7441	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	14795	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	12512	0.400	ng/ul	0.00
23) Perylene-d12	23.980	264	14423	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	25965	4.357	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.329	152	6841	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	14851	0.374	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.355	88	1112	0.176	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028133.D
Acq On : 07 Oct 2023 22:39
Operator : MA/JU
Sample : 04607-15
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHC1

Quant Time: Oct 08 00:53:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

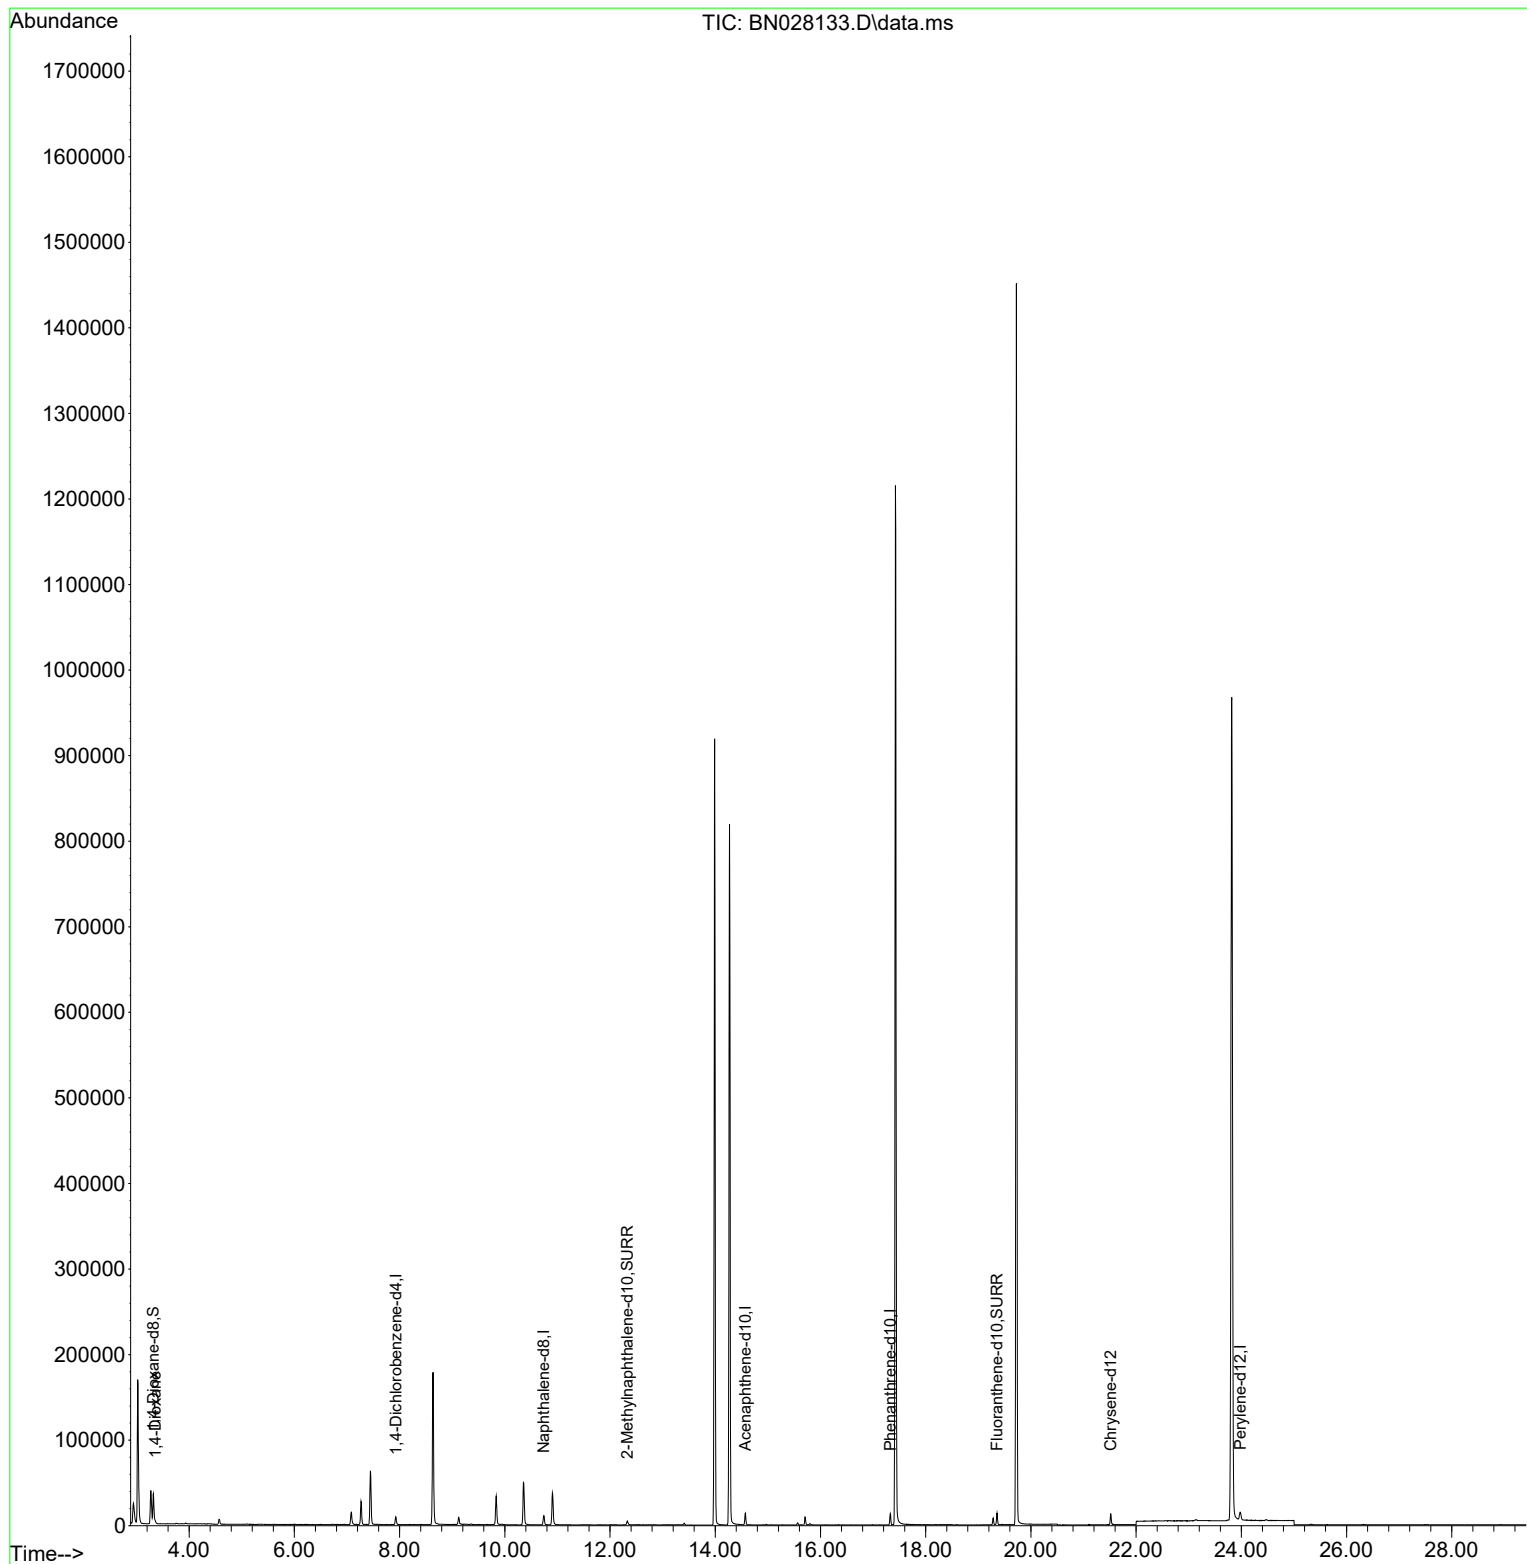

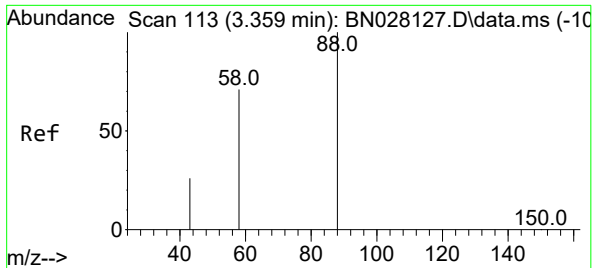

1,4-Dioxane
 Concen: 0.176 ng/ul
 RT: 3.355 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN028133.D
 Acq: 07 Oct 2023 22:39

Instrument :
 BNA_N
 ClientSampleId :
 BBHC1

Tgt Ion:	88	Resp:	1112
Ion	Ratio	Lower	Upper
88	100		
43	56.7	33.4	50.2#
58	53.7	45.7	68.5

