

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028136.D
 Acq On : 08 Oct 2023 00:29
 Operator : MA/JU
 Sample : 04607-18
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJP8

Quant Time: Oct 08 01:26:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	5040	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	14323	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.573	164	7715	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.329	188	15260	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	12844	0.400	ng/ul	0.00
23) Perylene-d12	23.980	264	14578	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	23976	3.787	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	6792	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	13947	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.359	88	1166	0.174	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028136.D
Acq On : 08 Oct 2023 00:29
Operator : MA/JU
Sample : 04607-18
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJP8

Quant Time: Oct 08 01:26:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

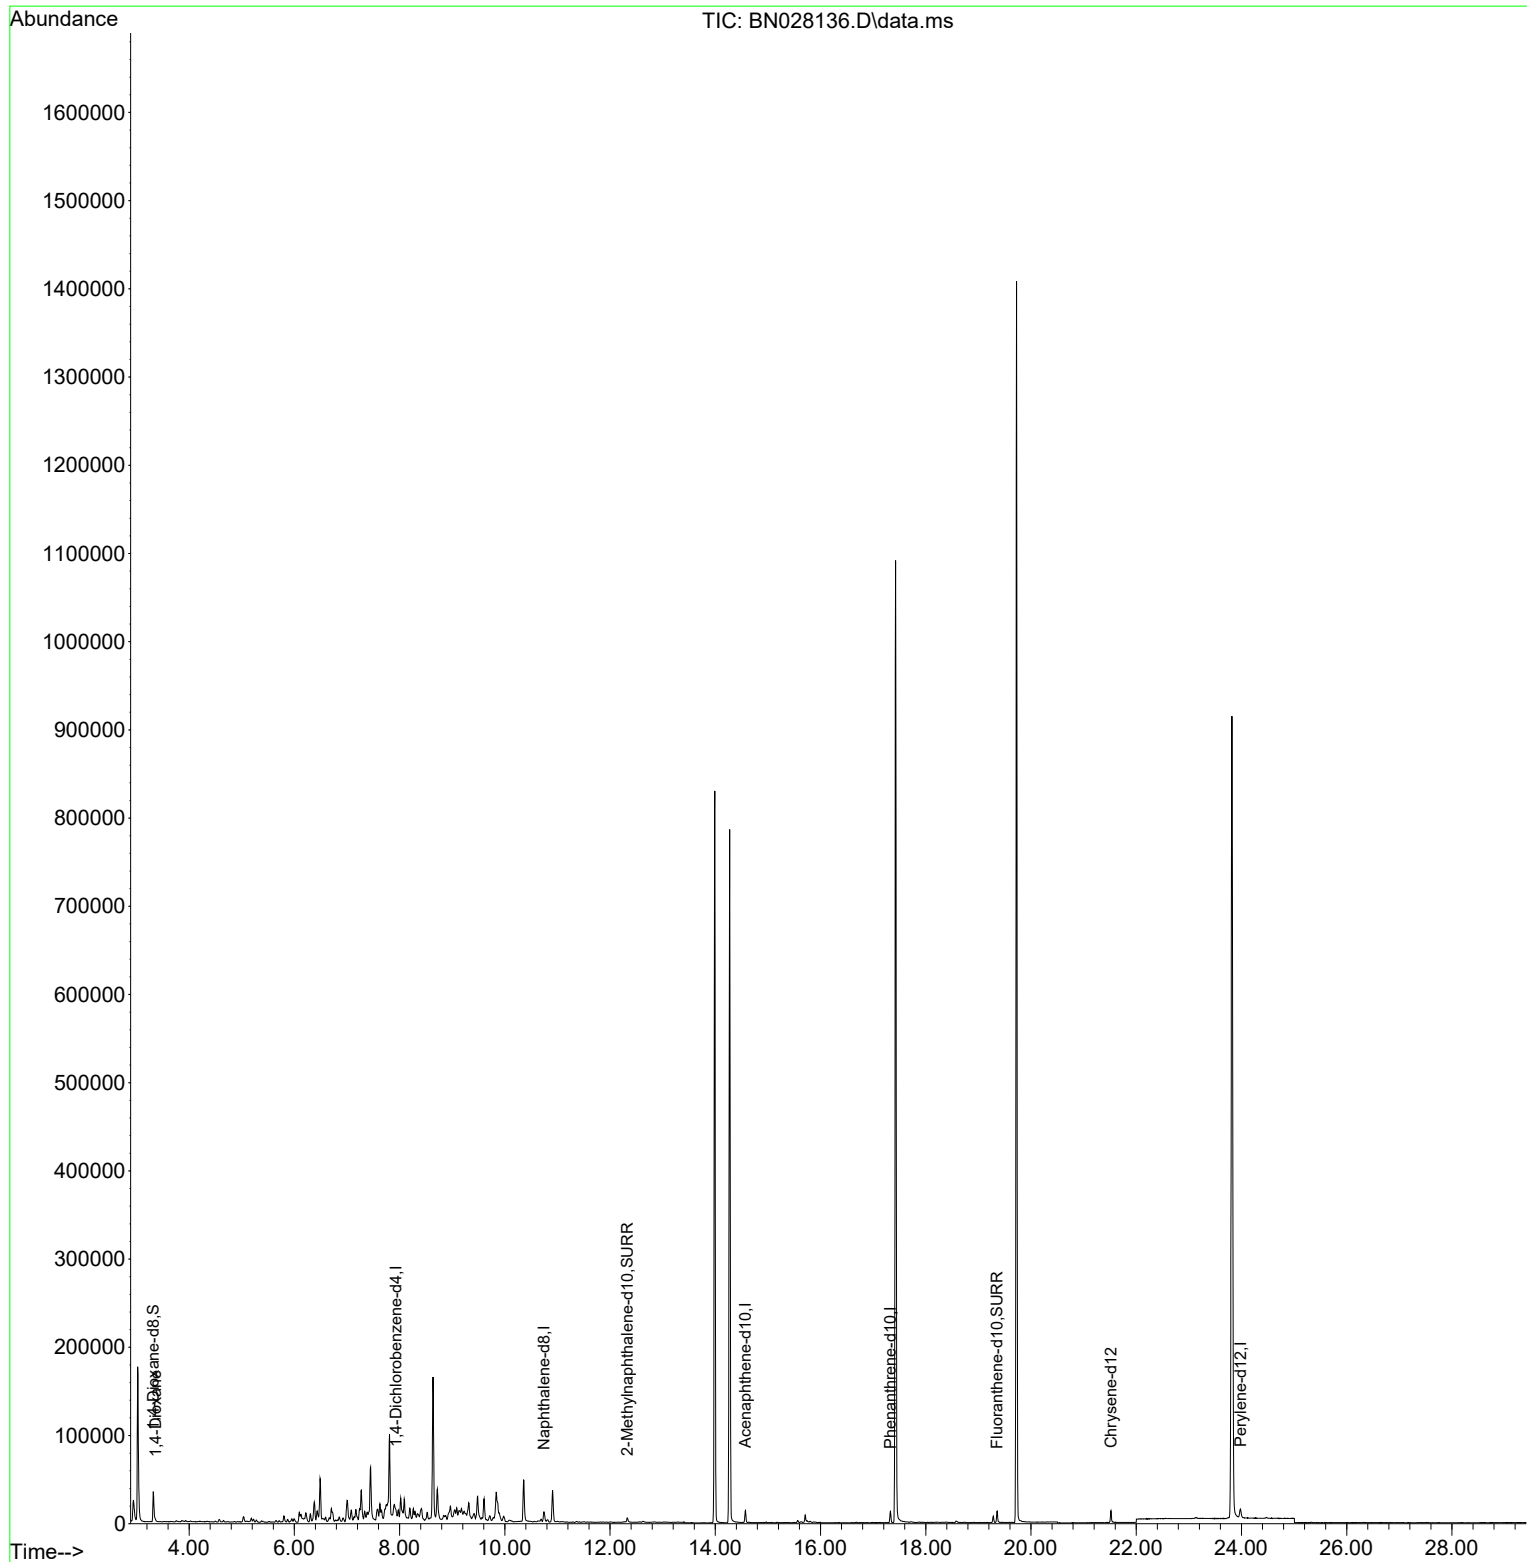

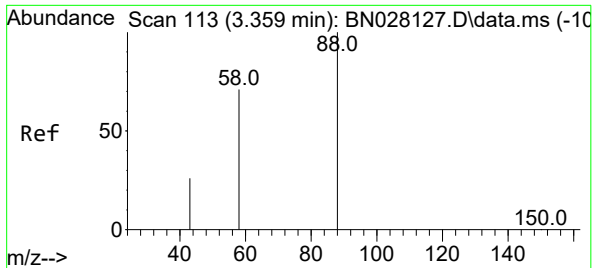

1,4-Dioxane
 Concen: 0.174 ng/ul
 RT: 3.359 min Scan# 11
 Delta R.T. -0.004 min
 Lab File: BN028136.D
 Acq: 08 Oct 2023 00:29

Instrument :
 BNA_N
 ClientSampleId :
 BBJP8

Tgt Ion: 88 Resp: 1166
 Ion Ratio Lower Upper
 88 100
 43 57.2 33.4 50.2#
 58 52.4 45.7 68.5

