

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028141.D
 Acq On : 08 Oct 2023 03:31
 Operator : MA/JU
 Sample : 04624-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJQ0

Quant Time: Oct 08 03:57:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	4310	0.400	ng/ul	0.00
4) Naphthalene-d8	10.740	136	13236	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.569	164	7065	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.329	188	13930	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	11938	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264	13809	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.321	96	28848	5.329	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152	7536	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	17073	0.451	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.355	88	2214	0.386	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028141.D
Acq On : 08 Oct 2023 03:31
Operator : MA/JU
Sample : 04624-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJQ0

Quant Time: Oct 08 03:57:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

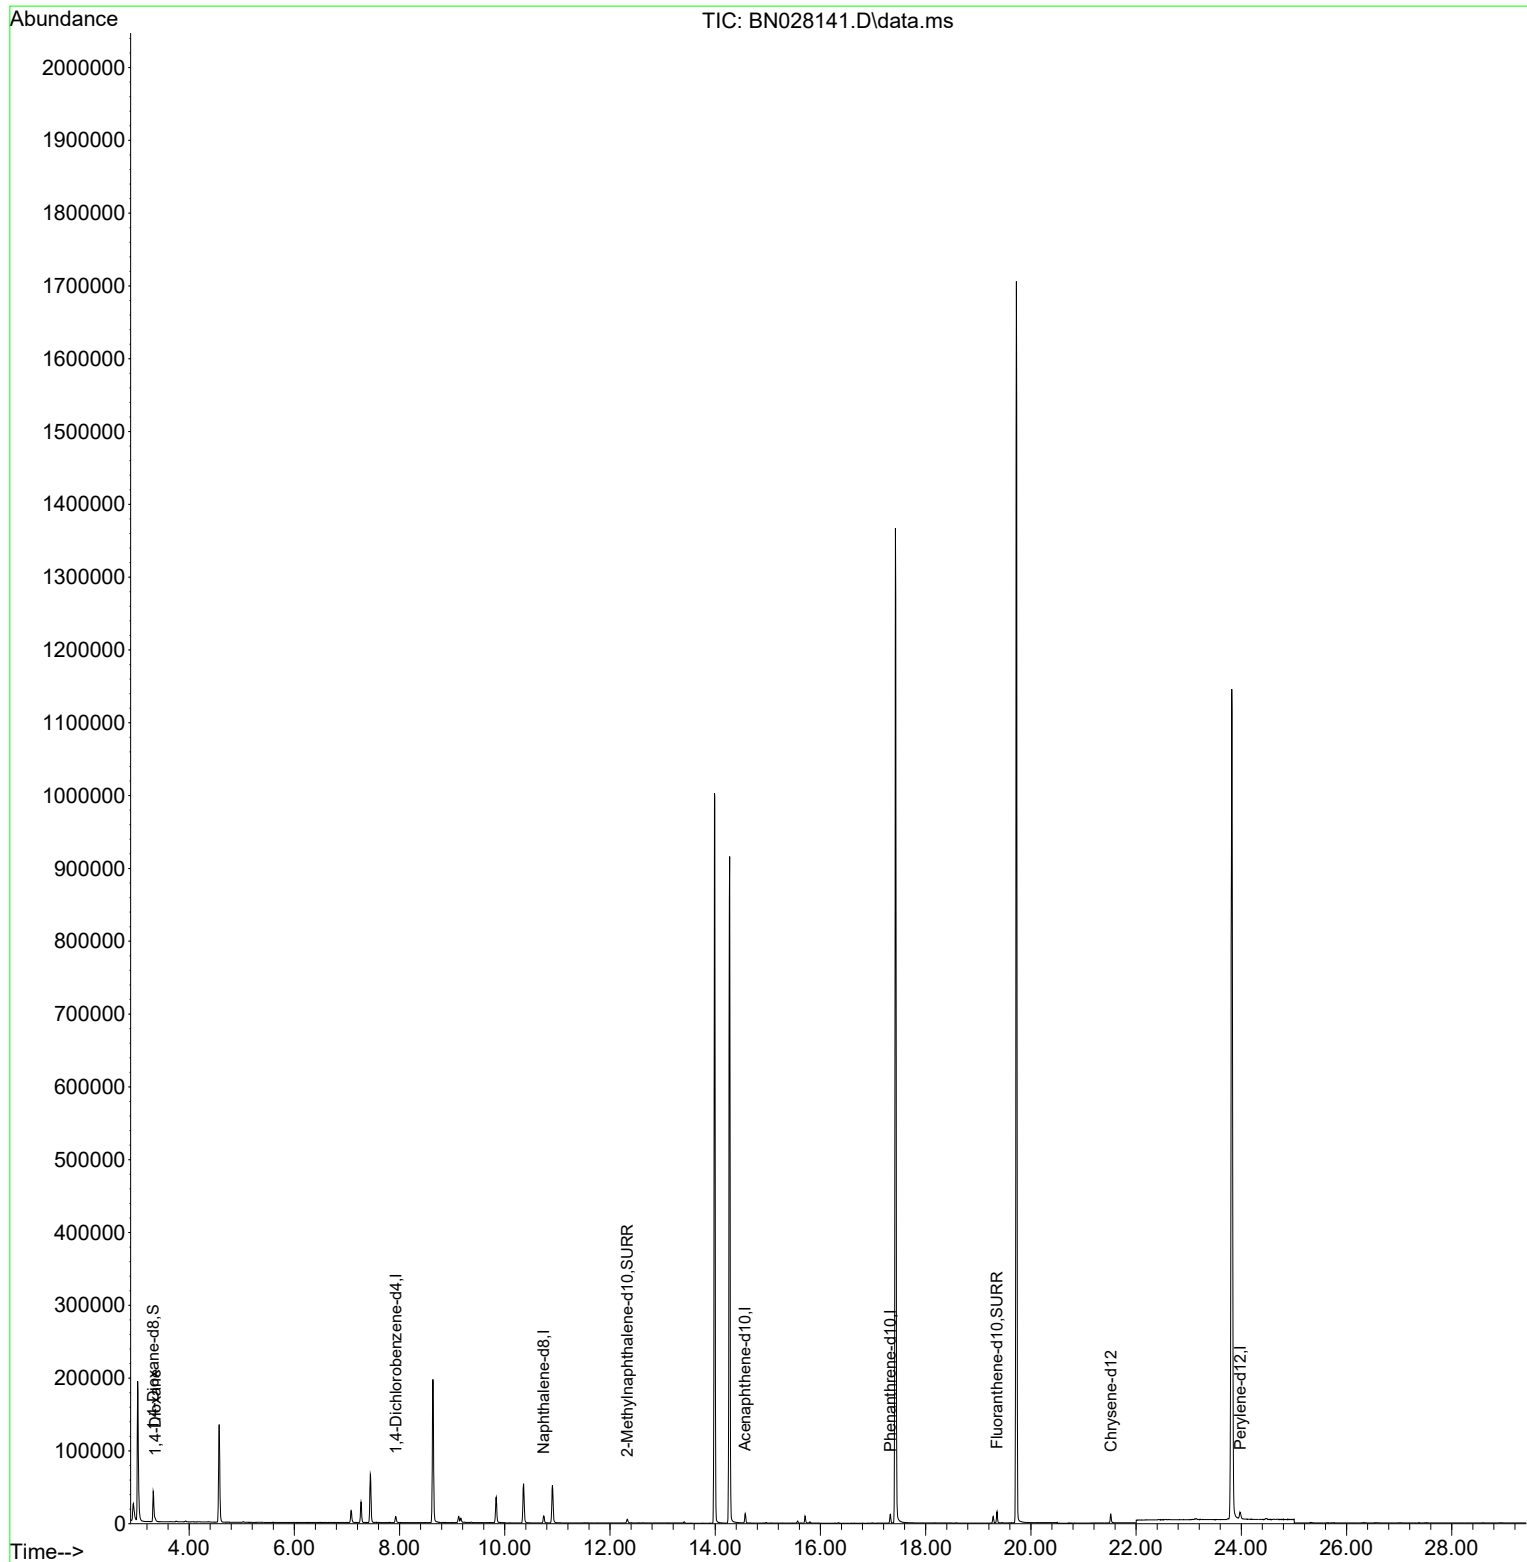

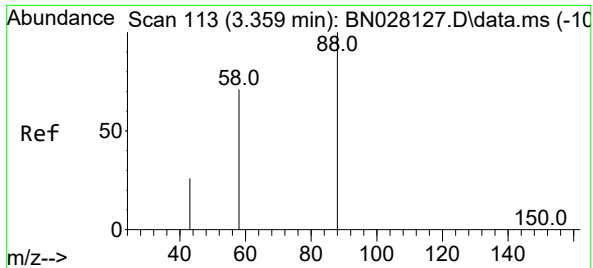

#2
1,4-Dioxane
Concen: 0.386 ng/ul
RT: 3.355 min Scan# 11
Delta R.T. -0.008 min
Lab File: BN028141.D
Acq: 08 Oct 2023 03:31

Instrument :
BNA_N
ClientSampleId :
BBJQ0

Tgt Ion: 88 Resp: 2214
Ion Ratio Lower Upper
88 100
43 41.6 33.4 50.2
58 50.7 45.7 68.5

