

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
 Data File : BN028148.D
 Acq On : 08 Oct 2023 08:21
 Operator : MA/JU
 Sample : 04624-05
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJQ4

Quant Time: Oct 09 00:46:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 06 05:15:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.924	152	3983	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.740	136	11966	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.569	164	6313	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.325	188	12271	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	10256	0.400	ng/ul	0.00
23) Perylene-d12	23.977	264	12039	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	26236	5.244	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.329	152	7214	0.374	ng/ul	0.00
18) Fluoranthene-d10	19.357	212	13856	0.426	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.355	88	1212	0.229	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100523\
Data File : BN028148.D
Acq On : 08 Oct 2023 08:21
Operator : MA/JU
Sample : 04624-05
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJQ4

Quant Time: Oct 09 00:46:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 06 05:15:40 2023
Response via : Initial Calibration

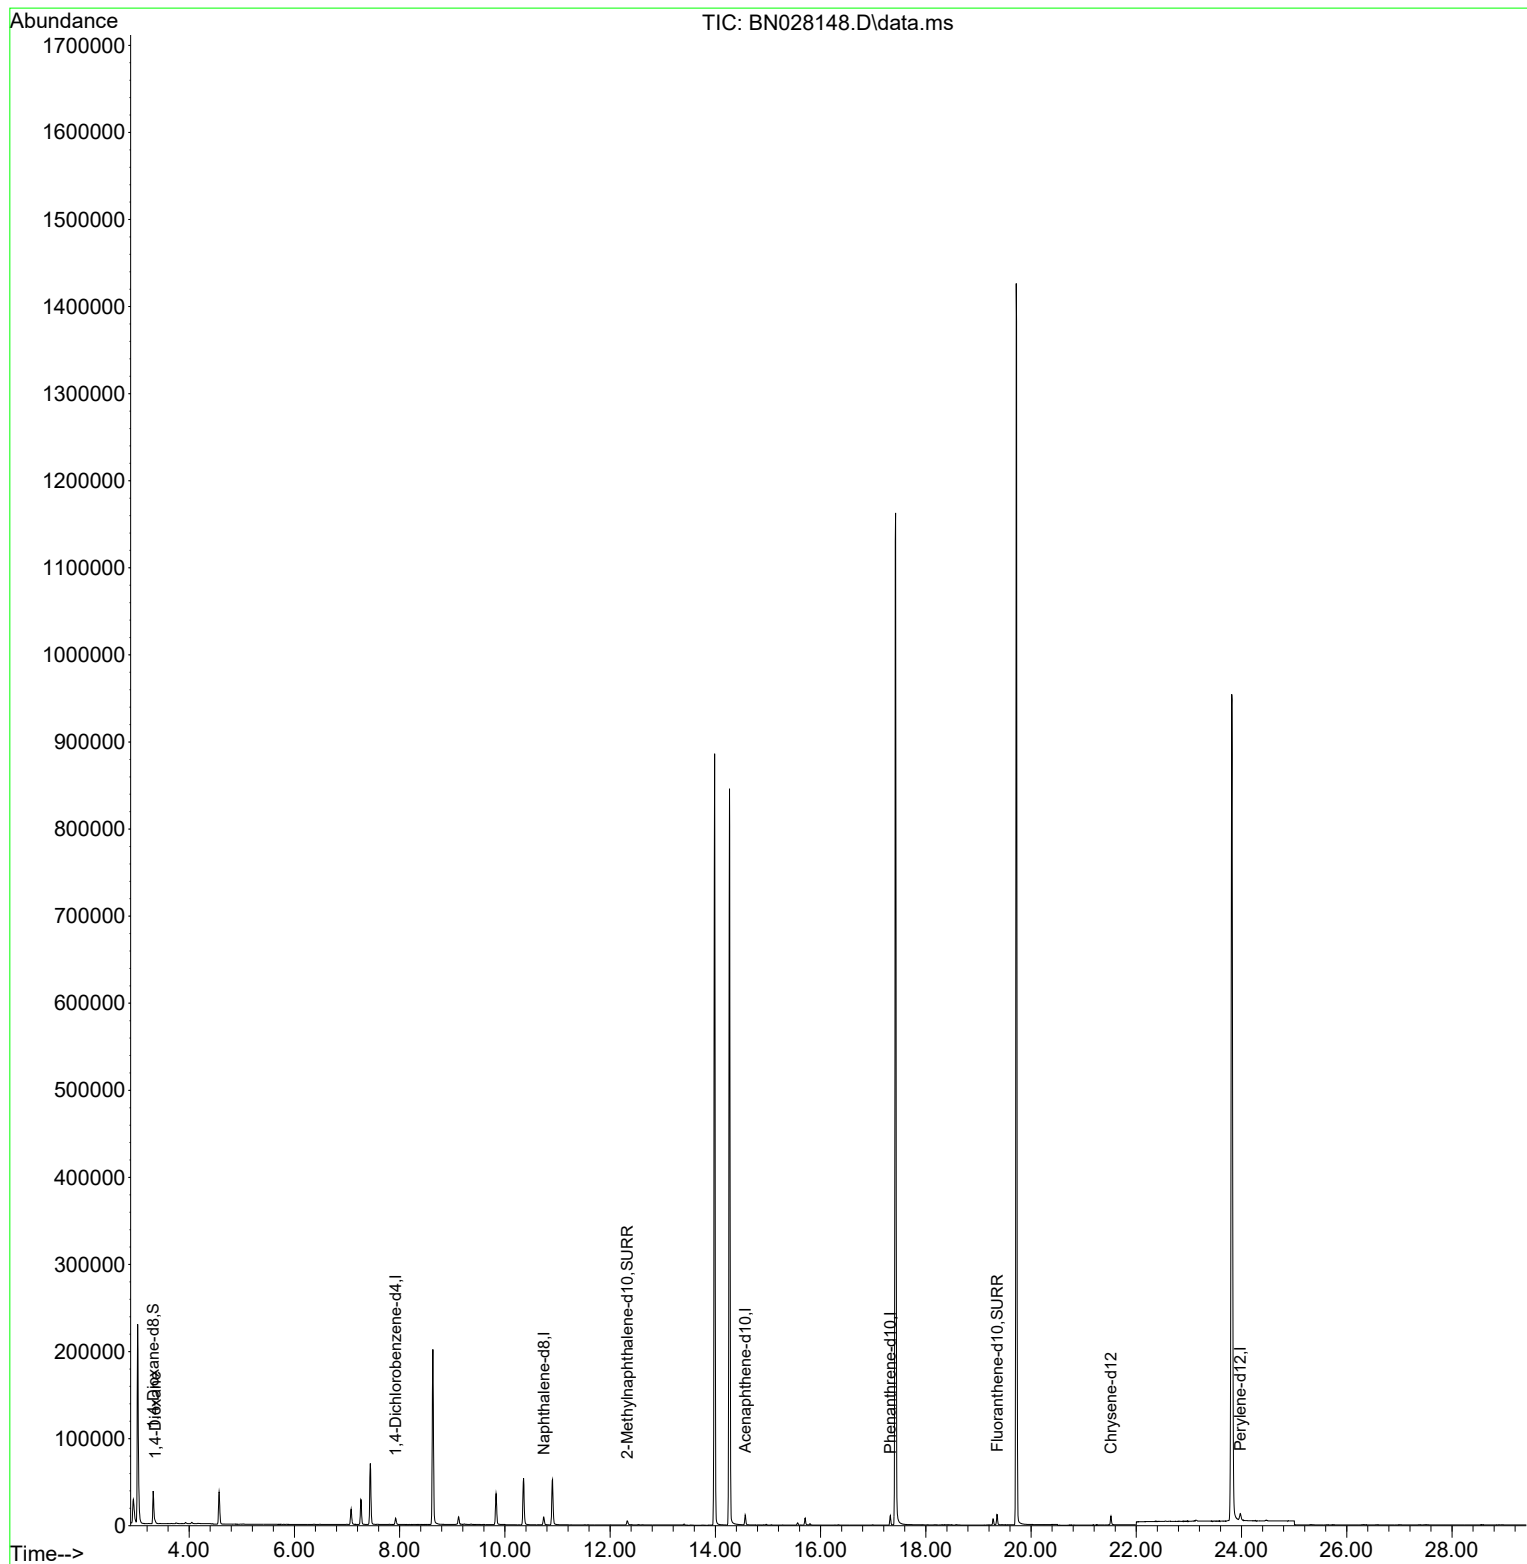

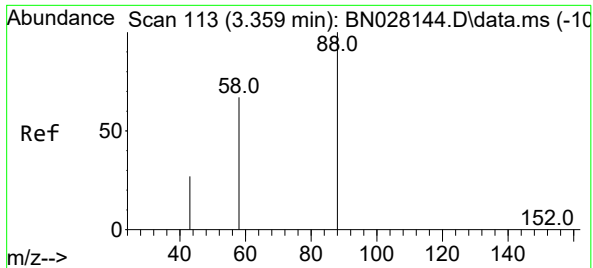

1,4-Dioxane
 Concen: 0.229 ng/ul
 RT: 3.355 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN028148.D
 Acq: 08 Oct 2023 08:21

Instrument :
 BNA_N
 ClientSampleId :
 BBJQ4

Tgt Ion: 88	Resp:	1212
Ion	Ratio	Lower Upper
88	100	
43	48.3	33.4 50.2
58	53.7	45.7 68.5

