

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100523\  
 Data File : BN028149.D  
 Acq On : 08 Oct 2023 08:57  
 Operator : MA/JU  
 Sample : 04624-06  
 Misc :  
 ALS Vial : 78 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BBKB3

Quant Time: Oct 09 00:47:01 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN100323.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Oct 06 05:15:40 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.924	152	3970	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.740	136	11962	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.569	164	6328	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.325	188	12403	0.400	ng/ul	0.00
17) Chrysene-d12	21.516	240	10349	0.400	ng/ul	0.00
23) Perylene-d12	23.974	264	11959	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	27743	5.564	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.324	152	7652	0.397	ng/ul	-0.01
18) Fluoranthene-d10	19.352	212	16081	0.490	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.355	88	939	0.178	ng/ul#	83
-----						


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100523\  
Data File : BN028149.D  
Acq On : 08 Oct 2023 08:57  
Operator : MA/JU  
Sample : 04624-06  
Misc :  
ALS Vial : 78 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
BBKB3

Quant Time: Oct 09 00:47:01 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN100323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 06 05:15:40 2023  
Response via : Initial Calibration

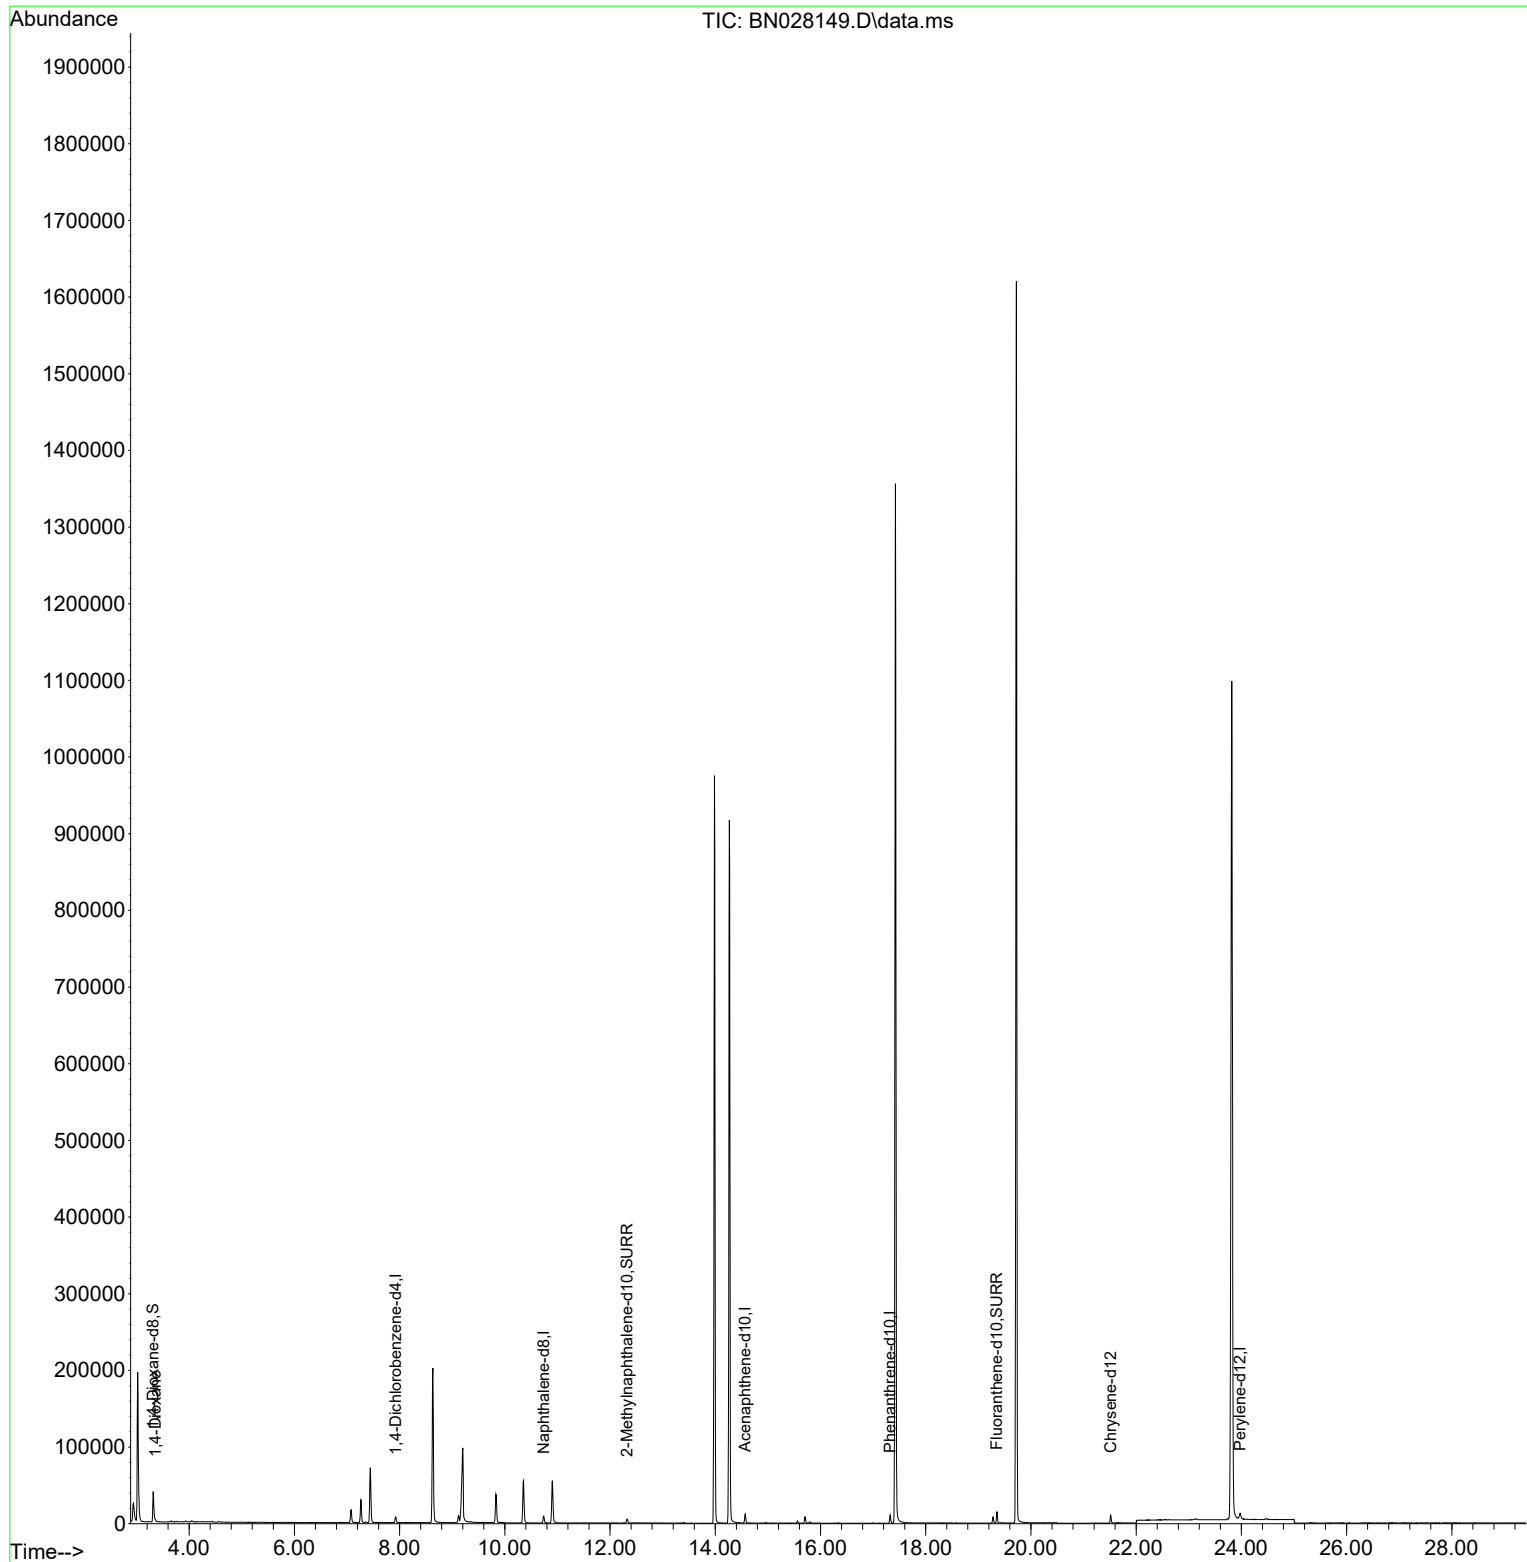

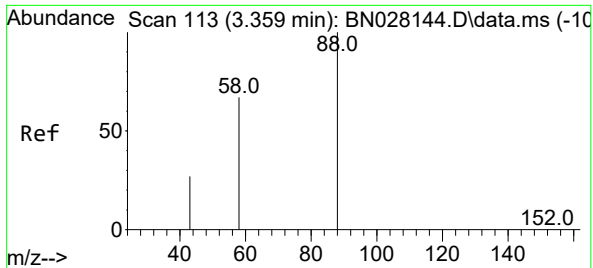

1,4-Dioxane  
 Concen: 0.178 ng/ul  
 RT: 3.355 min Scan# 11  
 Delta R.T. -0.009 min  
 Lab File: BN028149.D  
 Acq: 08 Oct 2023 08:57

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BBKB3

Tgt Ion: 88 Resp: 939

Ion	Ratio	Lower	Upper
88	100		
43	53.2	33.4	50.2#
58	45.0	45.7	68.5#

