
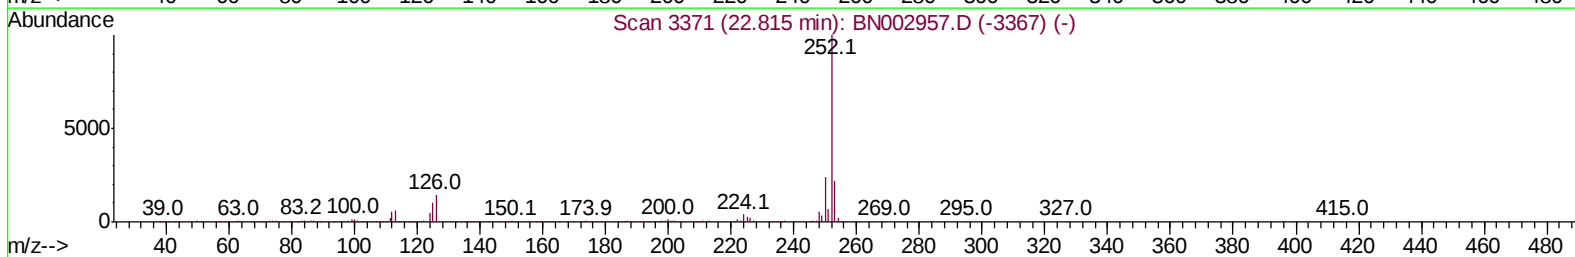
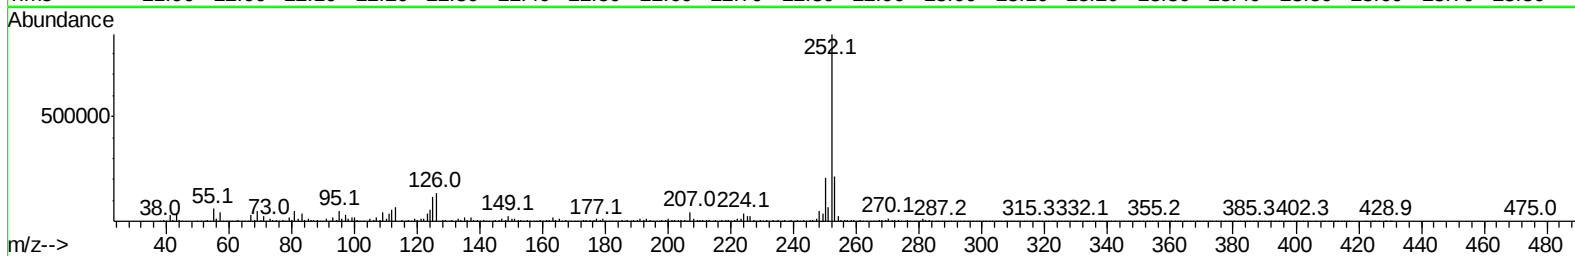


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002960.D
Acq On : 05 Oct 2018 11:02
Operator : MJ/SJ
Sample : J5183-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Oct 06 01:08:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

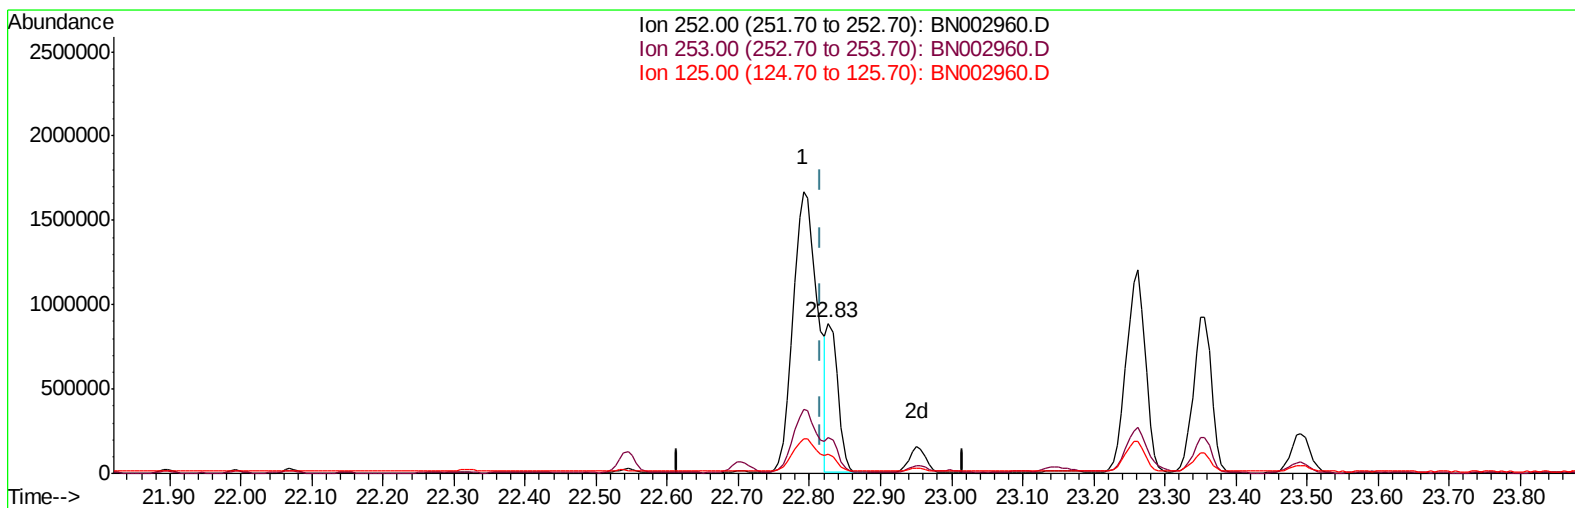

TIC: BN002960.D

(88) Benzo(k)fluoranthene

22.827min (+0.012) 31.22ng/ul m

response 943693

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.87
125.00	10.40	12.81#
0.00	0.00	0.00