
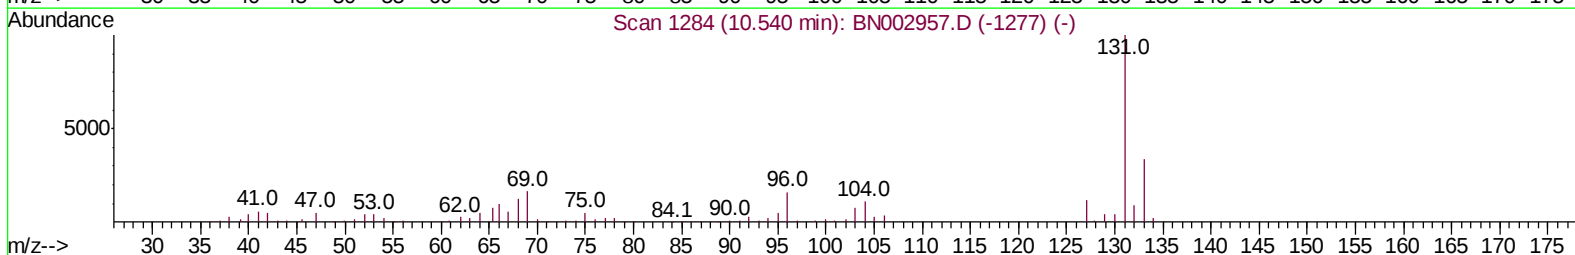
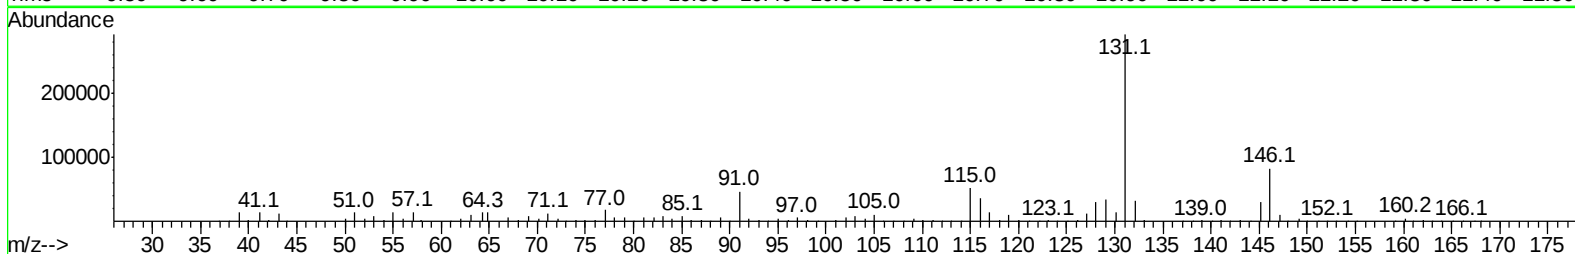


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 06 01:10:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

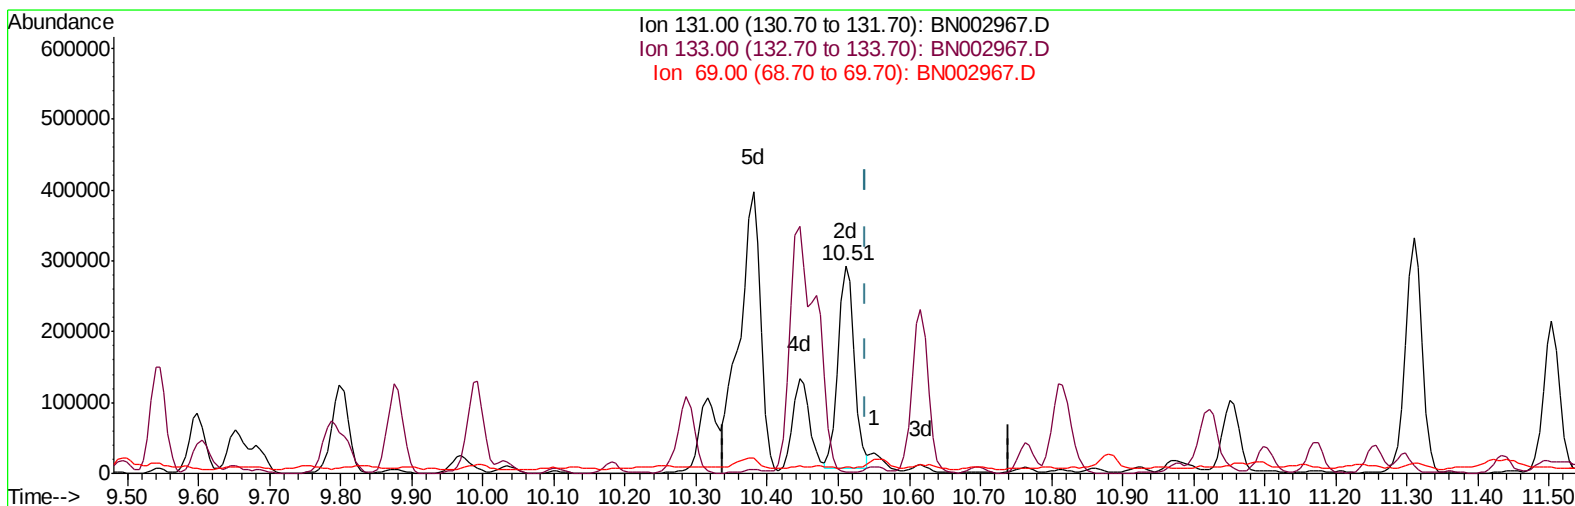

TIC: BN002967.D

(29) 4-Chloroaniline-d4 (S)

10.510min (-0.030) 40.44ng/ul m

response 453256

Ion	Exp%	Act%
131.00	100	100
133.00	32.90	0.94#
69.00	16.80	2.90#
0.00	0.00	0.00