
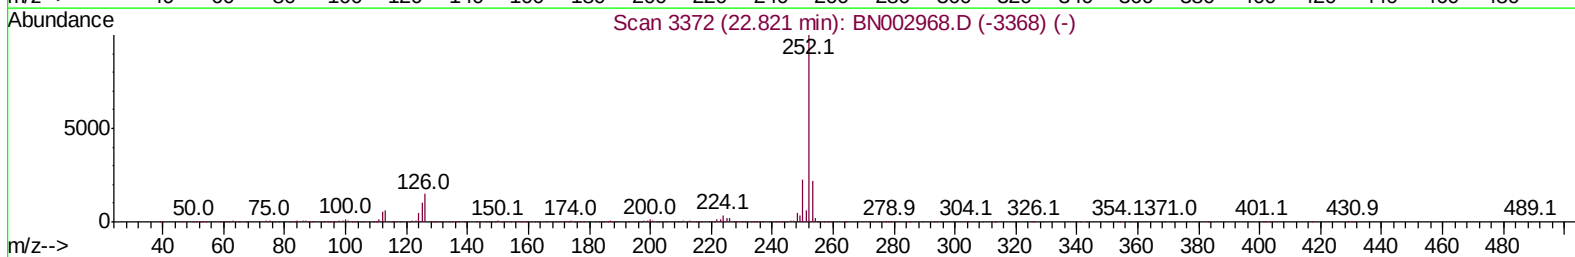
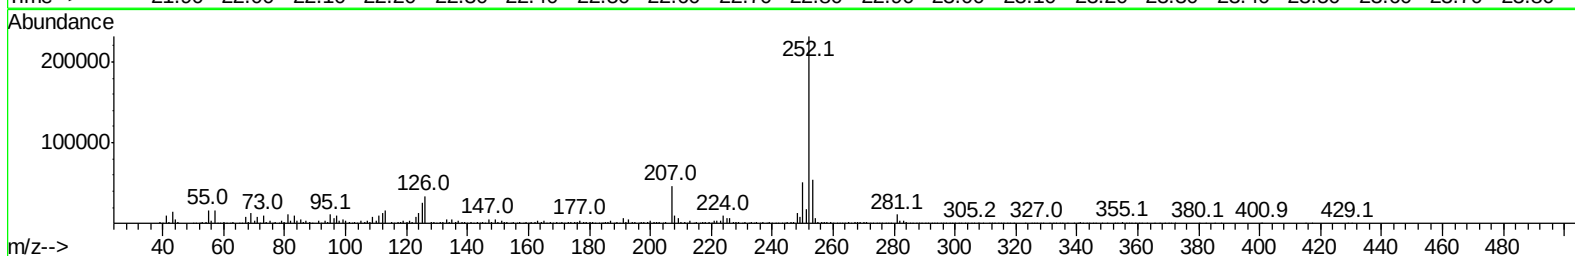


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002974.D
Acq On : 05 Oct 2018 21:55
Operator : MJ/SJ
Sample : J5230-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 06 02:56:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 02:55:40 2018
Response via : Initial Calibration

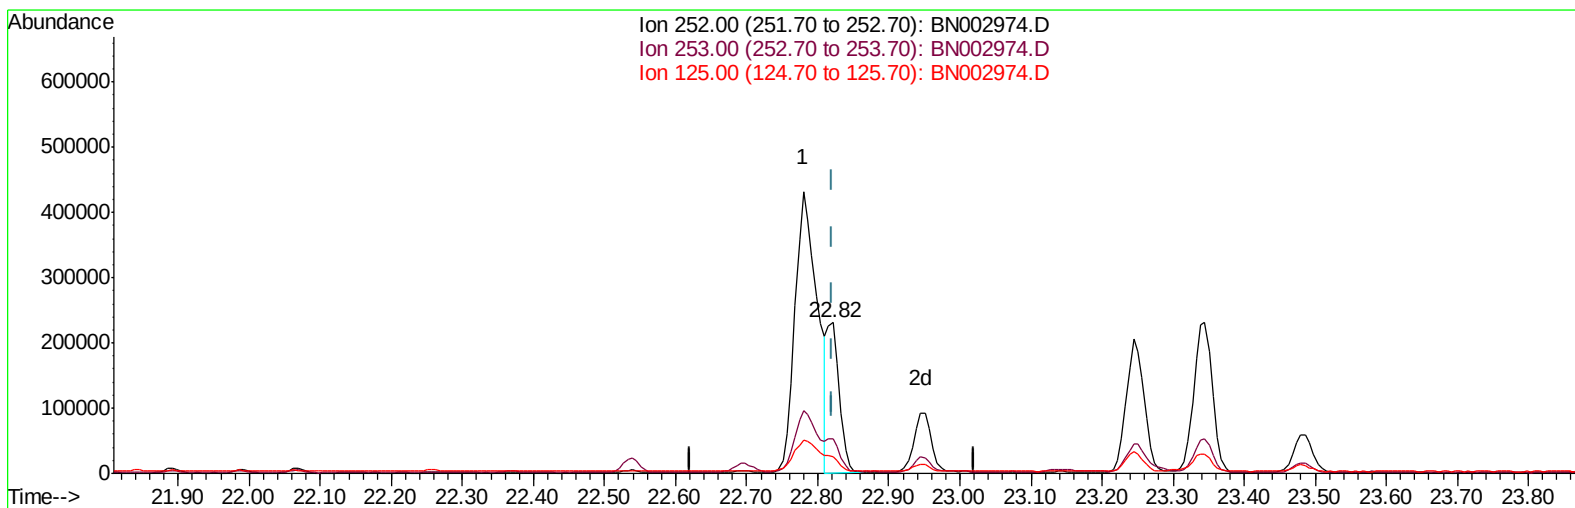

TIC: BN002974.D

(88) Benzo(k)fluoranthene

22.821min (-0.000) 6.98ng/ul m

response 269678

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.16
125.00	10.40	10.99
0.00	0.00	0.00