
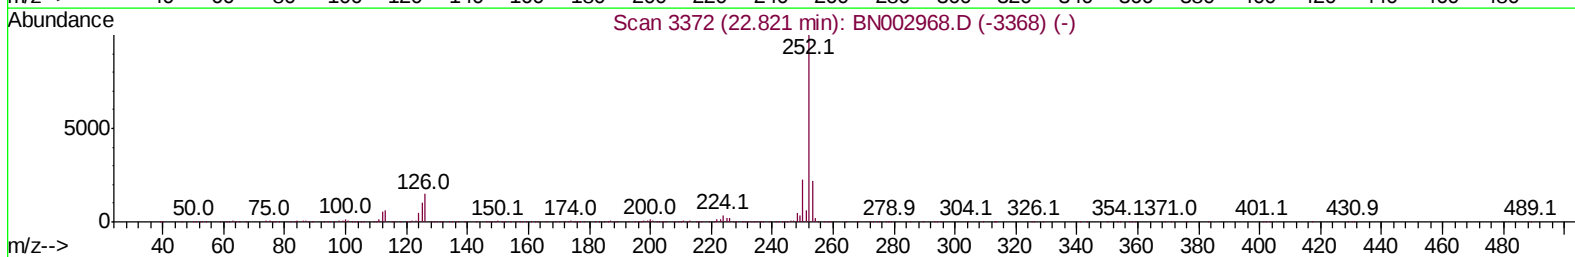
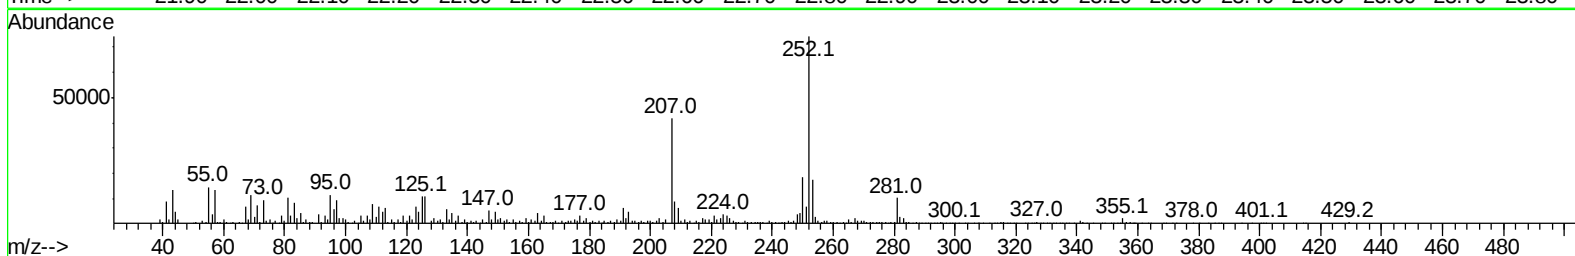


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002976.D
Acq On : 05 Oct 2018 23:05
Operator : MJ/SJ
Sample : J5230-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 06 02:57:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 02:55:40 2018
Response via : Initial Calibration

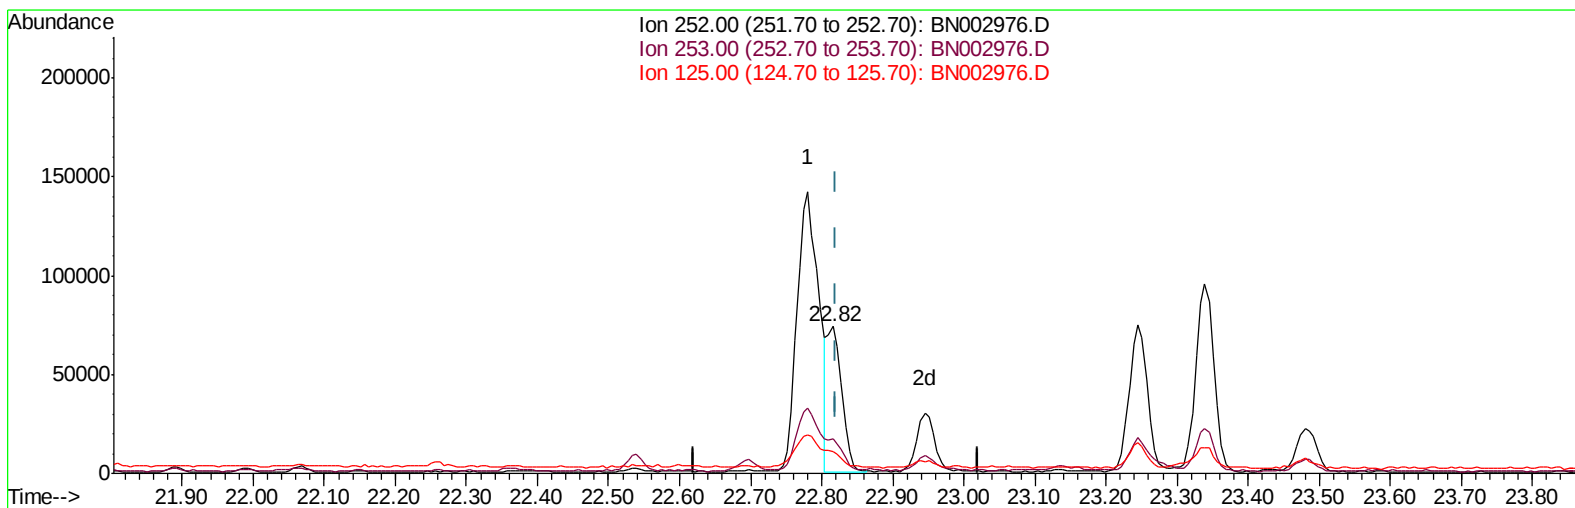

TIC: BN002976.D

(88) Benzo(k)fluoranthene

22.816min (-0.006) 2.76ng/ul m

response 101908

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.83
125.00	10.40	14.45#
0.00	0.00	0.00