

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
 Data File : BN002969.D
 Acq On : 05 Oct 2018 18:59
 Operator : MJ/SJ
 Sample : PB113526BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 06 02:56:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 06 02:55:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	113139	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	500681	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	320363	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	764903	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	790954	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	718366	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11653	4.75	ng/uL	0.00
5) Phenol-d5	6.82	99	230163	23.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	143298	24.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	195137	24.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	186471	25.06	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	96912	24.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	126525	28.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	194866	24.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	278876	30.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	713086	28.44	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	819031	25.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	101551	24.49	ng/ul	0.00
57) Fluorene-d10	15.26	176	592625	26.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	42745	8.93	ng/ul	0.00
70) Anthracene-d10	17.12	188	949151	25.99	ng/ul	0.00
78) Pyrene-d10	19.42	212	1034166	24.78	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	981038	25.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
75) Di-n-butylphthalate	17.99	149	197599	4.491	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
Data File : BN002969.D
Acq On : 05 Oct 2018 18:59
Operator : MJ/SJ
Sample : PB113526BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 06 02:56:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 02:55:40 2018
Response via : Initial Calibration

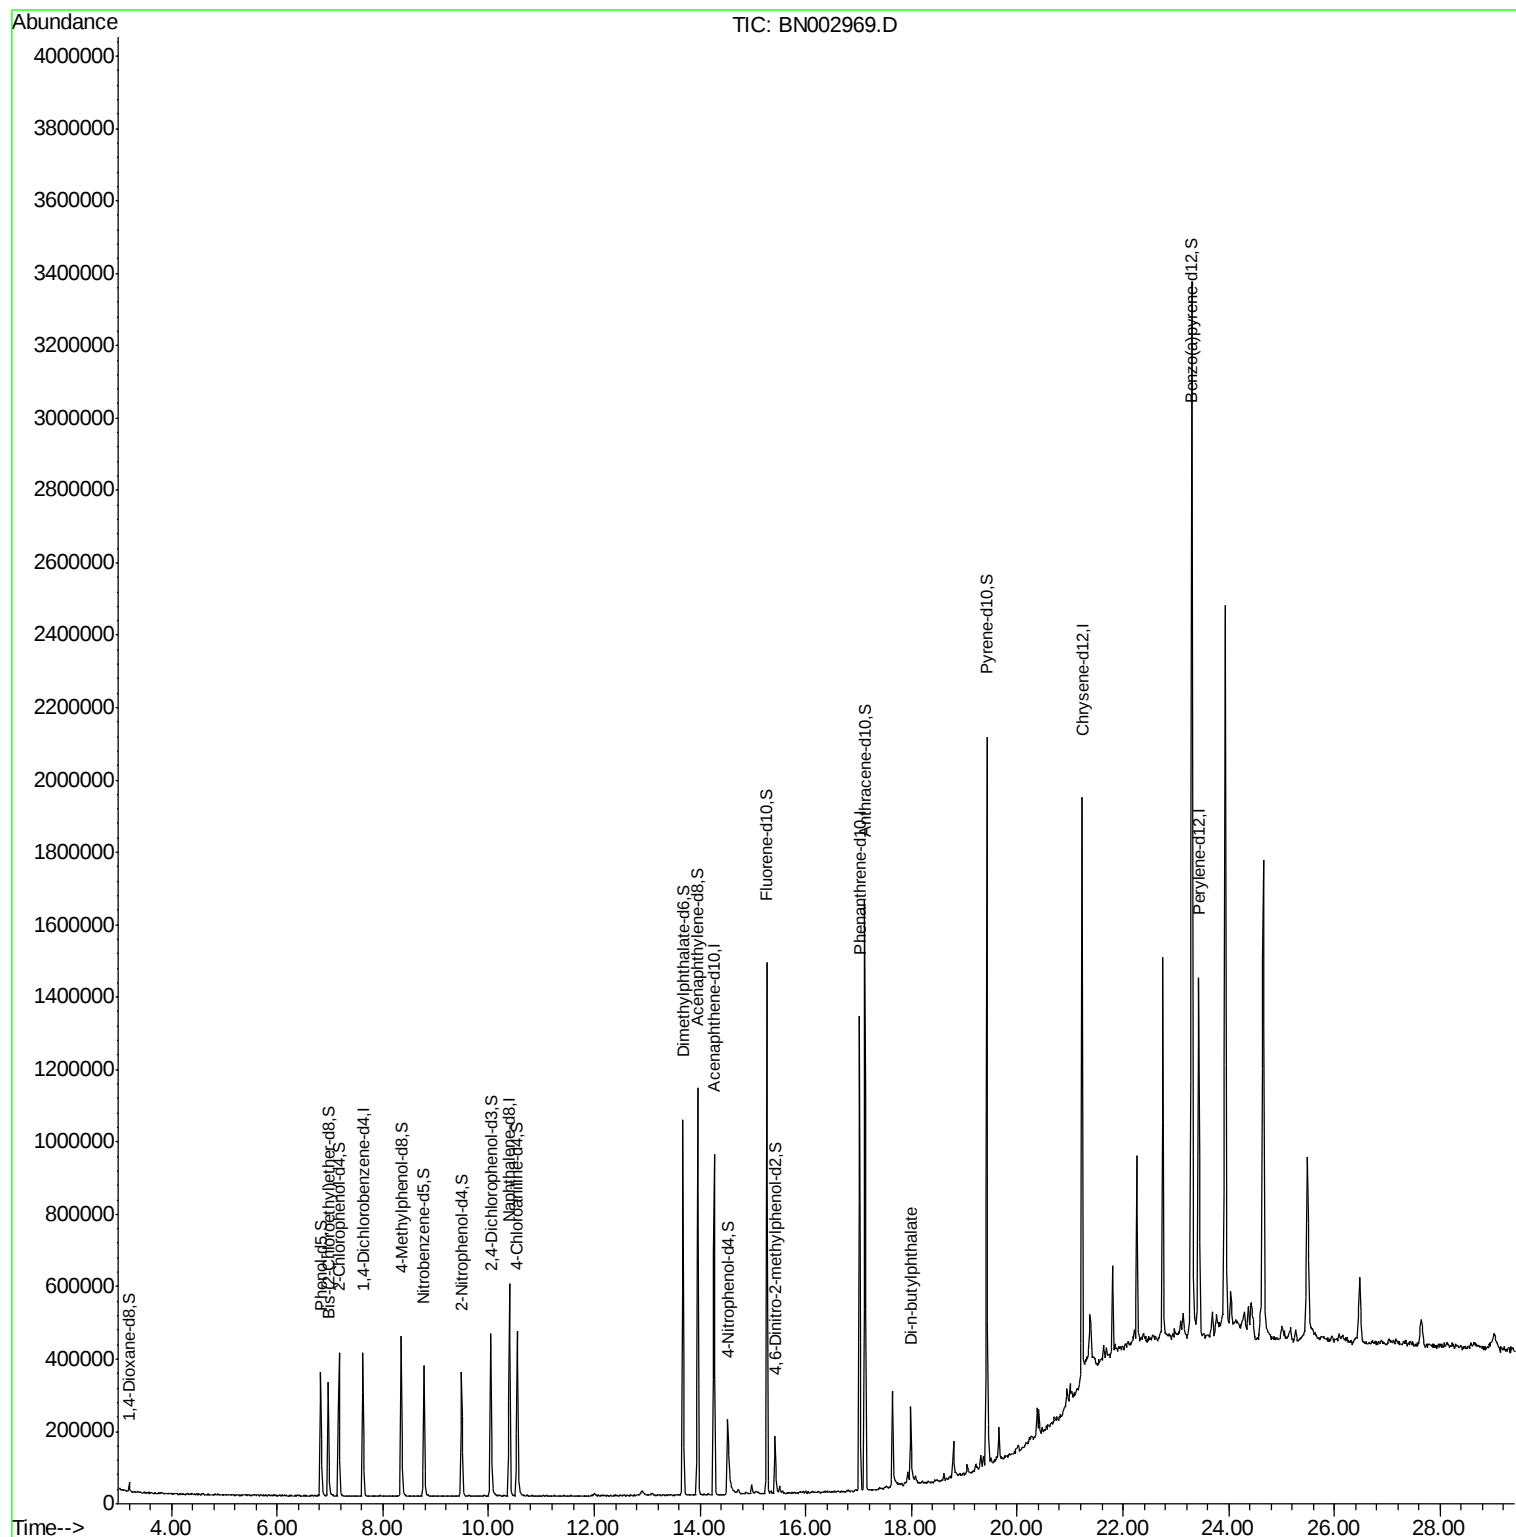


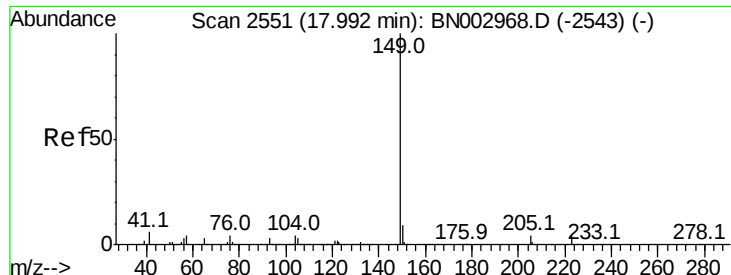

#75
 Di-n-butylphthalate
 Concen: 4.491 ng/ul
 RT: 17.99 min Scan# 2551
 Delta R.T. -0.00 min
 Lab File: BN002969.D
 Acq: 05 Oct 2018 18:59

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
149	100		
150	8.9	7.3	10.9
104	4.3	3.7	5.5

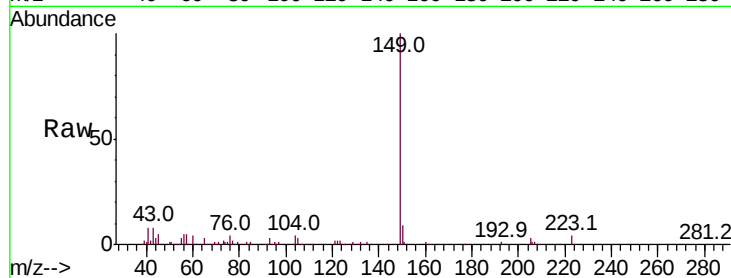

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 104.00 (103.70 to 104.70): E

