


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLC29DL

Manual Integrations
APPROVED

Sohil
10/8/2018 5:53:32 PM

Quant Time: Oct 06 02:37:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

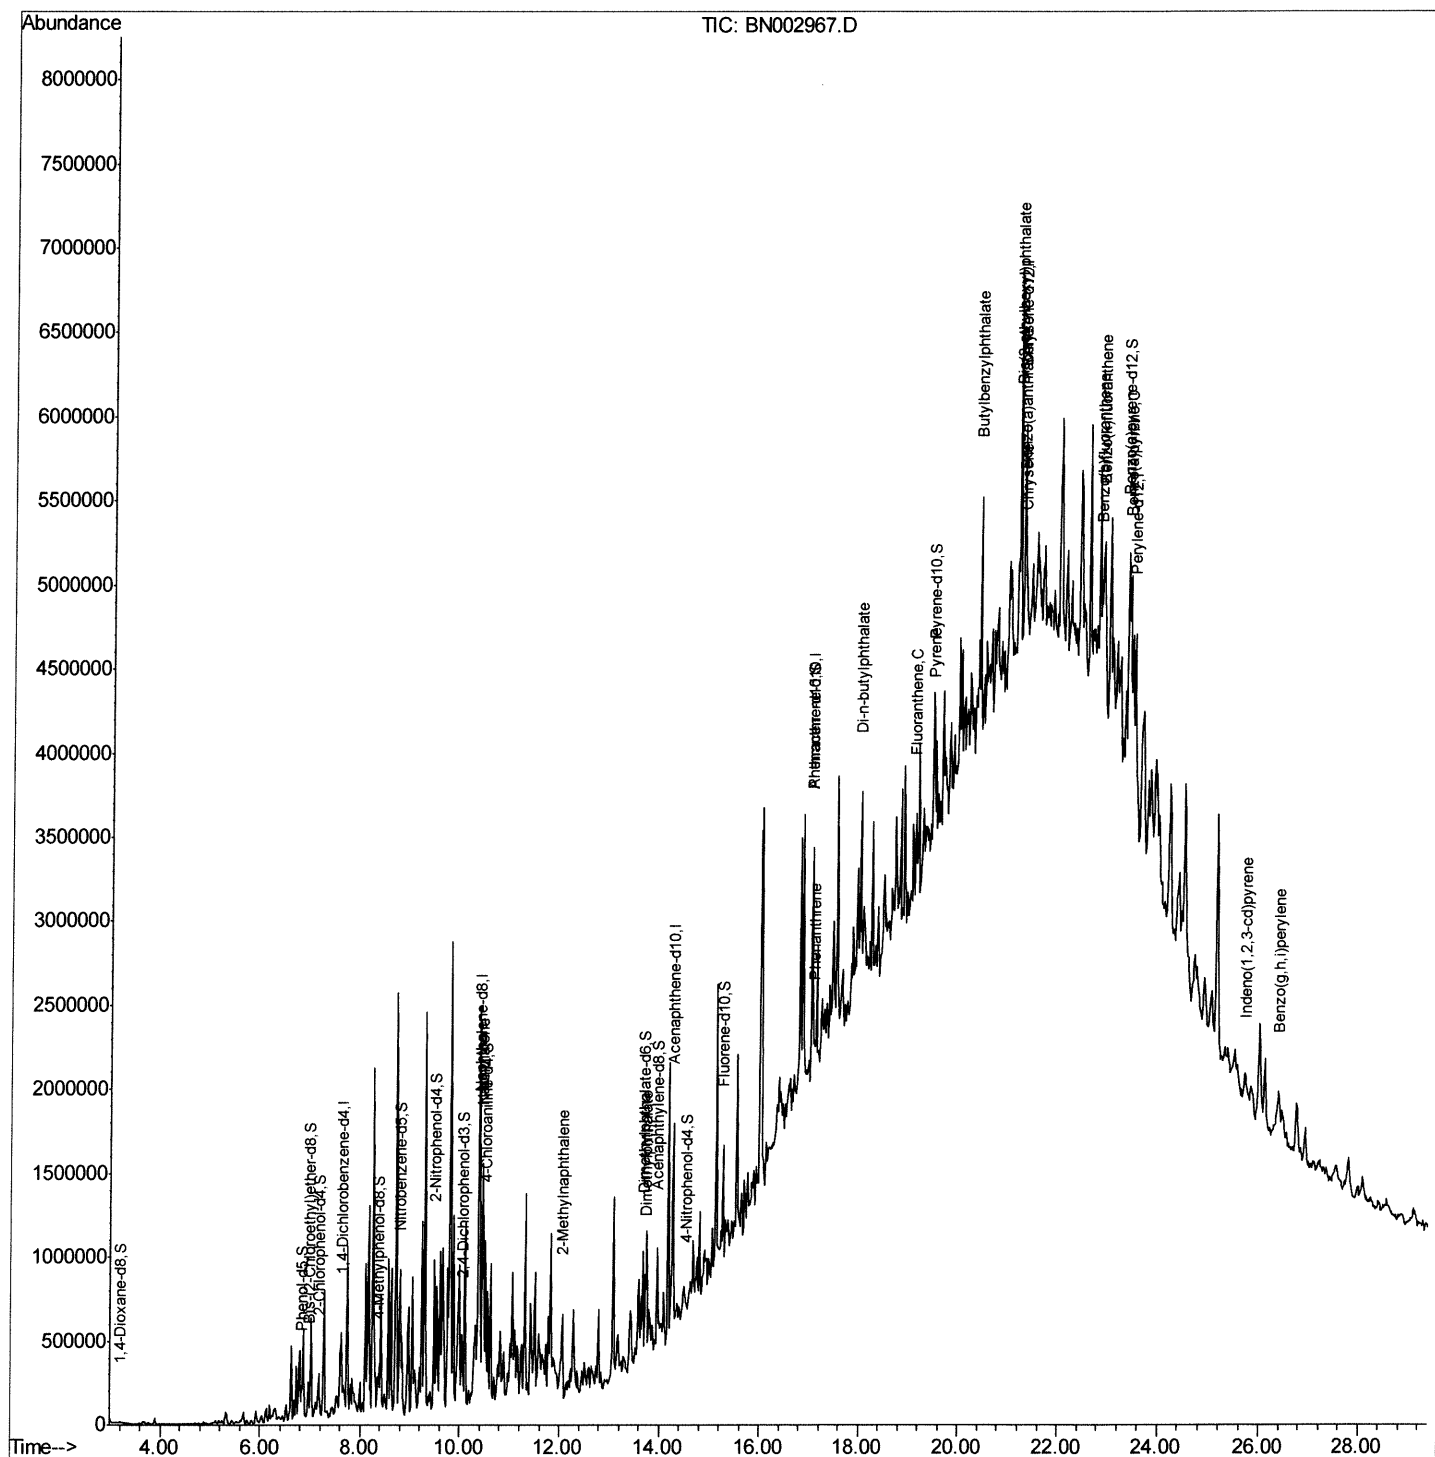

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC29DL

Manual Integrations
APPROVED

Sohil
10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

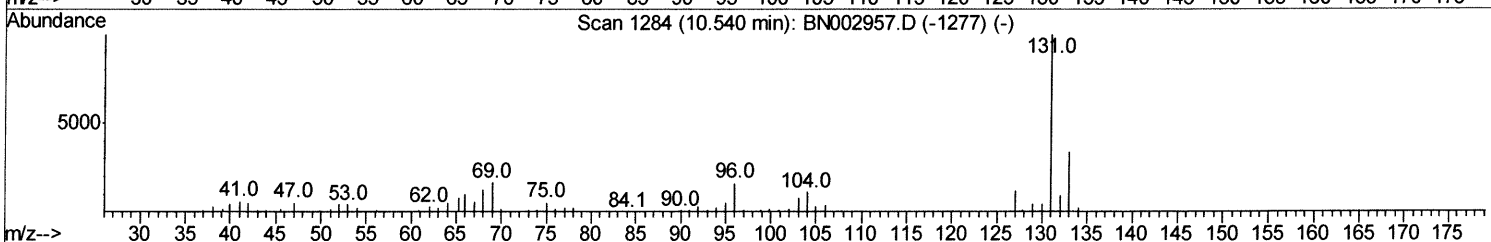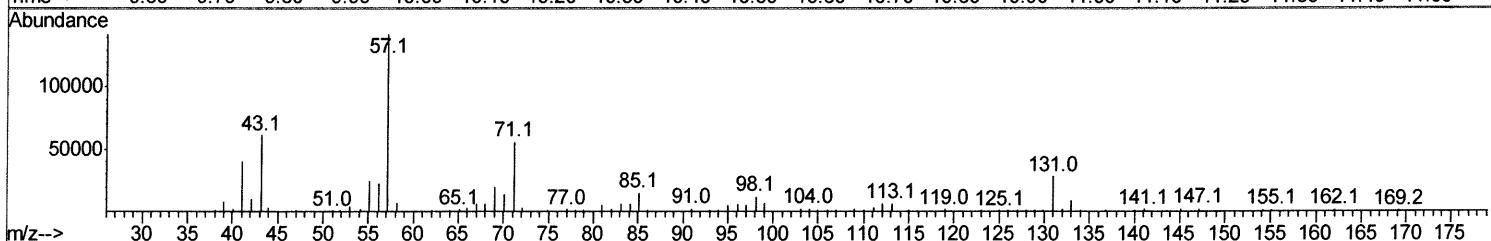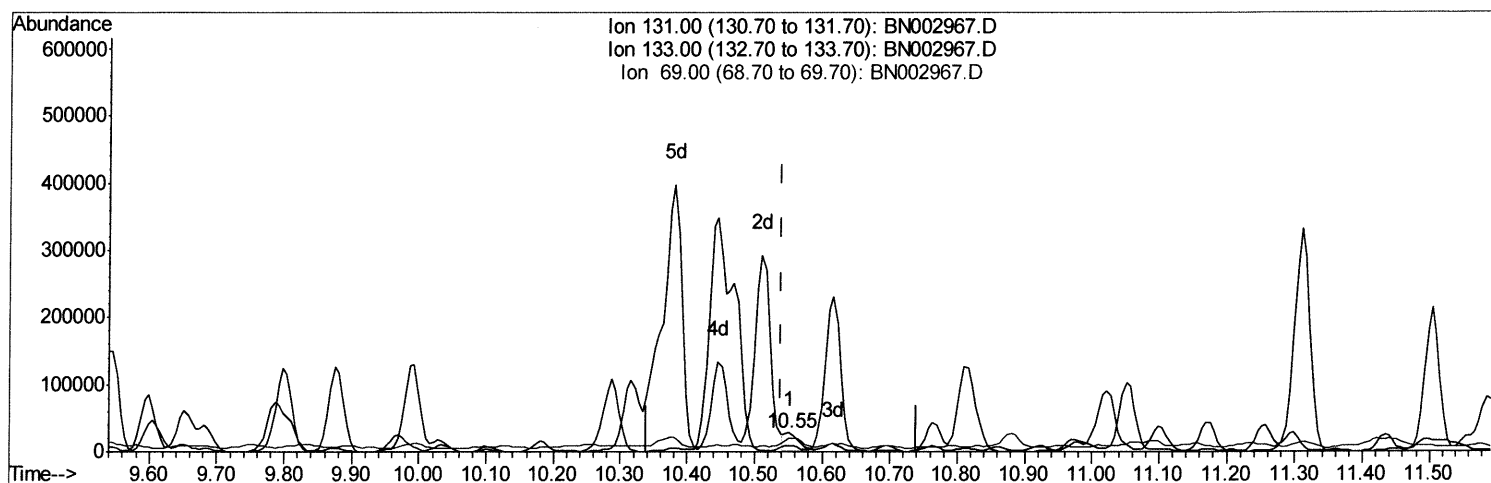

TIC: BN002967.D

(29) 4-Chloroaniline-d4 (S)

10.551min (+0.011) 3.67ng/ul

response 41078

Ion	Exp%	Act%
131.00	100	100
133.00	32.90	32.37
69.00	16.80	69.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC29DL

Manual Integrations
APPROVED

Sohil
10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

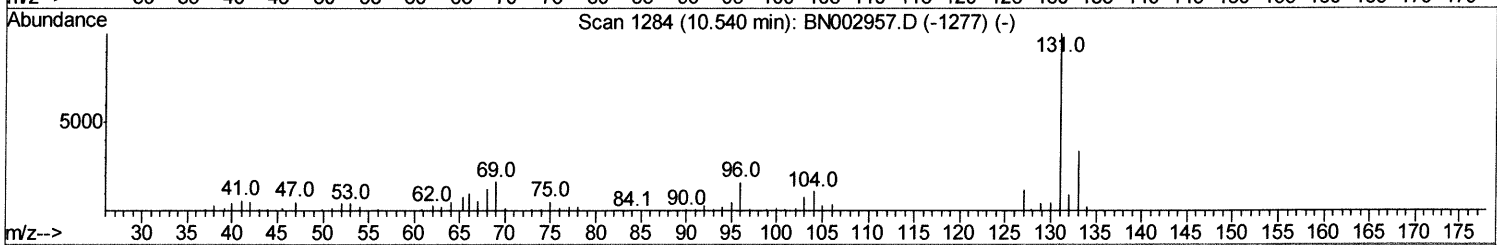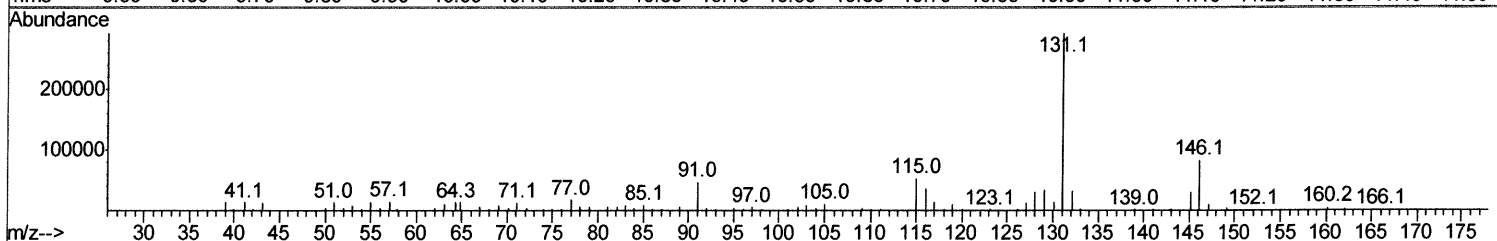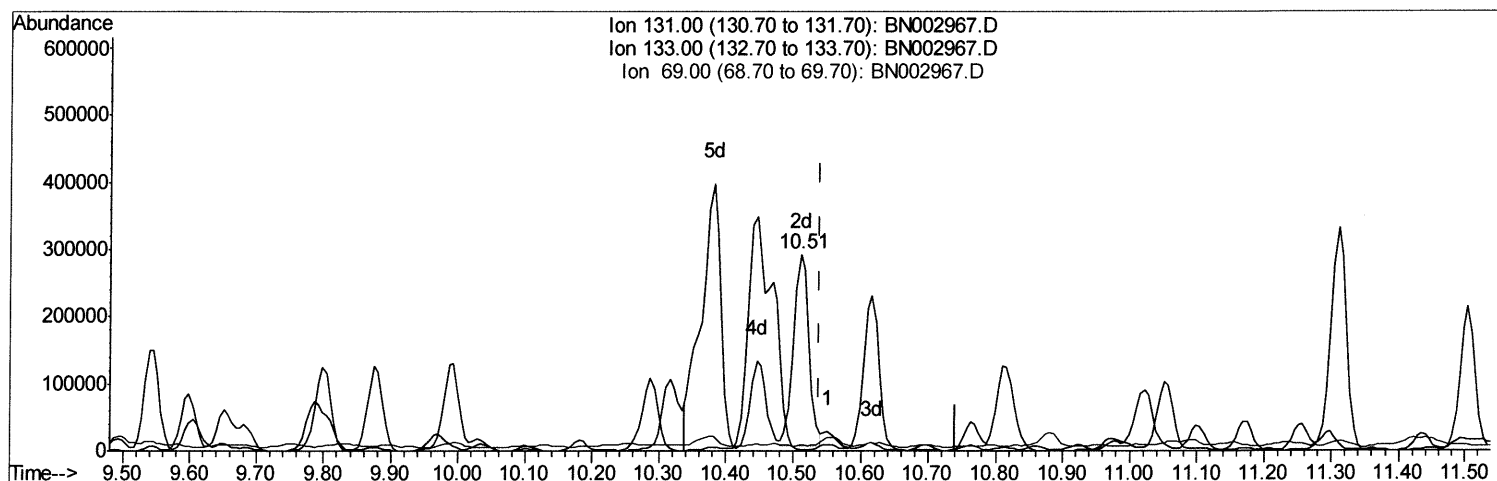

TIC: BN002967.D

(29) 4-Chloroaniline-d4 (S)

10.510min (-0.030) 40.44ng/ul m

response 453256

Ion	Exp%	Act%
131.00	100	100
133.00	32.90	0.94#
69.00	16.80	2.90#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
 Data File : BN002967.D
 Acq On : 05 Oct 2018 15:27
 Operator : MJ/SJ
 Sample : J5183-14DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC29DL

Manual Integrations
 APPROVED

Sohil
 10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 06 01:07:30 2018
 Response via : Initial Calibration

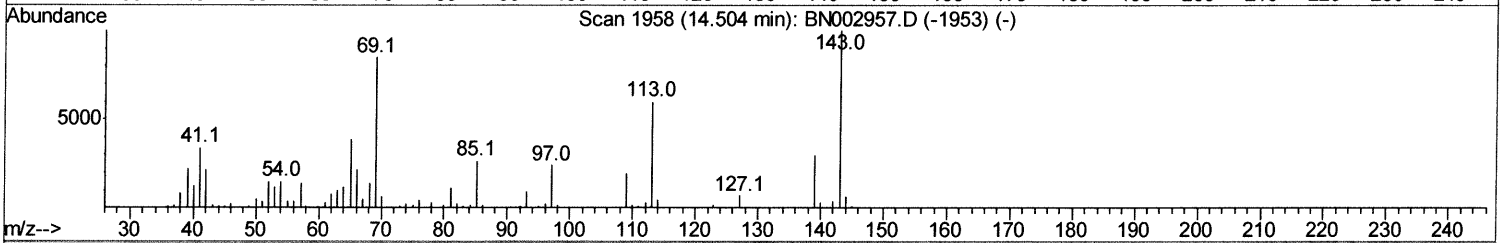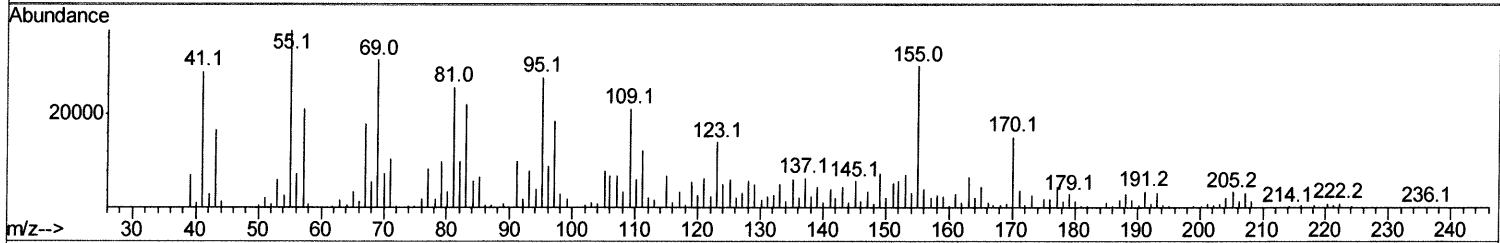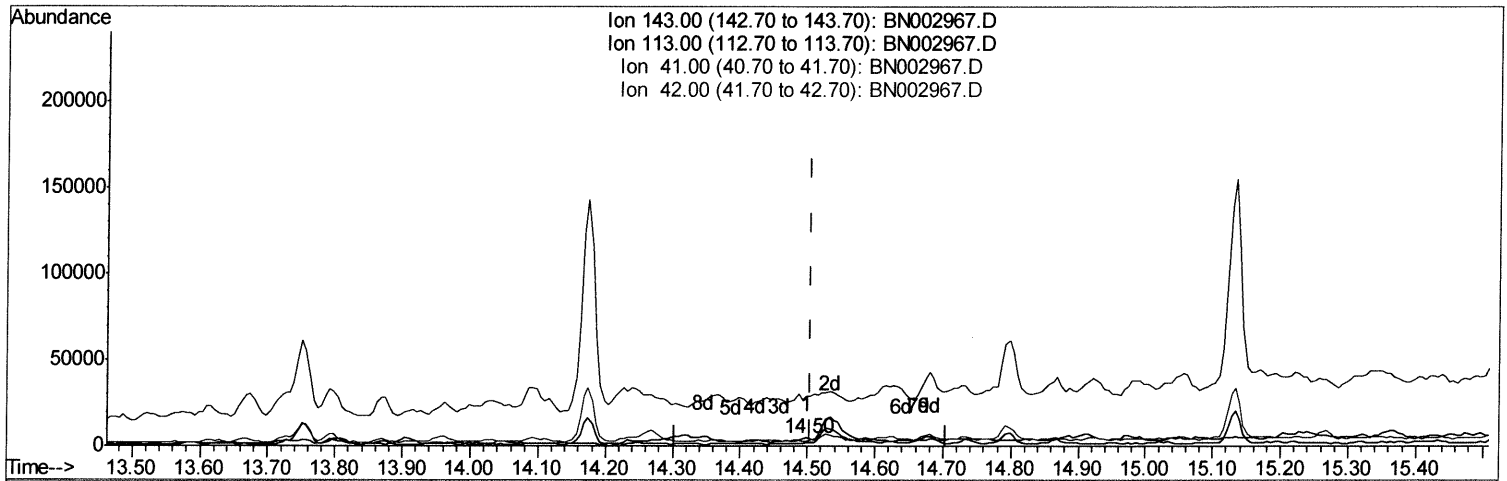

TIC: BN002967.D

(51) 4-Nitrophenol-d4 (S)
 14.498min (-0.006) 0.65ng/ul
 response 2992

Ion	Exp%	Act%
143.00	100	100
113.00	66.10	39.29#
41.00	39.90	617.16#
42.00	25.80	65.99#

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
 Data File : BN002967.D
 Acq On : 05 Oct 2018 15:27
 Operator : MJ/SJ
 Sample : J5183-14DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC29DL

Manual Integrations
 APPROVED

Sohil
 10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 06 01:07:30 2018
 Response via : Initial Calibration

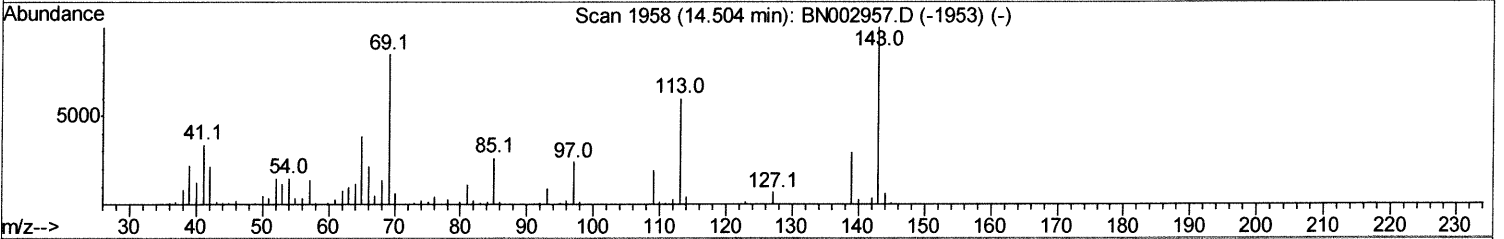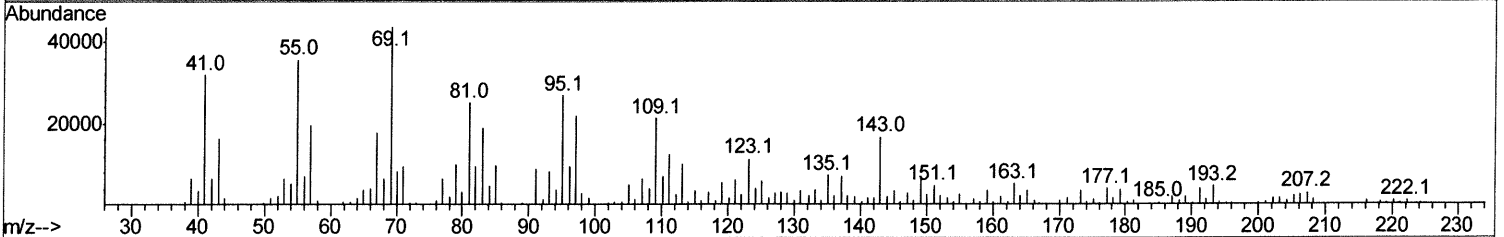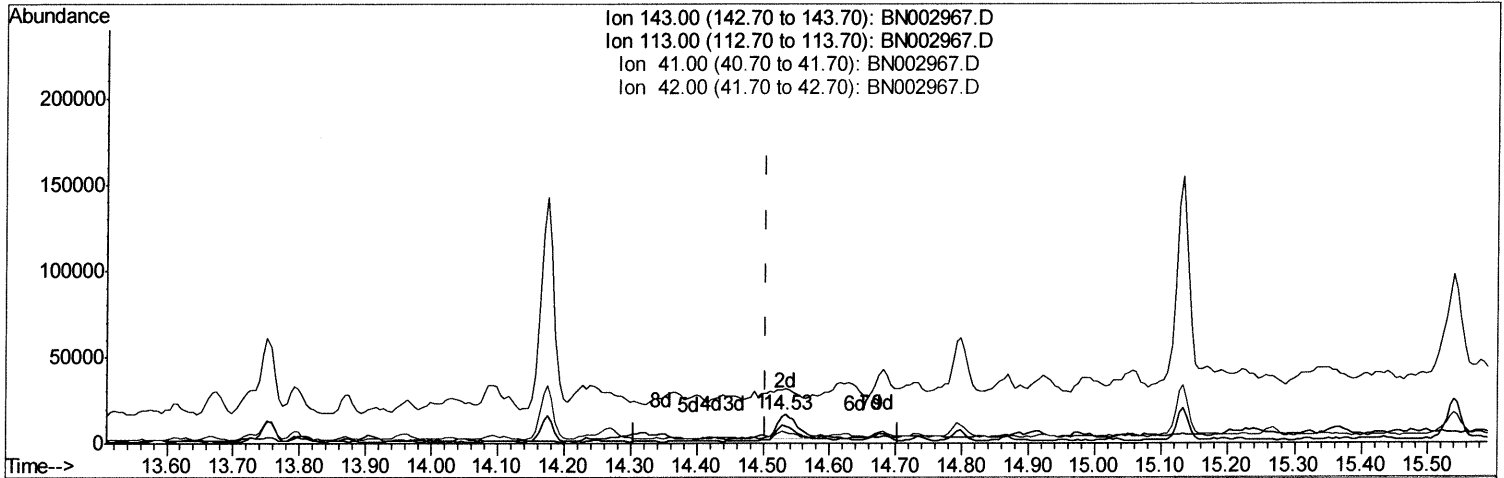

TIC: BN002967.D

(51) 4-Nitrophenol-d4 (S)

14.533min (+0.029) 6.73ng/ul m

response 31102

Ion	Exp%	Act%
143.00	100	100
113.00	66.10	61.12
41.00	39.90	191.52#
42.00	25.80	40.10#

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC29DL

Manual Integrations
APPROVED

Sohil
10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

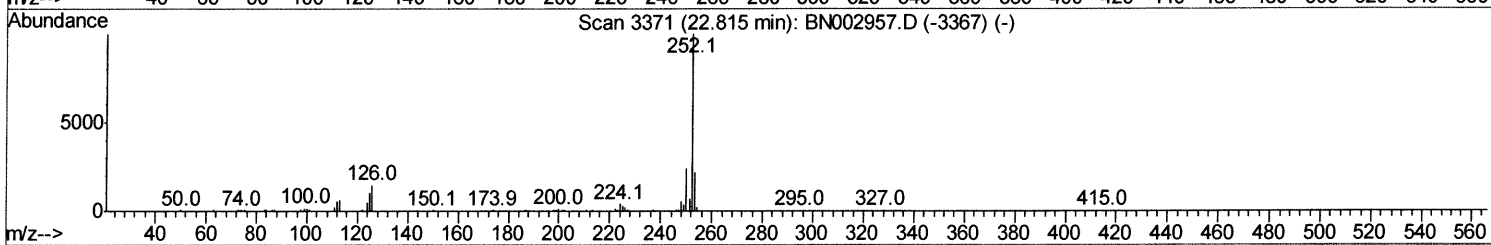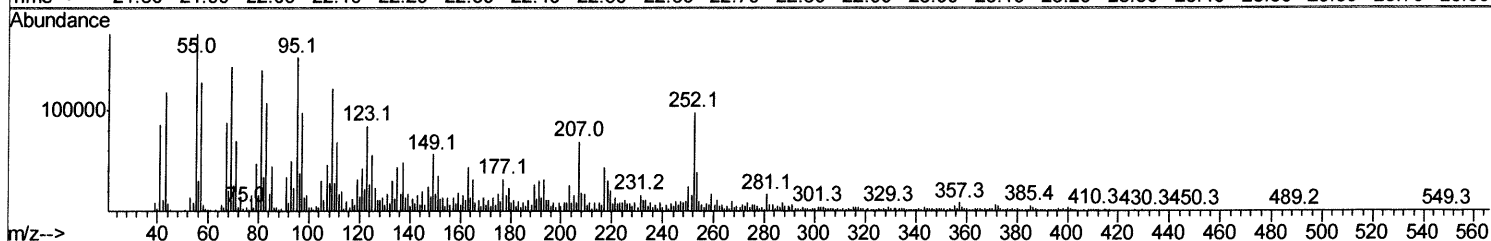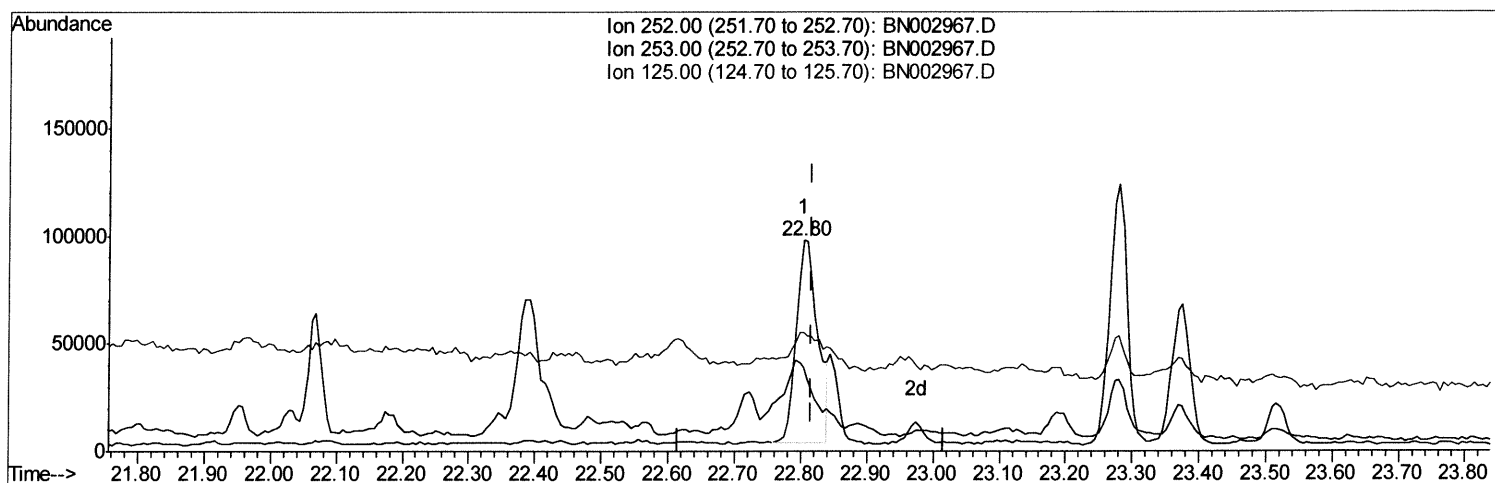

TIC: BN002967.D

(88) Benzo(k)fluoranthene

22.803min (-0.012) 6.94ng/ul

response 213780

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	39.46#
125.00	10.40	56.46#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100618\
Data File : BN002967.D
Acq On : 05 Oct 2018 15:27
Operator : MJ/SJ
Sample : J5183-14DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC29DL

Manual Integrations
APPROVED

Sohil
10/8/2018 5:53:32 PM

Quant Time: Oct 06 01:10:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 06 01:07:30 2018
Response via : Initial Calibration

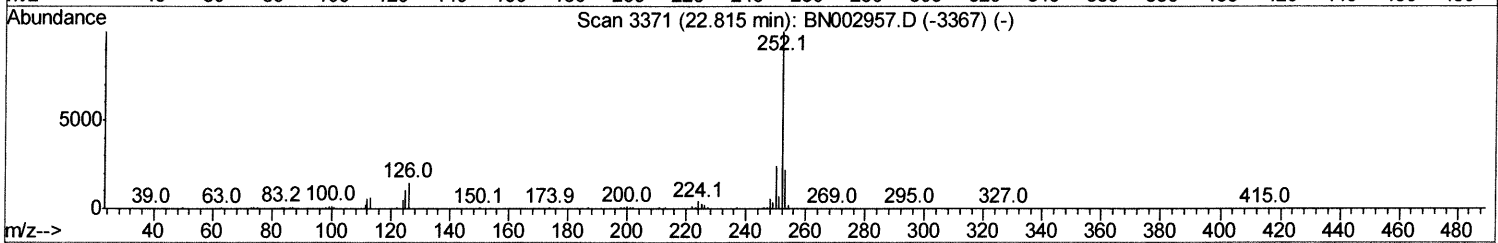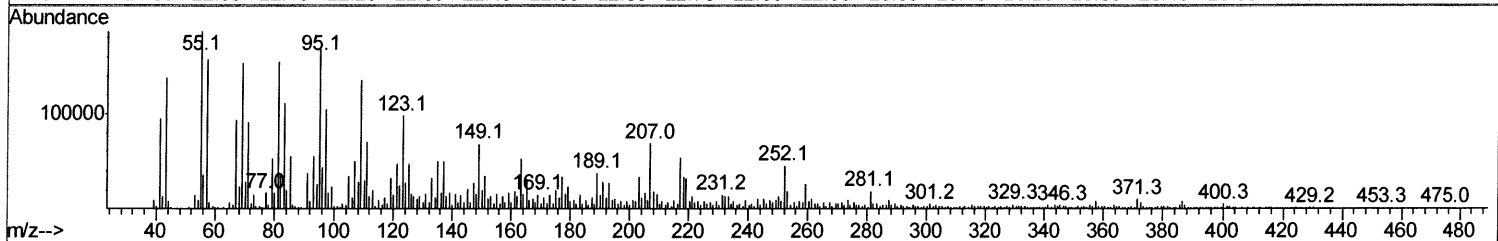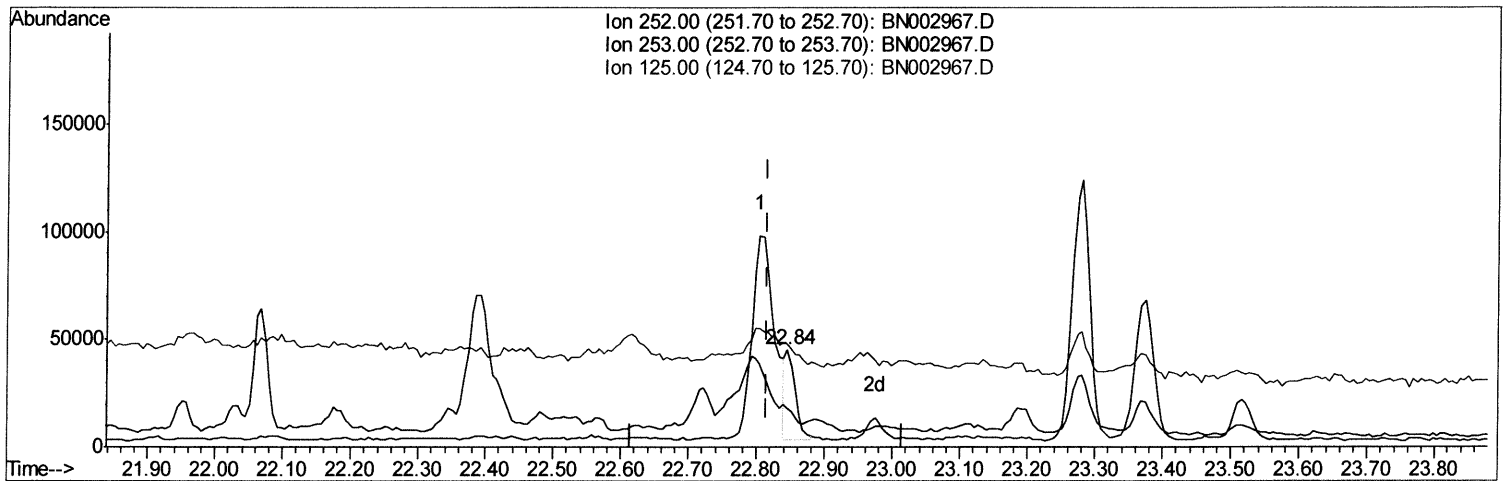

TIC: BN002967.D

(88) Benzo(k)fluoranthene

22.845min (+0.029) 1.36ng/ul m

response 42049

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	40.03#
125.00	10.40	106.56#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100618\
 Data File : BN002967.D
 Acq On : 05 Oct 2018 15:27
 Operator : MJ/SJ
 Sample : J5183-14DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC29DL

Manual Integrations
 APPROVED

Sohil
 10/8/2018 5:53:32 PM

Quant Time: Oct 06 02:37:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 06 01:07:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	138039	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	612156	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	357143	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	717428	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	534446	20.00	ng/ul	0.02
85) Perylene-d12	23.47	264	540676	20.00	ng/ul	0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	4033	1.35	ng/uL	0.00
5) Phenol-d5	6.83	99	111562	9.52	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.97	67	75958	10.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	92958	9.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	91400	10.07	ng/ul	0.01
19) Nitrobenzene-d5	8.78	128	62269	13.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	52843	9.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	97260	10.04	ng/ul	0.02
29) 4-Chloroaniline-d4	10.51	131	453256m	40.44	ng/ul	-0.03
43) Dimethylphthalate-d6	13.68	166	298551	10.68	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	391721	10.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	31102m	6.73	ng/ul	0.03
57) Fluorene-d10	15.27	176	268817	10.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	2979	0.66	ng/ul	-0.04
70) Anthracene-d10	17.02	188	717428	20.95	ng/ul	-0.09
78) Pyrene-d10	19.43	212	334356	11.86	ng/ul	0.02
89) Benzo(a)pyrene-d12	23.33	264	306802	10.78	ng/ul	0.04

SJ 10/10/18
 SJ 10/10/18

Target Compounds

					Ovalue	
28) Naphthalene	10.45	128	157059	4.978	ng/ul#	66
34) 2-Methylnaphthalene	12.07	142	225543	10.227	ng/ul	97
44) Dimethylphthalate	13.73	163	169126	6.199	ng/ul	98
69) Phenanthrene	17.07	178	120316	3.044	ng/ul#	85
75) Di-n-butylphthalate	18.00	149	815446	19.760	ng/ul	98
76) Fluoranthene	19.10	202	178554	4.234	ng/ul	97
79) Pyrene	19.46	202	273016	7.726	ng/ul	98
80) Butylbenzylphthalate	20.37	149	378467	25.739	ng/ul	97
82) Benzo(a)anthracene	21.22	228	78173	2.351	ng/ul#	71
83) Bis(2-ethylhexyl)phthalate	21.16	149	732202	34.300	ng/ul#	96
84) Chrysene	21.27	228	153526	4.927	ng/ul#	89
87) Benzo(b)fluoranthene	22.80	252	213780	6.474	ng/ul#	33
88) Benzo(k)fluoranthene	22.84	252	42049m	1.365	ng/ul	43
90) Benzo(a)pyrene	23.37	252	126833	4.063	ng/ul#	43
91) Indeno(1,2,3-cd)pyrene	25.69	276	123976	3.355	ng/ul#	90
93) Benzo(g,h,i)perylene	26.37	276	195332	6.323	ng/ul#	91

SJ 10/10/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed