

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100719\
 Data File : BN008052.D
 Acq On : 07 Oct 2019 16:27
 Operator : JU
 Sample : K5078-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PST-024-B282-092619

Manual Integrations
 APPROVED

mohammad
 10/8/2019 12:23:14 PM

Quant Time: Oct 08 00:01:26 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Oct 03 18:39:49 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	2840	0.40	ng	-0.03
7) Naphthalene-d8	10.43	136	11840	0.40	ng	-0.04
13) Acenaphthene-d10	14.29	164	7420	0.40	ng	-0.03
19) Phenanthrene-d10	17.04	188	15859	0.40	ng	-0.03
27) Chrysene-d12	21.24	240	23860	0.40	ng	-0.03
34) Perylene-d12	23.45	264	23974	0.40	ng	-0.04

System Monitoring Compounds

4) 2-Fluorophenol	5.29	112	2334	0.24	ng	-0.02
5) Phenol-d6	6.86	99	3147	0.26	ng	0.00
8) Nitrobenzene-d5	8.81	82	2649	0.26	ng	-0.03
11) 2-Methylnaphthalene-d10	12.03	152	5387	0.27	ng	-0.03
14) 2,4,6-Tribromophenol	15.80	330	1040	0.26	ng	-0.02
15) 2-Fluorobiphenyl	12.91	172	7341	0.24	ng	-0.03
25) Fluoranthene-d10	19.08	212	15195	0.28	ng	-0.02
29) Terphenyl-d14	19.68	244	14676	0.25	ng	-0.03

Target Compounds

						Qvalue
9) Naphthalene	10.48	128	4257	0.128	ng	# 89
12) 2-Methylnaphthalene	12.10	142	4131	0.184	ng	95
16) Acenaphthylene	14.01	152	50226	1.276	ng	99
17) Acenaphthene	14.36	154	2316	0.091	ng	99
18) Fluorene	15.35	166	6807	0.209	ng	# 12
22) Pentachlorophenol	16.71	266	147	0.038	ng	# 81
23) Phenanthrene	17.08	178	103941	2.104	ng	100
24) Anthracene	17.18	178	36294	0.813	ng	99
26) Fluoranthene	19.11	202	211764	3.447	ng	99
28) Pylene	19.48	202	246616	3.031	ng	97
30) Benzo(a)anthracene	21.23	228	128869	1.467	ng	91
31) Chrysene	21.28	228	156790	1.831	ng	96
32) Bis(2-ethylhexyl)phthalate	21.16	149	35245	0.780	ng	99
33) Indeno(1,2,3-cd)pyrene	25.66	276	101986	0.951	ng	96
35) Benzo(b)fluoranthene	22.80	252	199430	2.396	ng	# 94
36) Benzo(k)fluoranthene	22.83	252	65253m	0.793	ng	
37) Benzo(a)pyrene	23.36	252	130776	1.672	ng	# 95
38) Dibenzo(a,h)anthracene	25.67	278	29925	0.374	ng	# 75
39) Benzo(g,h,i)perylene	26.33	276	111827	1.412	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100719\
Data File : BN008052.D
Acq On : 07 Oct 2019 16:27
Operator : JU
Sample : K5078-12
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Quant Time: Oct 08 00:01:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 03 18:39:49 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



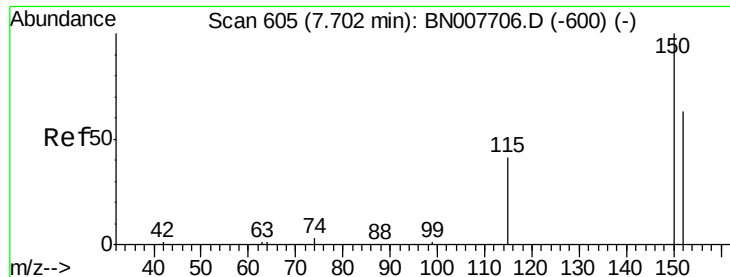

#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.67 min Scan# 601
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.0	125.6	188.4
115	68.8	53.3	79.9

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E



#4

2-Fluorophenol
Concen: 0.239 ng
RT: 5.29 min Scan# 306
Delta R.T. -0.02 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.5	46.6	70.0
63	31.0	23.1	34.7






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC





#5

Phenol-d6

Concen: 0.256 ng

RT: 6.86 min Scan# 501

Delta R.T. -0.01 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion:	99	Resp:	3147
Ion	Ratio	Lower	Upper
99	100		
42	27.9	12.8	19.2#
71	45.2	27.6	41.4#

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.43 min Scan# 848


Delta R.T. -0.04 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion:	136	Resp:	11840
Ion	Ratio	Lower	Upper
136	100		
137	12.4	9.2	13.8
54	10.8	5.8	8.8#
68	13.0	6.5	9.7#





#8

Nitrobenzene-d5

Concen: 0.256 ng

RT: 8.81 min Scan# 720

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion:	82	Resp:	2649
Ion	Ratio	Lower	Upper
82	100		
128	40.4	24.5	36.7#
54	42.6	35.2	52.8

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#9

Naphthalene

Concen: 0.128 ng




RT: 10.48 min Scan# 852


Delta R.T. -0.04 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion:	128	Resp:	4257
Ion	Ratio	Lower	Upper
128	100		
129	16.4	9.1	13.7#
127	16.8	10.6	15.8#









#11
2-Methylnaphthalene-d10
Concen: 0.270 ng
RT: 12.03 min Scan# 1051
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.6	15.4	23.2




Manual Integrations
APPROVED


mohammad
10/8/2019 12:23:14 PM



#12
2-Methylnaphthalene
Concen: 0.184 ng
RT: 12.10 min Scan# 1067
Delta R.T. -0.04 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.4	70.6	106.0
115	41.6	28.3	42.5





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.29 min Scan# 1318

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion:	164	Resp:	7420
Ion	Ratio	Lower	Upper
164	100		
162	103.2	81.7	122.5
160	47.6	37.0	55.4

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#14

2,4,6-Tribromophenol

Concen: 0.257 ng




RT: 15.80 min Scan# 1453


Delta R.T. -0.02 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion:	330	Resp:	1040
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	70.1	28.7	43.1#






#15
2-Fluorobiphenyl
Concen: 0.240 ng
RT: 12.91 min Scan# 1194
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
172	100		
171	37.2	28.8	43.2
170	25.2	19.5	29.3

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM






Abundance

Ion 172.00 (171.70 to 172.70): E


Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



#16
Acenaphthylene
Concen: 1.276 ng
RT: 14.01 min Scan# 1293
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.1	15.5	23.3
153	13.3	10.4	15.6






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E









#17
Acenaphthene
Concen: 0.091 ng
RT: 14.36 min Scan# 1324
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
154	100		
153	110.1	87.0	130.4
152	54.1	42.7	64.1




Manual Integrations
APPROVED


mohammad
10/8/2019 12:23:14 PM



#18
Fluorene
Concen: 0.209 ng
RT: 15.35 min Scan# 1413
Delta R.T. -0.02 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
166	100		
165	0.0	78.0	117.0#
167	19.2	10.9	16.3#





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.04 min Scan# 1569

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion:	188	Resp:	15859
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	14.3	7.4	11.2#

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#22

Pentachlorophenol

Concen: 0.038 ng




RT: 16.71 min Scan# 1538


Delta R.T. -0.02 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion:	266	Resp:	147
Ion Ratio	Lower	Upper	
266	100		
264	69.9	50.0	75.0
268	89.7	54.2	81.4#









#23
Phenanthrene
Concen: 2.104 ng
RT: 17.08 min Scan# 1573
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.9	22.3
179	15.9	12.5	18.7




Manual Integrations
APPROVED


mohammad
10/8/2019 12:23:14 PM



#24
Anthracene
Concen: 0.813 ng
RT: 17.18 min Scan# 1582
Delta R.T. -0.02 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
178	100		
176	17.9	14.6	21.8
179	16.0	12.2	18.4





#25

Fluoranthene-d10

Concen: 0.284 ng

RT: 19.08 min Scan# 1877

Delta R.T. -0.02 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N


ClientSampleId :

PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
212	100		
106	11.5	9.4	14.0
104	7.3	5.3	7.9

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM






Abundance

Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



#26

Fluoranthene

Concen: 3.447 ng

RT: 19.11 min Scan# 1882

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27




Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.4	8.4	12.6
203	17.8	13.8	20.8


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E






#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.24 min Scan# 2179
Delta R.T. -0.03 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
240	100		
120	21.2	5.4	8.2#
236	30.5	21.0	31.4

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM






Abundance

Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#28
Pyrene
Concen: 3.031 ng
RT: 19.48 min Scan# 1956
Delta R.T. -0.02 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.3	16.4	24.6
203	20.5	14.1	21.1






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E





#29

Terphenyl-d14

Concen: 0.250 ng

RT: 19.68 min Scan# 1998

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
244	100		
212	9.5	5.9	8.9#
122	13.1	7.4	11.2#

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#30

Benzo(a)anthracene

Concen: 1.467 ng




RT: 21.23 min Scan# 2178


Delta R.T. -0.02 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
228	100		
226	32.8	22.1	33.1
229	23.0	15.8	23.6









#31
Chrysene
Concen: 1.831 ng
RT: 21.28 min Scan# 2183
Delta R.T. -0.02 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Instrument :
BNA_N
ClientSampleId :
PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.3	23.9	35.9
229	23.4	15.8	23.6




Manual Integrations
APPROVED


mohammad
10/8/2019 12:23:14 PM



#32
Bis(2-ethylhexyl)phthalate
Concen: 0.780 ng
RT: 21.16 min Scan# 2172
Delta R.T. -0.04 min
Lab File: BN008052.D
Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
149	100		
167	29.3	23.7	35.5
279	5.7	4.2	6.2









#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.951 ng
 RT: 25.66 min Scan# 3239
 Delta R.T. -0.05 min
 Lab File: BN008052.D
 Acq: 07 Oct 2019 16:27

Instrument :
 BNA_N
 ClientSampleId :
 PST-024-B282-092619

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.7	17.1	25.7
277	25.0	20.0	30.0




Manual Integrations
 APPROVED


mohammad
 10/8/2019 12:23:14 PM



#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.45 min Scan# 2595
 Delta R.T. -0.04 min
 Lab File: BN008052.D
 Acq: 07 Oct 2019 16:27

Tgt Ion	Ratio	Lower	Upper
264	100		
260	28.4	19.3	28.9
265	65.4	26.9	40.3#





#35

Benzo(b)fluoranthene

Concen: 2.396 ng

RT: 22.80 min Scan# 2403

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N


ClientSampleId :

PST-024-B282-092619

Tot Ion:	252	Resp:	199430
Ion Ratio	Lower	Upper	
252	100		
253	24.7	18.3	27.5
125	14.0	8.2	12.4#

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#36

Benzo(k)fluoranthene

Concen: 0.793 ng m

RT: 22.83 min Scan# 2414

Delta R.T. -0.04 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27




Tgt Ion:	252	Resp:	65253
Ion Ratio	Lower	Upper	
252	100		
253	26.4	18.5	27.7
125	34.9	8.4	12.6#


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E





#37

Benzo(a)pyrene

Concen: 1.672 ng

RT: 23.36 min Scan# 2567

Delta R.T. -0.03 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Instrument :

BNA_N





ClientSampleId :

PST-024-B282-092619

Tot Ion:	252	Resp:	130776
Ion Ratio	Lower	Upper	
252	100		
253	25.0	18.6	27.8
125	15.0	9.4	14.0#

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM



#38

Dibenzo(a,h)anthracene

Concen: 0.374 ng




RT: 25.67 min Scan# 3241


Delta R.T. -0.05 min

Lab File: BN008052.D

Acq: 07 Oct 2019 16:27

Tgt Ion:	278	Resp:	29925
Ion Ratio	Lower	Upper	
278	100		
139	26.4	11.8	17.6#
279	35.3	19.4	29.2#





#39

Benzo(a,h,i)perylene

Concen: 1.412 ng

RT: 26.33 min Scan# 3436

Delta R.T. -0.05 min

Lab File: BN008052.D


Acq: 07 Oct 2019 16:27

Instrument :

BNA_N

ClientSampleId :

PST-024-B282-092619



Tot Ion:	276	Resp:	111827
Ion Ratio	Lower	Upper	
276	100		
277	25.9	19.8	29.8
138	19.6	15.1	22.7

Manual Integrations
APPROVED

mohammad
10/8/2019 12:23:14 PM

