


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100719\
 Data File : BN008049.D
 Acq On : 07 Oct 2019 14:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 03 18:39:49 2019

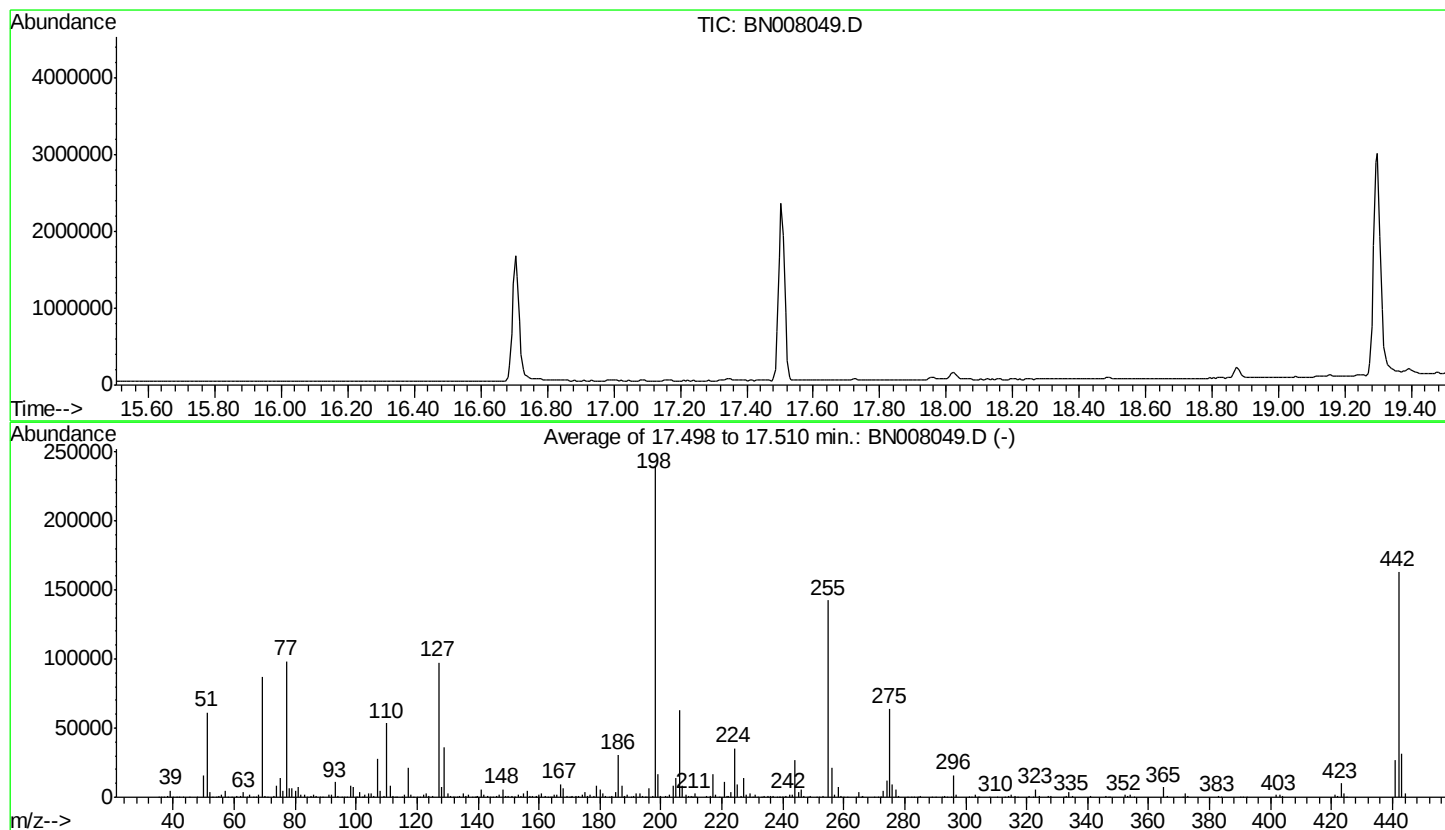

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	61354	PASS
68	69	0.00	2	1.8	1552	PASS
69	198	0.00	100	36.3	87114	PASS
70	69	0.00	2	0.6	536	PASS
127	198	10	80	40.6	97298	PASS
197	198	0.00	2	0.3	630	PASS
198	198	100	100	100.0	239808	PASS
199	198	5	9	6.8	16289	PASS
275	198	10	60	26.8	64322	PASS
365	198	1	100	3.1	7405	PASS
441	198	0.01	100	11.2	26845	PASS
442	198	50	100	67.9	162930	PASS
443	442	15	24	19.6	31917	PASS