

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016814.D
 Acq On : 07 Oct 2021 18:14
 Operator : CG/JU
 Sample : SSTDIC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.8

Quant Time: Oct 08 01:19:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 18:25:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.615	152	20505	0.400	ng	0.00
7) Naphthalene-d8	10.381	136	89278	0.400	ng	# 0.00
13) Acenaphthene-d10	14.243	164	47187	0.400	ng	0.00
19) Phenanthrene-d10	17.006	188	88673	0.400	ng	0.00
29) Chrysene-d12	21.206	240	93863	0.400	ng	#-0.01
35) Perylene-d12	23.454	264	99130	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.227	112	41902	0.801	ng	0.00
5) Phenol-d6	6.803	99	47910	0.825	ng	0.00
8) Nitrobenzene-d5	8.759	82	49517	0.791	ng	0.00
11) 2-Methylnaphthalene-d10	11.981	152	109245	0.821	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	19706	0.944	ng	0.00
15) 2-Fluorobiphenyl	12.873	172	151875	0.805	ng	0.00
27) Fluoranthene-d10	19.043	212	203386	0.838	ng	0.00
31) Terphenyl-d14	19.659	244	174506	0.831	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.217	88	7557	0.790	ng	# 81
3) n-Nitrosodimethylamine	3.549	42	13349	0.864	ng	# 99
6) bis(2-Chloroethyl)ether	7.052	93	47217	0.847	ng	100
9) Naphthalene	10.432	128	197275	0.808	ng	100
10) Hexachlorobutadiene	10.724	225	38006	0.832	ng	# 100
12) 2-Methylnaphthalene	12.052	142	128696	0.829	ng	100
16) Acenaphthylene	13.964	152	172684	0.829	ng	100
17) Acenaphthene	14.307	154	112259	0.816	ng	100
18) Fluorene	15.309	166	137279	0.827	ng	100
20) 4,6-Dinitro-2-methylph...	15.385	198	11338	1.849	ng	# 63
21) 4-Bromophenyl-phenylether	16.202	248	45326	0.839	ng	97
22) Hexachlorobenzene	16.312	284	51179	0.836	ng	99
23) Atrazine	16.482	200	35547	0.831	ng	100
24) Pentachlorophenol	16.653	266	18868	1.118	ng	98
25) Phenanthrene	17.042	178	214288	0.822	ng	100
26) Anthracene	17.139	178	194477	0.835	ng	100
28) Fluoranthene	19.073	202	248453	0.859	ng	100
30) Pyrene	19.440	202	250005	0.810	ng	100
32) Benzo(a)anthracene	21.196	228	251646	0.864	ng	98
33) Chrysene	21.249	228	261948	0.887	ng	98
34) Bis(2-ethylhexyl)phtha...	21.143	149	137450	0.779	ng	100
36) Indeno(1,2,3-cd)pyrene	25.716	276	335341	1.066	ng	99
37) Benzo(b)fluoranthene	22.779	252	272183	0.849	ng	99
38) Benzo(k)fluoranthene	22.824	252	274973	0.893	ng	99
39) Benzo(a)pyrene	23.355	252	253324	0.883	ng	99
40) Dibenzo(a,h)anthracene	25.737	278	274736	1.100	ng	99
41) Benzo(g,h,i)perylene	26.408	276	286953	1.027	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016814.D
Acq On : 07 Oct 2021 18:14
Operator : CG/JU
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Quant Time: Oct 08 01:19:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 18:25:32 2021
Response via : Initial Calibration




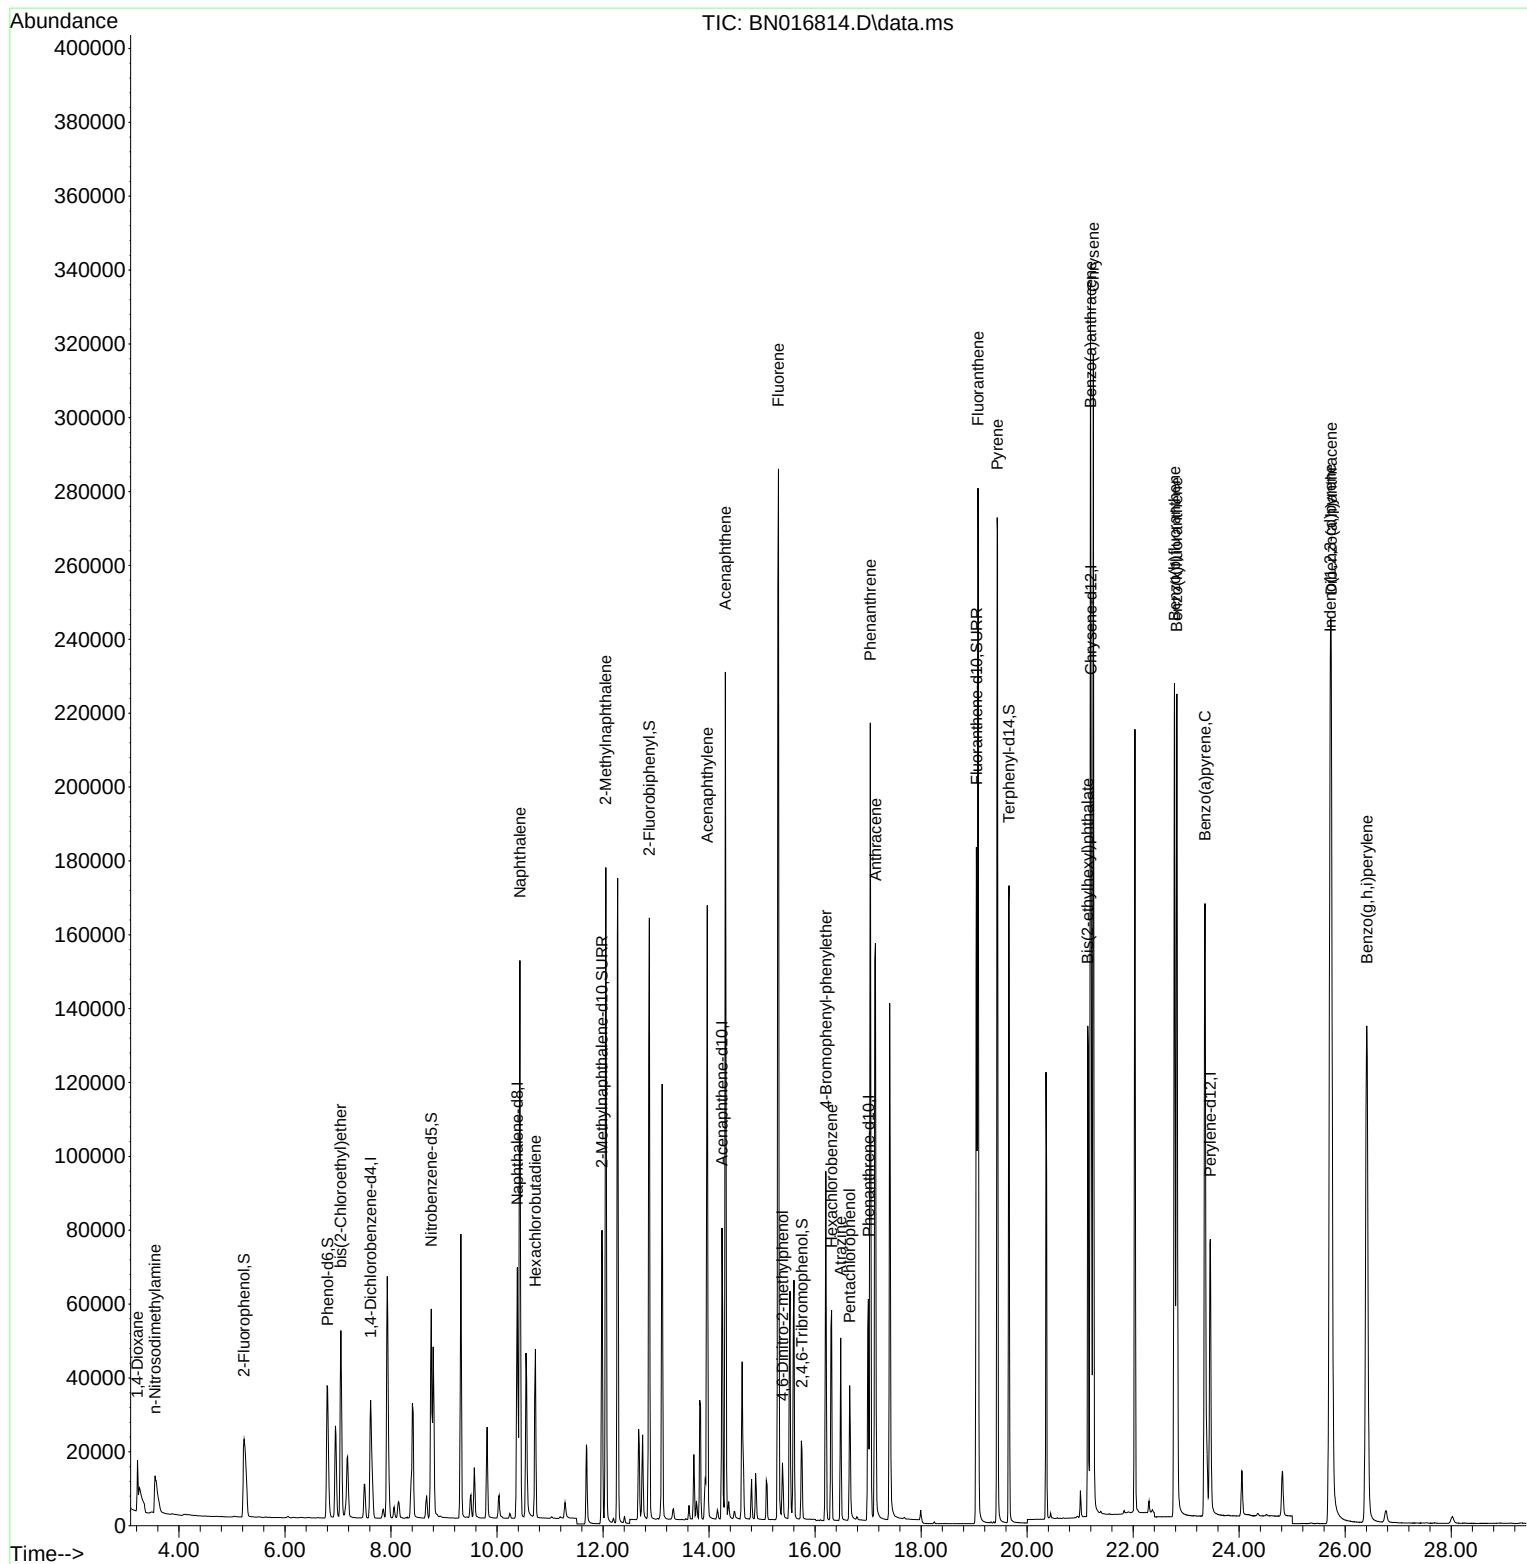




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.615 min Scan# 492
 Delta R.T. 0.001 min
 Lab File: BN016814.D
 Acq: 07 Oct 2021 18:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 20505
 Ion Ratio Lower Upper
 152 100
 150 156.6 123.3 184.9
 115 59.0 47.0 70.6

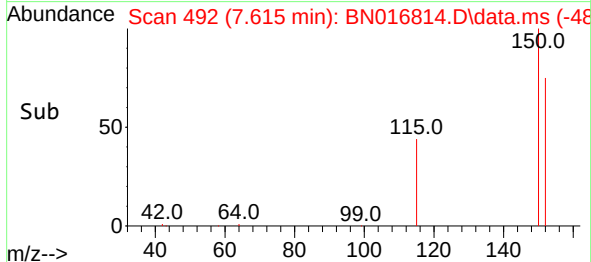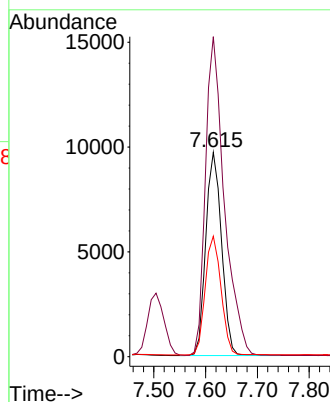

#2
 1,4-Dioxane
 Concen: 0.790 ng
 RT: 3.217 min Scan# 15
 Delta R.T. 0.000 min
 Lab File: BN016814.D
 Acq: 07 Oct 2021 18:14

Tgt Ion: 88 Resp: 7557
 Ion Ratio Lower Upper
 88 100
 43 47.2 61.7 92.5#
 58 75.1 62.2 93.2


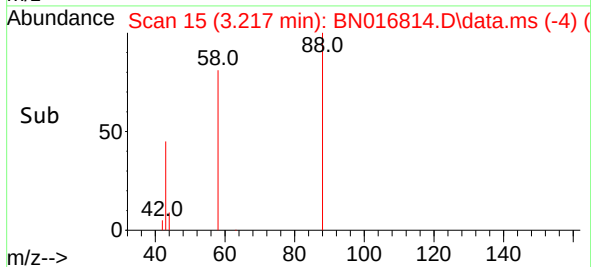
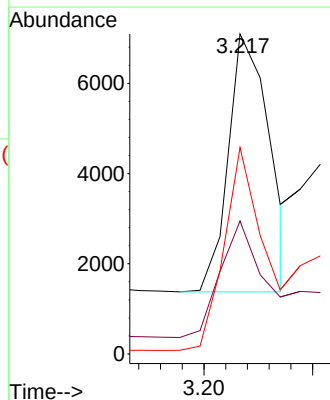
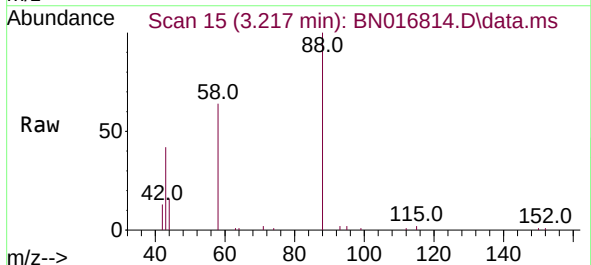


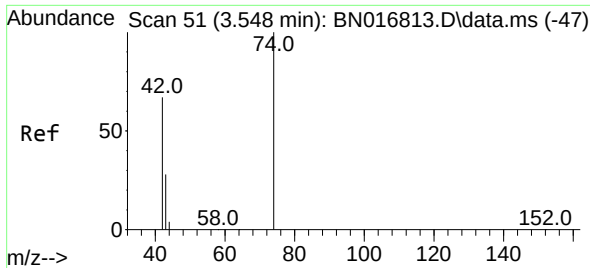

#3
n-Nitrosodimethylamine
Concen: 0.864 ng
RT: 3.549 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 13349
Ion Ratio Lower Upper
42 100
74 154.6 124.0 186.0
44 5.5 5.6 8.4#

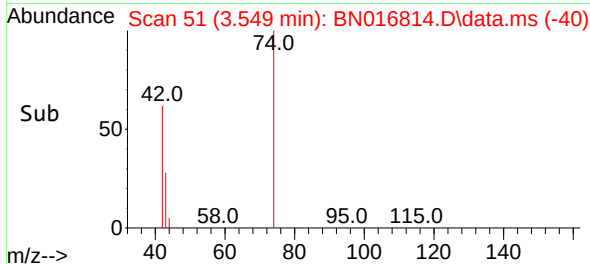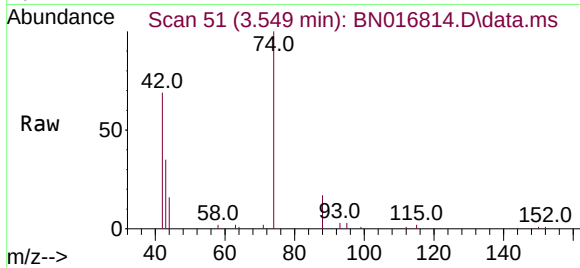

#4
2-Fluorophenol
Concen: 0.801 ng
RT: 5.227 min Scan# 233
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion: 112 Resp: 41902
Ion Ratio Lower Upper
112 100
64 54.3 42.9 64.3
63 27.5 21.5 32.3


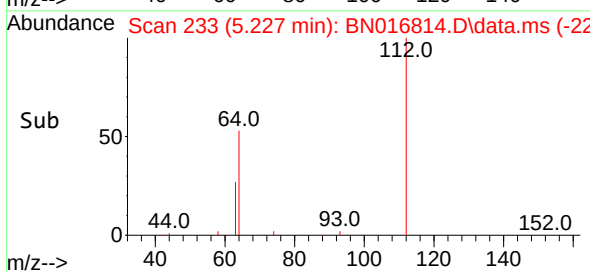

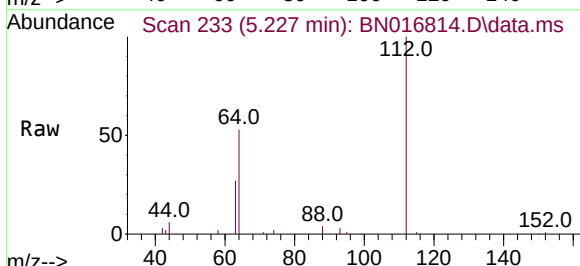




#5
Phenol-d6
Concen: 0.825 ng
RT: 6.803 min Scan# 404
Delta R.T. 0.010 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 99 Resp: 47910
Ion Ratio Lower Upper
99 100
42 16.8 13.4 20.2
71 30.2 24.0 36.0

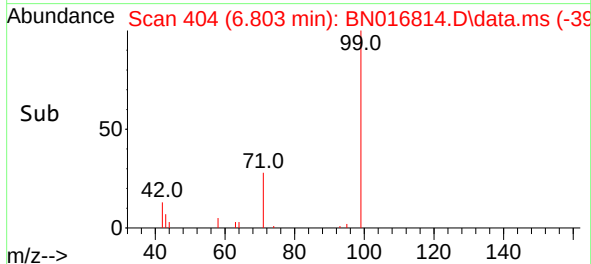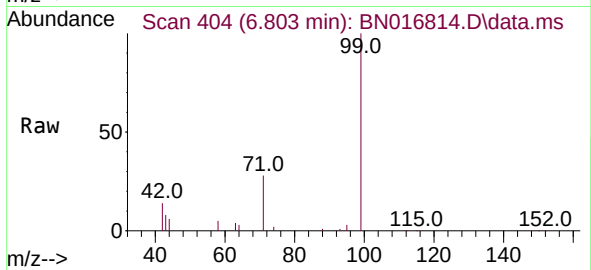

#6
bis(2-Chloroethyl)ether
Concen: 0.847 ng
RT: 7.052 min Scan# 431
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion: 93 Resp: 47217
Ion Ratio Lower Upper
93 100
63 73.7 59.0 88.6
95 32.8 26.4 39.6




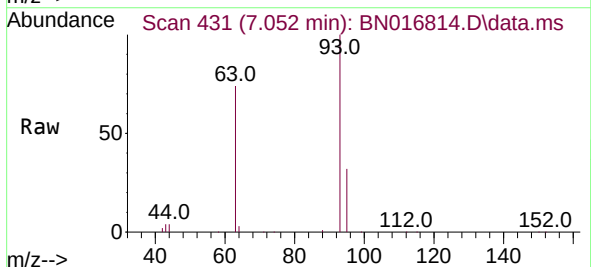




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.381 min Scan# 731
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	136	Resp:	89278
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.9	13.3
54	6.5	6.5	9.7#
68	5.6	5.3	7.9

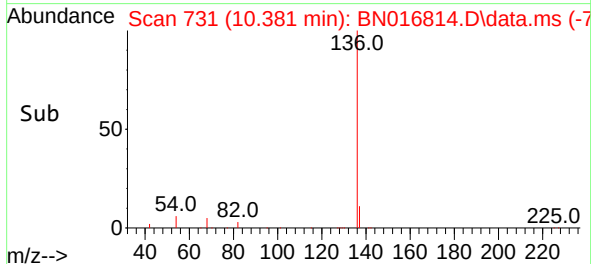

#8
Nitrobenzene-d5
Concen: 0.791 ng
RT: 8.759 min Scan# 603
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:	82	Resp:	49517
Ion Ratio	Lower	Upper	
82	100		
128	45.7	33.8	50.6
54	44.9	38.5	57.7


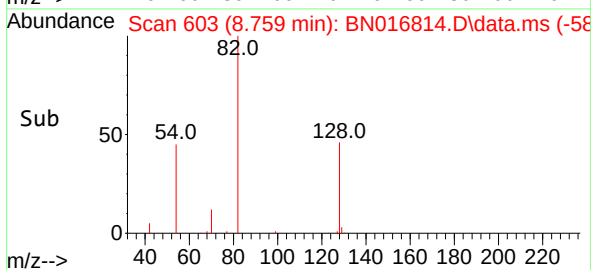

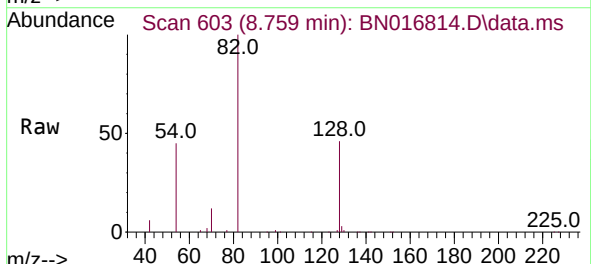




#9
Naphthalene
Concen: 0.808 ng
RT: 10.432 min Scan# 735
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	128	Resp:	197275
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.7	13.1
127	12.8	10.3	15.5

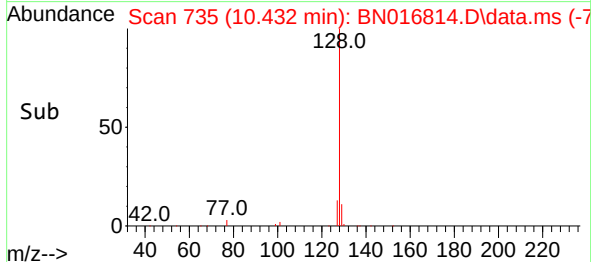

#10
Hexachlorobutadiene
Concen: 0.832 ng
RT: 10.724 min Scan# 758
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:	225	Resp:	38006
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	51.1	76.7


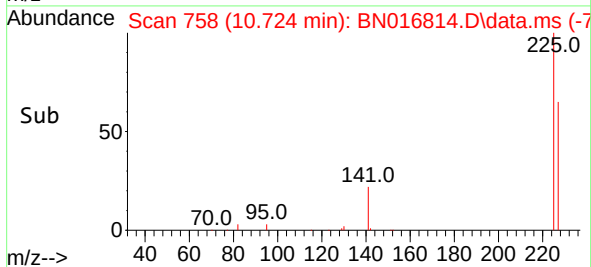

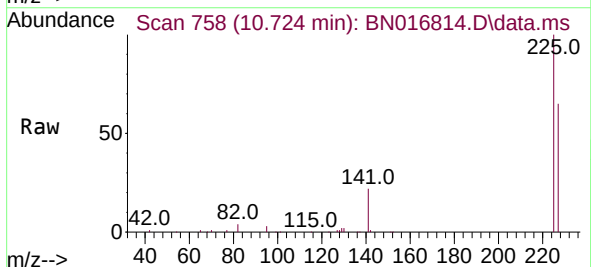


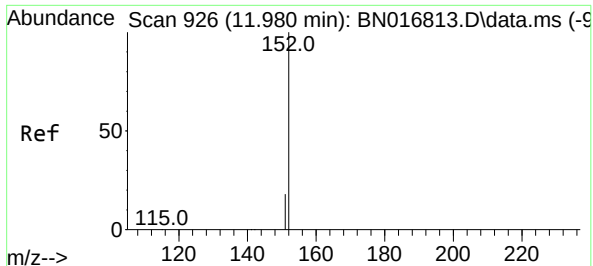

#11
2-Methylnaphthalene-d10
Concen: 0.821 ng
RT: 11.981 min Scan# 926
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:152 Resp: 109245
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

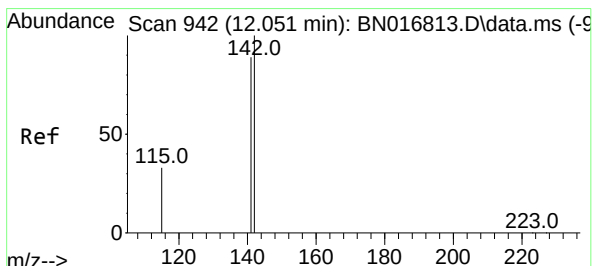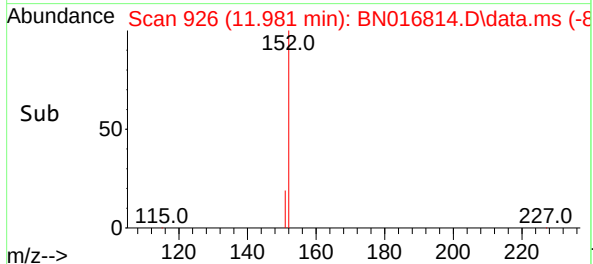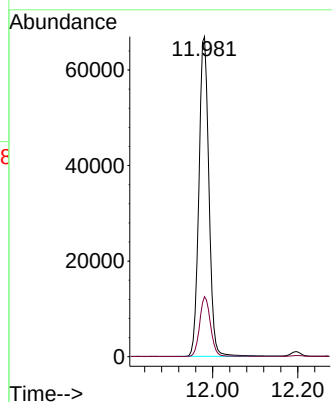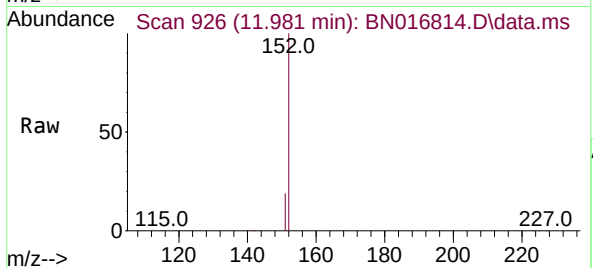

#12
2-Methylnaphthalene
Concen: 0.829 ng
RT: 12.052 min Scan# 942
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:142 Resp: 128696
Ion Ratio Lower Upper
142 100
141 88.8 70.6 106.0
115 32.8 26.1 39.1


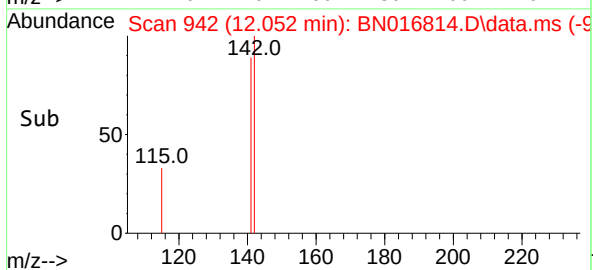
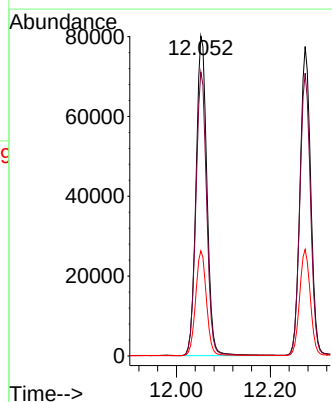
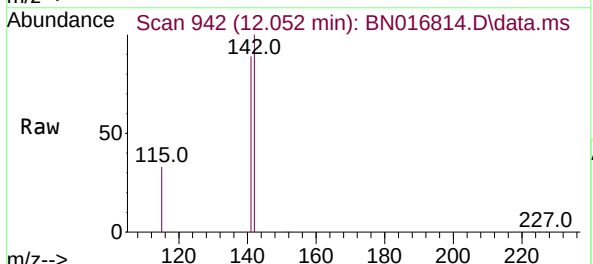


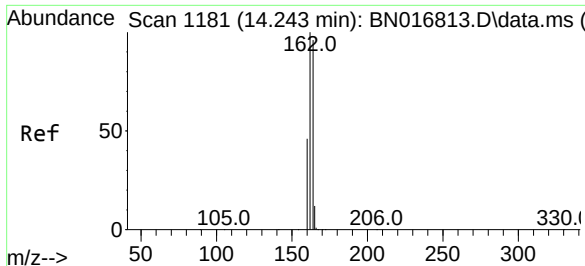

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.243 min Scan# 1181
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 47187
Ion Ratio Lower Upper
164 100
162 104.5 82.6 124.0
160 47.8 38.2 57.2

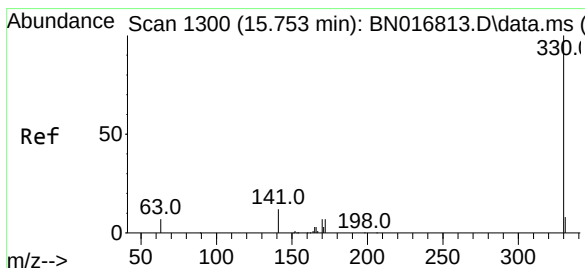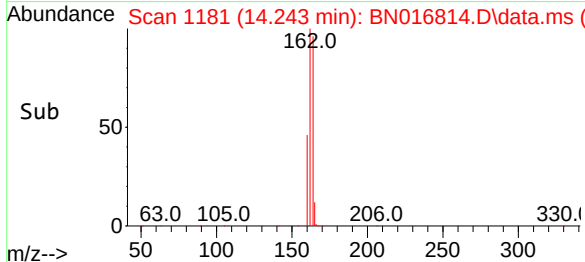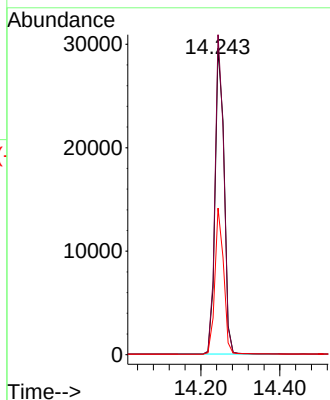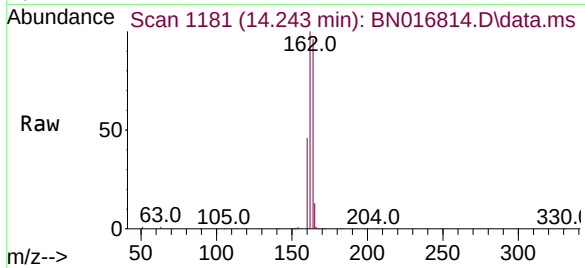

#14
2,4,6-Tribromophenol
Concen: 0.944 ng
RT: 15.753 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:330 Resp: 19706
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.4 24.2 36.2


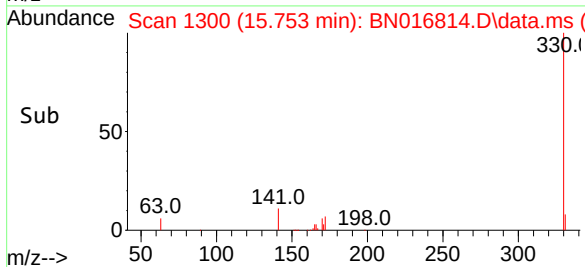
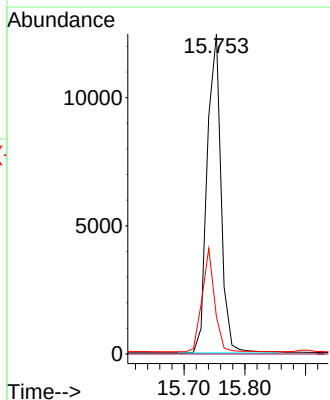
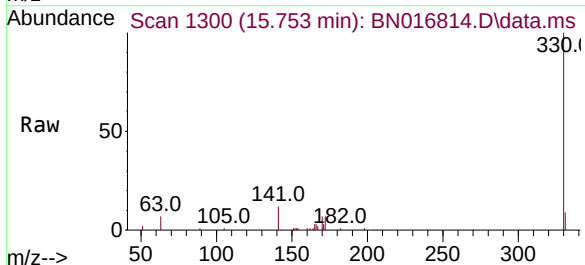




#15
2-Fluorobiphenyl
Concen: 0.805 ng
RT: 12.873 min Scan# 1073
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	172	Resp:	151875
Ion Ratio	Lower	Upper	
172	100		
171	33.6	26.9	40.3
170	21.6	17.4	26.0

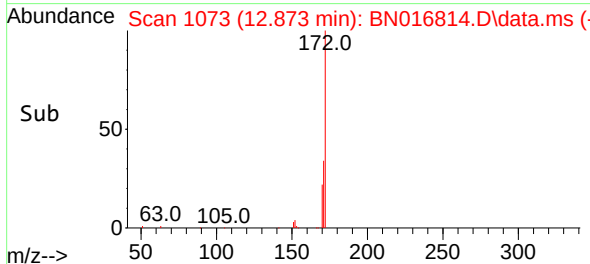

#16
Acenaphthylene
Concen: 0.829 ng
RT: 13.964 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:	152	Resp:	172684
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.5	23.3
153	13.0	10.4	15.6


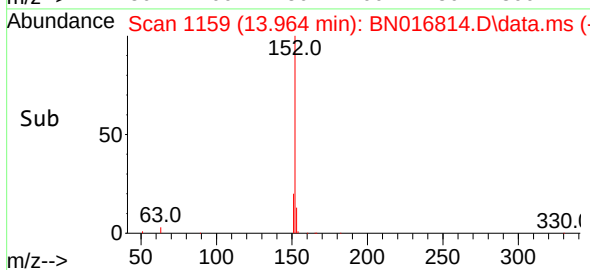

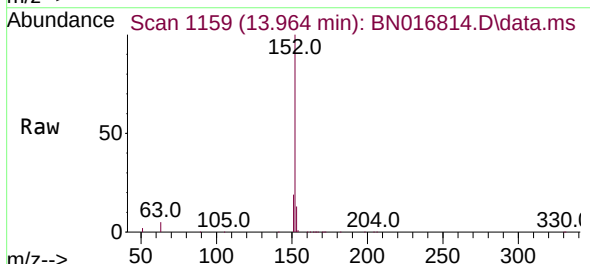


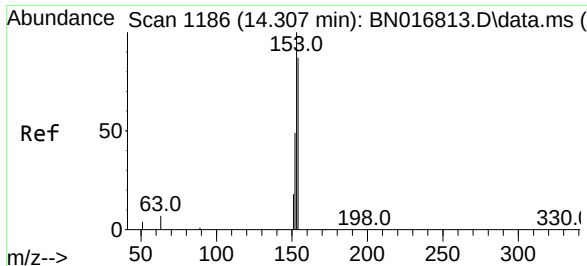

#17
Acenaphthene
Concen: 0.816 ng
RT: 14.307 min Scan# 1186
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 112259
Ion Ratio Lower Upper
154 100
153 112.6 90.1 135.1
152 54.3 43.6 65.4

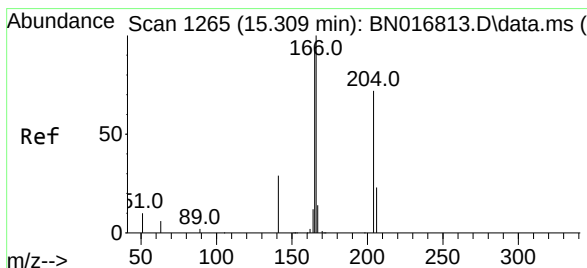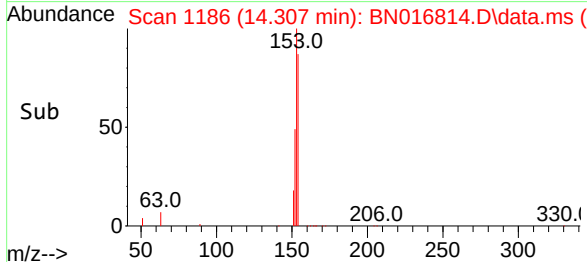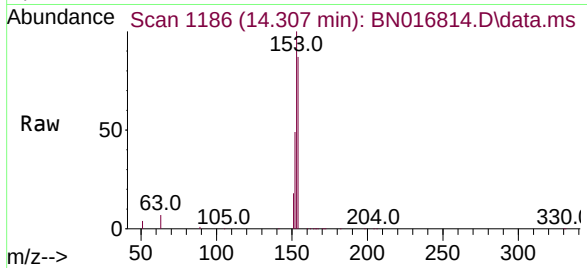

#18
Fluorene
Concen: 0.827 ng
RT: 15.309 min Scan# 1265
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:166 Resp: 137279
Ion Ratio Lower Upper
166 100
165 97.3 78.1 117.1
167 13.4 10.7 16.1


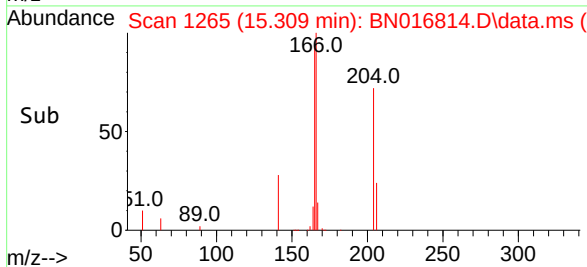

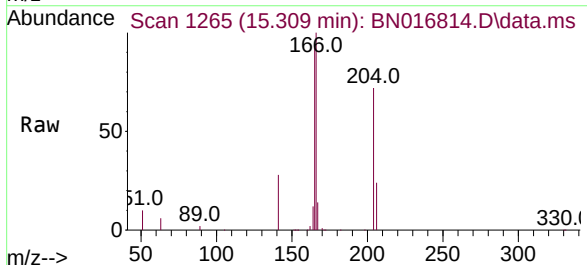




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.006 min Scan# 1402
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:188 Resp: 88673
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.7 5.8 8.8

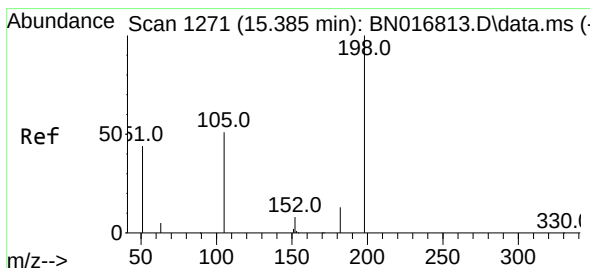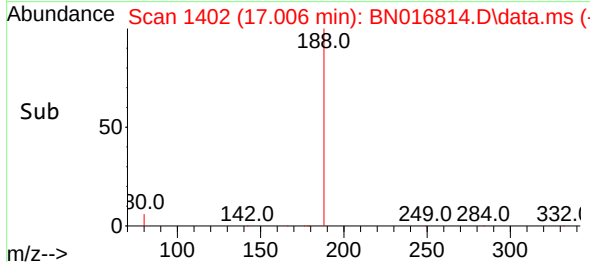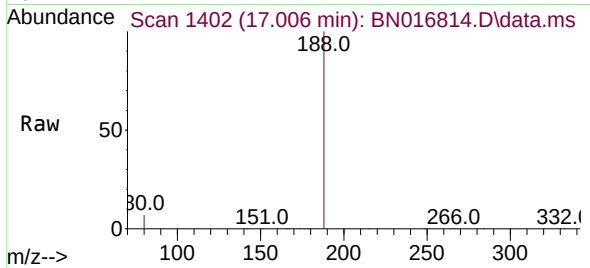

#20
4,6-Dinitro-2-methylphenol
Concen: 1.849 ng
RT: 15.385 min Scan# 1271
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:198 Resp: 11338
Ion Ratio Lower Upper
198 100
182 12.0 26.2 39.2#
77 0.0 0.0 0.0


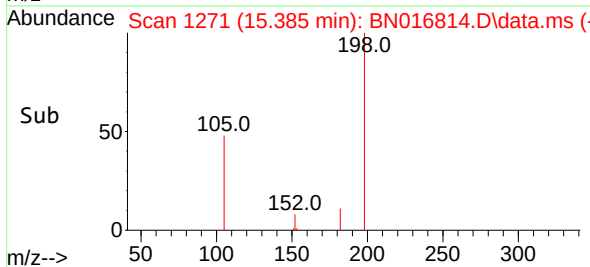

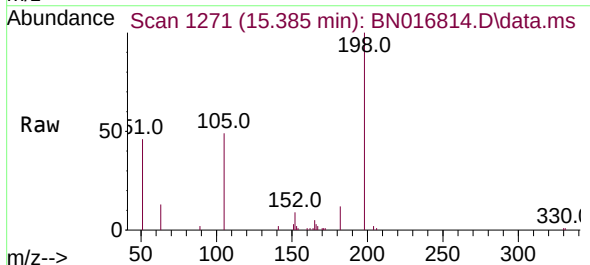




#21
4-Bromophenyl-phenylether
Concen: 0.839 ng
RT: 16.202 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:248 Resp: 45326
Ion Ratio Lower Upper
248 100
250 96.0 76.2 114.4
141 51.3 45.6 68.4

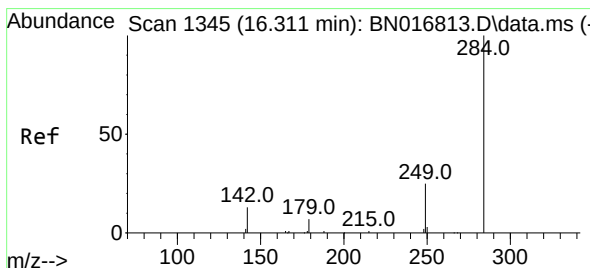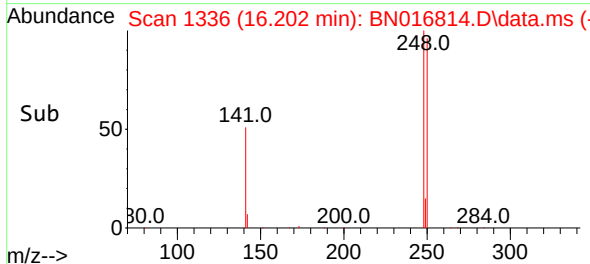

#22
Hexachlorobenzene
Concen: 0.836 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:284 Resp: 51179
Ion Ratio Lower Upper
284 100
142 31.5 25.8 38.6
249 29.2 23.3 34.9


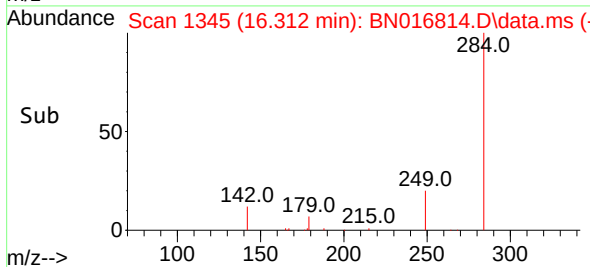

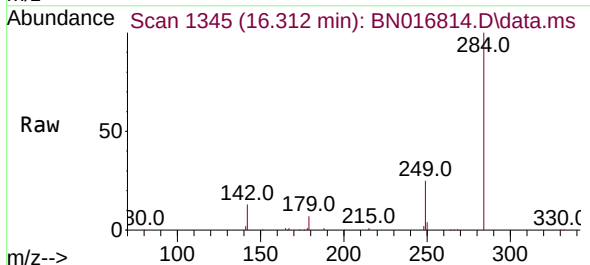


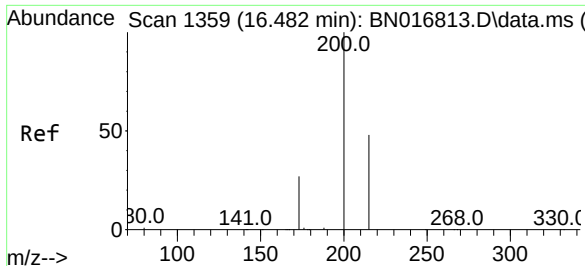

#23
Atrazine
Concen: 0.831 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:200 Resp: 35547
Ion Ratio Lower Upper
200 100
173 25.6 20.1 30.1
215 48.5 38.8 58.2

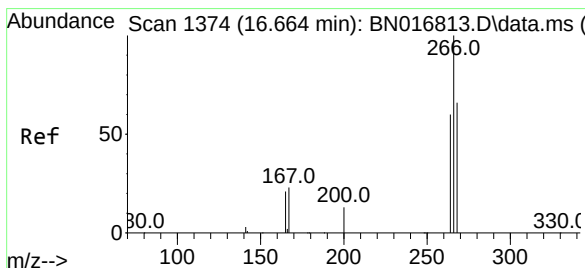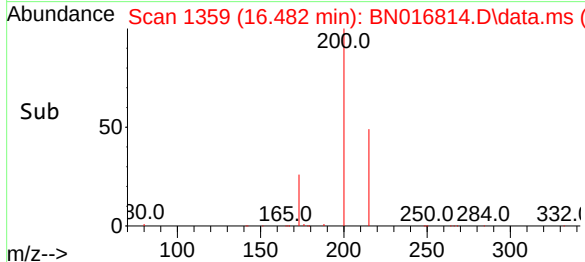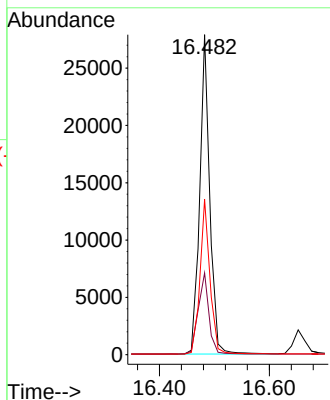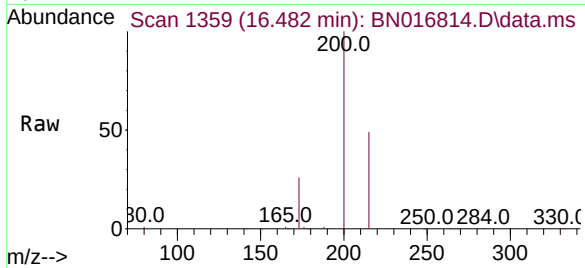

#24
Pentachlorophenol
Concen: 1.118 ng
RT: 16.653 min Scan# 1373
Delta R.T. -0.012 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:266 Resp: 18868
Ion Ratio Lower Upper
266 100
264 62.8 49.3 73.9
268 63.5 51.8 77.8


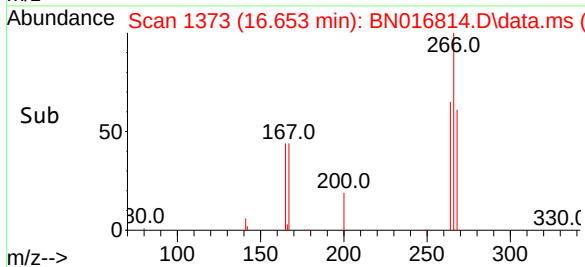
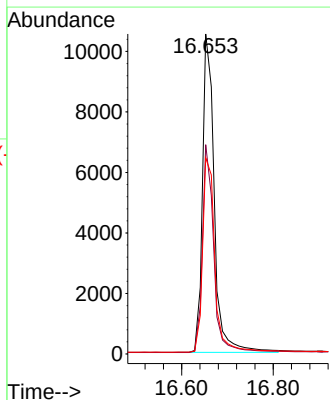
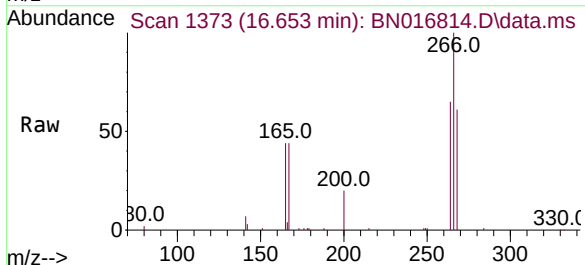




#25
Phenanthrene
Concen: 0.822 ng
RT: 17.042 min Scan# 1405
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 214288
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.3 12.4 18.6

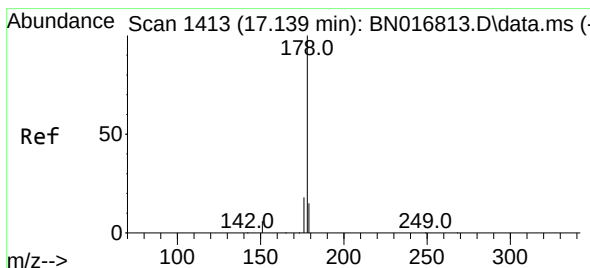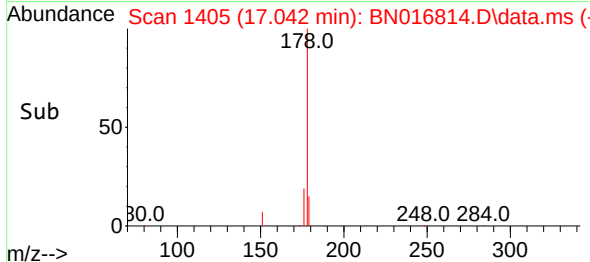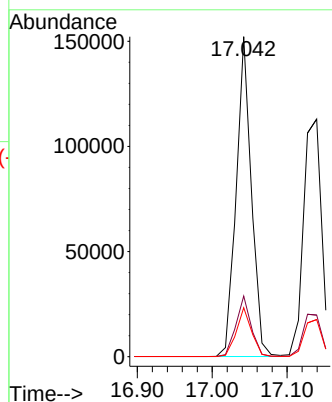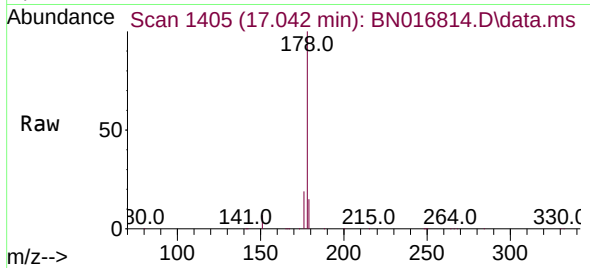

#26
Anthracene
Concen: 0.835 ng
RT: 17.139 min Scan# 1413
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:178 Resp: 194477
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 15.4 12.2 18.4


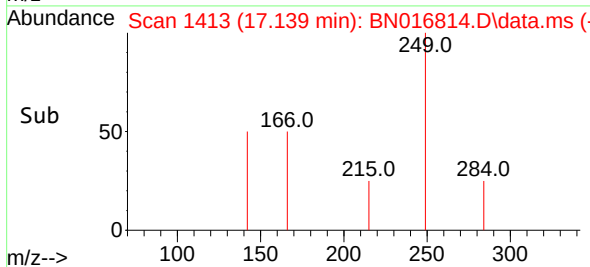

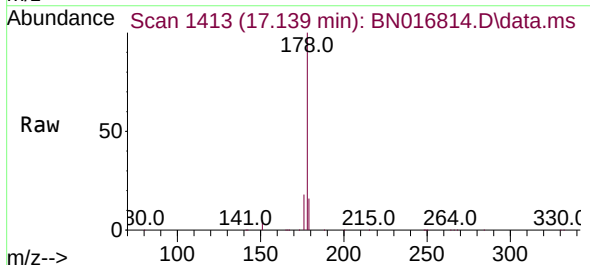




#27
Fluoranthene-d10
Concen: 0.838 ng
RT: 19.043 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 203386
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.8 8.8

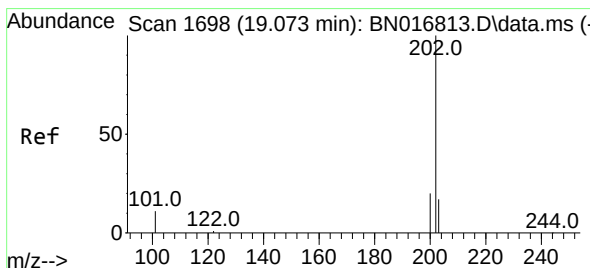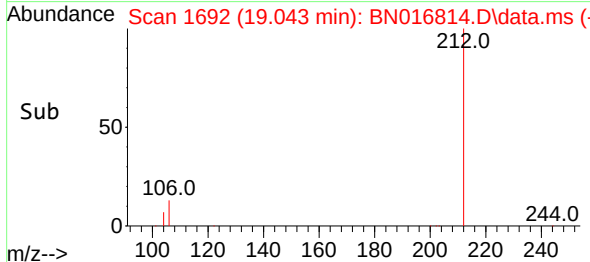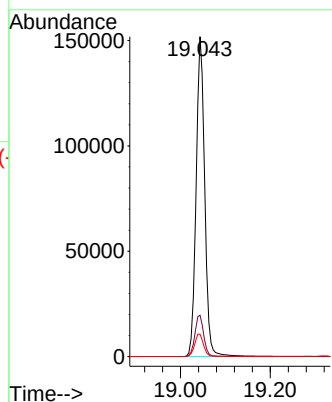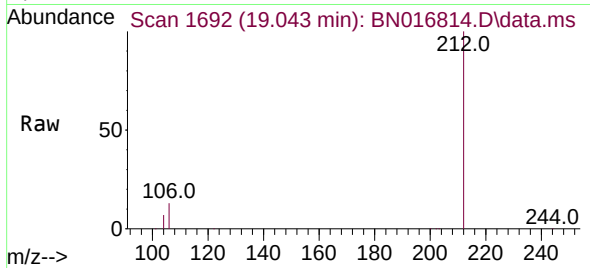

#28
Fluoranthene
Concen: 0.859 ng
RT: 19.073 min Scan# 1698
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:202 Resp: 248453
Ion Ratio Lower Upper
202 100
101 11.2 8.9 13.3
203 17.4 13.8 20.8


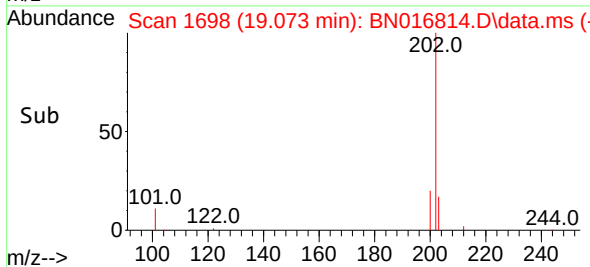

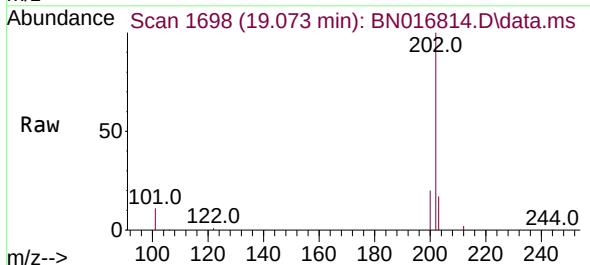




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.010 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:240 Resp: 93863
Ion Ratio Lower Upper
240 100
120 14.5 6.6 10.0#
236 27.0 20.7 31.1

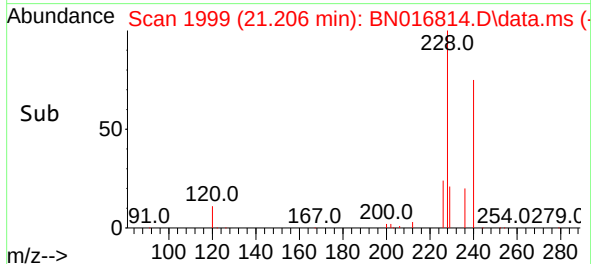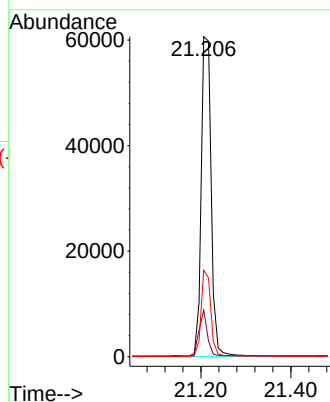

#30
Pyrene
Concen: 0.810 ng
RT: 19.440 min Scan# 1772
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:202 Resp: 250005
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 13.9 20.9



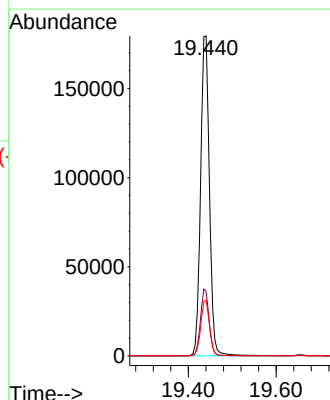
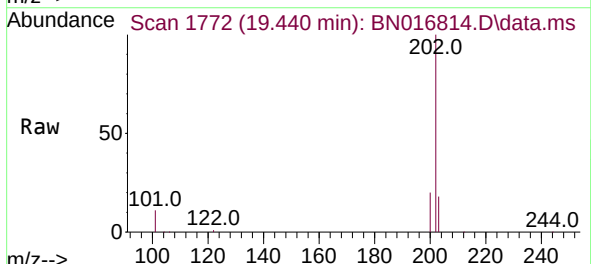




#31
Terphenyl-d14
Concen: 0.831 ng
RT: 19.659 min Scan# 1816
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:244 Resp: 174506
Ion Ratio Lower Upper
244 100
212 6.9 5.8 8.6
122 10.8 8.9 13.3

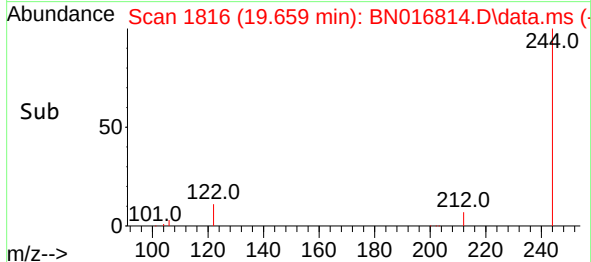

#32
Benzo(a)anthracene
Concen: 0.864 ng
RT: 21.196 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:228 Resp: 251646
Ion Ratio Lower Upper
228 100
226 26.6 22.3 33.5
229 19.7 15.4 23.0


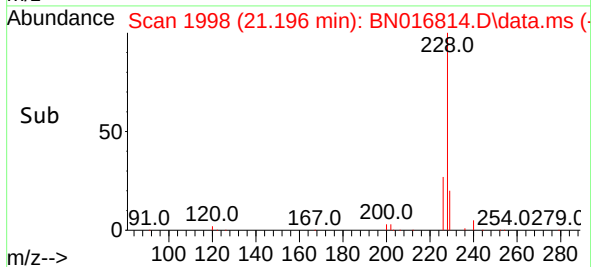

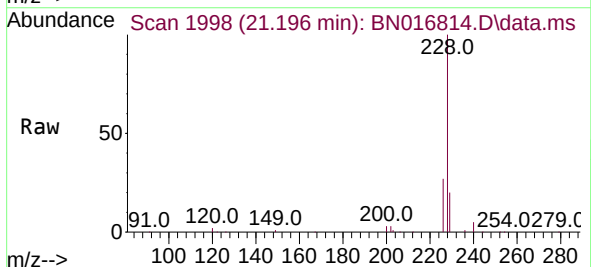




#33
Chrysene
Concen: 0.887 ng
RT: 21.249 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:228 Resp: 261948
Ion Ratio Lower Upper
228 100
226 28.7 24.2 36.4
229 19.7 15.4 23.0

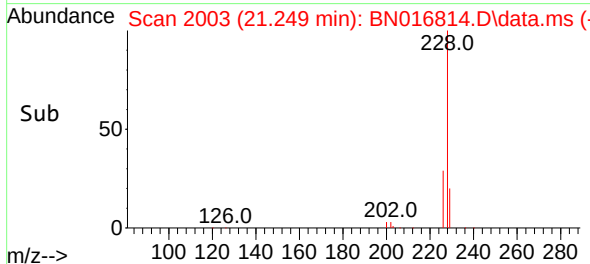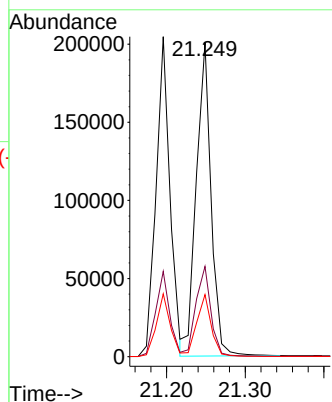

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.779 ng
RT: 21.143 min Scan# 1993
Delta R.T. -0.010 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:149 Resp: 137450
Ion Ratio Lower Upper
149 100
167 28.0 22.2 33.4
279 4.4 3.4 5.2


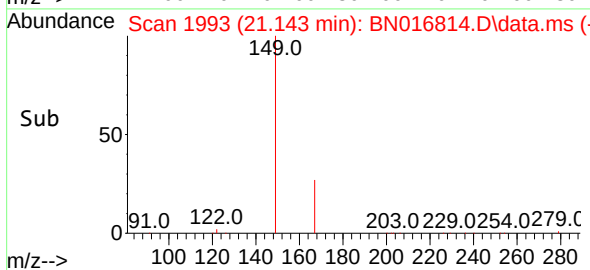

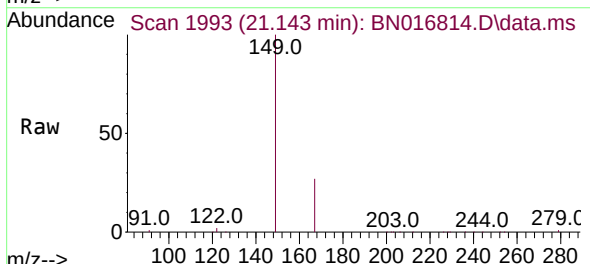


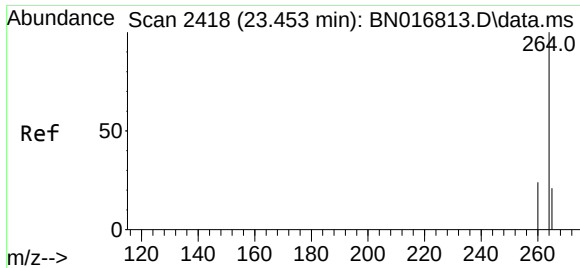

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.454 min Scan# 2418
 Delta R.T. 0.000 min
 Lab File: BN016814.D
 Acq: 07 Oct 2021 18:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:264	Resp:	99130
Ion Ratio	Lower	Upper
264	100	
260	24.4	19.8 29.6
265	23.6	20.3 30.5

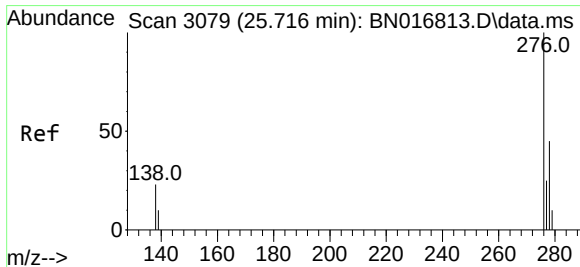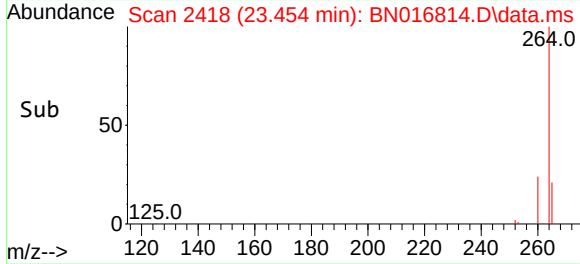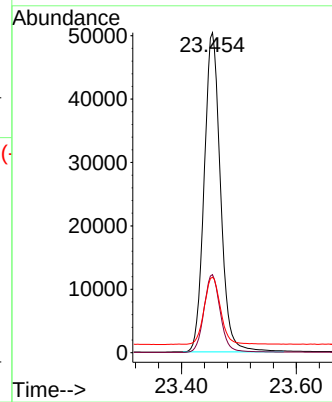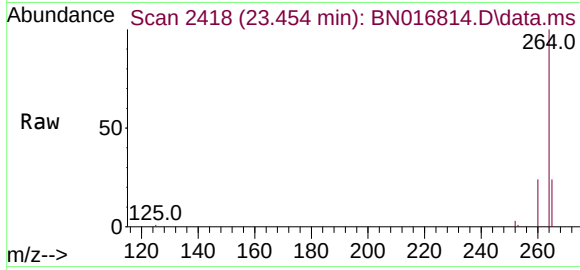

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 1.066 ng
 RT: 25.716 min Scan# 3079
 Delta R.T. 0.000 min
 Lab File: BN016814.D
 Acq: 07 Oct 2021 18:14

Tgt Ion:276	Resp:	335341
Ion Ratio	Lower	Upper
276	100	
138	24.8	19.2 28.8
277	25.1	20.0 30.0


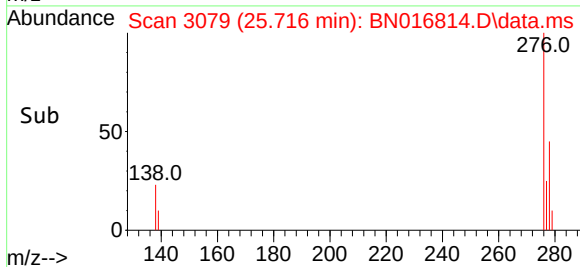

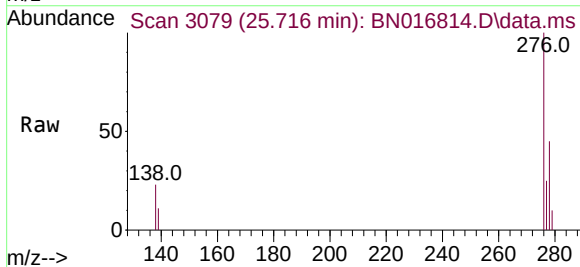




#37
Benzo(b)fluoranthene
Concen: 0.849 ng
RT: 22.779 min Scan# 2221
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 272183
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 9.8 8.3 12.5

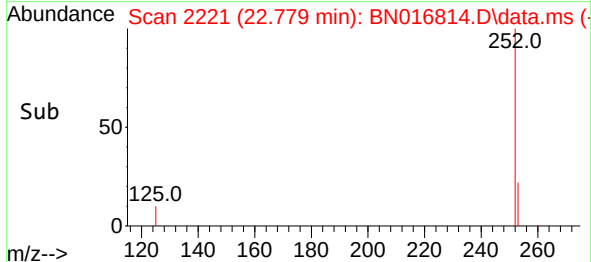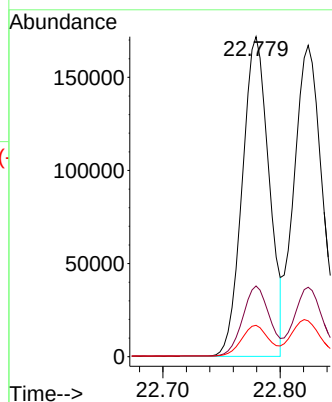

#38
Benzo(k)fluoranthene
Concen: 0.893 ng
RT: 22.824 min Scan# 2234
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14


Tgt Ion:252 Resp: 274973
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 11.5 8.5 12.7

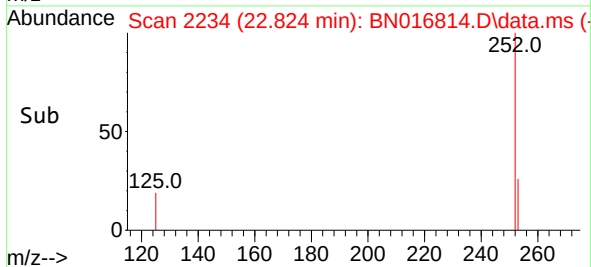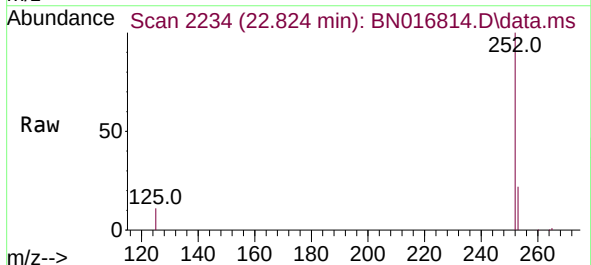






#39
Benzo(a)pyrene
Concen: 0.883 ng
RT: 23.355 min Scan# 2389
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8







Tgt Ion:252 Resp: 253324
Ion Ratio Lower Upper
252 100
253 22.1 17.9 26.9
125 10.7 9.4 14.2

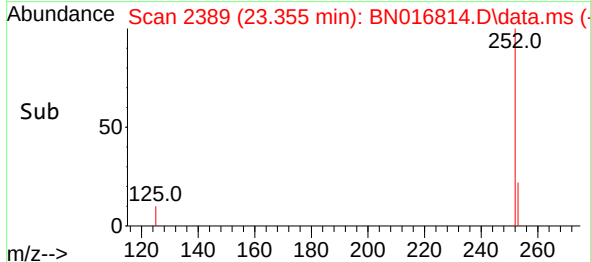

#40
Dibenzo(a,h)anthracene
Concen: 1.100 ng
RT: 25.737 min Scan# 3085
Delta R.T. 0.000 min
Lab File: BN016814.D
Acq: 07 Oct 2021 18:14

Tgt Ion:278 Resp: 274736
Ion Ratio Lower Upper
278 100
139 16.8 13.1 19.7
279 23.6 19.3 28.9

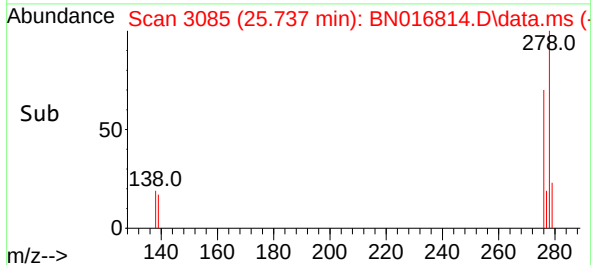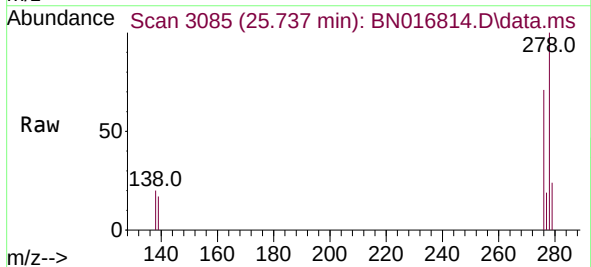

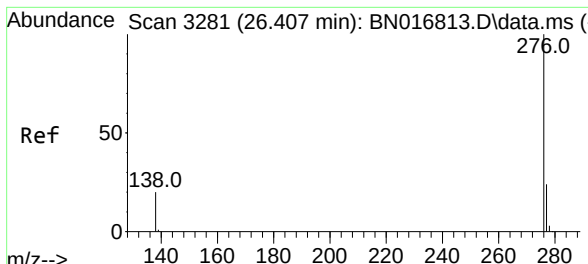

#41
 Benzo(g,h,i)perylene
 Concen: 1.027 ng
 RT: 26.408 min Scan# 3281
 Delta R.T. 0.000 min
 Lab File: BN016814.D
 Acq: 07 Oct 2021 18:14

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:276 Resp: 286953

Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.0	28.4
138	20.5	17.0	25.6

