

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016817.D
 Acq On : 07 Oct 2021 20:04
 Operator : CG/JU
 Sample : SSTDIC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC5.0

Quant Time: Oct 08 01:20:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 18:25:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.615	152	21471	0.400	ng	0.00
7) Naphthalene-d8	10.381	136	85703	0.400	ng	# 0.00
13) Acenaphthene-d10	14.243	164	45730	0.400	ng	0.00
19) Phenanthrene-d10	17.006	188	89110	0.400	ng	0.00
29) Chrysene-d12	21.217	240	90842	0.400	ng	# 0.00
35) Perylene-d12	23.454	264	100102	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.227	112	250617	4.575	ng	0.00
5) Phenol-d6	6.794	99	296380	4.877	ng	0.00
8) Nitrobenzene-d5	8.759	82	327240	5.446	ng	0.00
11) 2-Methylnaphthalene-d10	11.981	152	612300	4.796	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	142335	7.037	ng	0.00
15) 2-Fluorobiphenyl	12.873	172	862175	4.714	ng	0.00
27) Fluoranthene-d10	19.043	212	1228315	5.038	ng	0.00
31) Terphenyl-d14	19.659	244	1029586	5.065	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.217	88	44589	4.450	ng	# 70
3) n-Nitrosodimethylamine	3.539	42	85385	5.280	ng	99
6) bis(2-Chloroethyl)ether	7.052	93	264513	4.534	ng	100
9) Naphthalene	10.432	128	1098817	4.686	ng	100
10) Hexachlorobutadiene	10.724	225	212135	4.840	ng	# 100
12) 2-Methylnaphthalene	12.052	142	694943	4.665	ng	100
16) Acenaphthylene	13.964	152	1056677	5.234	ng	100
17) Acenaphthene	14.307	154	655313	4.913	ng	99
18) Fluorene	15.297	166	807187	5.017	ng	99
20) 4,6-Dinitro-2-methylph...	15.385	198	117758	19.106	ng	# 52
21) 4-Bromophenyl-phenylether	16.202	248	282920	5.213	ng	94
22) Hexachlorobenzene	16.312	284	302525	4.916	ng	99
23) Atrazine	16.482	200	245064	5.702	ng	98
24) Pentachlorophenol	16.653	266	167218	9.859	ng	99
25) Phenanthrene	17.042	178	1261507	4.816	ng	100
26) Anthracene	17.139	178	1202116	5.138	ng	100
28) Fluoranthene	19.073	202	1397055	4.806	ng	99
30) Pyrene	19.435	202	1480854	4.958	ng	100
32) Benzo(a)anthracene	21.196	228	1510455	5.361	ng	97
33) Chrysene	21.249	228	1468327	5.137	ng	98
34) Bis(2-ethylhexyl)phtha...	21.143	149	1023215	5.988	ng	98
36) Indeno(1,2,3-cd)pyrene	25.720	276	1919023	6.038	ng	99
37) Benzo(b)fluoranthene	22.779	252	1637380	5.058	ng	99
38) Benzo(k)fluoranthene	22.824	252	1528748	4.915	ng	99
39) Benzo(a)pyrene	23.351	252	1511908	5.220	ng	99
40) Dibenzo(a,h)anthracene	25.740	278	1589358	6.303	ng	99
41) Benzo(g,h,i)perylene	26.411	276	1676075	5.941	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016817.D
Acq On : 07 Oct 2021 20:04
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC5.0

Quant Time: Oct 08 01:20:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 18:25:32 2021
Response via : Initial Calibration




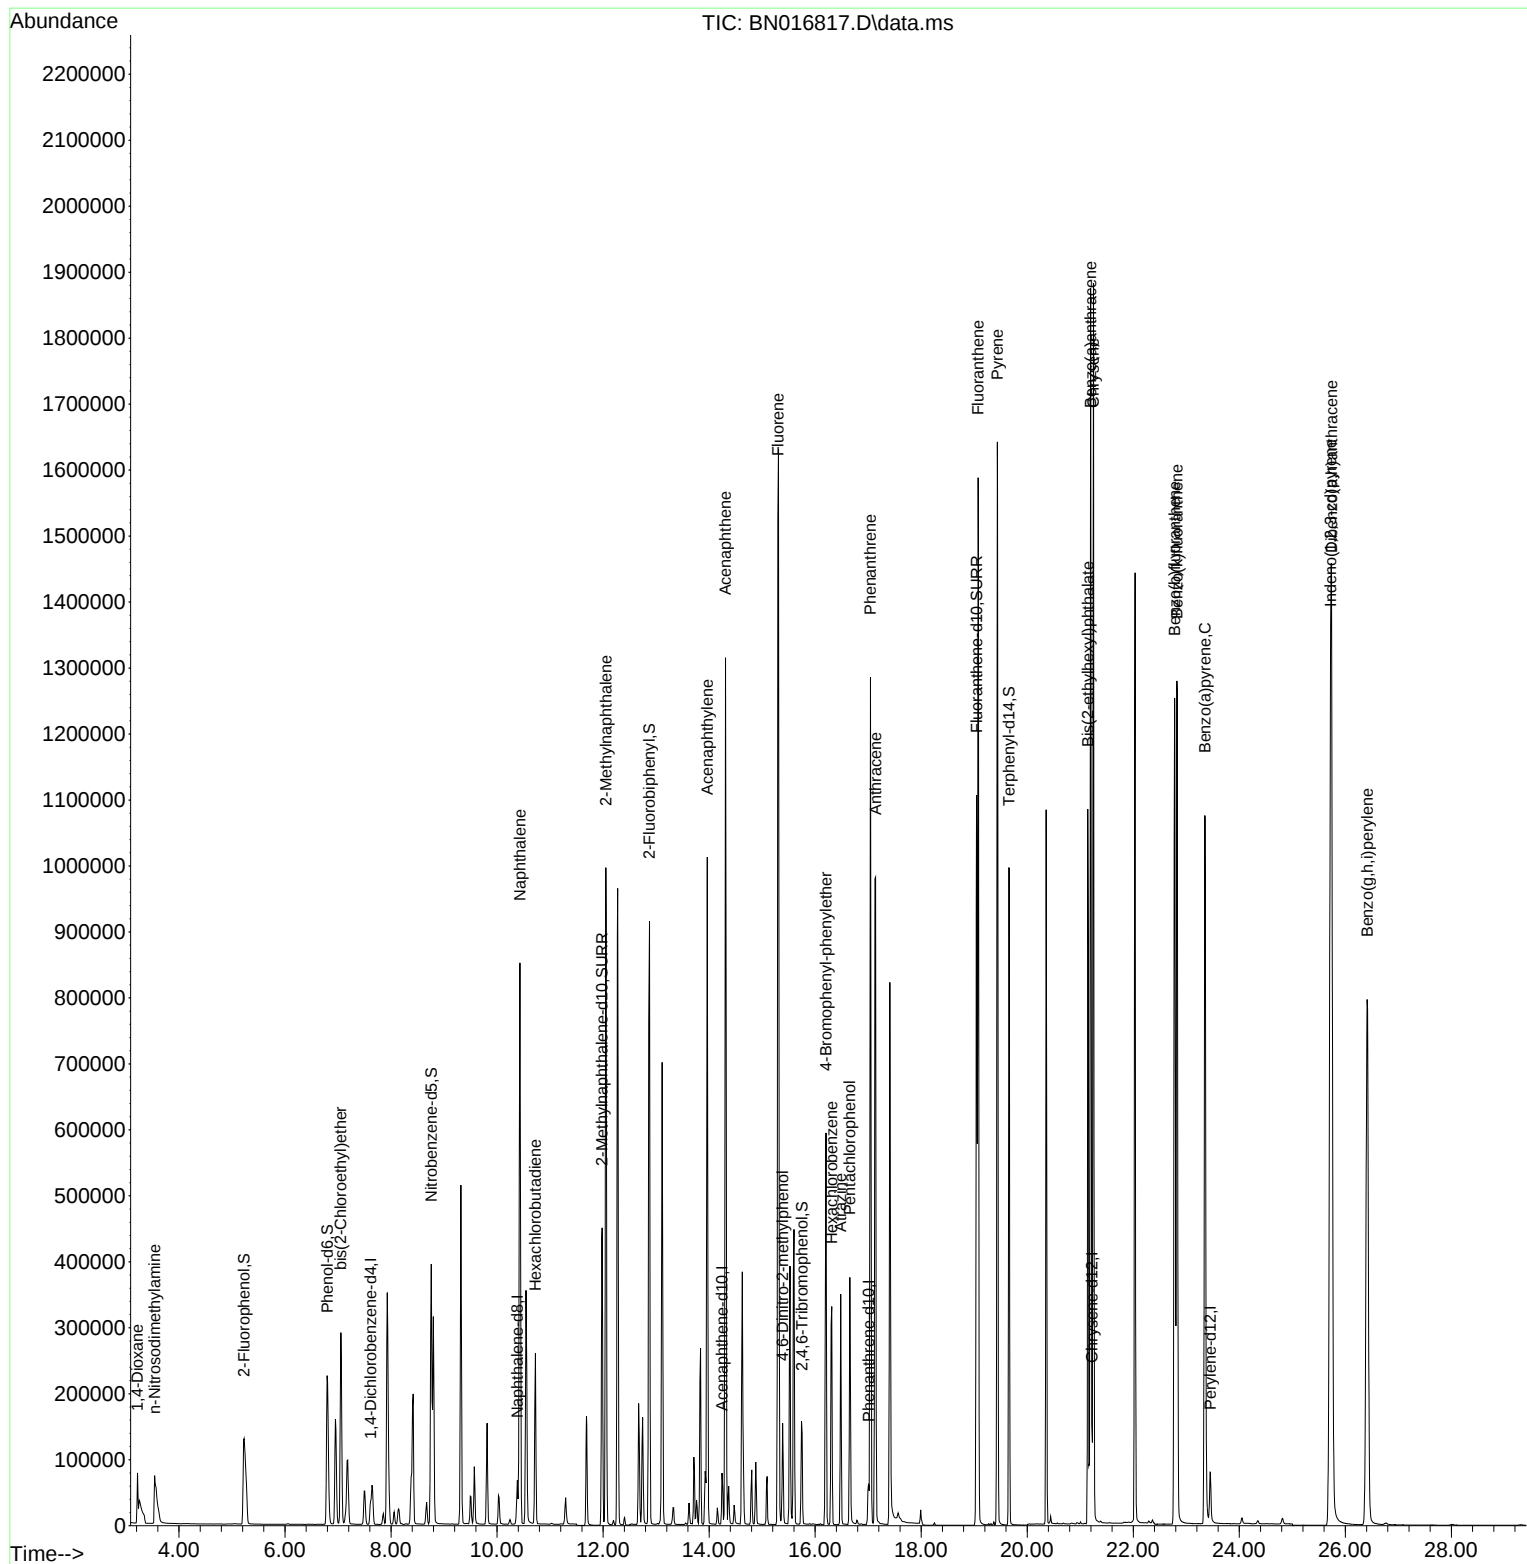




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.615 min Scan# 492
 Delta R.T. 0.001 min
 Lab File: BN016817.D
 Acq: 07 Oct 2021 20:04




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 21471
 Ion Ratio Lower Upper
 152 100
 150 157.4 123.3 184.9
 115 58.2 47.0 70.6

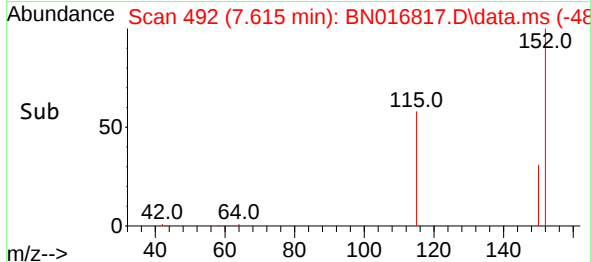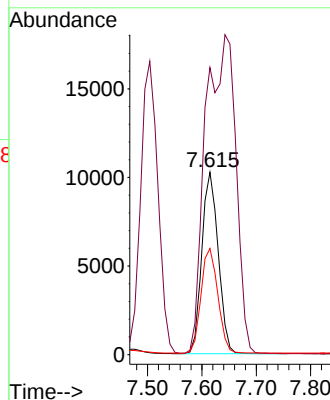

#2
 1,4-Dioxane
 Concen: 4.450 ng
 RT: 3.217 min Scan# 15
 Delta R.T. 0.000 min
 Lab File: BN016817.D
 Acq: 07 Oct 2021 20:04

Tgt Ion: 88 Resp: 44589
 Ion Ratio Lower Upper
 88 100
 43 28.9 61.7 92.5#
 58 74.3 62.2 93.2


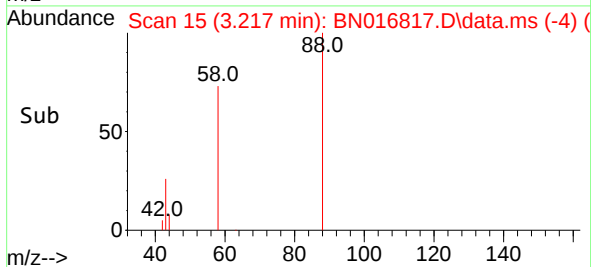
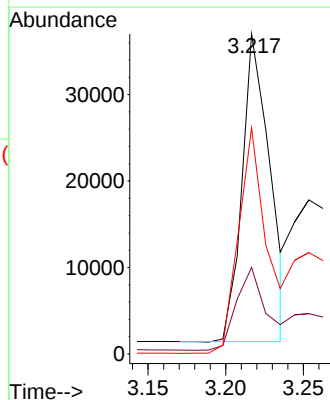
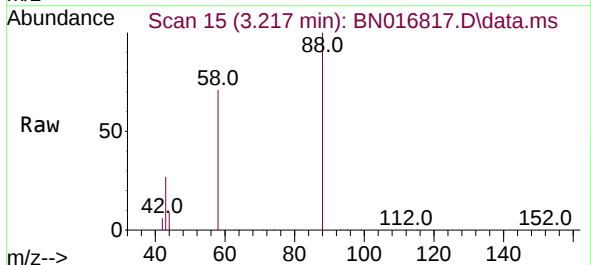




#3
n-Nitrosodimethylamine
Concen: 5.280 ng
RT: 3.539 min Scan# 50
Delta R.T. -0.009 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 85385
Ion Ratio Lower Upper
42 100
74 153.8 124.0 186.0
44 6.4 5.6 8.4

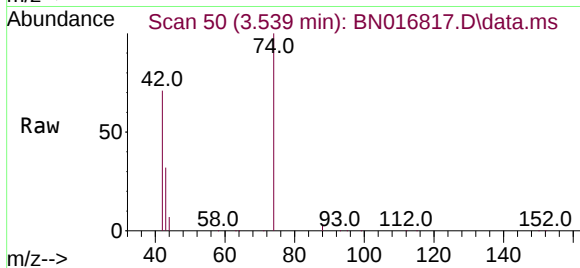

#4
2-Fluorophenol
Concen: 4.575 ng
RT: 5.227 min Scan# 233
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion: 112 Resp: 250617
Ion Ratio Lower Upper
112 100
64 54.5 42.9 64.3
63 27.3 21.5 32.3


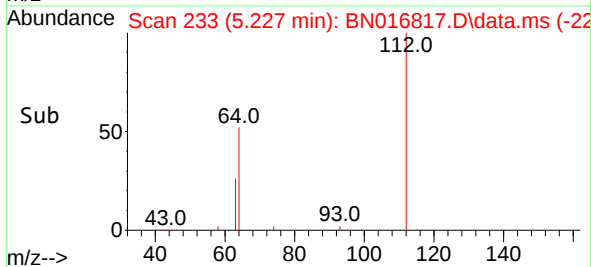

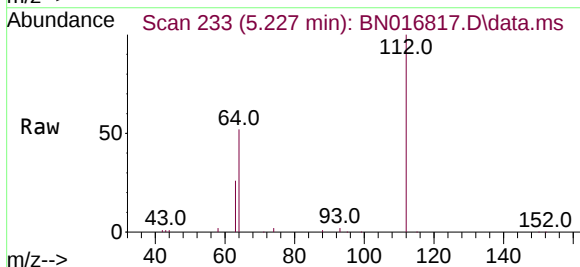


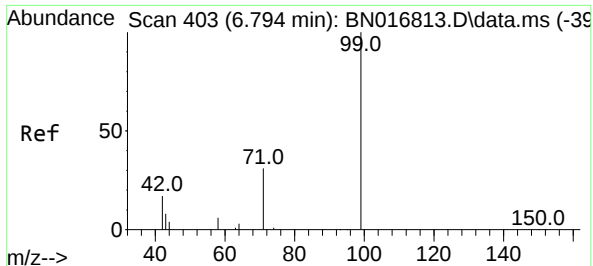

#5
Phenol-d6
Concen: 4.877 ng
RT: 6.794 min Scan# 403
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 296380
Ion Ratio Lower Upper
99 100
42 16.6 13.4 20.2
71 30.1 24.0 36.0

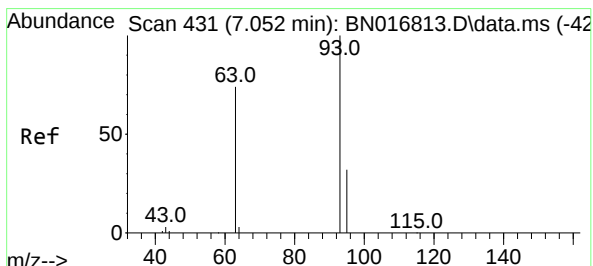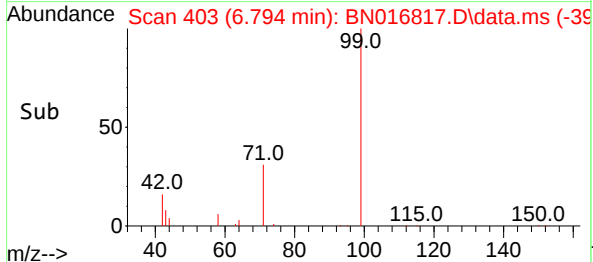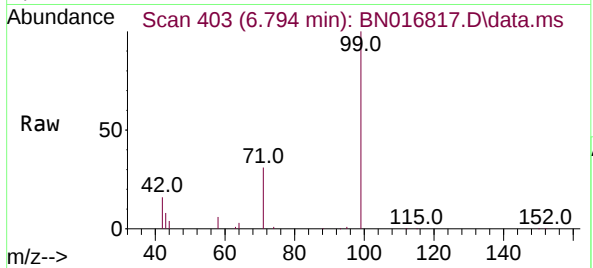

#6
bis(2-Chloroethyl)ether
Concen: 4.534 ng
RT: 7.052 min Scan# 431
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion: 93 Resp: 264513
Ion Ratio Lower Upper
93 100
63 73.4 59.0 88.6
95 32.7 26.4 39.6


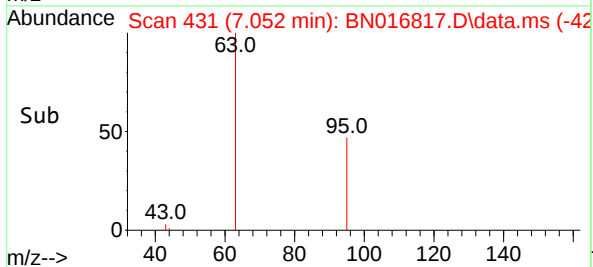

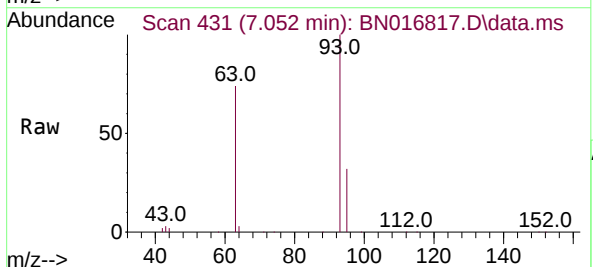




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.381 min Scan# 731
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	85703
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	6.4	6.5	9.7#
68	5.5	5.3	7.9

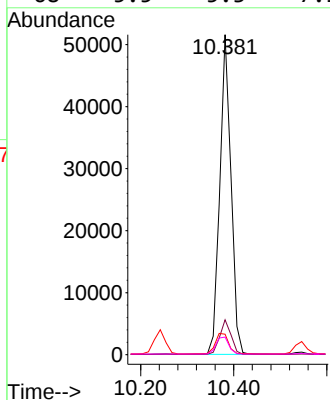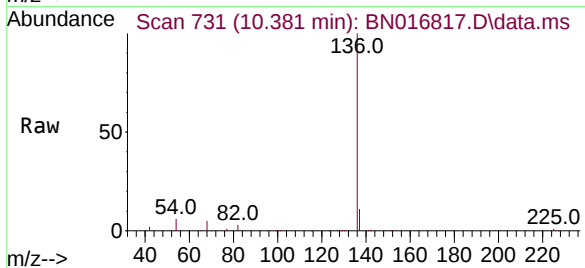

#8
Nitrobenzene-d5
Concen: 5.446 ng
RT: 8.759 min Scan# 603
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:	82	Resp:	327240
Ion	Ratio	Lower	Upper
82	100		
128	48.8	33.8	50.6
54	43.4	38.5	57.7


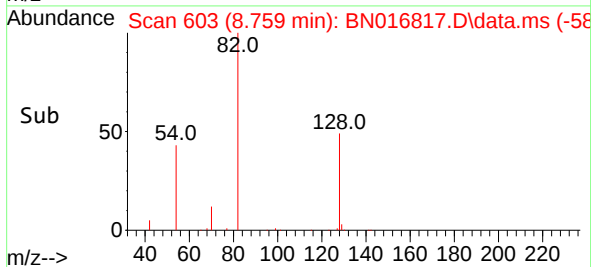
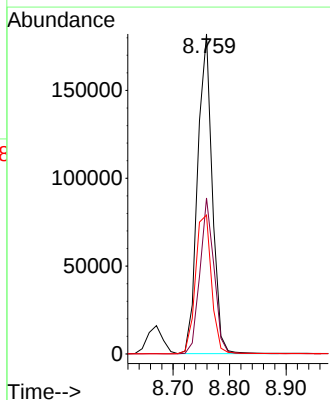
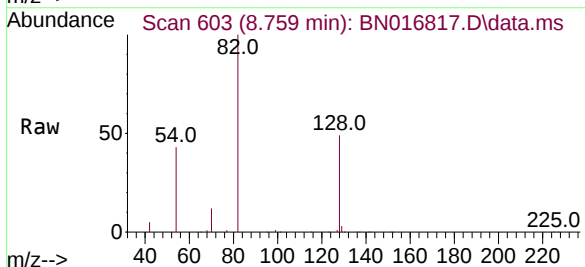




#9
Naphthalene
Concen: 4.686 ng
RT: 10.432 min Scan# 735
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1098817
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 12.8 10.3 15.5



#10
Hexachlorobutadiene
Concen: 4.840 ng
RT: 10.724 min Scan# 758
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:225 Resp: 212135
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.1 76.7


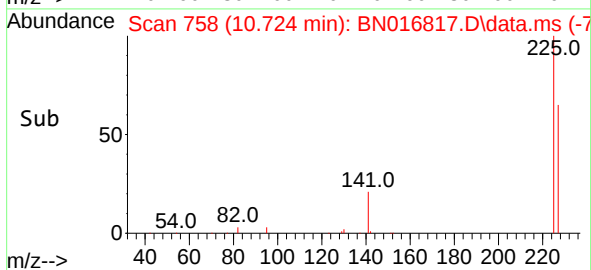




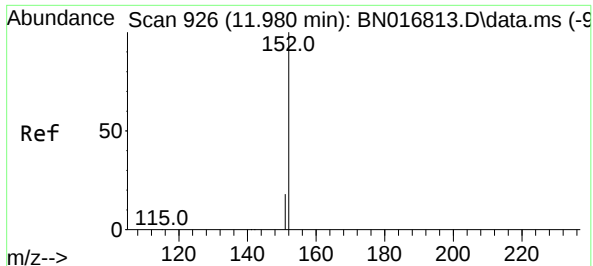

#11
2-Methylnaphthalene-d10
Concen: 4.796 ng
RT: 11.981 min Scan# 926
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 612300
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4

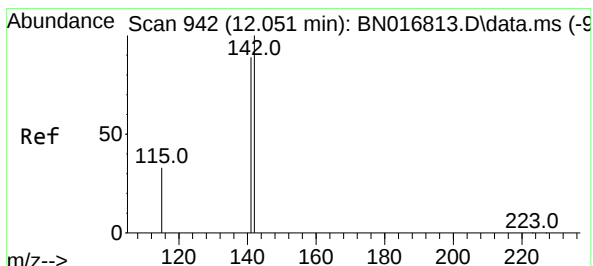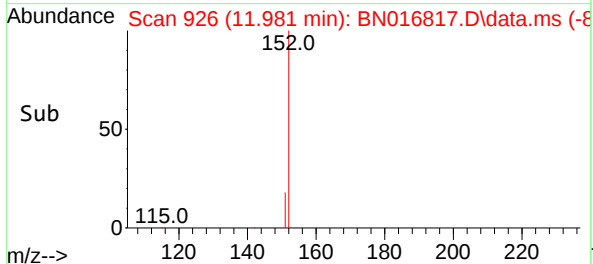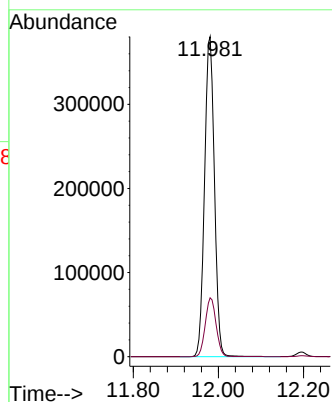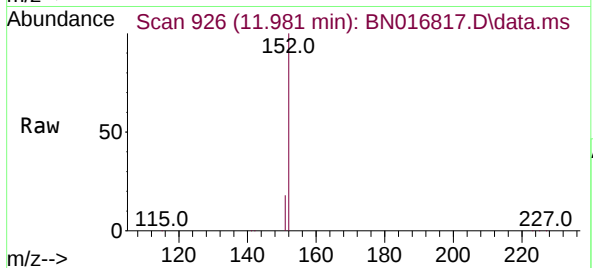

#12
2-Methylnaphthalene
Concen: 4.665 ng
RT: 12.052 min Scan# 942
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:142 Resp: 694943
Ion Ratio Lower Upper
142 100
141 88.0 70.6 106.0
115 32.7 26.1 39.1


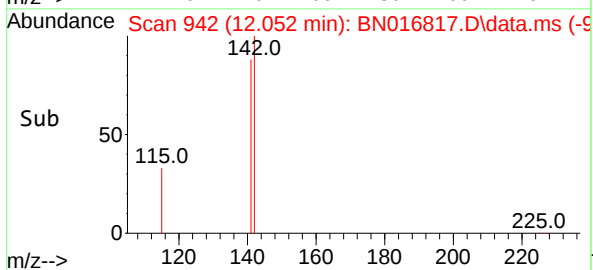

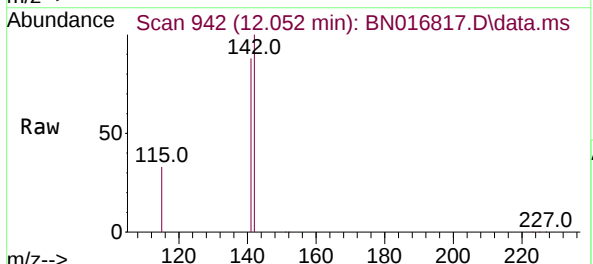


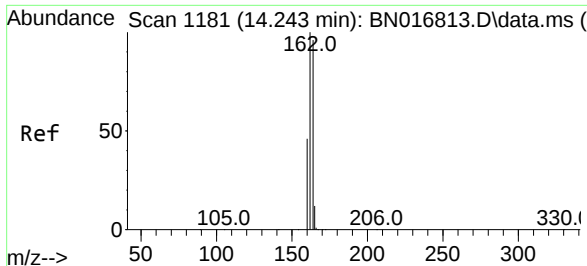

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.243 min Scan# 1181
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 45730
Ion Ratio Lower Upper
164 100
162 103.8 82.6 124.0
160 47.2 38.2 57.2

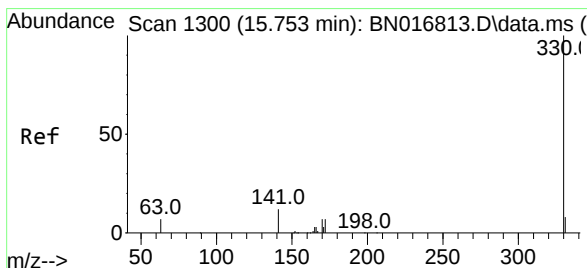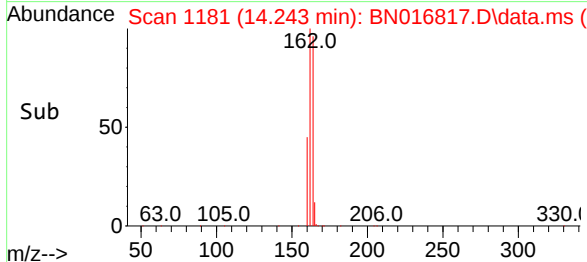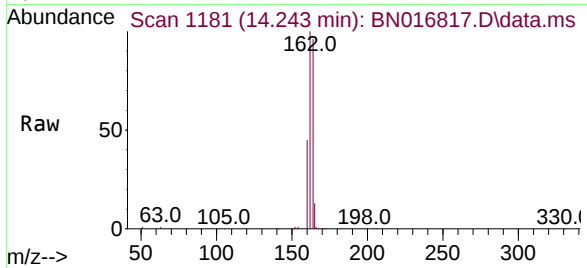

#14
2,4,6-Tribromophenol
Concen: 7.037 ng
RT: 15.753 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:330 Resp: 142335
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 28.9 24.2 36.2


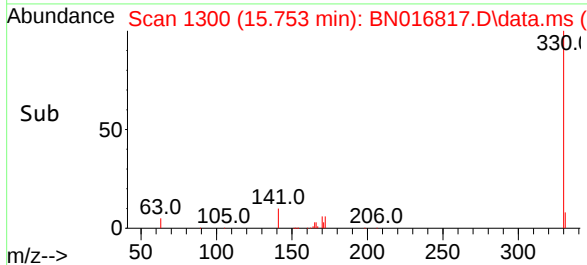

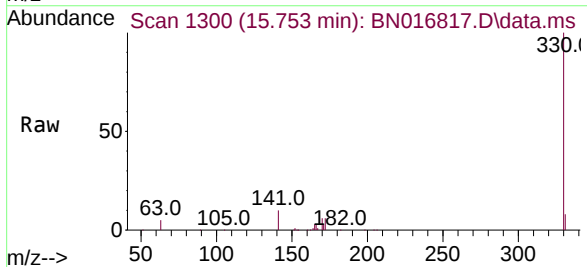


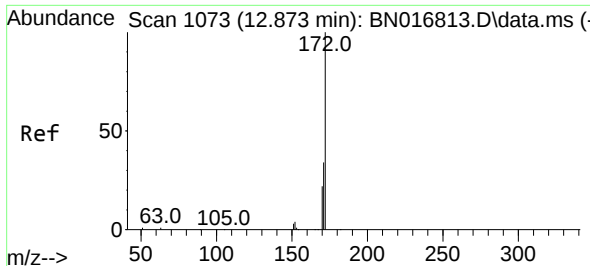

#15
2-Fluorobiphenyl
Concen: 4.714 ng
RT: 12.873 min Scan# 1073
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 862175
Ion Ratio Lower Upper
172 100
171 33.5 26.9 40.3
170 21.6 17.4 26.0

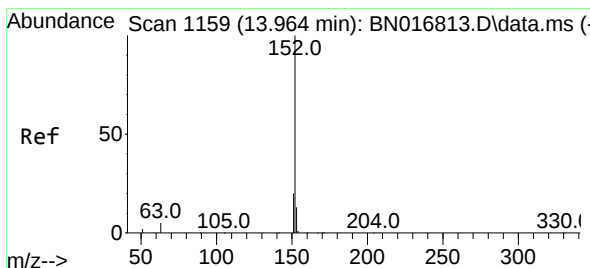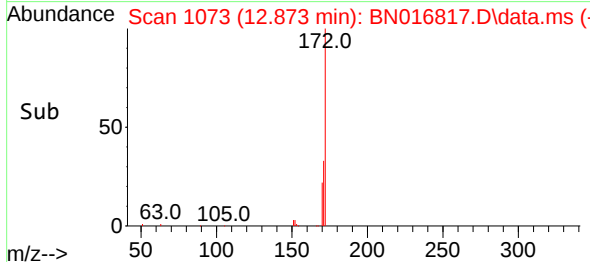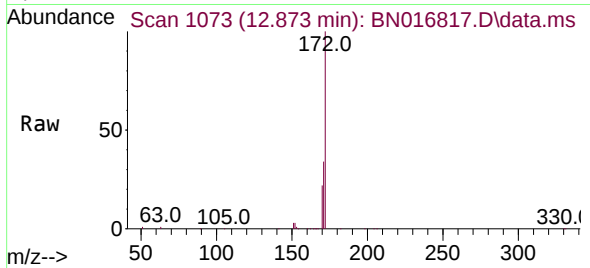

#16
Acenaphthylene
Concen: 5.234 ng
RT: 13.964 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:152 Resp: 1056677
Ion Ratio Lower Upper
152 100
151 19.5 15.5 23.3
153 13.1 10.4 15.6


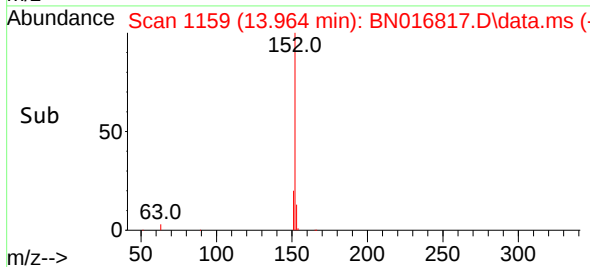

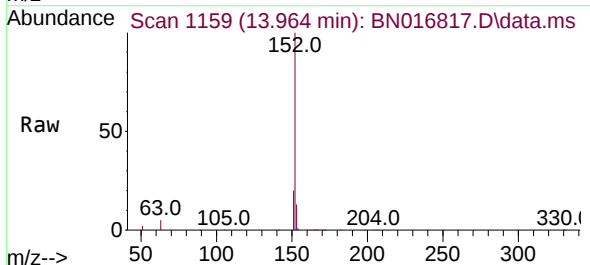


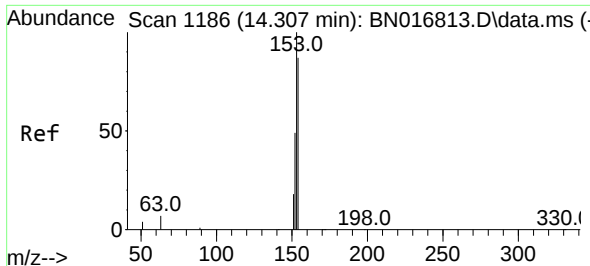

#17
Acenaphthene
Concen: 4.913 ng
RT: 14.307 min Scan# 1186
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 655313
Ion Ratio Lower Upper
154 100
153 111.7 90.1 135.1
152 53.0 43.6 65.4

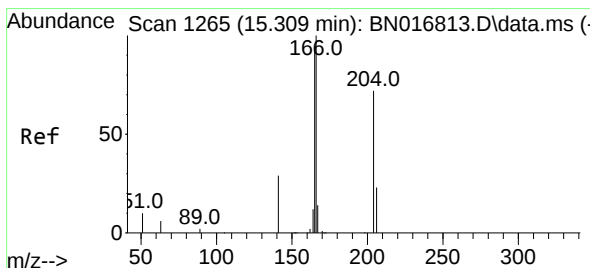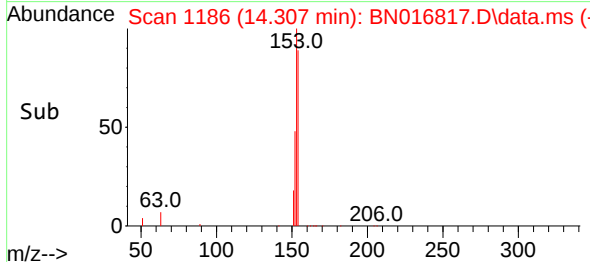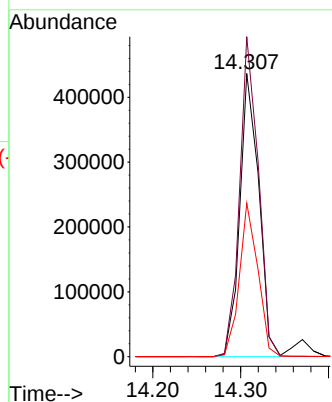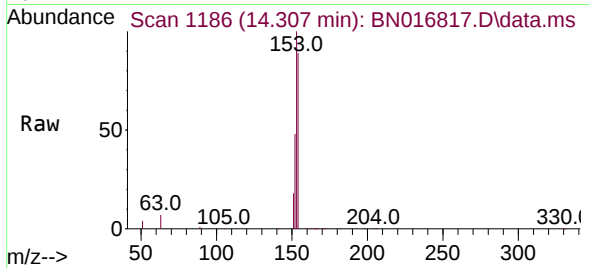

#18
Fluorene
Concen: 5.017 ng
RT: 15.297 min Scan# 1264
Delta R.T. -0.012 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:166 Resp: 807187
Ion Ratio Lower Upper
166 100
165 96.6 78.1 117.1
167 13.6 10.7 16.1


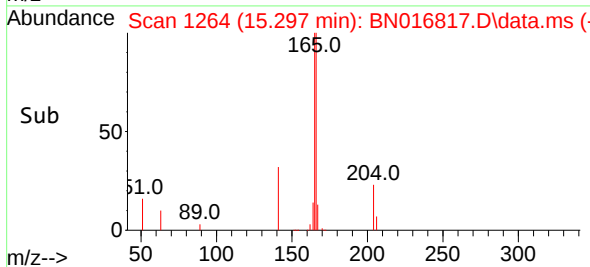
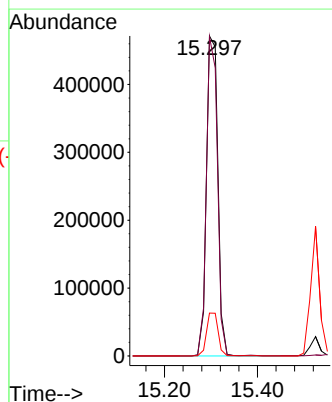
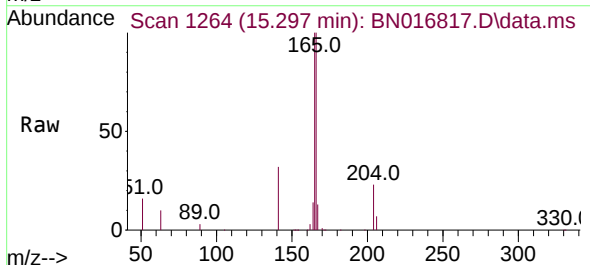




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.006 min Scan# 1402
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 89110
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.5 5.8 8.8

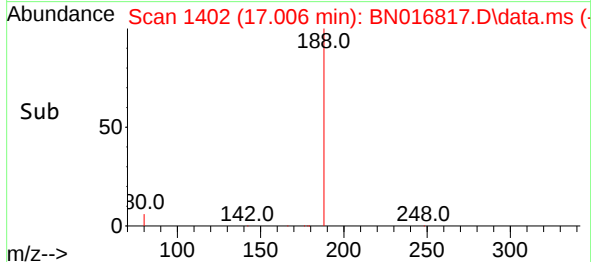

#20
4,6-Dinitro-2-methylphenol
Concen: 19.106 ng
RT: 15.385 min Scan# 1271
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:198 Resp: 117758
Ion Ratio Lower Upper
198 100
182 5.8 26.2 39.2#
77 0.0 0.0 0.0


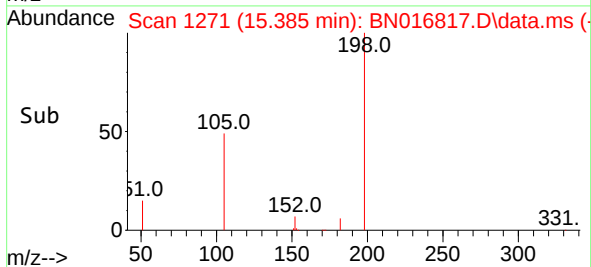

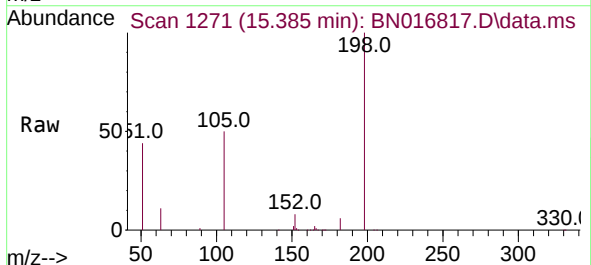




#21
4-Bromophenyl-phenylether
Concen: 5.213 ng
RT: 16.202 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 282920
Ion Ratio Lower Upper
248 100
250 97.3 76.2 114.4
141 47.3 45.6 68.4



#22
Hexachlorobenzene
Concen: 4.916 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:284 Resp: 302525
Ion Ratio Lower Upper
284 100
142 31.2 25.8 38.6
249 29.0 23.3 34.9


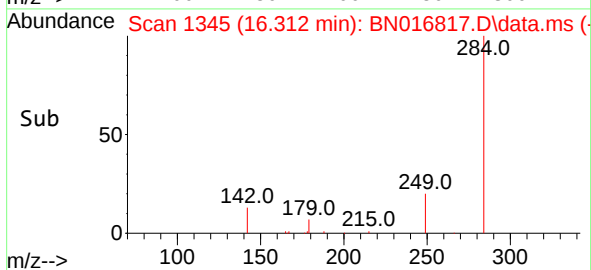




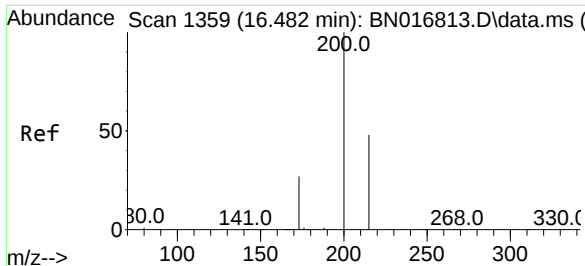

#23
Atrazine
Concen: 5.702 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:200 Resp: 245064
Ion Ratio Lower Upper
200 100
173 27.3 20.1 30.1
215 48.5 38.8 58.2

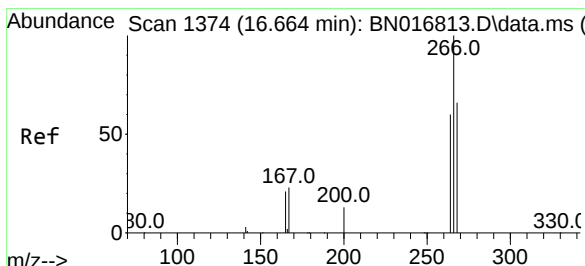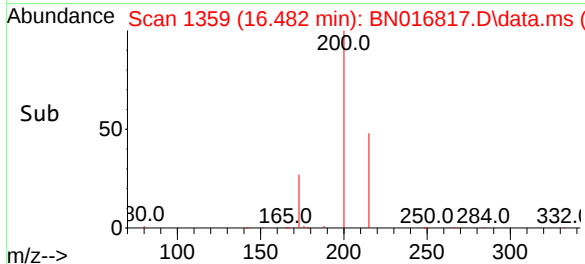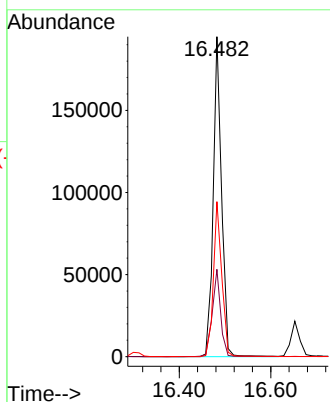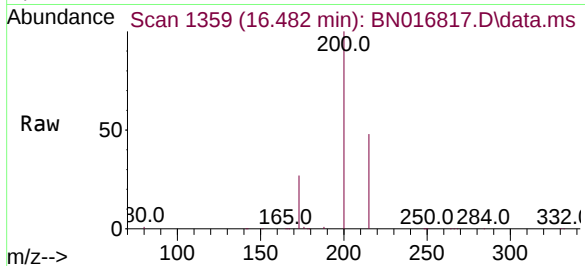

#24
Pentachlorophenol
Concen: 9.859 ng
RT: 16.653 min Scan# 1373
Delta R.T. -0.012 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:266 Resp: 167218
Ion Ratio Lower Upper
266 100
264 62.6 49.3 73.9
268 64.0 51.8 77.8


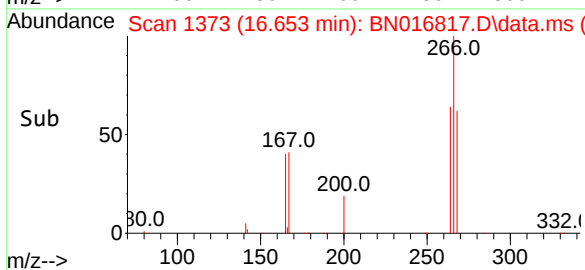
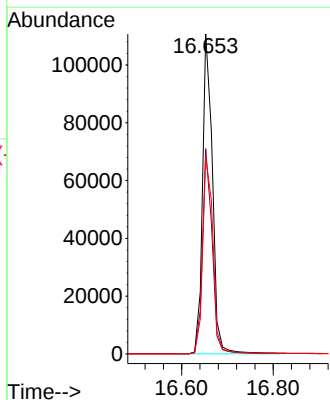
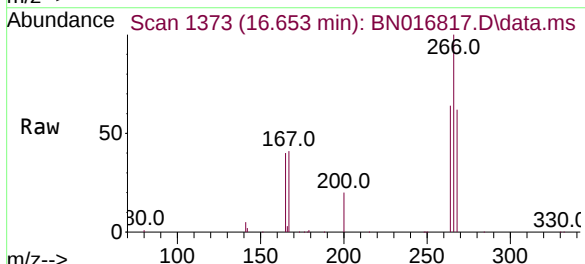




#25
Phenanthrene
Concen: 4.816 ng
RT: 17.042 min Scan# 1405
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 1261507
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.5 12.4 18.6



#26
Anthracene
Concen: 5.138 ng
RT: 17.139 min Scan# 1413
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:178 Resp: 1202116
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 15.4 12.2 18.4


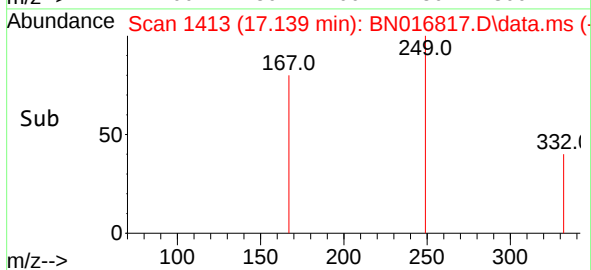




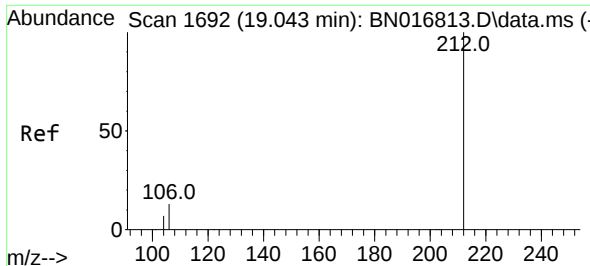

#27
Fluoranthene-d10
Concen: 5.038 ng
RT: 19.043 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 1228315
Ion Ratio Lower Upper
212 100
106 13.6 10.6 16.0
104 7.4 5.8 8.8

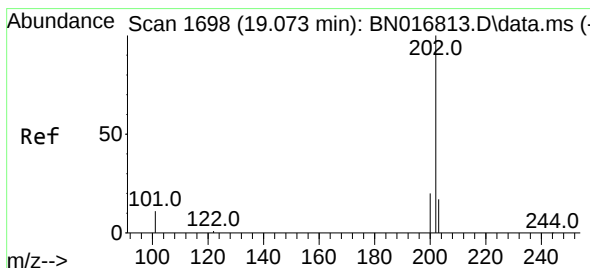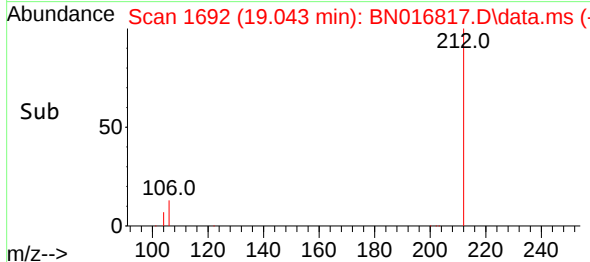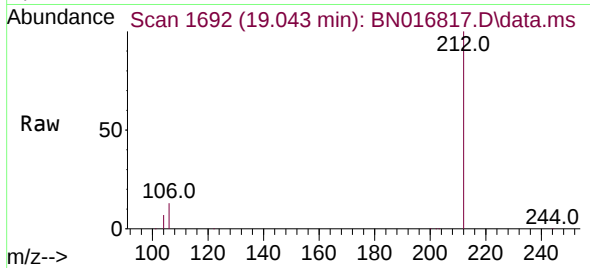

#28
Fluoranthene
Concen: 4.806 ng
RT: 19.073 min Scan# 1698
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:202 Resp: 1397055
Ion Ratio Lower Upper
202 100
101 11.5 8.9 13.3
203 17.6 13.8 20.8


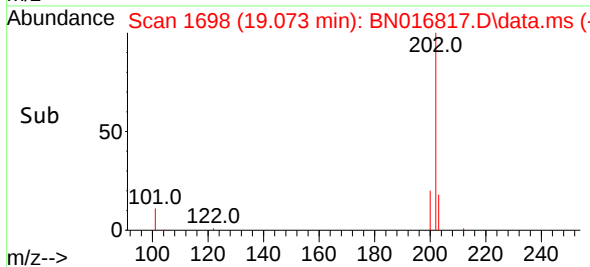

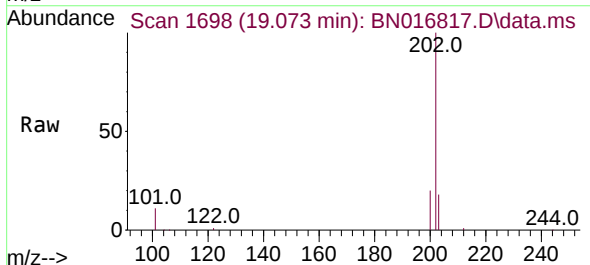


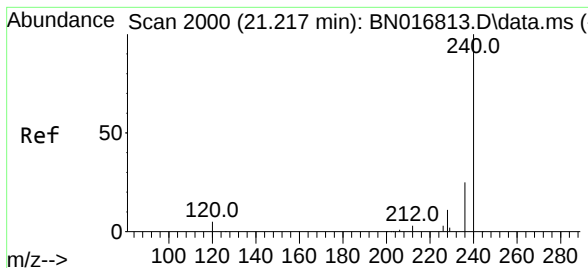

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 90842
Ion Ratio Lower Upper
240 100
120 4.9 6.6 10.0#
236 24.9 20.7 31.1

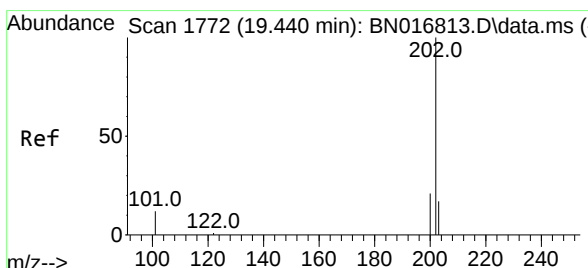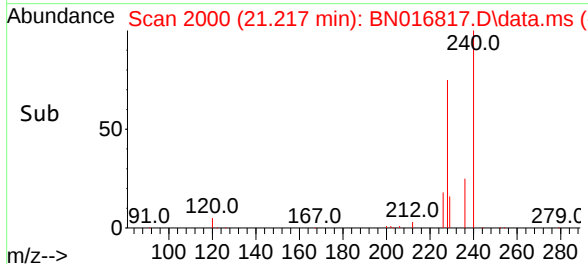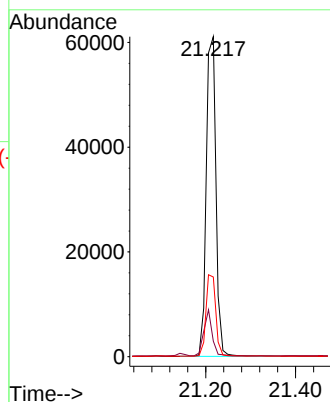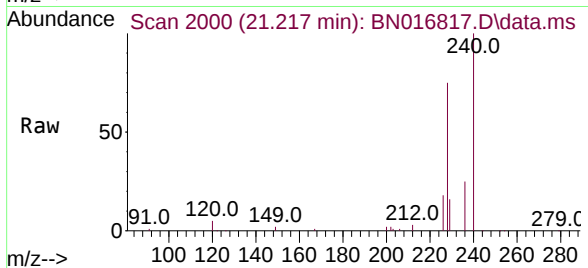

#30
Pyrene
Concen: 4.958 ng
RT: 19.435 min Scan# 1771
Delta R.T. -0.005 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:202 Resp: 1480854
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.7 13.9 20.9


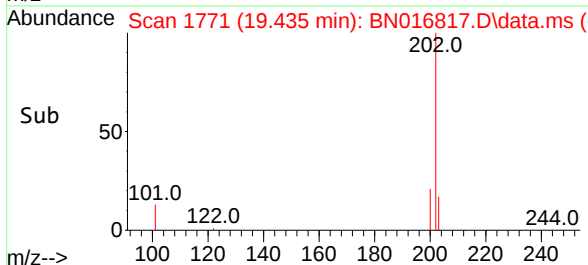
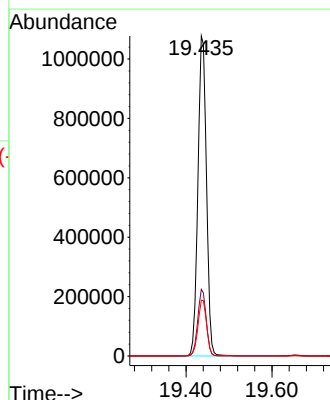
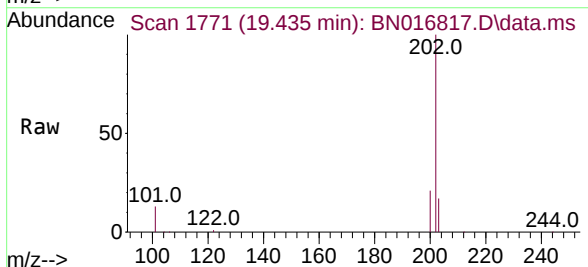




#31
 Terphenyl-d14
 Concen: 5.065 ng
 RT: 19.659 min Scan# 1816
 Delta R.T. 0.000 min
 Lab File: BN016817.D
 Acq: 07 Oct 2021 20:04




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 1029586
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.8 8.6
 122 10.9 8.9 13.3

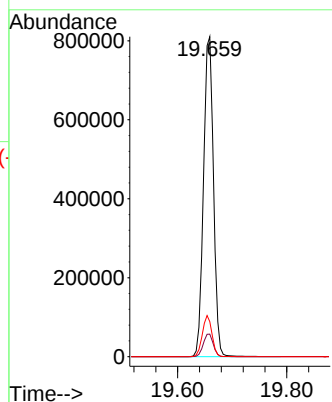

#32
 Benzo(a)anthracene
 Concen: 5.361 ng
 RT: 21.196 min Scan# 1998
 Delta R.T. 0.000 min
 Lab File: BN016817.D
 Acq: 07 Oct 2021 20:04

Tgt Ion:228 Resp: 1510455
 Ion Ratio Lower Upper
 228 100
 226 26.4 22.3 33.5
 229 20.2 15.4 23.0


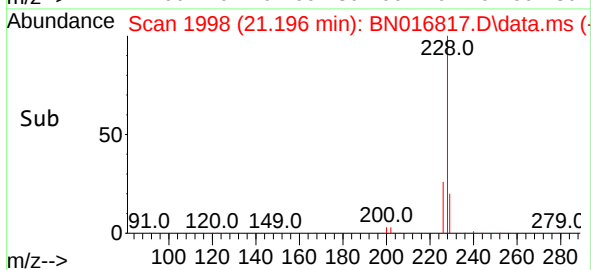
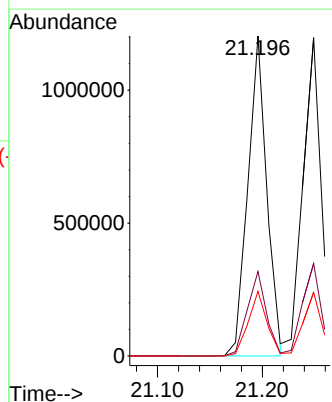



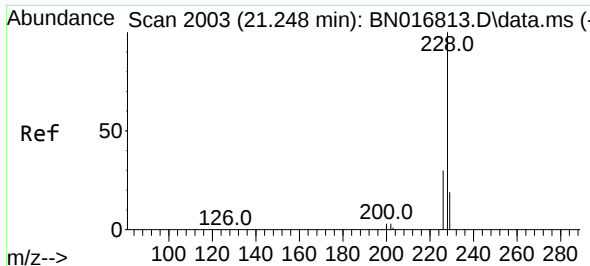

#33
Chrysene
Concen: 5.137 ng
RT: 21.249 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 1468327
Ion Ratio Lower Upper
228 100
226 29.1 24.2 36.4
229 20.0 15.4 23.0

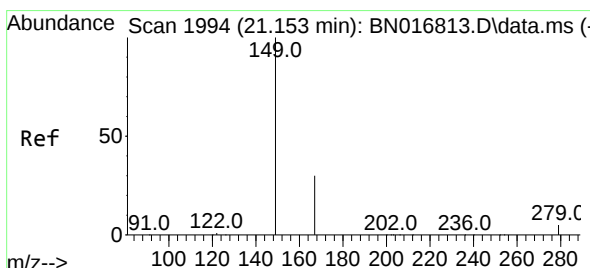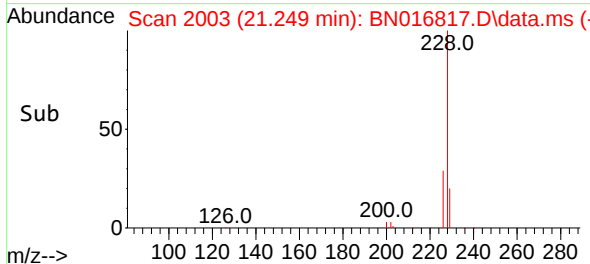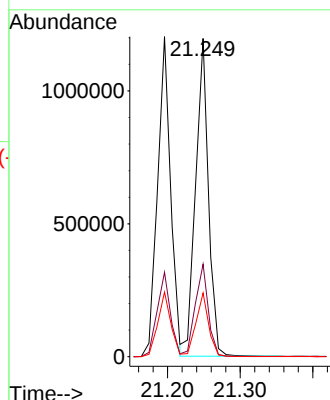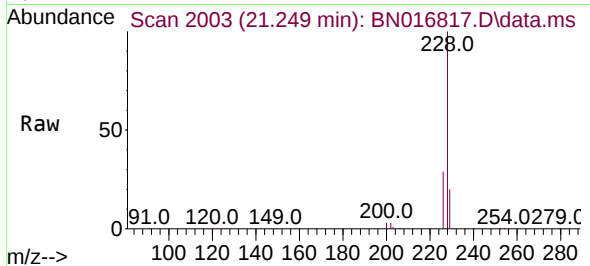

#34
Bis(2-ethylhexyl)phthalate
Concen: 5.988 ng
RT: 21.143 min Scan# 1993
Delta R.T. -0.010 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:149 Resp: 1023215
Ion Ratio Lower Upper
149 100
167 28.6 22.2 33.4
279 4.7 3.4 5.2


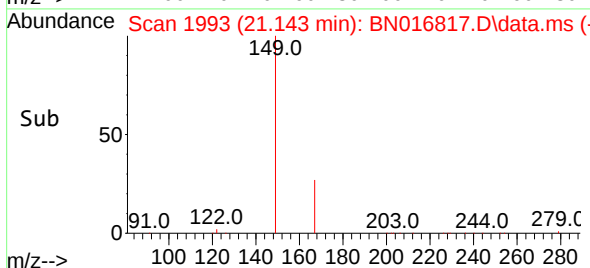
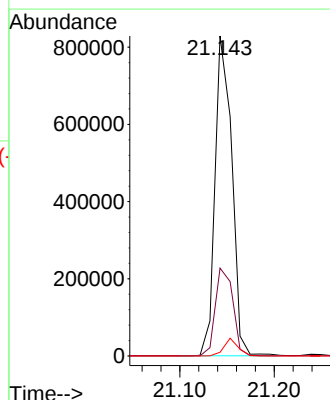
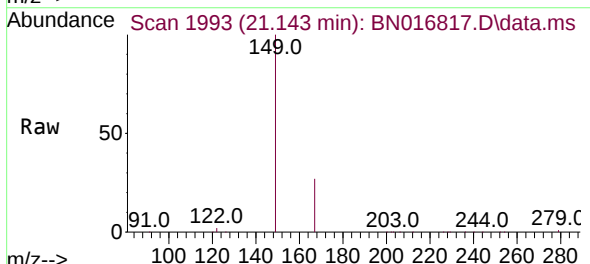




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.454 min Scan# 2418
Delta R.T. 0.000 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:264 Resp: 100102
Ion Ratio Lower Upper
264 100
260 24.5 19.8 29.6
265 23.6 20.3 30.5

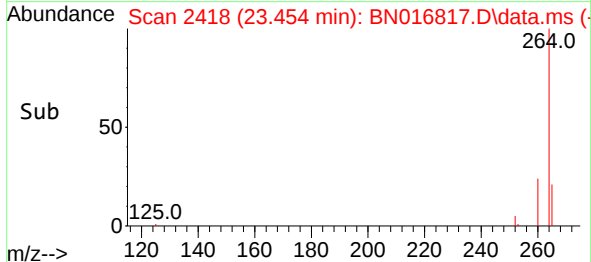

#36
Indeno(1,2,3-cd)pyrene
Concen: 6.038 ng
RT: 25.720 min Scan# 3080
Delta R.T. 0.004 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Tgt Ion:276 Resp: 1919023
Ion Ratio Lower Upper
276 100
138 24.4 19.2 28.8
277 25.2 20.0 30.0

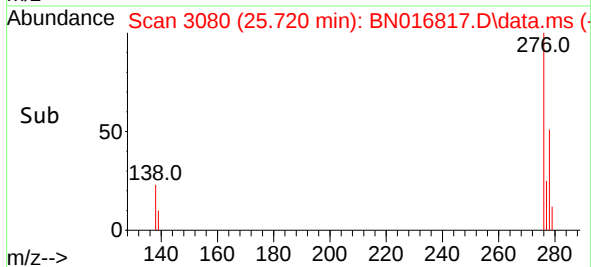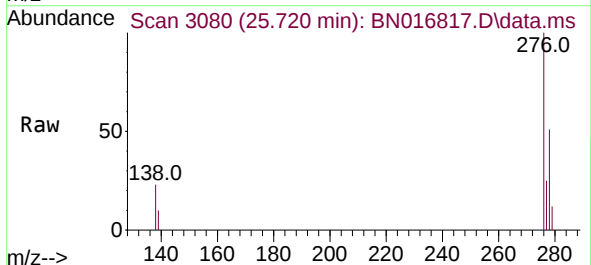



#37

Benzo(b)fluoranthene

Concen: 5.058 ng

RT: 22.779 min Scan# 2221

Delta R.T. 0.000 min

Lab File: BN016817.D

Acq: 07 Oct 2021 20:04





Tgt Ion:252 Resp: 1637380

Ion Ratio Lower Upper

252 100

253 22.1 17.8 26.8

125 9.8 8.3 12.5



#38

Benzo(k)fluoranthene

Concen: 4.915 ng

RT: 22.824 min Scan# 2234

Delta R.T. 0.000 min

Lab File: BN016817.D

Acq: 07 Oct 2021 20:04




Tgt Ion:252 Resp: 1528748


Ion Ratio Lower Upper

252 100

253 22.1 17.8 26.8


125 10.1 8.5 12.7

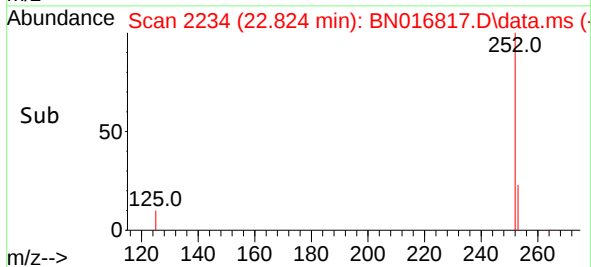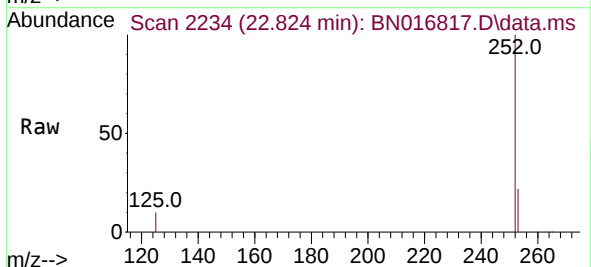






#39
Benzo(a)pyrene
Concen: 5.220 ng
RT: 23.351 min Scan# 2388
Delta R.T. -0.003 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0





Tgt Ion:252 Resp: 1511908
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 11.0 9.4 14.2

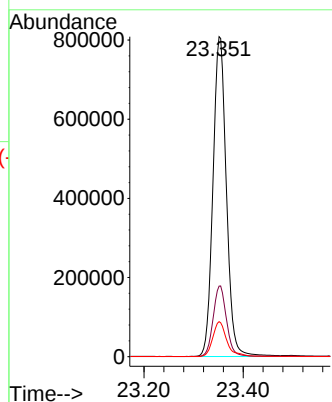


#40
Dibenzo(a,h)anthracene
Concen: 6.303 ng
RT: 25.740 min Scan# 3086
Delta R.T. 0.004 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04



Tgt Ion:278 Resp: 1589358
Ion Ratio Lower Upper
278 100
139 16.2 13.1 19.7
279 23.9 19.3 28.9

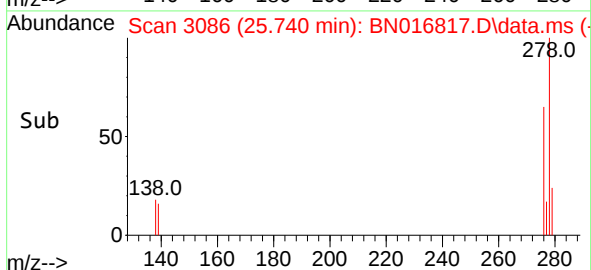

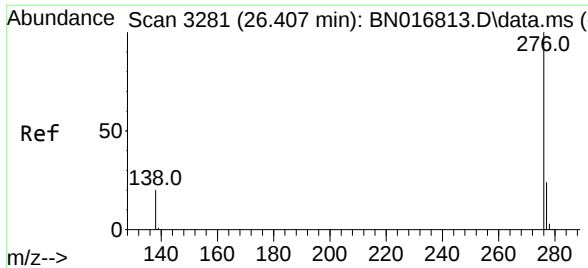

#41
Benzo(g,h,i)perylene
Concen: 5.941 ng
RT: 26.411 min Scan# 3282
Delta R.T. 0.004 min
Lab File: BN016817.D
Acq: 07 Oct 2021 20:04

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:276 Resp: 1676075
Ion Ratio Lower Upper
276 100
277 23.9 19.0 28.4
138 20.9 17.0 25.6

