

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016811.D
 Acq On : 07 Oct 2021 16:25
 Operator : CG/JU
 Sample : SSTDIC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.1

Quant Time: Oct 07 18:26:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 18:25:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.614	152	17535	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	77801	0.40	ng	0.00
13) Acenaphthene-d10	14.243	164	40824	0.40	ng	0.00
19) Phenanthrene-d10	17.005	188	76172	0.40	ng	0.00
29) Chrysene-d12	21.217	240	77115	0.40	ng	# 0.00
35) Perylene-d12	23.453	264	84356	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.226	112	4402	0.10	ng	0.00
5) Phenol-d6	6.803	99	4742	0.10	ng	0.00
8) Nitrobenzene-d5	8.759	82	4946	0.09	ng	0.00
11) 2-Methylnaphthalene-d10	11.980	152	11284	0.10	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	1598	0.09	ng	0.00
15) 2-Fluorobiphenyl	12.873	172	16948	0.10	ng	0.00
27) Fluoranthene-d10	19.043	212	19897	0.10	ng	0.00
31) Terphenyl-d14	19.658	244	18463	0.11	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.225	88	807	0.10	ng	# 33
3) n-Nitrosodimethylamine	3.548	42	1202	0.09	ng	# 1
6) bis(2-Chloroethyl)ether	7.052	93	4849	0.10	ng	100
9) Naphthalene	10.432	128	21584	0.10	ng	99
10) Hexachlorobutadiene	10.723	225	4072	0.10	ng	# 99
12) 2-Methylnaphthalene	12.056	142	13499	0.10	ng	100
16) Acenaphthylene	13.964	152	15400	0.09	ng	100
17) Acenaphthene	14.307	154	11633	0.10	ng	99
18) Fluorene	15.309	166	13514	0.09	ng	99
20) 4,6-Dinitro-2-methylph...	15.398	198	602	0.11	ng	# 88
21) 4-Bromophenyl-phenylether	16.202	248	4367	0.09	ng	98
22) Hexachlorobenzene	16.311	284	5404	0.10	ng	98
23) Atrazine	16.482	200	3160	0.09	ng	97
24) Pentachlorophenol	16.664	266	1400	0.10	ng	99
25) Phenanthrene	17.042	178	22074	0.10	ng	100
26) Anthracene	17.139	178	17577	0.09	ng	100
28) Fluoranthene	19.073	202	24178	0.10	ng	99
30) Pyrene	19.440	202	24833	0.10	ng	100
32) Benzo(a)anthracene	21.195	228	24180	0.10	ng	98
33) Chrysene	21.248	228	25076	0.10	ng	99
34) Bis(2-ethylhexyl)phtha...	21.153	149	12925	0.09	ng	99
36) Indeno(1,2,3-cd)pyrene	25.719	276	33010	0.12	ng	96
37) Benzo(b)fluoranthene	22.779	252	27054	0.10	ng	96
38) Benzo(k)fluoranthene	22.824	252	27373	0.10	ng	# 87
39) Benzo(a)pyrene	23.354	252	24704	0.10	ng	94
40) Dibenzo(a,h)anthracene	25.740	278	26817	0.13	ng	# 94
41) Benzo(g,h,i)perylene	26.407	276	29263	0.12	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016811.D
Acq On : 07 Oct 2021 16:25
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Oct 07 18:26:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 18:25:32 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.614 min Scan# 492
 Delta R.T. 0.000 min
 Lab File: BN016811.D
 Acq: 07 Oct 2021 16:25

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion: 152 Resp: 17535




Ion	Ratio	Lower	Upper
152	100		
150	154.4	123.3	184.9
115	58.3	47.0	70.6




#2
 1,4-Dioxane
 Concen: 0.10 ng
 RT: 3.225 min Scan# 16
 Delta R.T. 0.009 min
 Lab File: BN016811.D
 Acq: 07 Oct 2021 16:25

Tgt Ion: 88 Resp: 807

Ion	Ratio	Lower	Upper
88	100		
43	190.2	61.7	92.5#
58	74.0	62.2	93.2









#3
n-Nitrosodimethylamine
Concen: 0.09 ng
RT: 3.548 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 1202
Ion Ratio Lower Upper
42 100
74 0.0 124.0 186.0#
44 3.2 5.6 8.4#



#4
2-Fluorophenol
Concen: 0.10 ng
RT: 5.226 min Scan# 233
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion: 112 Resp: 4402
Ion Ratio Lower Upper
112 100
64 54.5 42.9 64.3
63 27.7 21.5 32.3









#5
Phenol-d6
Concen: 0.10 ng
RT: 6.803 min Scan# 404
Delta R.T. 0.009 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion: 99 Resp: 4742
Ion Ratio Lower Upper
99 100
42 16.8 13.4 20.2
71 30.9 24.0 36.0



#6
bis(2-Chloroethyl)ether
Concen: 0.10 ng
RT: 7.052 min Scan# 431
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion: 93 Resp: 4849
Ion Ratio Lower Upper
93 100
63 73.5 59.0 88.6
95 33.5 26.4 39.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:136 Resp: 77801




Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	6.8	6.5	9.7
68	5.7	5.3	7.9




#8
Nitrobenzene-d5
Concen: 0.09 ng
RT: 8.759 min Scan# 603
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion: 82 Resp: 4946

Ion	Ratio	Lower	Upper
82	100		
128	44.2	33.8	50.6
54	51.1	38.5	57.7









#9
Naphthalene
Concen: 0.10 ng
RT: 10.432 min Scan# 735
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:128 Resp: 21584




Ion	Ratio	Lower	Upper
128	100		
129	11.4	8.7	13.1
127	13.4	10.3	15.5




#10
Hexachlorobutadiene
Concen: 0.10 ng
RT: 10.723 min Scan# 758
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:225 Resp: 4072

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.4	51.1	76.7









#11
2-Methylnaphthalene-d10
Concen: 0.10 ng
RT: 11.980 min Scan# 926
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 11284
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.10 ng
RT: 12.056 min Scan# 943
Delta R.T. 0.004 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:142 Resp: 13499
Ion Ratio Lower Upper
142 100
141 88.0 70.6 106.0
115 33.2 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.243 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:164 Resp: 40824
Ion Ratio Lower Upper
164 100
162 103.6 82.6 124.0
160 47.6 38.2 57.2



#14
2,4,6-Tribromophenol
Concen: 0.09 ng
RT: 15.753 min Scan# 1300
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:330 Resp: 1598
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.6 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 0.10 ng
RT: 12.873 min Scan# 1073
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:172 Resp: 16948
Ion Ratio Lower Upper
172 100
171 34.4 26.9 40.3
170 22.5 17.4 26.0



#16
Acenaphthylene
Concen: 0.09 ng
RT: 13.964 min Scan# 1159
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:152 Resp: 15400
Ion Ratio Lower Upper
152 100
151 19.6 15.5 23.3
153 13.1 10.4 15.6









#17
Acenaphthene
Concen: 0.10 ng
RT: 14.307 min Scan# 1186
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:154 Resp: 11633
Ion Ratio Lower Upper
154 100
153 114.0 90.1 135.1
152 54.9 43.6 65.4



#18
Fluorene
Concen: 0.09 ng
RT: 15.309 min Scan# 1265
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:166 Resp: 13514
Ion Ratio Lower Upper
166 100
165 98.5 78.1 117.1
167 13.6 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.005 min Scan# 1402
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:188 Resp: 76172
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.2 5.8 8.8



#20
4,6-Dinitro-2-methylphenol
Concen: 0.11 ng
RT: 15.398 min Scan# 1272
Delta R.T. 0.013 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:198 Resp: 602
Ion Ratio Lower Upper
198 100
182 26.1 26.2 39.2#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.09 ng
RT: 16.202 min Scan# 1336
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:248 Resp: 4367




Ion	Ratio	Lower	Upper
248	100		
250	93.9	76.2	114.4
141	59.7	45.6	68.4




#22
Hexachlorobenzene
Concen: 0.10 ng
RT: 16.311 min Scan# 1345
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:284 Resp: 5404

Ion	Ratio	Lower	Upper
284	100		
142	31.2	25.8	38.6
249	28.4	23.3	34.9







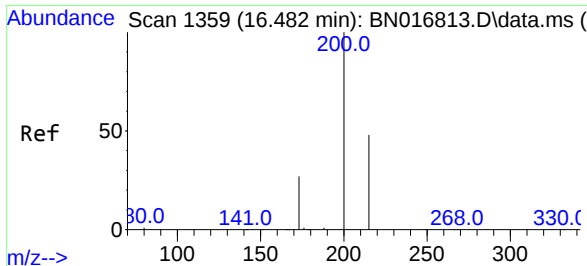

#23
Atrazine
Concen: 0.09 ng
RT: 16.482 min Scan# 1359
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	200	Resp:	3160
Ion	Ratio	Lower	Upper
200	100		
173	28.3	20.1	30.1
215	48.9	38.8	58.2



#24
Pentachlorophenol
Concen: 0.10 ng
RT: 16.664 min Scan# 1374
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:	266	Resp:	1400
Ion	Ratio	Lower	Upper
266	100		
264	62.6	49.3	73.9
268	65.6	51.8	77.8









#25
Phenanthrene
Concen: 0.10 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:178 Resp: 22074
Ion Ratio Lower Upper
178 100
176 19.0 15.0 22.6
179 15.6 12.4 18.6



#26
Anthracene
Concen: 0.09 ng
RT: 17.139 min Scan# 1413
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:178 Resp: 17577
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.10 ng
RT: 19.043 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:212 Resp: 19897




Ion	Ratio	Lower	Upper
212	100		
106	13.2	10.6	16.0
104	7.3	5.8	8.8




#28
Fluoranthene
Concen: 0.10 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:202 Resp: 24178

Ion	Ratio	Lower	Upper
202	100		
101	11.3	8.9	13.3
203	17.0	13.8	20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.217 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:240 Resp: 77115
Ion Ratio Lower Upper
240 100
120 5.7 6.6 10.0#
236 25.0 20.7 31.1



#30
Pyrene
Concen: 0.10 ng
RT: 19.440 min Scan# 1772
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:202 Resp: 24833
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 17.5 13.9 20.9









#31
Terphenyl-d14
Concen: 0.11 ng
RT: 19.658 min Scan# 1816
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:244 Resp: 18463
Ion Ratio Lower Upper
244 100
212 7.4 5.8 8.6
122 11.9 8.9 13.3



#32
Benzo(a)anthracene
Concen: 0.10 ng
RT: 21.195 min Scan# 1998
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:228 Resp: 24180
Ion Ratio Lower Upper
228 100
226 26.8 22.3 33.5
229 19.7 15.4 23.0









#33
Chrysene
Concen: 0.10 ng
RT: 21.248 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	228	Resp:	25076
Ion	Ratio	Lower	Upper
228	100		
226	29.6	24.2	36.4
229	19.8	15.4	23.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.09 ng
RT: 21.153 min Scan# 1994
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25


Tgt Ion:	149	Resp:	12925
Ion	Ratio	Lower	Upper
149	100		
167	27.4	22.2	33.4
279	4.5	3.4	5.2








#35
Perylene-d12
Concen: 0.40 ng
RT: 23.453 min Scan# 2418
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1



Tgt Ion:264 Resp: 84356




Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.8	29.6
265	24.7	20.3	30.5




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.12 ng
RT: 25.719 min Scan# 3080
Delta R.T. 0.003 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:276 Resp: 33010

Ion	Ratio	Lower	Upper
276	100		
138	27.6	19.2	28.8
277	25.2	20.0	30.0









#37
Benzo(b)fluoranthene
Concen: 0.10 ng
RT: 22.779 min Scan# 2221
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Tgt Ion:252 Resp: 27054
Ion Ratio Lower Upper
252 100
253 24.2 17.8 26.8
125 12.1 8.3 12.5


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1



#38
Benzo(k)fluoranthene
Concen: 0.10 ng
RT: 22.824 min Scan# 2234
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:252 Resp: 27373
Ion Ratio Lower Upper
252 100
253 25.6 17.8 26.8
125 20.8 8.5 12.7#









#39
Benzo(a)pyrene
Concen: 0.10 ng
RT: 23.354 min Scan# 2389
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:252	Resp:	24704
Ion Ratio	Lower	Upper
252	100	
253	25.3	17.9 26.9
125	13.7	9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 0.13 ng
RT: 25.740 min Scan# 3086
Delta R.T. 0.003 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Tgt Ion:278	Resp:	26817
Ion Ratio	Lower	Upper
278	100	
139	20.8	13.1 19.7#
279	25.4	19.3 28.9





#41
Benzo(g,h,i)perylene
Concen: 0.12 ng
RT: 26.407 min Scan# 3281
Delta R.T. -0.000 min
Lab File: BN016811.D
Acq: 07 Oct 2021 16:25

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:276 Resp: 29263
Ion Ratio Lower Upper
276 100
277 24.0 19.0 28.4
138 22.0 17.0 25.6

