

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016823.D
 Acq On : 08 Oct 2021 00:55
 Operator : CG/JU
 Sample : M4020-13MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 S-820-N-SO-1-1.5-093021MS

Manual Integrations
 APPROVED

mohammad
 10/11/2021 2:09:48 PM

Quant Time: Oct 08 05:20:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 01:39:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.614	152	20251	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	92731	0.40	ng	# 0.00
13) Acenaphthene-d10	14.243	164	48636	0.40	ng	0.00
19) Phenanthrene-d10	17.005	188	92654	0.40	ng	0.00
29) Chrysene-d12	21.206	240	91756	0.40	ng	#-0.01
35) Perylene-d12	23.450	264	103737	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.263	112	17102	0.34	ng	0.04
5) Phenol-d6	6.812	99	18799	0.33	ng	0.02
8) Nitrobenzene-d5	8.759	82	20216	0.31	ng	0.00
11) 2-Methylnaphthalene-d10	11.976	152	52749	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	7082	0.28	ng	0.00
15) 2-Fluorobiphenyl	12.873	172	57442	0.29	ng	0.00
27) Fluoranthene-d10	19.043	212	87395	0.34	ng	0.00
31) Terphenyl-d14	19.653	244	65567	0.33	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	5986m	0.66	ng	
3) n-Nitrosodimethylamine	3.557	42	6544	0.41	ng	# 94
6) bis(2-Chloroethyl)ether	7.052	93	23076	0.41	ng	100
9) Naphthalene	10.432	128	96987	0.38	ng	100
10) Hexachlorobutadiene	10.723	225	17897	0.37	ng	# 100
12) 2-Methylnaphthalene	12.051	142	63318	0.39	ng	100
16) Acenaphthylene	13.964	152	82631	0.39	ng	100
17) Acenaphthene	14.307	154	53338	0.37	ng	100
18) Fluorene	15.296	166	65388	0.38	ng	100
20) 4,6-Dinitro-2-methylph...	15.385	198	2691	0.31	ng	# 69
21) 4-Bromophenyl-phenylether	16.202	248	23013	0.40	ng	# 91
22) Hexachlorobenzene	16.311	284	24788	0.38	ng	99
23) Atrazine	16.482	200	17811	0.39	ng	99
24) Pentachlorophenol	16.652	266	4641	0.25	ng	99
25) Phenanthrene	17.042	178	112824	0.41	ng	100
26) Anthracene	17.127	178	98690	0.40	ng	99
28) Fluoranthene	19.073	202	134878	0.44	ng	100
30) Pyrene	19.435	202	137103	0.49	ng	99
32) Benzo(a)anthracene	21.195	228	126305	0.45	ng	97
33) Chrysene	21.248	228	125121	0.43	ng	97
34) Bis(2-ethylhexyl)phtha...	21.142	149	967070	6.71	ng	100
36) Indeno(1,2,3-cd)pyrene	25.712	276	168105	0.43	ng	99
37) Benzo(b)fluoranthene	22.776	252	143857	0.44	ng	99
38) Benzo(k)fluoranthene	22.820	252	129953	0.41	ng	# 97
39) Benzo(a)pyrene	23.351	252	134924	0.45	ng	99
40) Dibenzo(a,h)anthracene	25.733	278	134980	0.42	ng	99
41) Benzo(g,h,i)perylene	26.404	276	145801	0.43	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016823.D
Acq On : 08 Oct 2021 00:55
Operator : CG/JU
Sample : M4020-13MS
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:48 PM

Quant Time: Oct 08 05:20:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 01:39:08 2021
Response via : Initial Calibration





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.614 min Scan# 492
 Delta R.T. 0.000 min
 Lab File: BN016823.D
 Acq: 08 Oct 2021 00:55





Tgt Ion: 152 Resp: 20251

Ion	Ratio	Lower	Upper
152	100		
150	155.7	123.3	184.9
115	59.2	47.0	70.6

Instrument :
 BNA_N
 ClientSampleId :
 S-820-N-SO-1-1.5-093021MS

Manual Integrations
 APPROVED




mohammad
 10/11/2021 2:09:48 PM




#2
 1,4-Dioxane
 Concen: 0.66 ng m
 RT: 3.253 min Scan# 19
 Delta R.T. 0.037 min
 Lab File: BN016823.D
 Acq: 08 Oct 2021 00:55

Tgt Ion: 88 Resp: 5986

Ion	Ratio	Lower	Upper
88	100		
43	0.0	61.7	92.5#
58	0.0	62.2	93.2#









#3
n-Nitrosodimethylamine
Concen: 0.41 ng
RT: 3.557 min Scan# 52
Delta R.T. 0.009 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion: 42 Resp: 6544
Ion Ratio Lower Upper
42 100
74 162.5 124.0 186.0
44 0.0 5.6 8.4#

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM



#4
2-Fluorophenol
Concen: 0.34 ng
RT: 5.263 min Scan# 237
Delta R.T. 0.037 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55


Tgt Ion: 112 Resp: 17102
Ion Ratio Lower Upper
112 100
64 55.1 42.9 64.3
63 28.3 21.5 32.3





#5
Phenol-d6
Concen: 0.33 ng
RT: 6.812 min Scan# 405
Delta R.T. 0.018 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Tgt Ion: 99 Resp: 18799
Ion Ratio Lower Upper
99 100
42 17.6 13.4 20.2
71 31.3 24.0 36.0

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#6
bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 7.052 min Scan# 431
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion: 93 Resp: 23076
Ion Ratio Lower Upper
93 100
63 73.9 59.0 88.6
95 32.4 26.4 39.6





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55



Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Tgt Ion:	136	Resp:	92731
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	5.9	6.5	9.7#
68	5.2	5.3	7.9#

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#8
Nitrobenzene-d5
Concen: 0.31 ng
RT: 8.759 min Scan# 603
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55



Tgt Ion:	82	Resp:	20216
Ion	Ratio	Lower	Upper
82	100		
128	47.4	33.8	50.6
54	43.4	38.5	57.7









#9
Naphthalene
Concen: 0.38 ng
RT: 10.432 min Scan# 735
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:	128	Resp:	96987
Ion Ratio	Lower	Upper	
128	100		
129	10.9	8.7	13.1
127	12.7	10.3	15.5

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM



#10
Hexachlorobutadiene
Concen: 0.37 ng
RT: 10.723 min Scan# 758
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:	225	Resp:	17897
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.9	51.1	76.7









#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 11.976 min Scan# 925
Delta R.T. -0.004 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:152 Resp: 52749
Ion Ratio Lower Upper
152 100
151 18.2 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM



#12
2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.051 min Scan# 942
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55


Tgt Ion:142 Resp: 63318
Ion Ratio Lower Upper
142 100
141 87.9 70.6 106.0
115 32.6 26.1 39.1





#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.243 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS



Tgt Ion:164 Resp: 48636
Ion Ratio Lower Upper
164 100
162 101.9 82.6 124.0
160 46.4 38.2 57.2




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM

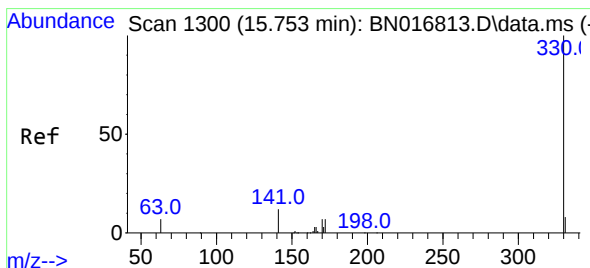

#14
2,4,6-Tribromophenol
Concen: 0.28 ng
RT: 15.753 min Scan# 1300
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:330 Resp: 7082
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.3 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 0.29 ng
RT: 12.873 min Scan# 1073
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:	172	Resp:	57442
Ion Ratio	Lower	Upper	
172	100		
171	33.5	26.9	40.3
170	21.5	17.4	26.0

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM



#16
Acenaphthylene
Concen: 0.39 ng
RT: 13.964 min Scan# 1159
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55


Tgt Ion:	152	Resp:	82631
Ion Ratio	Lower	Upper	
152	100		
151	19.6	15.5	23.3
153	13.0	10.4	15.6





#17
Acenaphthene
Concen: 0.37 ng
RT: 14.307 min Scan# 1186
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Tgt Ion:154 Resp: 53338
Ion Ratio Lower Upper
154 100
153 113.1 90.1 135.1
152 54.2 43.6 65.4

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#18
Fluorene
Concen: 0.38 ng
RT: 15.296 min Scan# 1264
Delta R.T. -0.013 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:166 Resp: 65388
Ion Ratio Lower Upper
166 100
165 97.1 78.1 117.1
167 13.6 10.7 16.1







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.005 min Scan# 1402
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:188 Resp: 92654
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.1 5.8 8.8




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.31 ng
RT: 15.385 min Scan# 1271
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:198 Resp: 2691
Ion Ratio Lower Upper
198 100
182 15.2 26.2 39.2#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.202 min Scan# 1336
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:248 Resp: 23013
Ion Ratio Lower Upper
248 100
250 99.3 76.2 114.4
141 44.1 45.6 68.4#



#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.311 min Scan# 1345
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:284 Resp: 24788
Ion Ratio Lower Upper
284 100
142 31.4 25.8 38.6
249 28.8 23.3 34.9



Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS


Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:48 PM

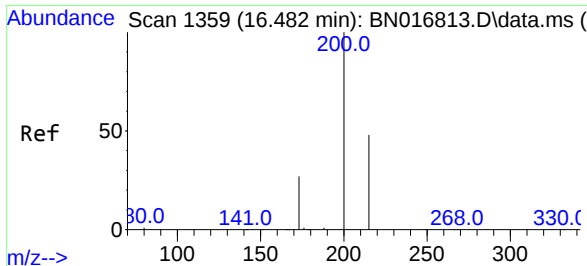

#23
Atrazine
Concen: 0.39 ng
RT: 16.482 min Scan# 1359
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Tgt Ion:200 Resp: 17811
Ion Ratio Lower Upper
200 100
173 24.5 20.1 30.1
215 49.5 38.8 58.2

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#24
Pentachlorophenol
Concen: 0.25 ng
RT: 16.652 min Scan# 1373
Delta R.T. -0.012 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55



Tgt Ion:266 Resp: 4641
Ion Ratio Lower Upper
266 100
264 62.9 49.3 73.9
268 63.9 51.8 77.8





#25
Phenanthrene
Concen: 0.41 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:178 Resp: 112824

Ion	Ratio	Lower	Upper
178	100		
176	18.7	15.0	22.6
179	15.7	12.4	18.6

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED




mohammad
10/11/2021 2:09:48 PM




#26
Anthracene
Concen: 0.40 ng
RT: 17.127 min Scan# 1412
Delta R.T. -0.012 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:178 Resp: 98690

Ion	Ratio	Lower	Upper
178	100		
176	18.1	14.5	21.7
179	14.8	12.2	18.4









#27
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.043 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion: 212 Resp: 87395
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.8 8.8

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM



#28
Fluoranthene
Concen: 0.44 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion: 202 Resp: 134878
Ion Ratio Lower Upper
202 100
101 10.9 8.9 13.3
203 17.1 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.011 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:240 Resp: 91756
Ion Ratio Lower Upper
240 100
120 11.9 6.6 10.0#
236 26.3 20.7 31.1

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:48 PM




#30
Pyrene
Concen: 0.49 ng
RT: 19.435 min Scan# 1771
Delta R.T. -0.005 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55

Tgt Ion:202 Resp: 137103
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 18.2 13.9 20.9






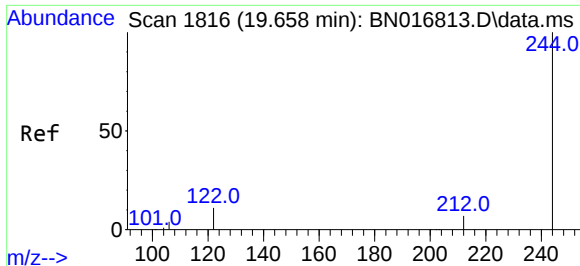


#31
Terphenyl-d14
Concen: 0.33 ng
RT: 19.653 min Scan# 1815
Delta R.T. -0.005 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:244 Resp: 65567
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 12.2 8.9 13.3

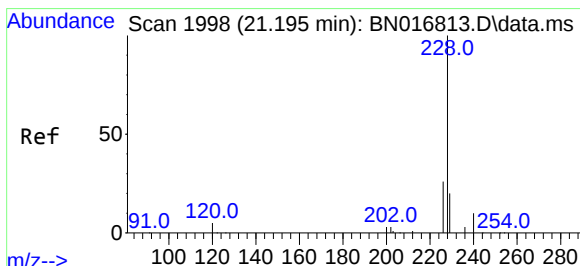

#32
Benzo(a)anthracene
Concen: 0.45 ng
RT: 21.195 min Scan# 1998
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:228 Resp: 126305
Ion Ratio Lower Upper
228 100
226 26.4 22.3 33.5
229 20.1 15.4 23.0




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED




mohammad
10/11/2021 2:09:48 PM




#33
Chrysene
Concen: 0.43 ng
RT: 21.248 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:228 Resp: 125121
Ion Ratio Lower Upper
228 100
226 28.7 24.2 36.4
229 20.4 15.4 23.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 6.71 ng
RT: 21.142 min Scan# 1993
Delta R.T. -0.011 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:149 Resp: 967070
Ion Ratio Lower Upper
149 100
167 27.9 22.2 33.4
279 4.3 3.4 5.2



Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS


Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:48 PM



#35
Perylene-d12
Concen: 0.40 ng
RT: 23.450 min Scan# 2417
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS




Tgt Ion:264 Resp: 103737
Ion Ratio Lower Upper
264 100
260 24.6 19.8 29.6
265 23.6 20.3 30.5

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.43 ng
RT: 25.712 min Scan# 3078
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:276 Resp: 168105
Ion Ratio Lower Upper
276 100
138 24.4 19.2 28.8
277 24.8 20.0 30.0









#37
Benzo(b)fluoranthene
Concen: 0.44 ng
RT: 22.776 min Scan# 2220
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:252 Resp: 143857
Ion Ratio Lower Upper
252 100
253 22.5 17.8 26.8
125 11.1 8.3 12.5

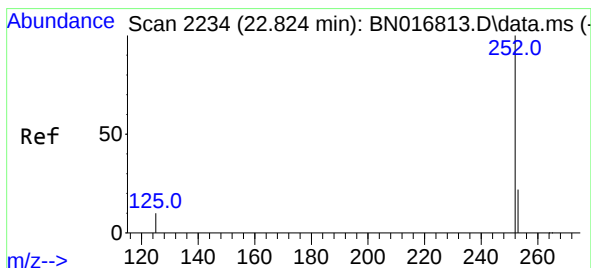

#38
Benzo(k)fluoranthene
Concen: 0.41 ng
RT: 22.820 min Scan# 2233
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:252 Resp: 129953
Ion Ratio Lower Upper
252 100
253 22.7 17.8 26.8
125 13.1 8.5 12.7#




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED




mohammad
10/11/2021 2:09:48 PM




#39
Benzo(a)pyrene
Concen: 0.45 ng
RT: 23.351 min Scan# 2388
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55





Tgt Ion:252 Resp: 134924
Ion Ratio Lower Upper
252 100
253 22.6 17.9 26.9
125 12.2 9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 0.42 ng
RT: 25.733 min Scan# 3084
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55




Tgt Ion:278 Resp: 134980
Ion Ratio Lower Upper
278 100
139 16.7 13.1 19.7
279 23.8 19.3 28.9




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:48 PM



#41
Benzo(g,h,i)perylene
Concen: 0.43 ng
RT: 26.404 min Scan# 3280
Delta R.T. -0.003 min
Lab File: BN016823.D
Acq: 08 Oct 2021 00:55



Tgt Ion: 276 Resp: 145801
Ion Ratio Lower Upper
276 100
277 23.9 19.0 28.4
138 21.0 17.0 25.6



Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MS

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:48 PM