

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016824.D
 Acq On : 08 Oct 2021 01:31
 Operator : CG/JU
 Sample : M4020-14MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 S-820-N-SO-1-1.5-093021MSD

Manual Integrations
 APPROVED

mohammad
 10/11/2021 2:09:50 PM

Quant Time: Oct 08 05:20:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 01:39:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.615	152	20656	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	95279	0.40	ng	# 0.00
13) Acenaphthene-d10	14.243	164	50030	0.40	ng	0.00
19) Phenanthrene-d10	17.005	188	95028	0.40	ng	0.00
29) Chrysene-d12	21.206	240	91134	0.40	ng	#-0.01
35) Perylene-d12	23.450	264	103237	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.263	112	17732	0.34	ng	0.04
5) Phenol-d6	6.812	99	19555	0.33	ng	0.02
8) Nitrobenzene-d5	8.759	82	20967	0.31	ng	0.00
11) 2-Methylnaphthalene-d10	11.976	152	52647	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	7364	0.28	ng	0.00
15) 2-Fluorobiphenyl	12.873	172	59979	0.30	ng	0.00
27) Fluoranthene-d10	19.043	212	88464	0.34	ng	0.00
31) Terphenyl-d14	19.654	244	66276	0.33	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	6319m	0.68	ng	
3) n-Nitrosodimethylamine	3.558	42	6860	0.42	ng	# 95
6) bis(2-Chloroethyl)ether	7.052	93	23715	0.42	ng	100
9) Naphthalene	10.432	128	99119	0.38	ng	100
10) Hexachlorobutadiene	10.723	225	18209	0.37	ng	# 100
12) 2-Methylnaphthalene	12.052	142	65170	0.39	ng	100
16) Acenaphthylene	13.964	152	85945	0.39	ng	100
17) Acenaphthene	14.307	154	55534	0.38	ng	99
18) Fluorene	15.296	166	67774	0.38	ng	100
20) 4,6-Dinitro-2-methylph...	15.385	198	2894	0.32	ng	# 69
21) 4-Bromophenyl-phenylether	16.202	248	23618	0.40	ng	93
22) Hexachlorobenzene	16.312	284	25163	0.37	ng	100
23) Atrazine	16.482	200	18201	0.39	ng	99
24) Pentachlorophenol	16.652	266	4610	0.25	ng	99
25) Phenanthrene	17.042	178	116071	0.41	ng	100
26) Anthracene	17.127	178	101032	0.40	ng	99
28) Fluoranthene	19.073	202	136003	0.43	ng	100
30) Pyrene	19.435	202	137897	0.49	ng	99
32) Benzo(a)anthracene	21.195	228	128019	0.45	ng	97
33) Chrysene	21.249	228	125510	0.44	ng	98
34) Bis(2-ethylhexyl)phtha...	21.142	149	950511	6.64	ng	100
36) Indeno(1,2,3-cd)pyrene	25.713	276	166434	0.43	ng	100
37) Benzo(b)fluoranthene	22.776	252	143017	0.44	ng	99
38) Benzo(k)fluoranthene	22.820	252	129733	0.41	ng	# 98
39) Benzo(a)pyrene	23.351	252	134908	0.45	ng	99
40) Dibenzo(a,h)anthracene	25.733	278	134112	0.42	ng	100
41) Benzo(g,h,i)perylene	26.401	276	145164	0.43	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016824.D
Acq On : 08 Oct 2021 01:31
Operator : CG/JU
Sample : M4020-14MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

Quant Time: Oct 08 05:20:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 01:39:08 2021
Response via : Initial Calibration



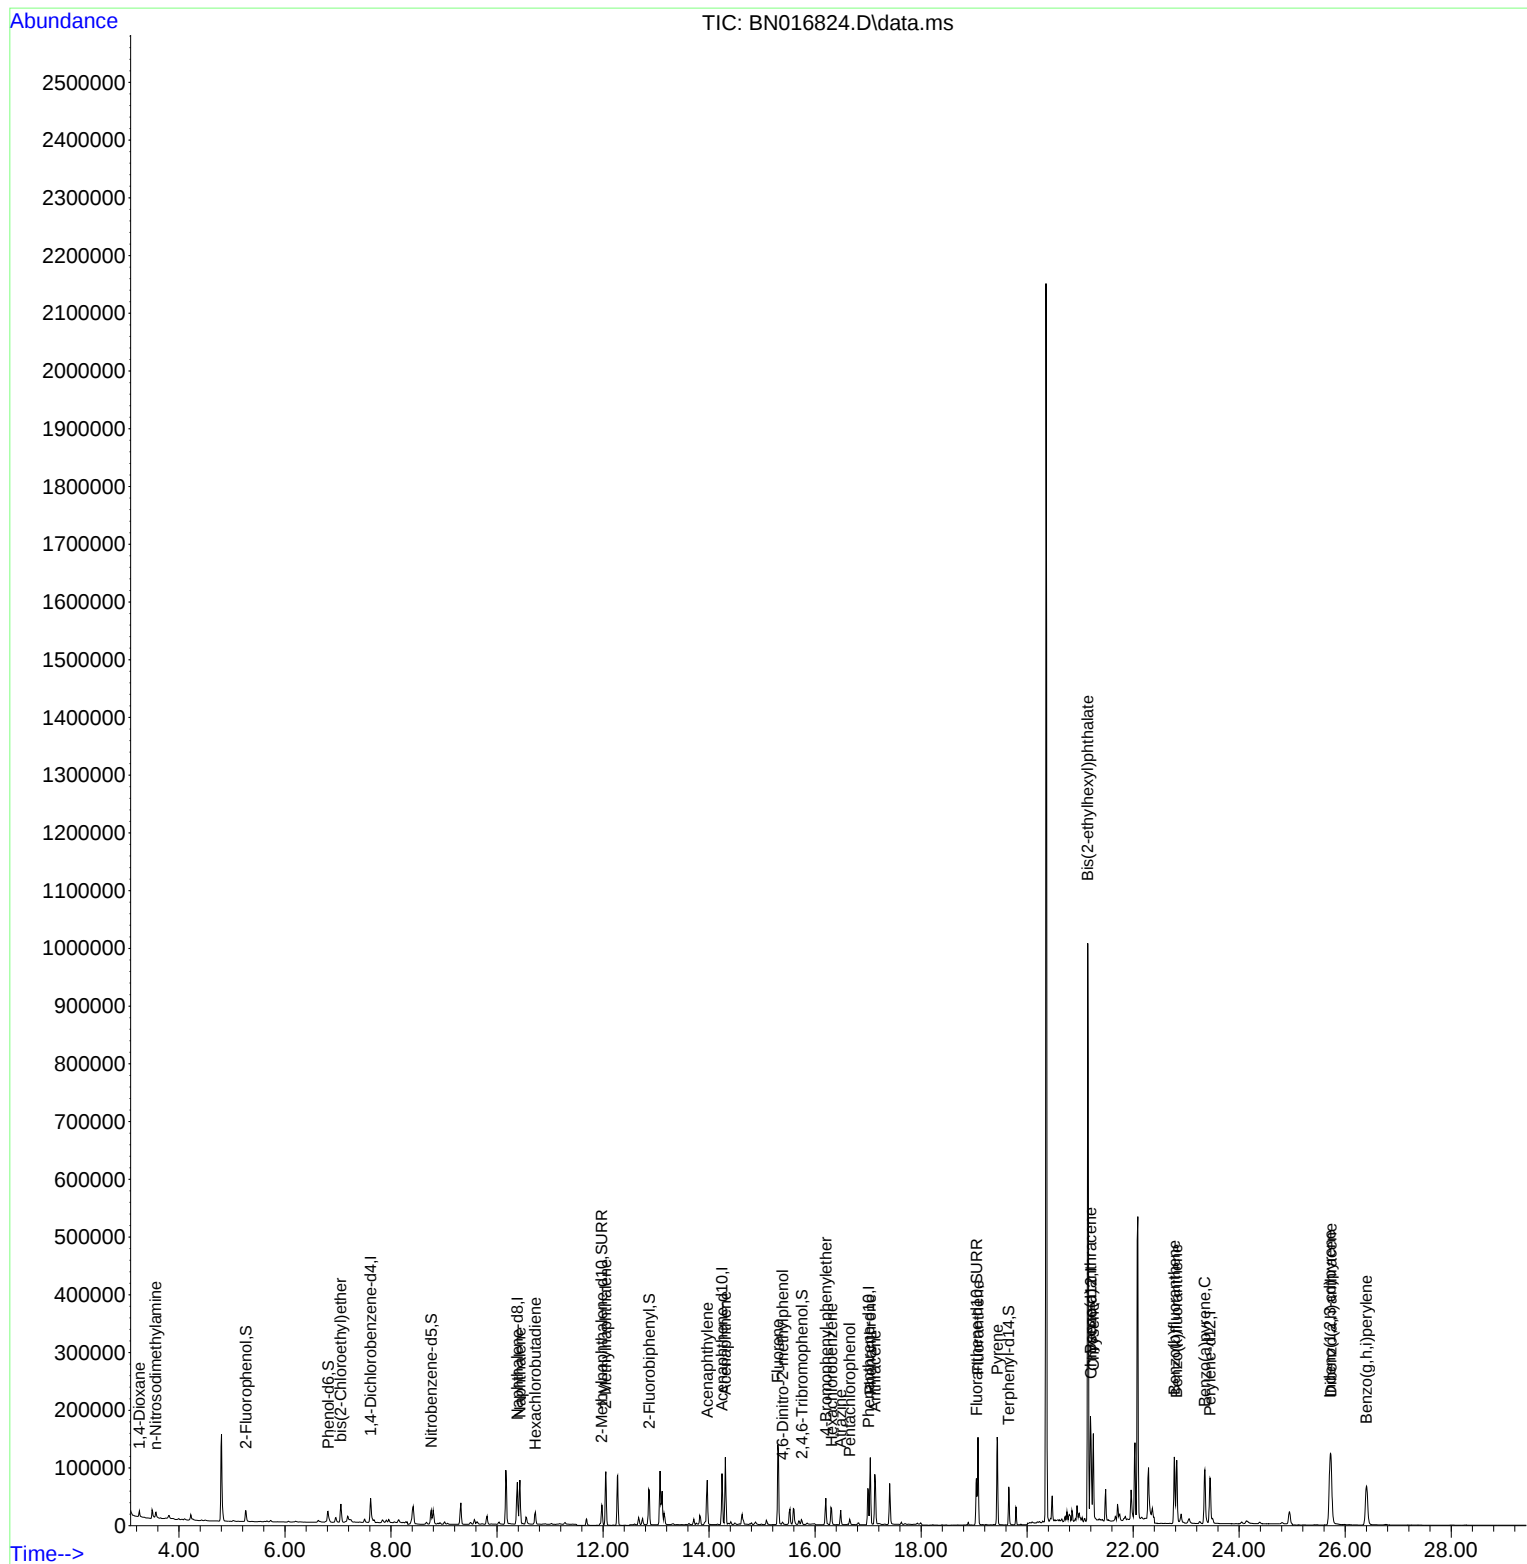





#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.615 min Scan# 492
Delta R.T. 0.001 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

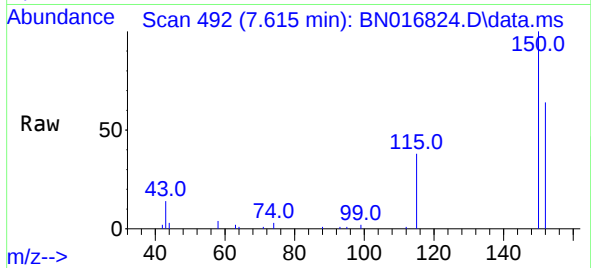



Tgt Ion: 152 Resp: 20656
Ion Ratio Lower Upper
152 100
150 156.9 123.3 184.9
115 59.8 47.0 70.6

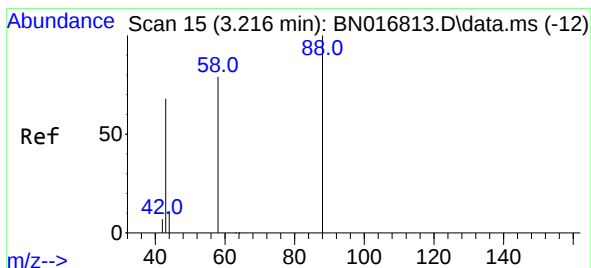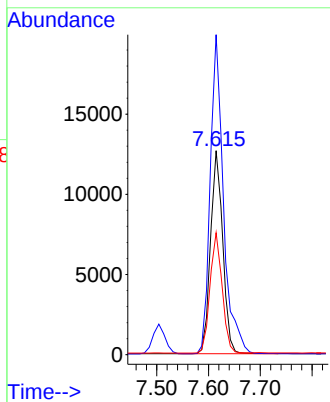

#2
1,4-Dioxane
Concen: 0.68 ng m
RT: 3.253 min Scan# 19
Delta R.T. 0.037 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

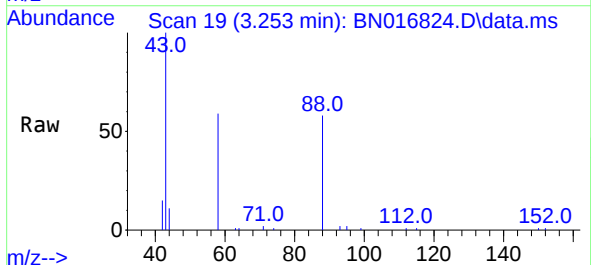


Tgt Ion: 88 Resp: 6319
Ion Ratio Lower Upper
88 100
43 0.0 61.7 92.5#
58 0.0 62.2 93.2#

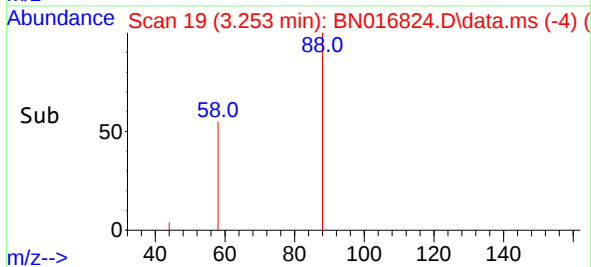

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM







#3
n-Nitrosodimethylamine
Concen: 0.42 ng
RT: 3.558 min Scan# 52
Delta R.T. 0.009 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion: 42 Resp: 6860
Ion Ratio Lower Upper
42 100
74 161.0 124.0 186.0
44 0.0 5.6 8.4#

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

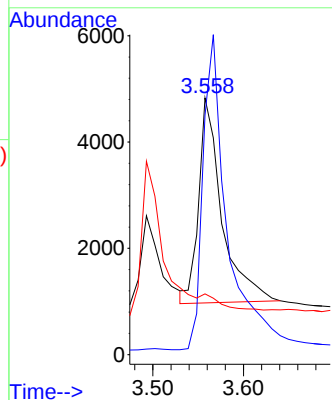

#4
2-Fluorophenol
Concen: 0.34 ng
RT: 5.263 min Scan# 237
Delta R.T. 0.037 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion: 112 Resp: 17732
Ion Ratio Lower Upper
112 100
64 54.4 42.9 64.3
63 28.1 21.5 32.3

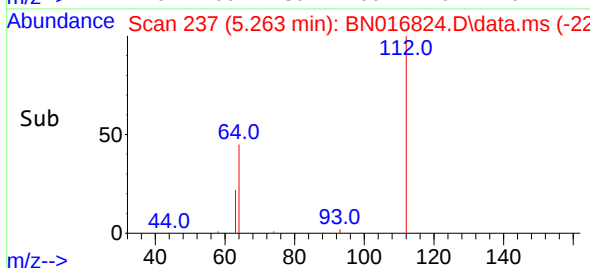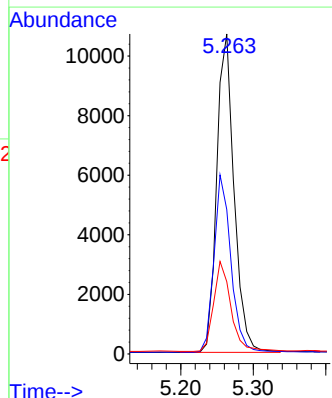

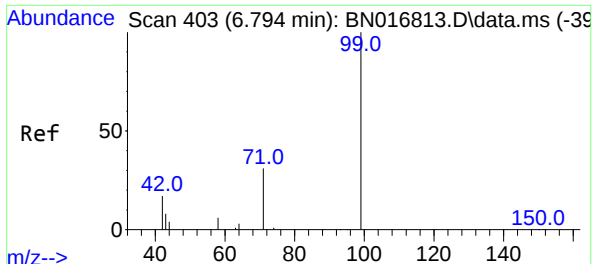





#5
Phenol-d6
Concen: 0.33 ng
RT: 6.812 min Scan# 405
Delta R.T. 0.019 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion: 99 Resp: 19555
Ion Ratio Lower Upper
99 100
42 17.4 13.4 20.2
71 31.5 24.0 36.0

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

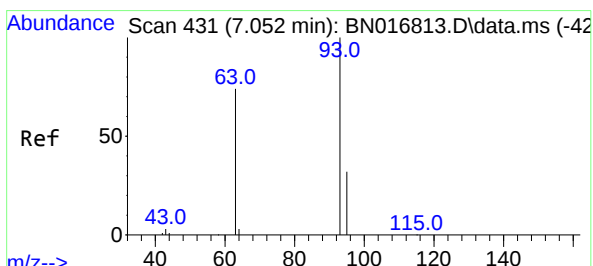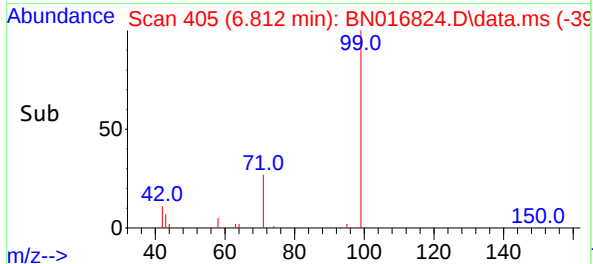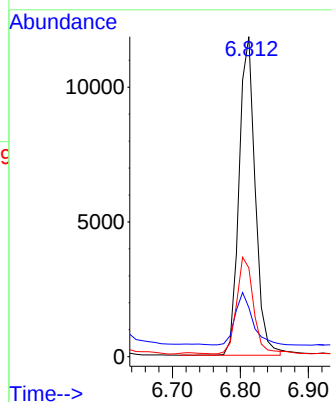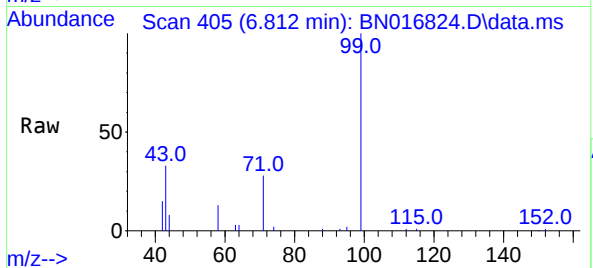

#6
bis(2-Chloroethyl)ether
Concen: 0.42 ng
RT: 7.052 min Scan# 431
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31


Tgt Ion: 93 Resp: 23715
Ion Ratio Lower Upper
93 100
63 73.8 59.0 88.6
95 32.2 26.4 39.6

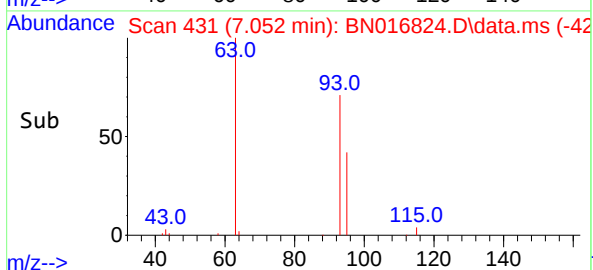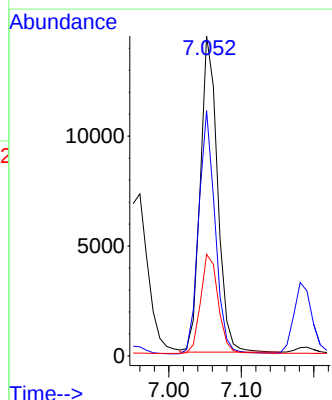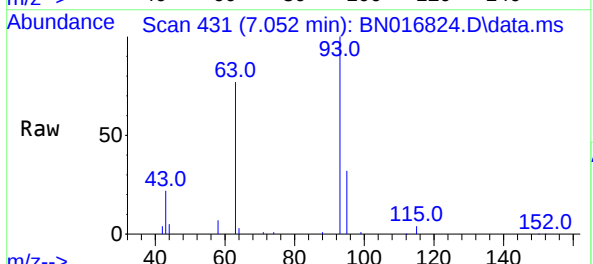



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Tgt Ion: 136 Resp: 95279
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 5.9 6.5 9.7#
68 5.2 5.3 7.9#

Manual Integrations
APPROVED



mohammad
10/11/2021 2:09:50 PM

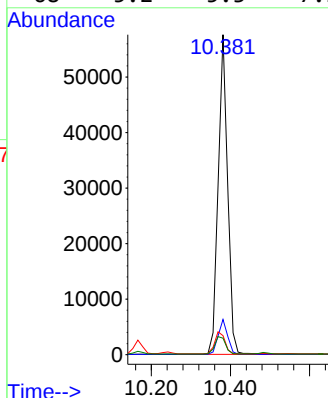


#8
Nitrobenzene-d5
Concen: 0.31 ng
RT: 8.759 min Scan# 603
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31



Tgt Ion: 82 Resp: 20967
Ion Ratio Lower Upper
82 100
128 48.2 33.8 50.6
54 43.5 38.5 57.7

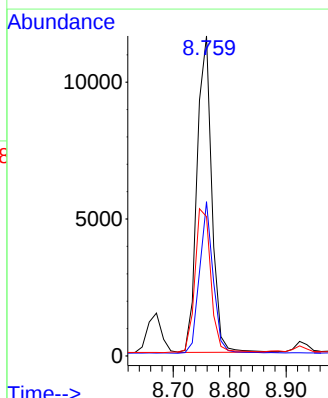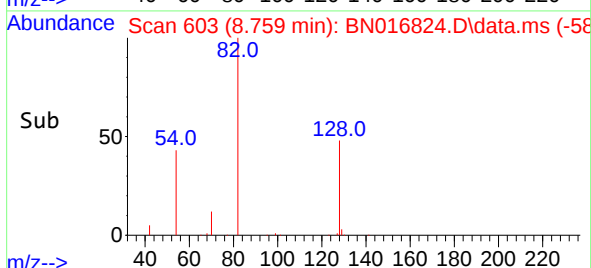







#9
Naphthalene
Concen: 0.38 ng
RT: 10.432 min Scan# 735
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	128	Resp:	99119
Ion Ratio	Lower	Upper	
128	100		
129	11.1	8.7	13.1
127	12.8	10.3	15.5

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM



#10
Hexachlorobutadiene
Concen: 0.37 ng
RT: 10.723 min Scan# 758
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	225	Resp:	18209
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.2	51.1	76.7

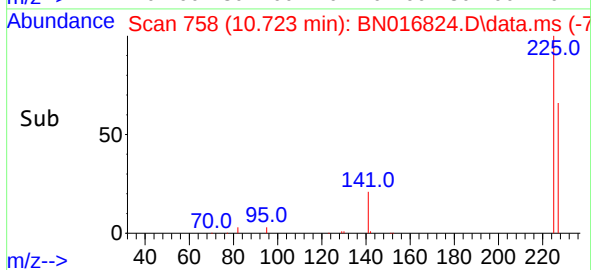

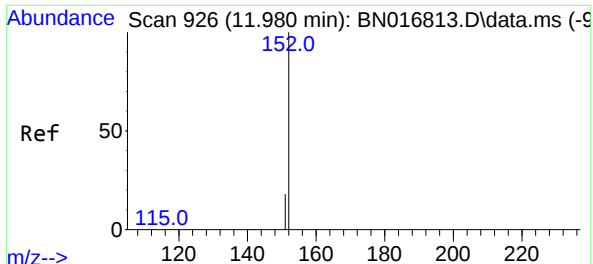





#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 11.976 min Scan# 925
Delta R.T. -0.004 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:152 Resp: 52647
Ion Ratio Lower Upper
152 100
151 18.7 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

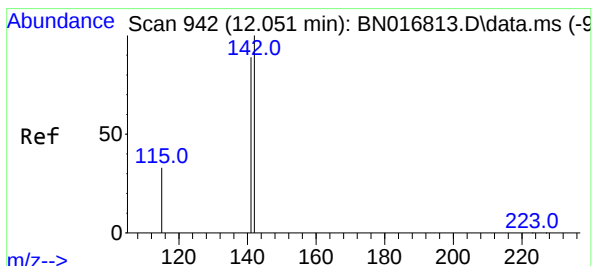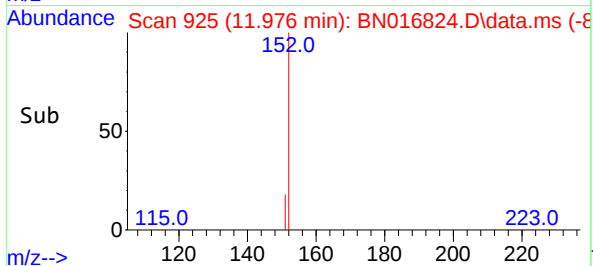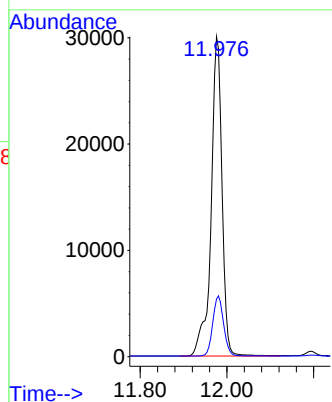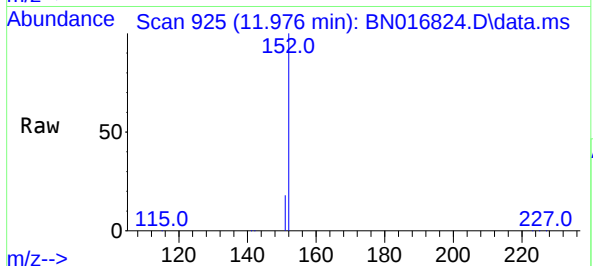

#12
2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.052 min Scan# 942
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31


Tgt Ion:142 Resp: 65170
Ion Ratio Lower Upper
142 100
141 88.5 70.6 106.0
115 32.7 26.1 39.1

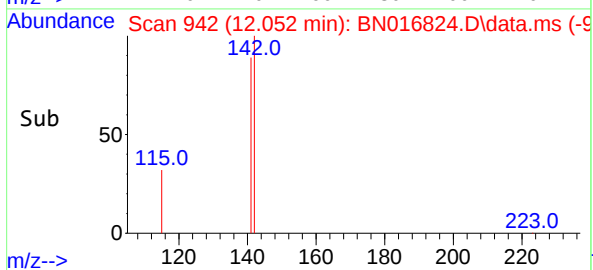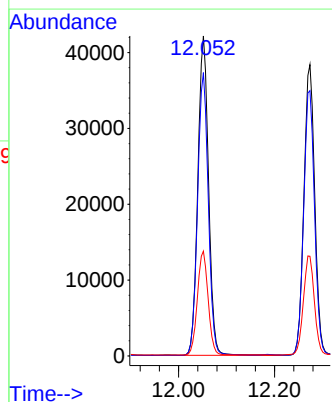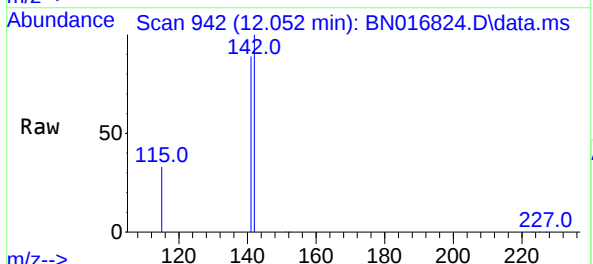



#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.243 min Scan# 1181
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31




Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

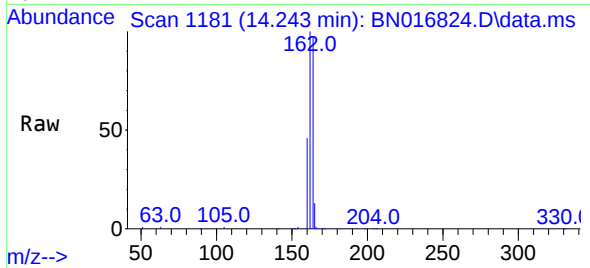

Tgt Ion:164 Resp: 50030
Ion Ratio Lower Upper
164 100
162 102.6 82.6 124.0
160 46.7 38.2 57.2




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

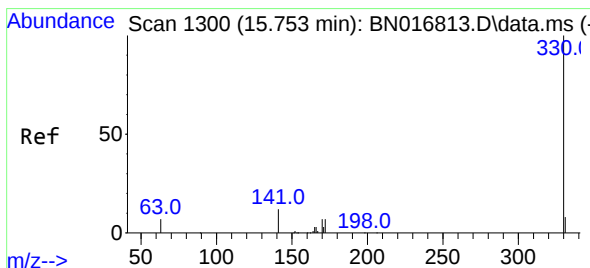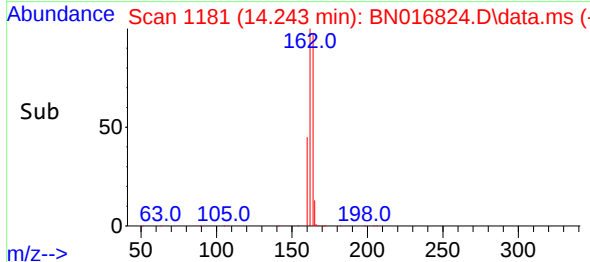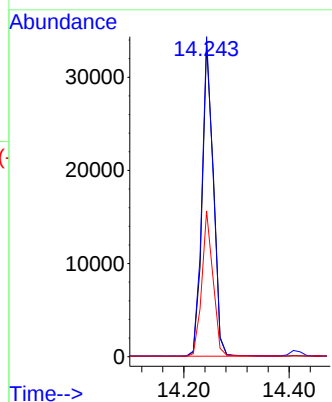

#14
2,4,6-Tribromophenol
Concen: 0.28 ng
RT: 15.753 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:330 Resp: 7364
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.7 24.2 36.2

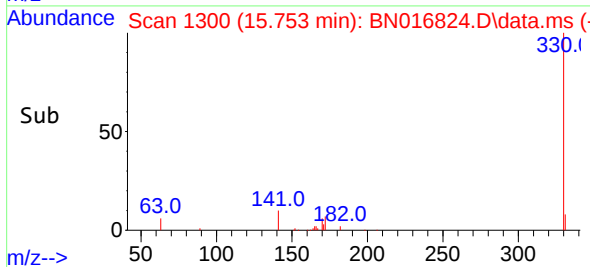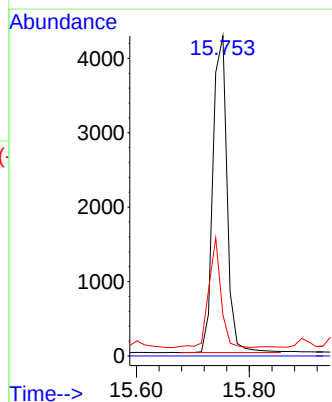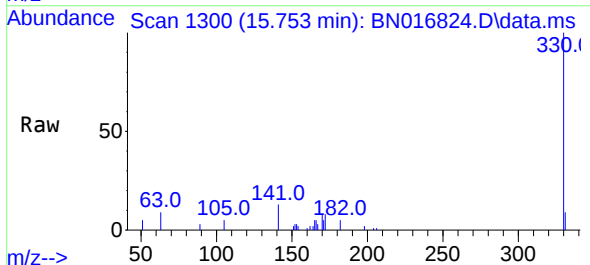







#15
2-Fluorobiphenyl
Concen: 0.30 ng
RT: 12.873 min Scan# 1073
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	172	Resp:	59979
Ion Ratio	Lower	Upper	
172	100		
171	33.6	26.9	40.3
170	21.4	17.4	26.0

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

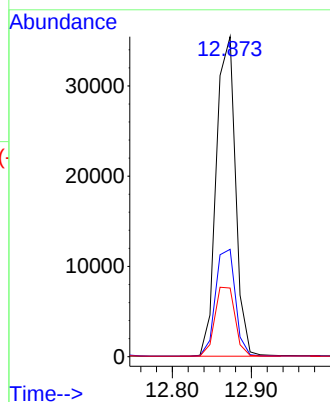


#16
Acenaphthylene
Concen: 0.39 ng
RT: 13.964 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	152	Resp:	85945
Ion Ratio	Lower	Upper	
152	100		
151	19.7	15.5	23.3
153	13.0	10.4	15.6

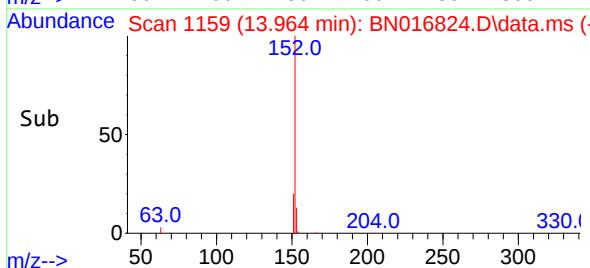







#17
Acenaphthene
Concen: 0.38 ng
RT: 14.307 min Scan# 1186
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

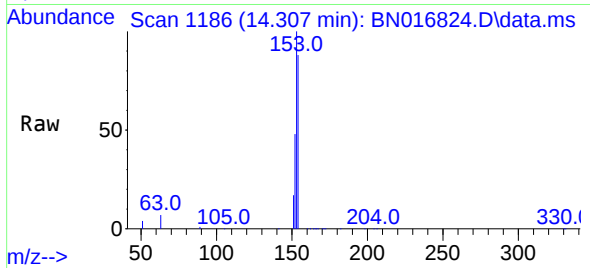



Tgt Ion:154 Resp: 55534
Ion Ratio Lower Upper
154 100
153 113.0 90.1 135.1
152 53.6 43.6 65.4

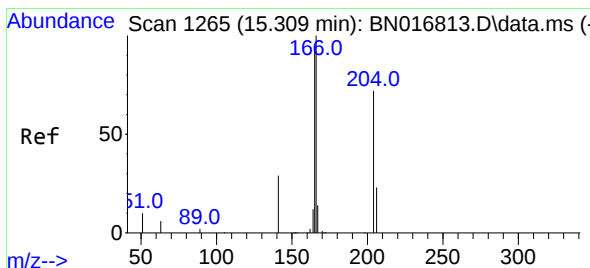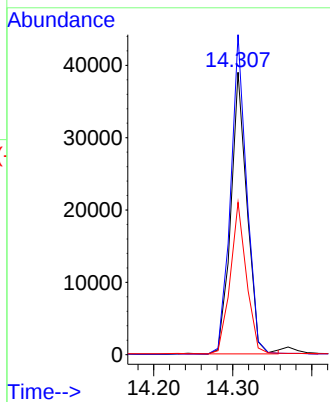

#18
Fluorene
Concen: 0.38 ng
RT: 15.296 min Scan# 1264
Delta R.T. -0.013 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

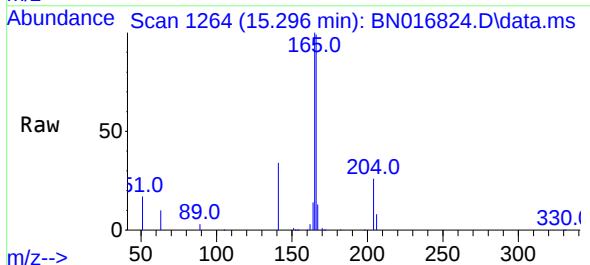


Tgt Ion:166 Resp: 67774
Ion Ratio Lower Upper
166 100
165 97.6 78.1 117.1
167 13.5 10.7 16.1

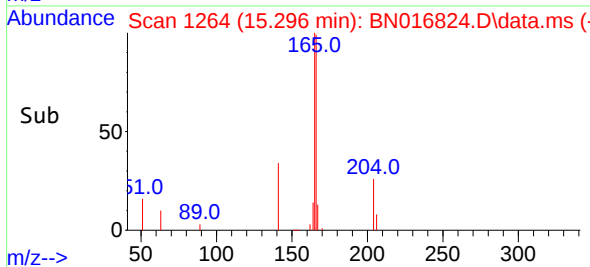

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.005 min Scan# 1402
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	188	Resp:	95028
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	6.0	5.8	8.8

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM



#20
4,6-Dinitro-2-methylphenol
Concen: 0.32 ng
RT: 15.385 min Scan# 1271
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	198	Resp:	2894
Ion Ratio	Lower	Upper	
198	100		
182	15.2	26.2	39.2#
77	0.0	0.0	0.0

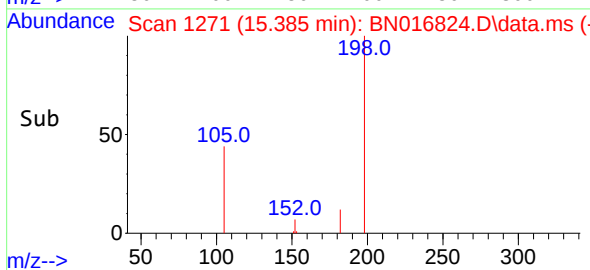







#21
4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.202 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	248	Resp:	23618
Ion Ratio	Lower	Upper	
248	100		
250	98.8	76.2	114.4
141	47.3	45.6	68.4

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

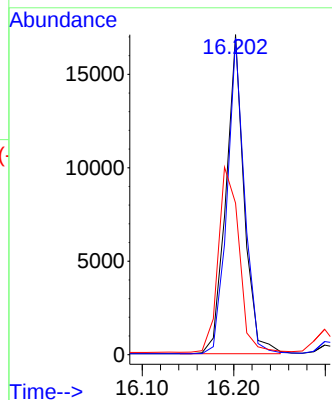


#22
Hexachlorobenzene
Concen: 0.37 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	284	Resp:	25163
Ion Ratio	Lower	Upper	
284	100		
142	32.0	25.8	38.6
249	29.1	23.3	34.9

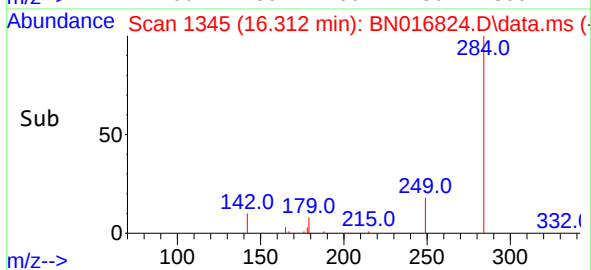
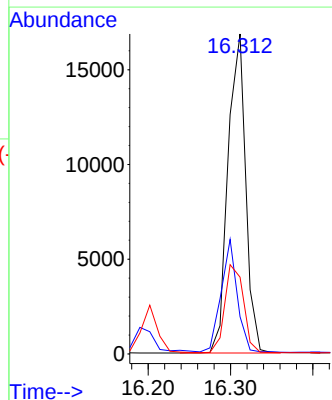



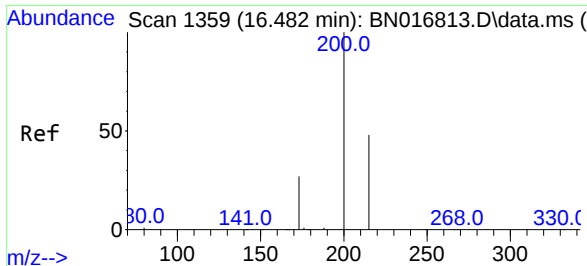


#23
Atrazine
Concen: 0.39 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

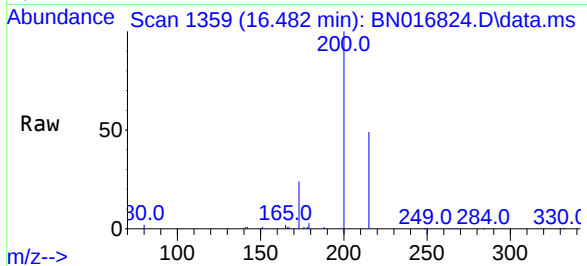



Tgt Ion:	200	Resp:	18201
Ion Ratio	Lower	Upper	
200	100		
173	24.4	20.1	30.1
215	49.1	38.8	58.2

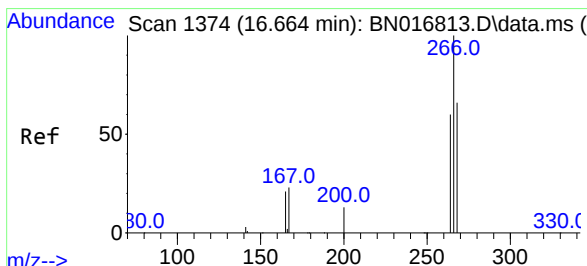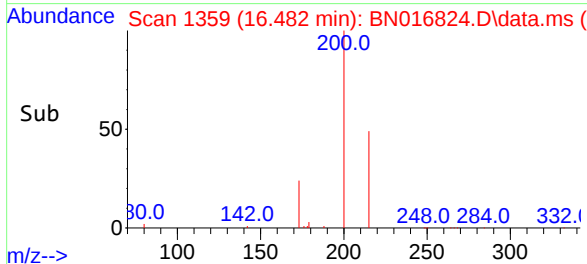

#24
Pentachlorophenol
Concen: 0.25 ng
RT: 16.652 min Scan# 1373
Delta R.T. -0.012 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

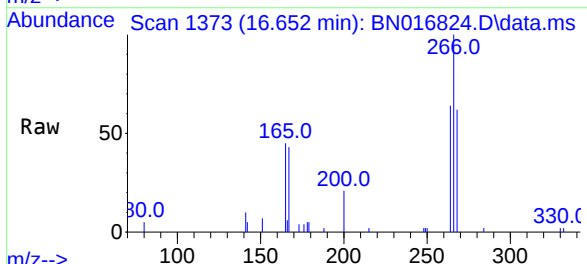


Tgt Ion:	266	Resp:	4610
Ion Ratio	Lower	Upper	
266	100		
264	62.5	49.3	73.9
268	63.5	51.8	77.8

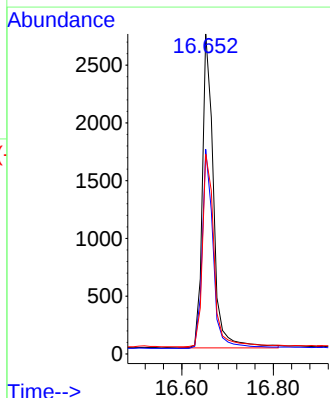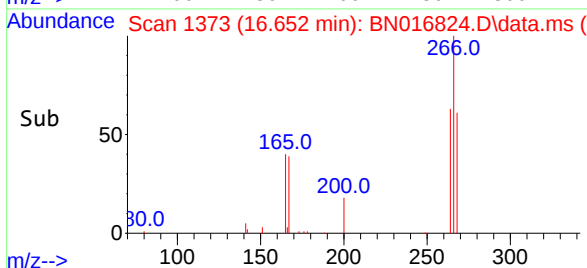

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM







#25
Phenanthrene
Concen: 0.41 ng
RT: 17.042 min Scan# 1405
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:178 Resp: 116071
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.6
179 15.8 12.4 18.6

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM



#26
Anthracene
Concen: 0.40 ng
RT: 17.127 min Scan# 1412
Delta R.T. -0.012 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:178 Resp: 101032
Ion Ratio Lower Upper
178 100
176 18.2 14.5 21.7
179 14.9 12.2 18.4

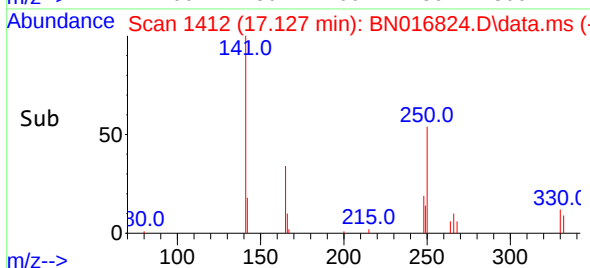







#27
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.043 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:212 Resp: 88464
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.3 5.8 8.8

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

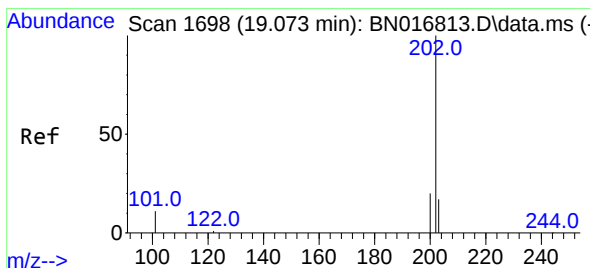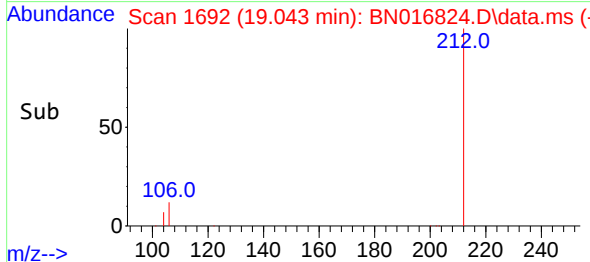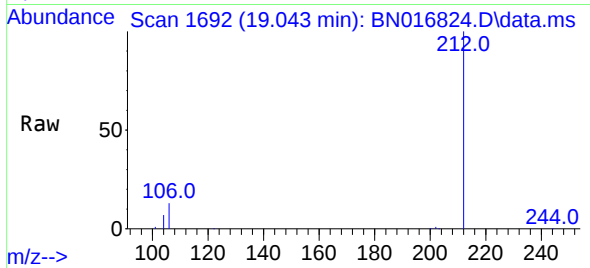

#28
Fluoranthene
Concen: 0.43 ng
RT: 19.073 min Scan# 1698
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:202 Resp: 136003
Ion Ratio Lower Upper
202 100
101 10.9 8.9 13.3
203 17.1 13.8 20.8

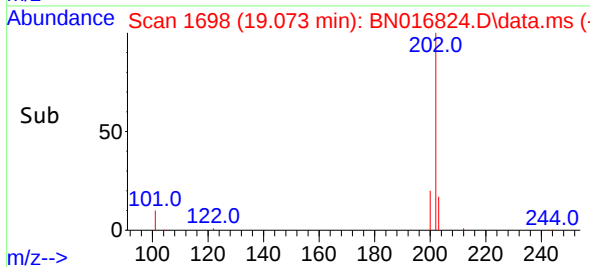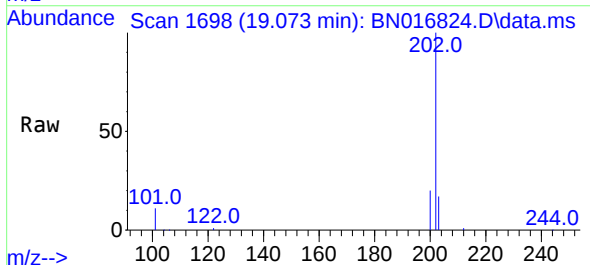







#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.011 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:240 Resp: 91134
Ion Ratio Lower Upper
240 100
120 12.6 6.6 10.0#
236 26.5 20.7 31.1

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM




#30
Pyrene
Concen: 0.49 ng
RT: 19.435 min Scan# 1771
Delta R.T. -0.005 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:202 Resp: 137897
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 18.2 13.9 20.9

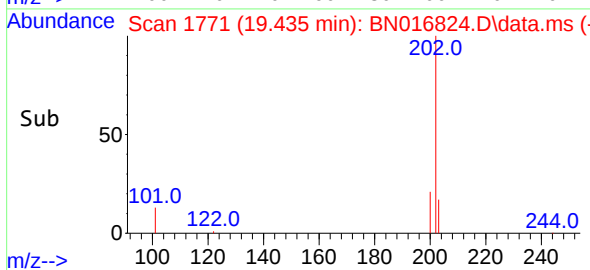




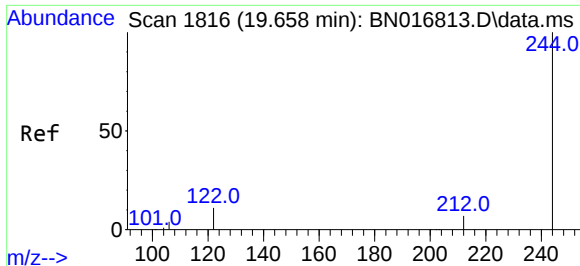


#31
Terphenyl-d14
Concen: 0.33 ng
RT: 19.654 min Scan# 1815
Delta R.T. -0.005 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

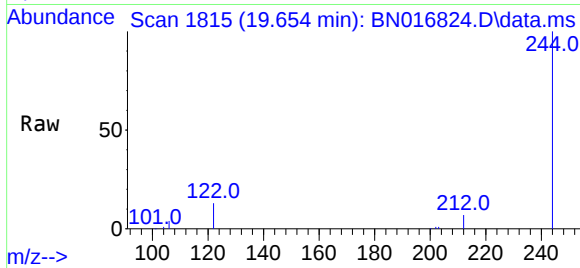



Tgt Ion:244 Resp: 66276
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.6
122 12.9 8.9 13.3

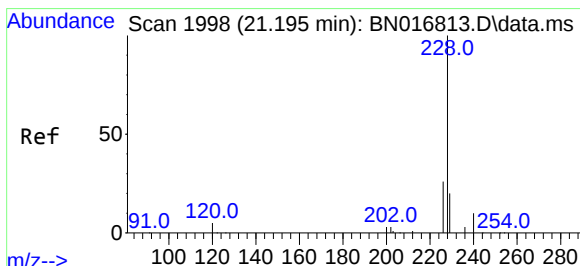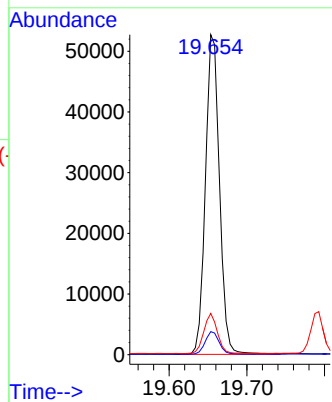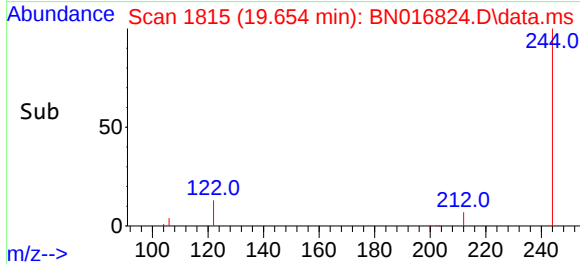

#32
Benzo(a)anthracene
Concen: 0.45 ng
RT: 21.195 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

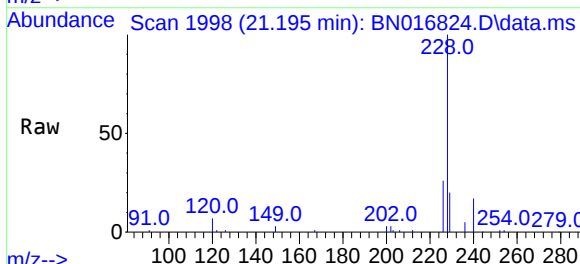


Tgt Ion:228 Resp: 128019
Ion Ratio Lower Upper
228 100
226 26.2 22.3 33.5
229 20.3 15.4 23.0

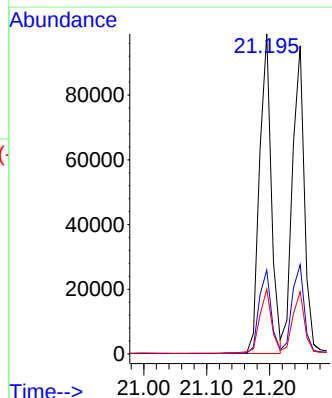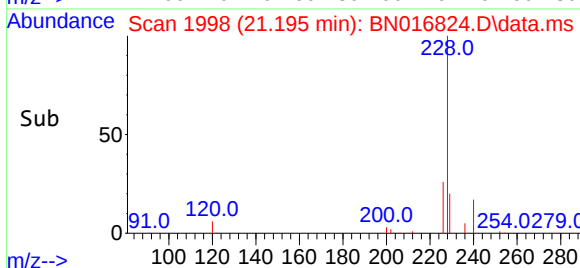

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM







#33
Chrysene
Concen: 0.44 ng
RT: 21.249 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:228 Resp: 125510
Ion Ratio Lower Upper
228 100
226 29.0 24.2 36.4
229 20.2 15.4 23.0

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

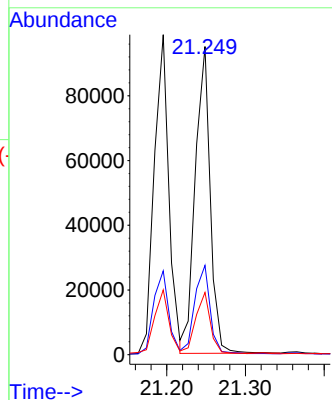


#34
Bis(2-ethylhexyl)phthalate
Concen: 6.64 ng
RT: 21.142 min Scan# 1993
Delta R.T. -0.011 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:149 Resp: 950511
Ion Ratio Lower Upper
149 100
167 27.9 22.2 33.4
279 4.4 3.4 5.2

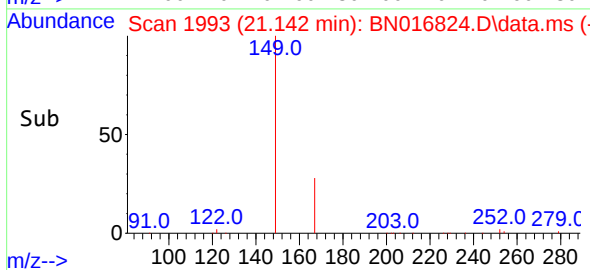
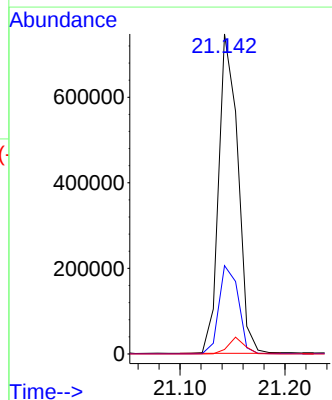






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.450 min Scan# 2417
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

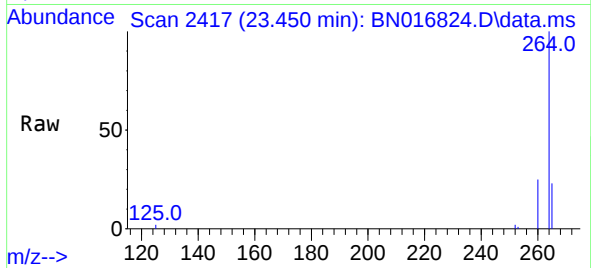



Tgt Ion:264 Resp: 103237
Ion Ratio Lower Upper
264 100
260 24.6 19.8 29.6
265 23.5 20.3 30.5

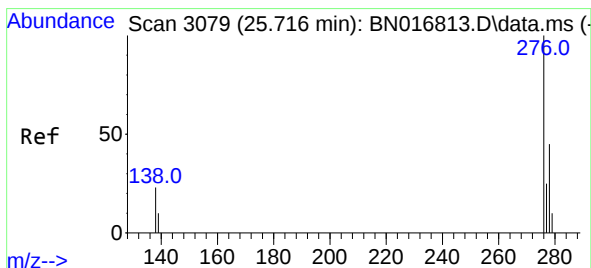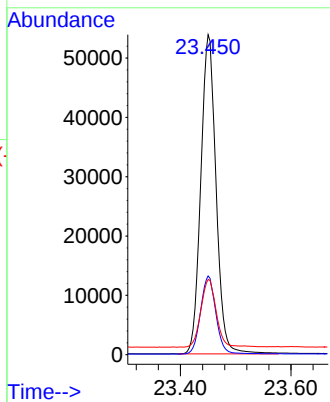

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.43 ng
RT: 25.713 min Scan# 3078
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

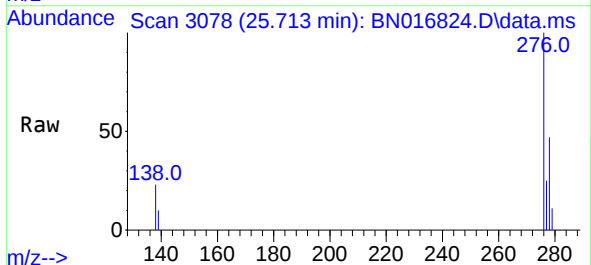


Tgt Ion:276 Resp: 166434
Ion Ratio Lower Upper
276 100
138 24.2 19.2 28.8
277 25.0 20.0 30.0

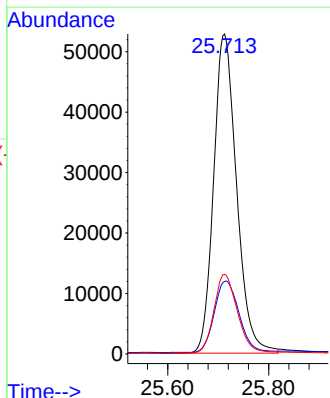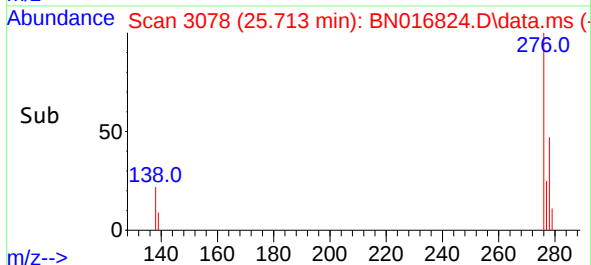


Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED




mohammad
10/11/2021 2:09:50 PM




#37
Benzo(b)fluoranthene
Concen: 0.44 ng
RT: 22.776 min Scan# 2220
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

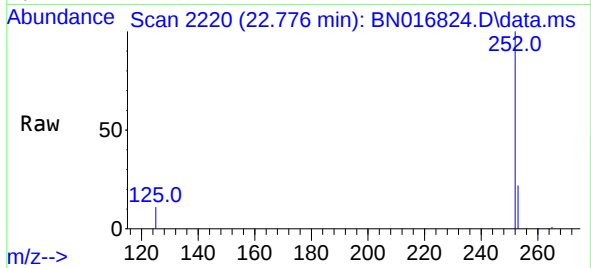



Tgt Ion:252 Resp: 143017
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.8
125 11.2 8.3 12.5

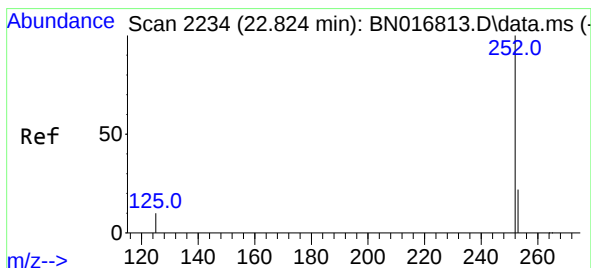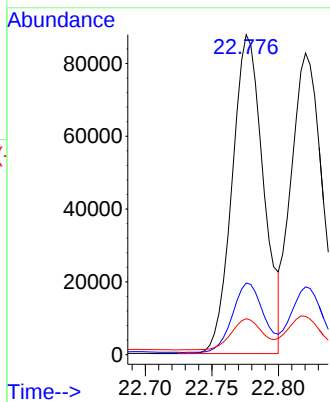

#38
Benzo(k)fluoranthene
Concen: 0.41 ng
RT: 22.820 min Scan# 2233
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

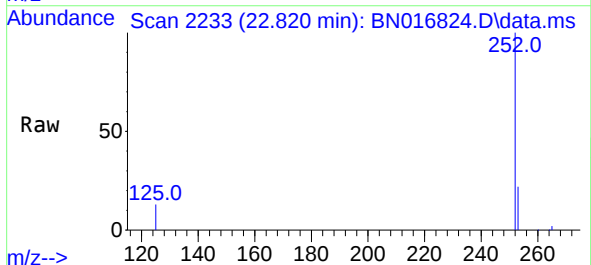


Tgt Ion:252 Resp: 129733
Ion Ratio Lower Upper
252 100
253 22.5 17.8 26.8
125 12.8 8.5 12.7#

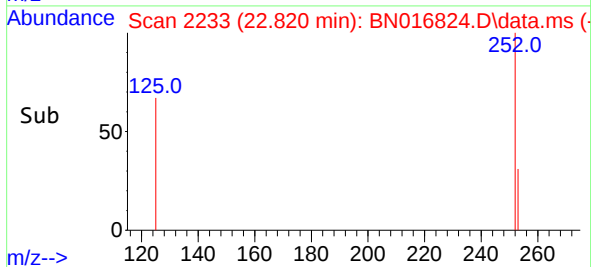

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM







#39
Benzo(a)pyrene
Concen: 0.45 ng
RT: 23.351 min Scan# 2388
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	252	Resp:	134908
Ion Ratio	Lower	Upper	
252	100		
253	22.6	17.9	26.9
125	12.2	9.4	14.2

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD




Manual Integrations
APPROVED


mohammad
10/11/2021 2:09:50 PM

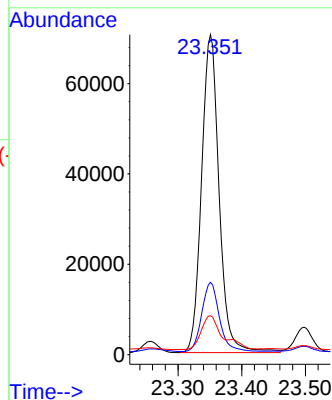

#40
Dibenzo(a,h)anthracene
Concen: 0.42 ng
RT: 25.733 min Scan# 3084
Delta R.T. -0.003 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31


Tgt Ion:	278	Resp:	134112
Ion Ratio	Lower	Upper	
278	100		
139	16.6	13.1	19.7
279	24.1	19.3	28.9

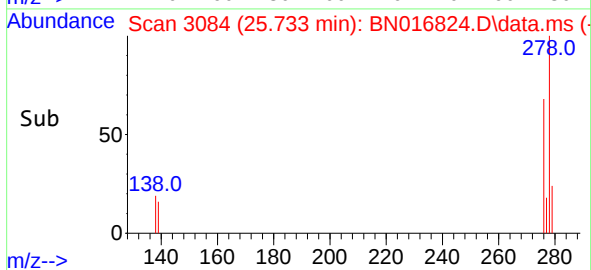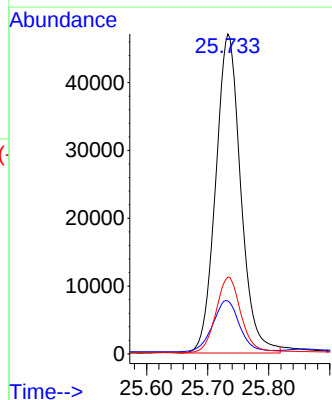

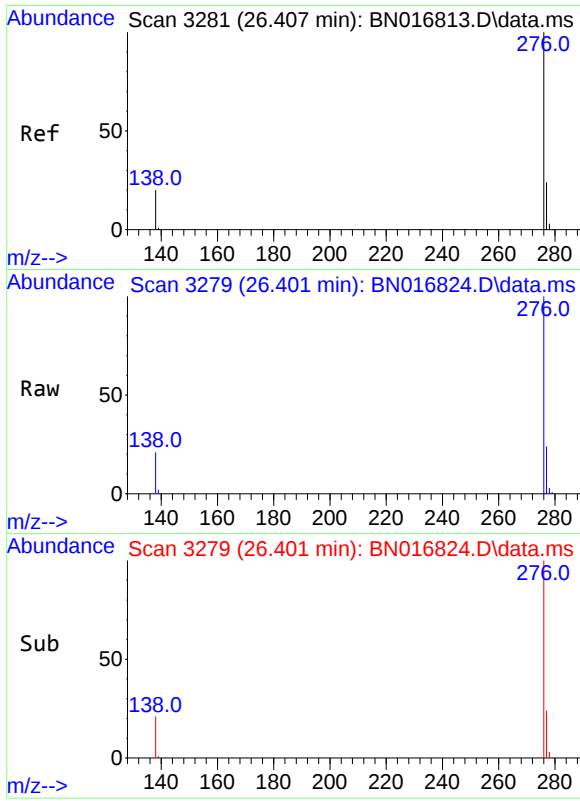

#41
Benzo(g,h,i)perylene
Concen: 0.43 ng
RT: 26.401 min Scan# 3279
Delta R.T. -0.007 min
Lab File: BN016824.D
Acq: 08 Oct 2021 01:31

Tgt Ion:	276	Resp:	145164
Ion Ratio	Lower	Upper	
276	100		
277	24.1	19.0	28.4
138	21.4	17.0	25.6

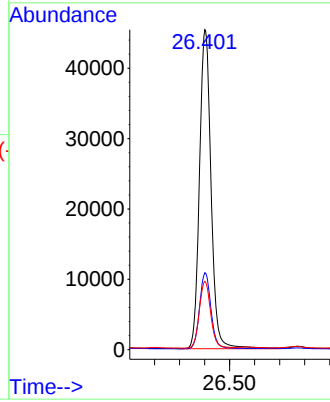

Instrument :
BNA_N
ClientSampleId :
S-820-N-SO-1-1.5-093021MSD

Manual Integrations
APPROVED

mohammad
10/11/2021 2:09:50 PM