


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
 Data File : BN016810.D
 Acq On : 07 Oct 2021 15:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 01:39:08 2021

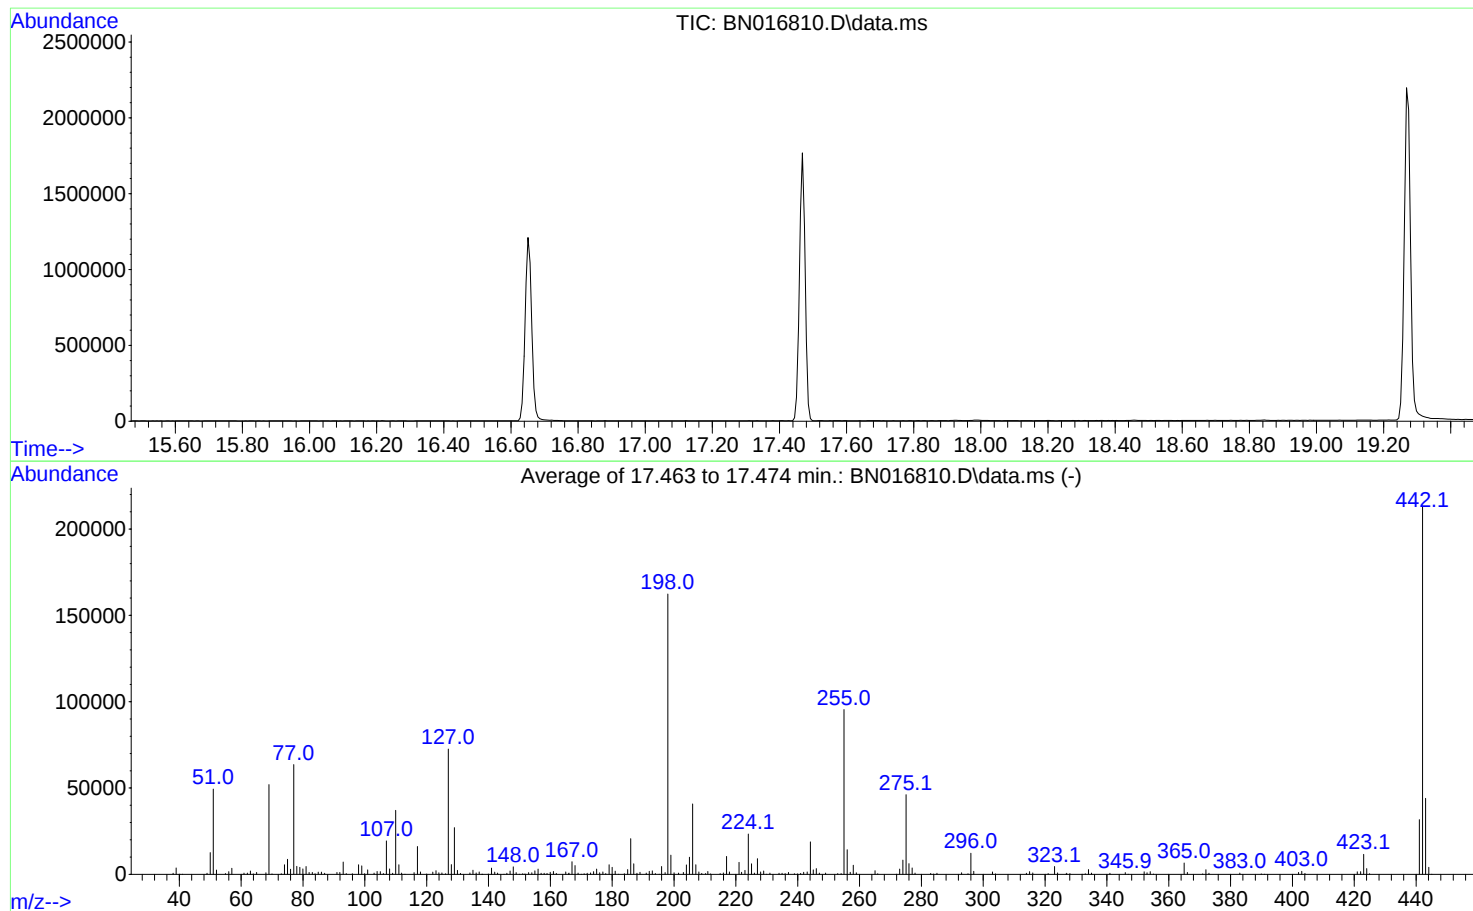




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	49387	PASS
68	69	0.00	2	1.9	971	PASS
69	198	0.00	100	32.0	51952	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	44.7	72595	PASS
197	198	0.00	2	0.6	987	PASS
198	198	100	100	100.0	162389	PASS
199	198	5	9	6.9	11159	PASS
275	198	10	60	28.4	46168	PASS
365	198	1	100	4.0	6565	PASS
441	198	0.01	100	19.5	31664	PASS
442	442	50	100	100.0	213056	PASS
443	442	15	24	20.7	44064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016810.D
Acq On : 07 Oct 2021 15:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 18:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

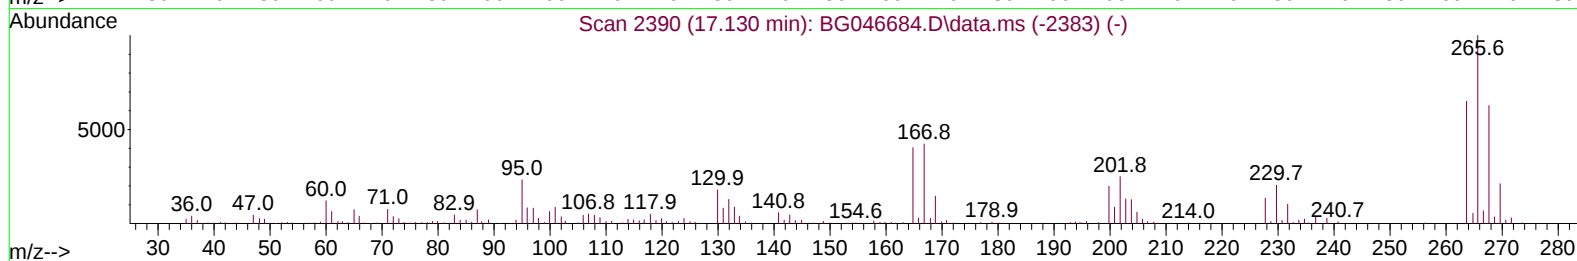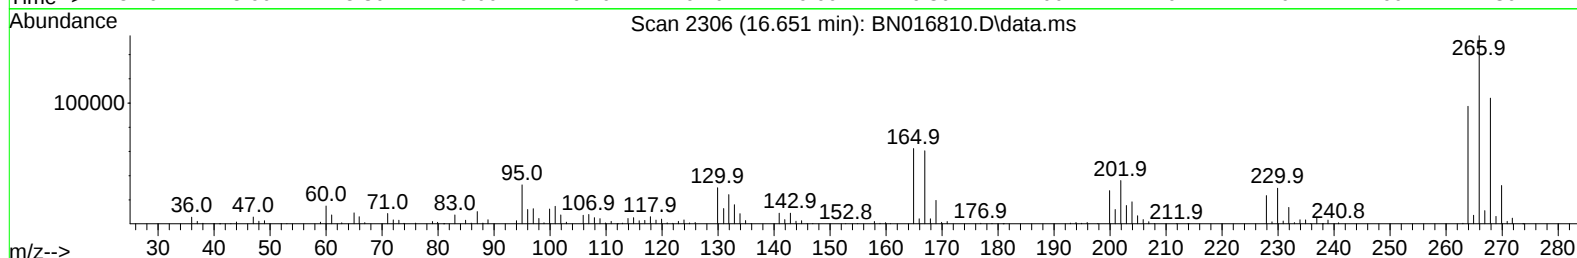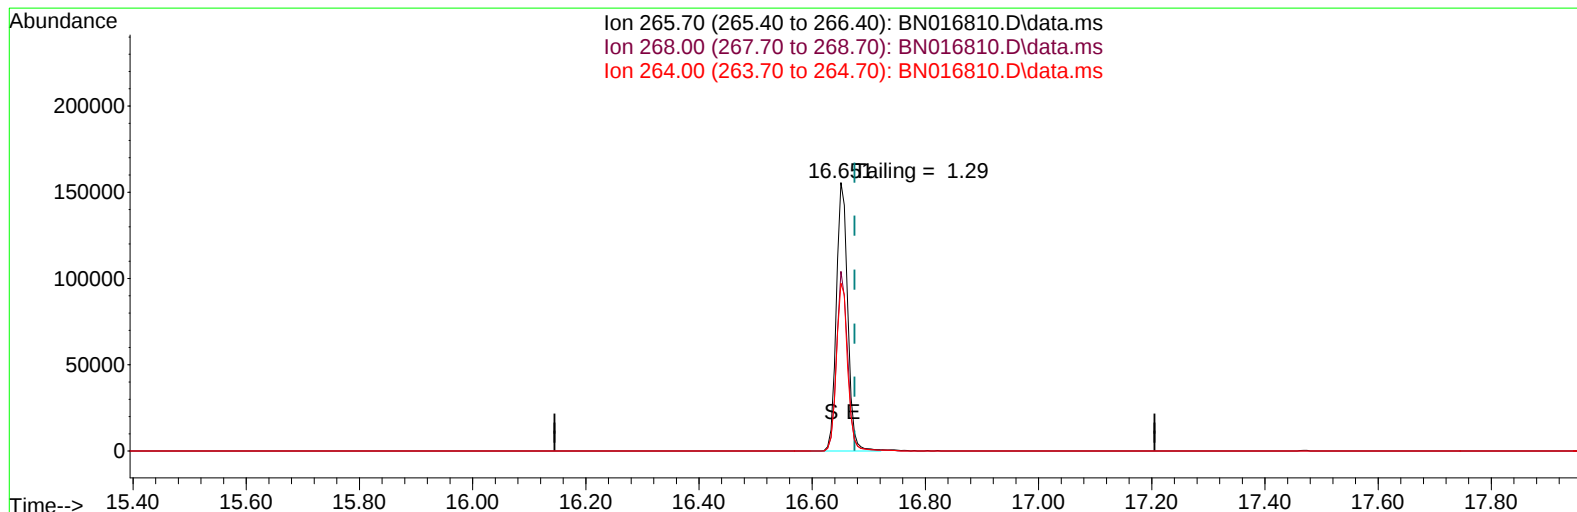

TIC: BN016810.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.024) 31665.42 ng




response 217688

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.89
264.00	61.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100721\
Data File : BN016810.D
Acq On : 07 Oct 2021 15:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 07 18:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

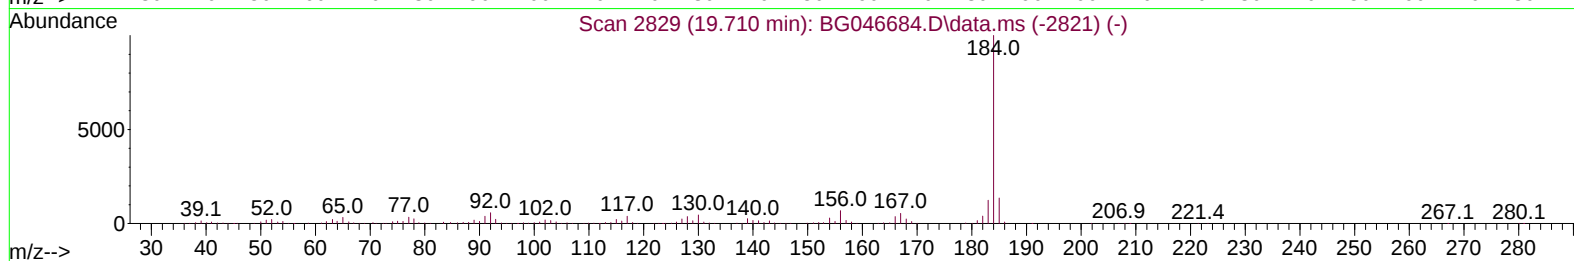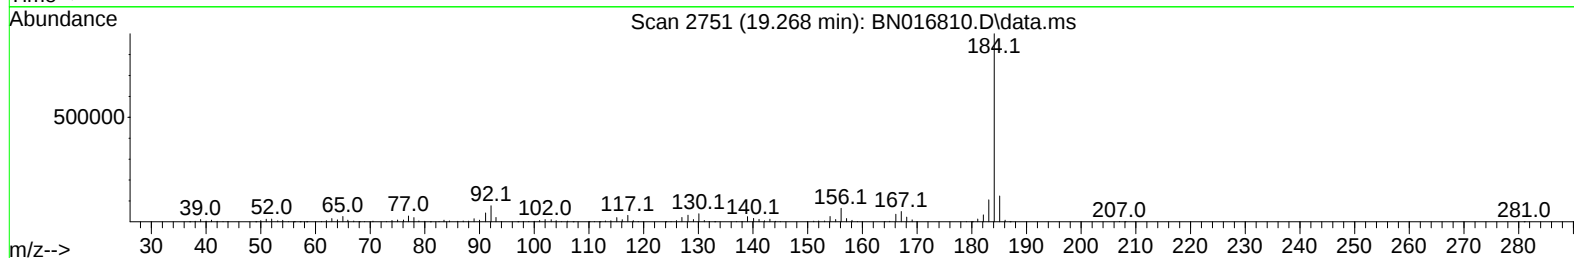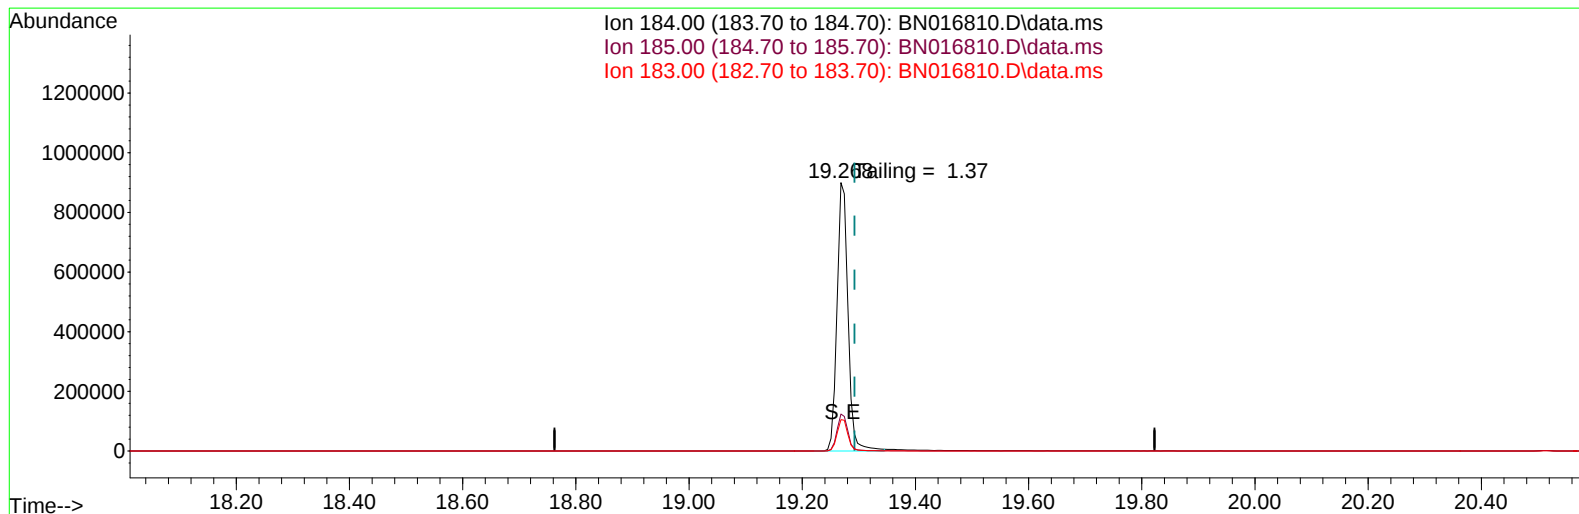

TIC: BN016810.D\data.ms

(77) Benzidine

19.268min (-0.024) 0.00 ng

response 1235857

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2021	BNA_N	<u>BN016810.D</u>
Compound Name	Response	Retention Time
DDT	588486	20.51
DDD	431	20.07
DDE	0	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
431	588917	0.07