
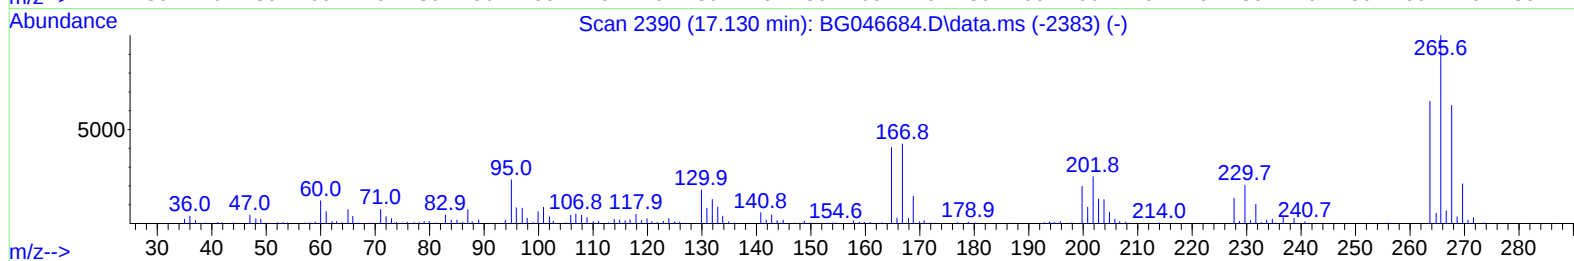
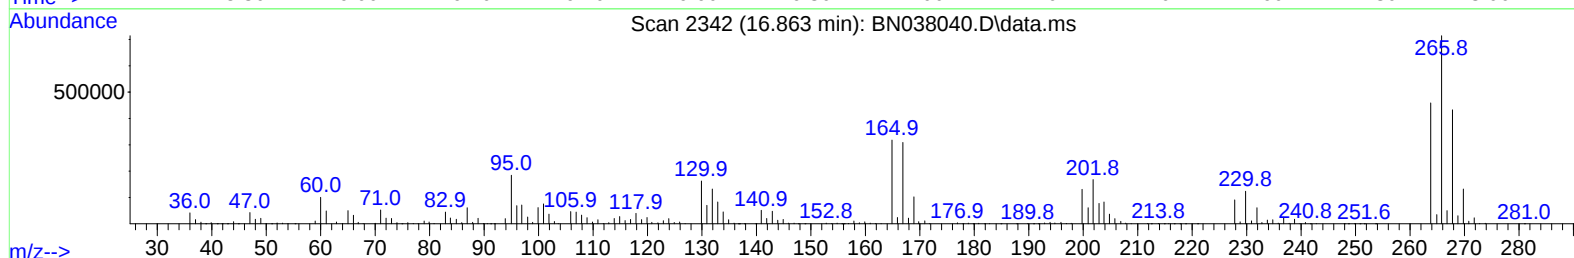


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038040.D
Acq On : 07 Oct 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 11:58:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

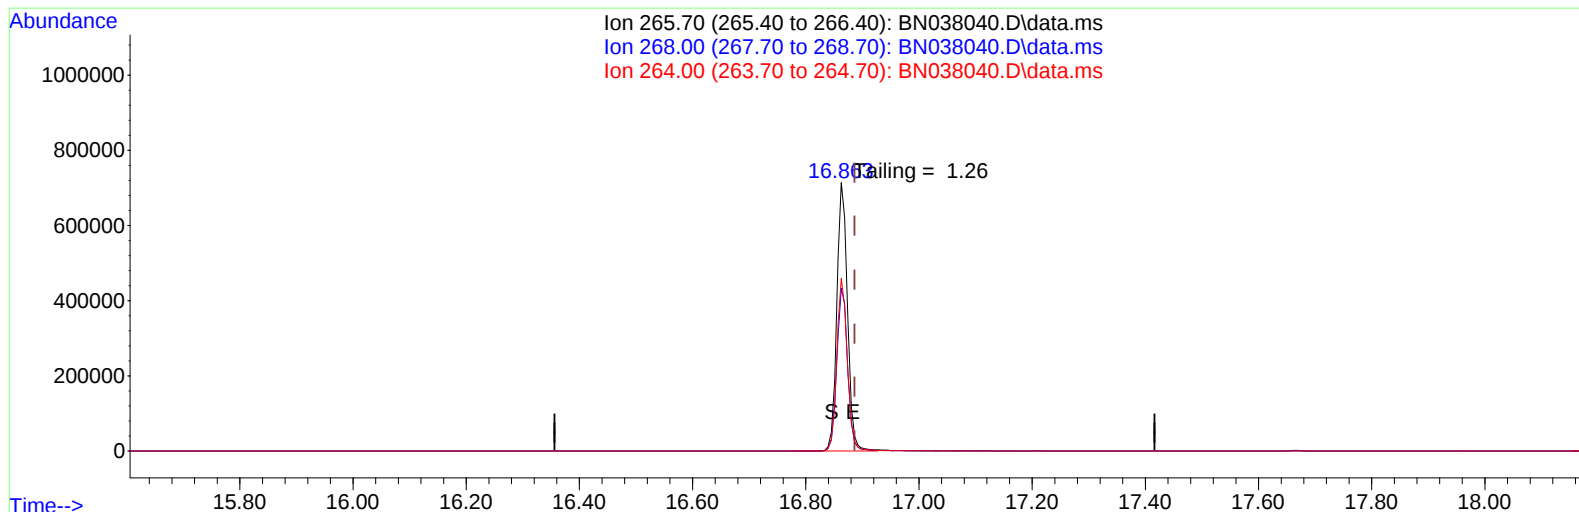

TIC: BN038040.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.023) 28552.74 ng

response 938649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.61
264.00	61.60	64.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038040.D
Acq On : 07 Oct 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 11:58:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

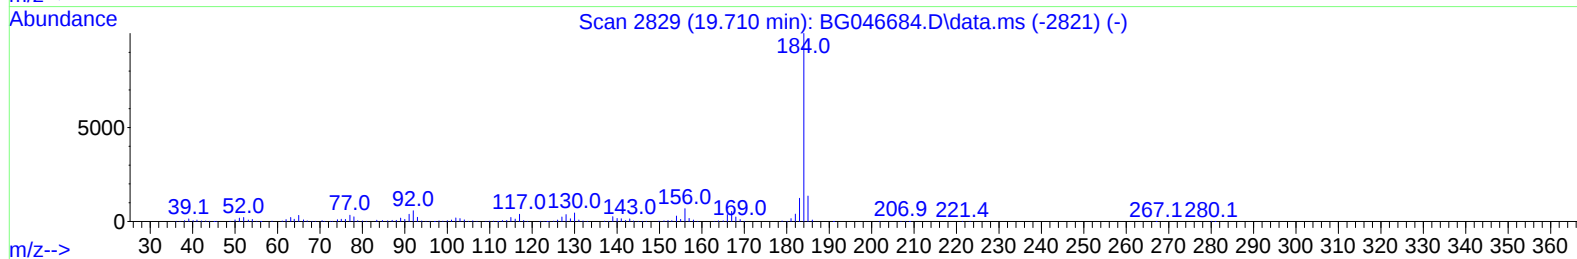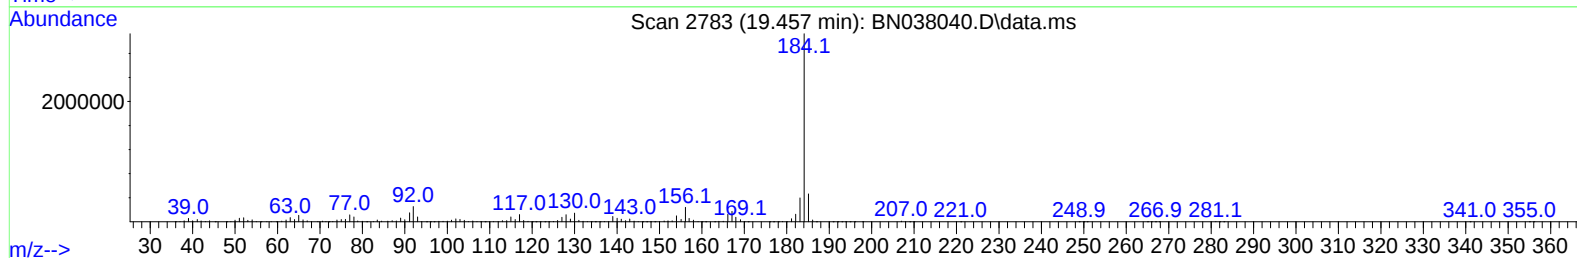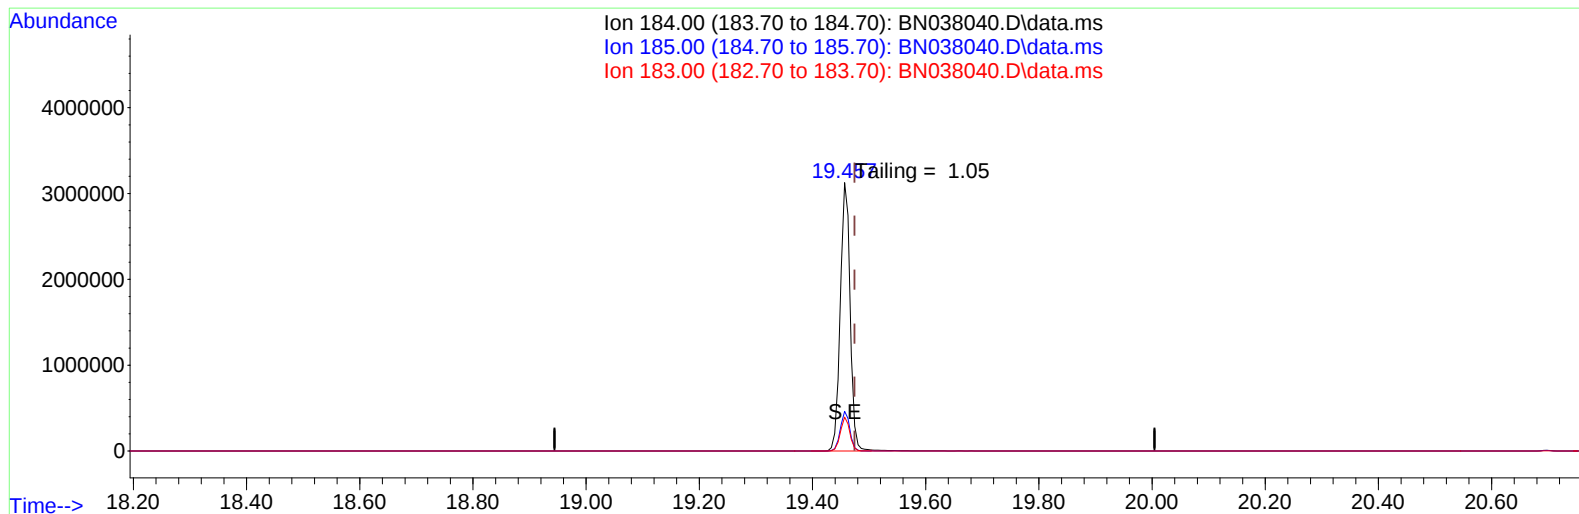

TIC: BN038040.D\data.ms

(77) Benzidine

19.457min (-0.017) 0.00 ng

response 3786107

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.66
0.00	0.00	0.00