
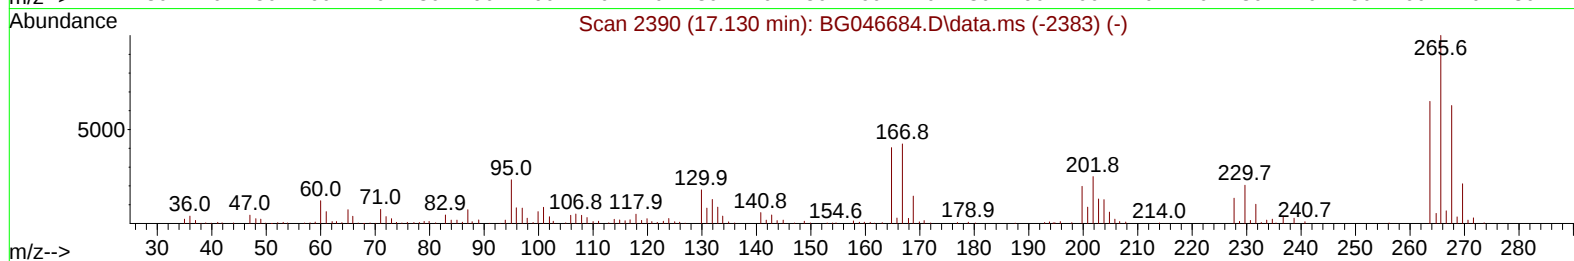
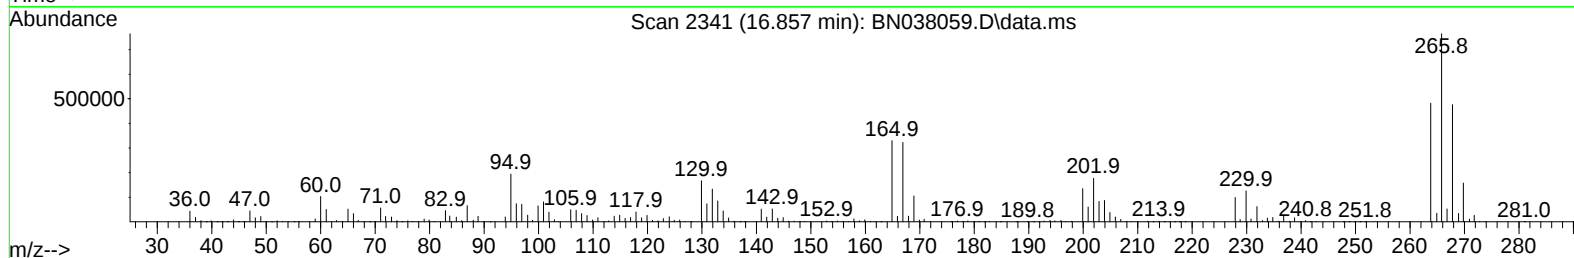


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100725\  
Data File : BN038059.D  
Acq On : 07 Oct 2025 22:58  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 02:11:14 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 29 10:34:59 2025  
Response via : Initial Calibration

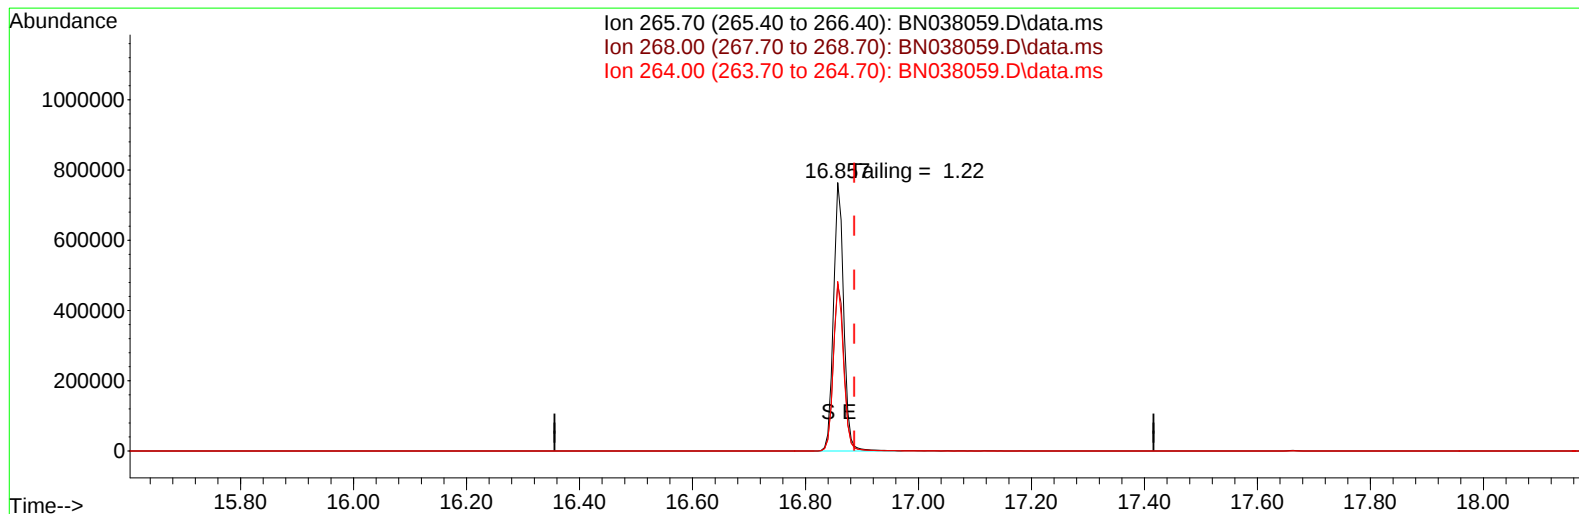

TIC: BN038059.D\data.ms




**(70) Pentachlorophenol (C)**

16.857min (-0.029) 29125.84 ng

response 962975

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.29  |
| 264.00 | 61.60  | 63.12  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Oct 08 02:11:14 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 29 10:34:59 2025  
Response via : Initial Calibration

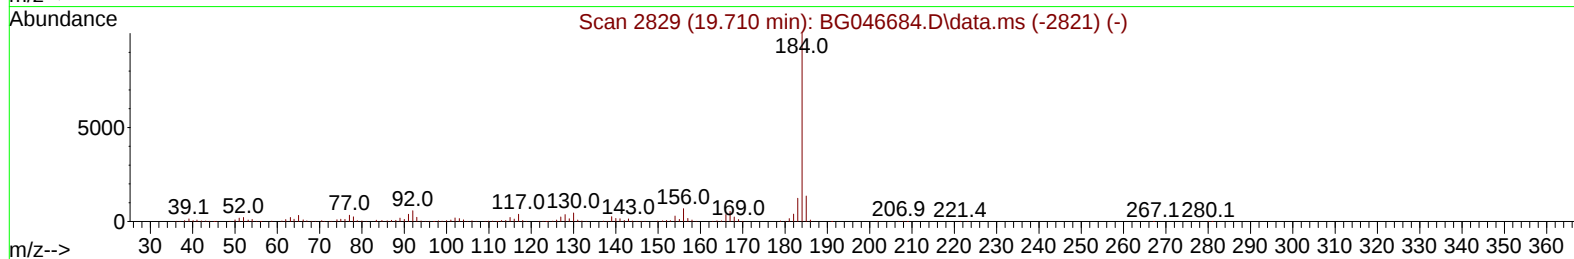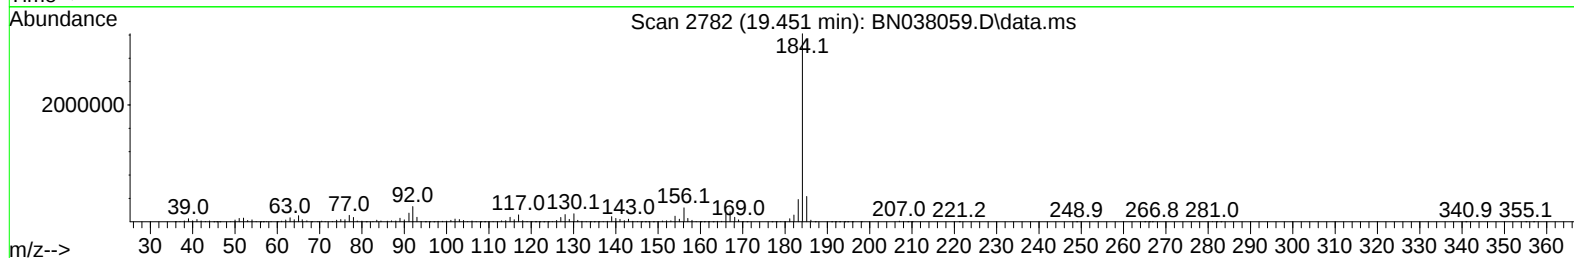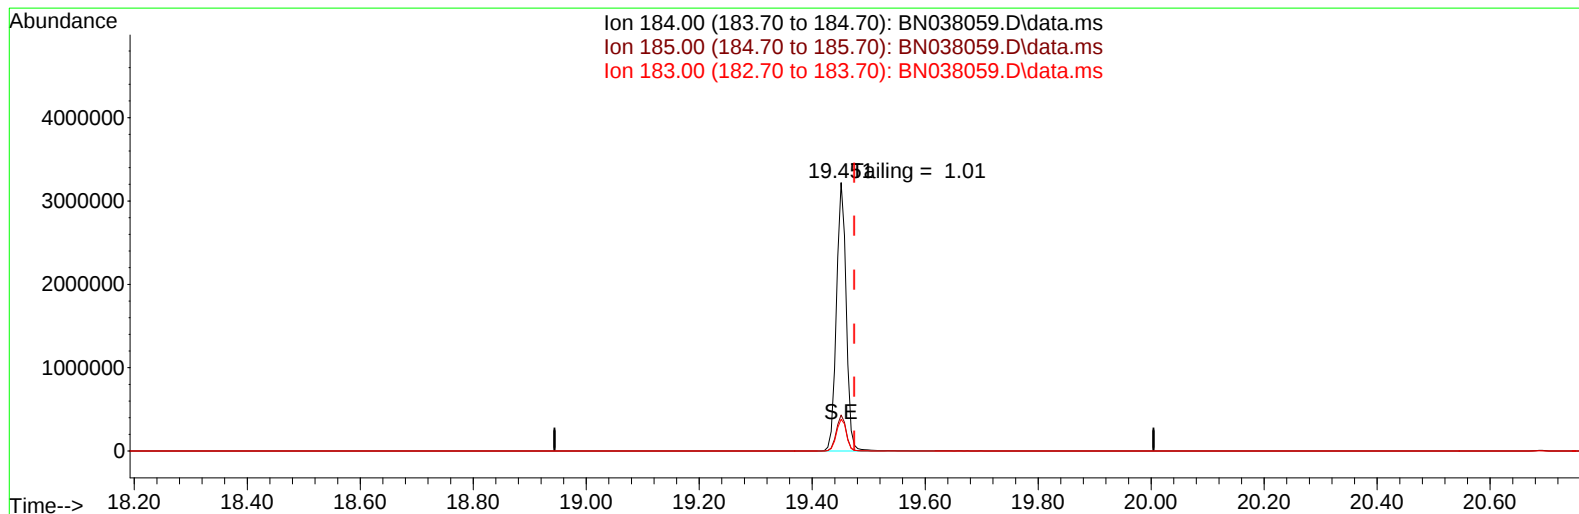

TIC: BN038059.D\data.ms

(77) Benzidine

**19.451min (-0.023) 0.00 ng**

**response**      **3860749**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.41  |
| 183.00 | 13.20  | 11.81  |
| 0.00   | 0.00   | 0.00   |