


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038059.D
Acq On : 07 Oct 2025 22:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

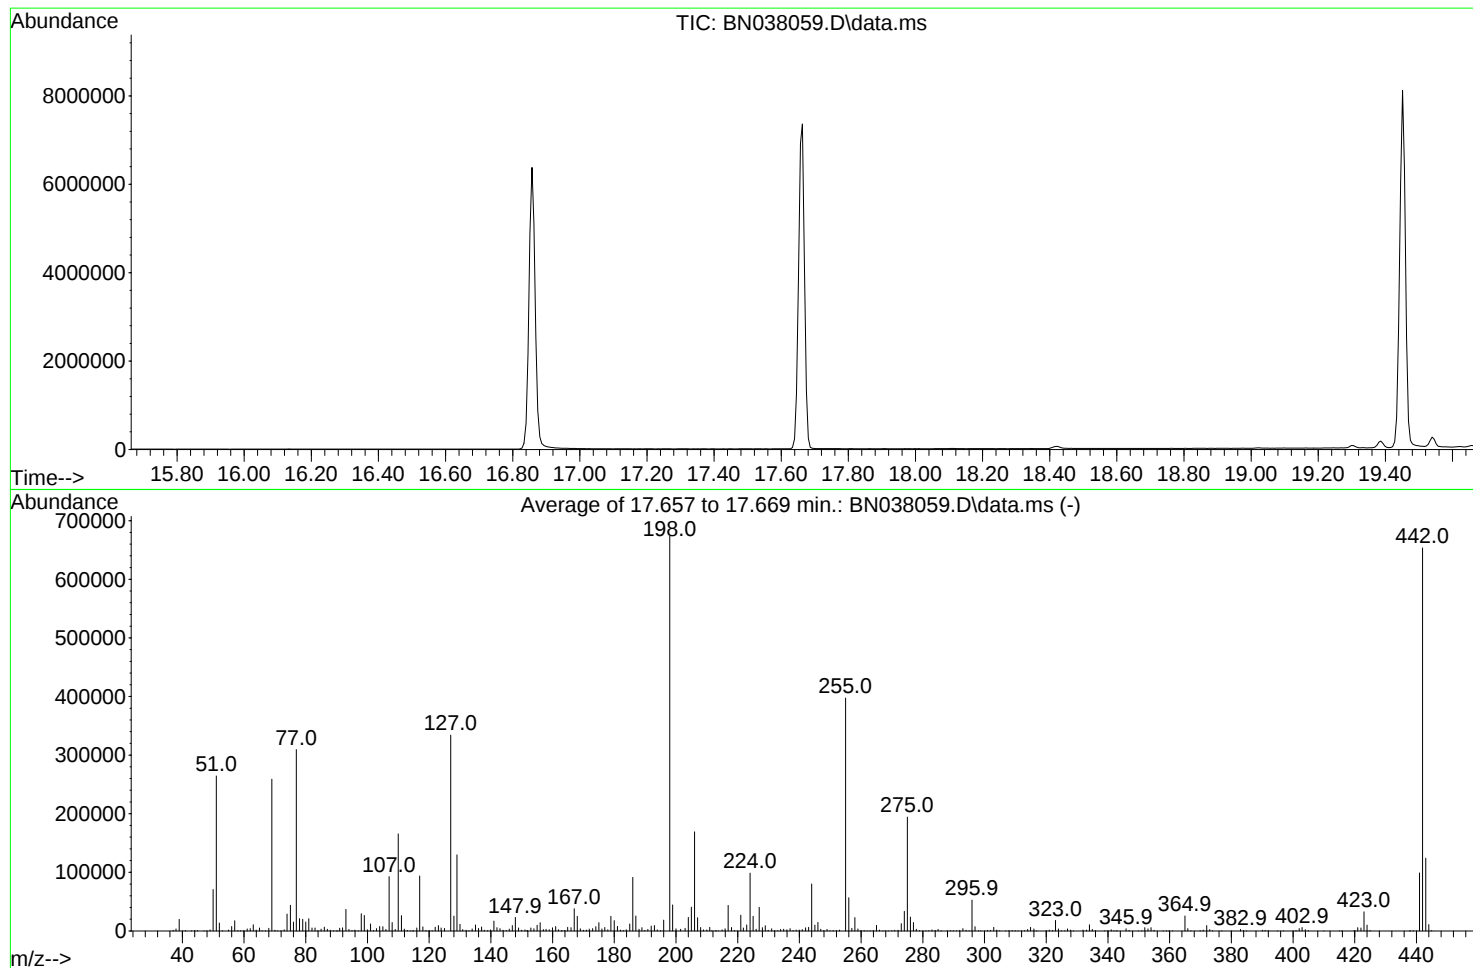




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4627	PASS
69	69	100	100	100.0	259029	PASS
70	69	0.00	2	0.5	1341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	673728	PASS
199	198	5	9	6.6	44347	PASS
365	198	1	100	3.8	25485	PASS
441	443	0.01	150	79.9	99053	PASS
442	442	100	100	100.0	653397	PASS
443	442	15	24	19.0	124008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100725\
Data File : BN038059.D
Acq On : 07 Oct 2025 22:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 08 02:11:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 29 10:34:59 2025
Response via : Initial Calibration

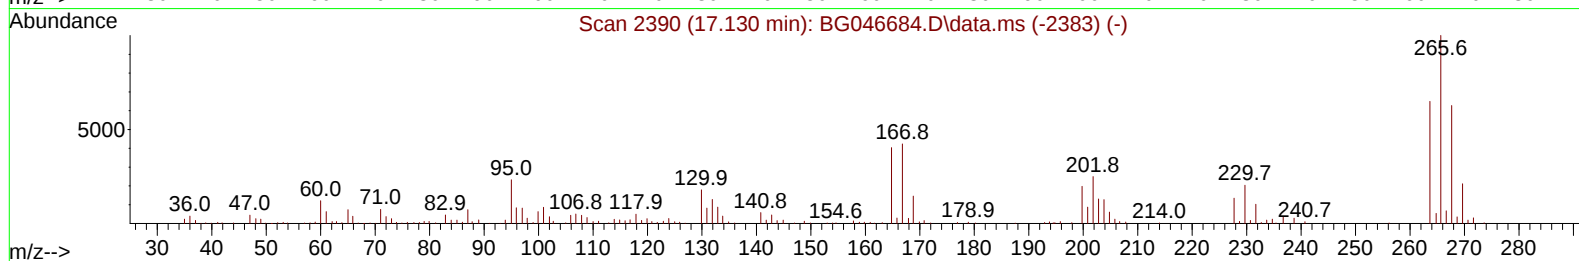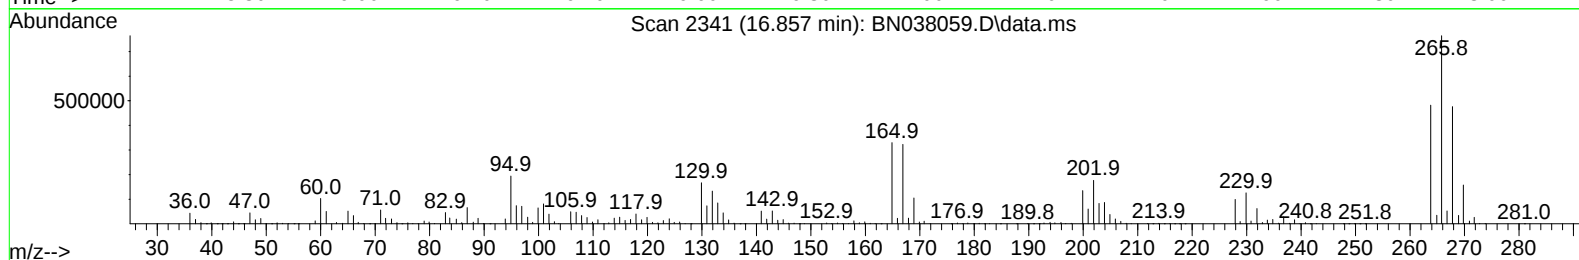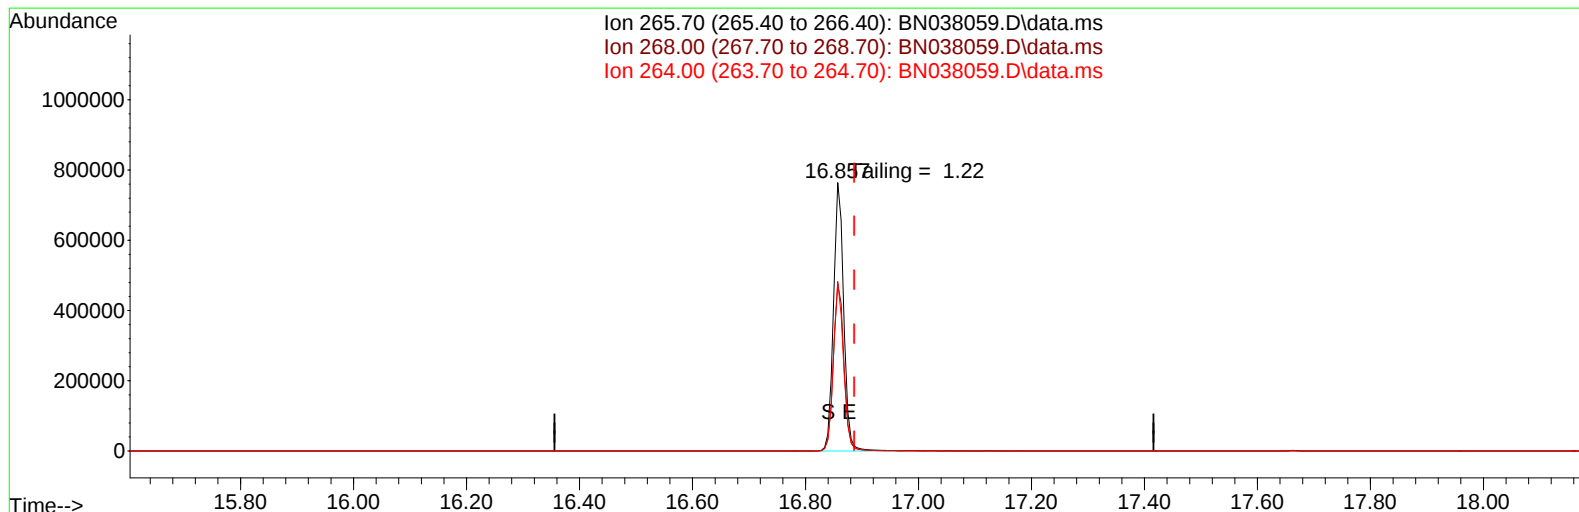

TIC: BN038059.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.029) 29125.84 ng

response 962975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.29
264.00	61.60	63.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2025	BNA_N	<u>BN038059.D</u>
Compound Name	Response	Retention Time
DDT	1940262	20.692
DDD	18010	20.245
DDE	592	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18602	1958864	0.95

Instrument :
BNA_N
ClientSampleId :
DFTPP