
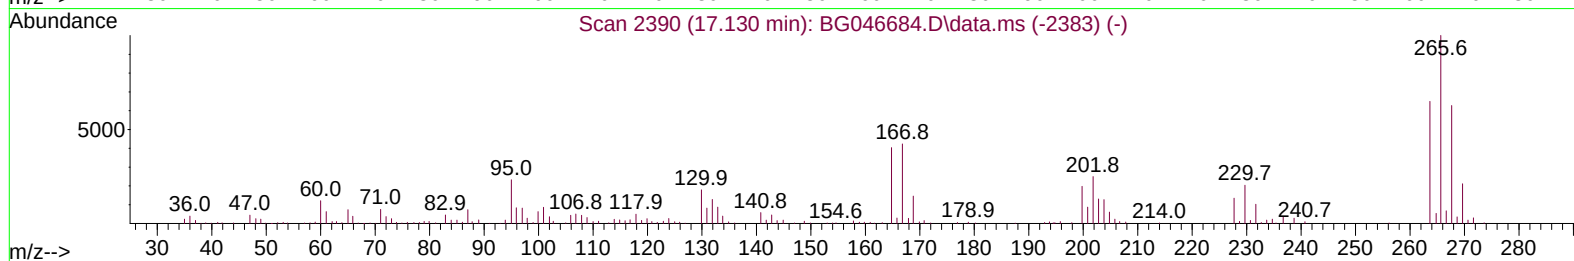
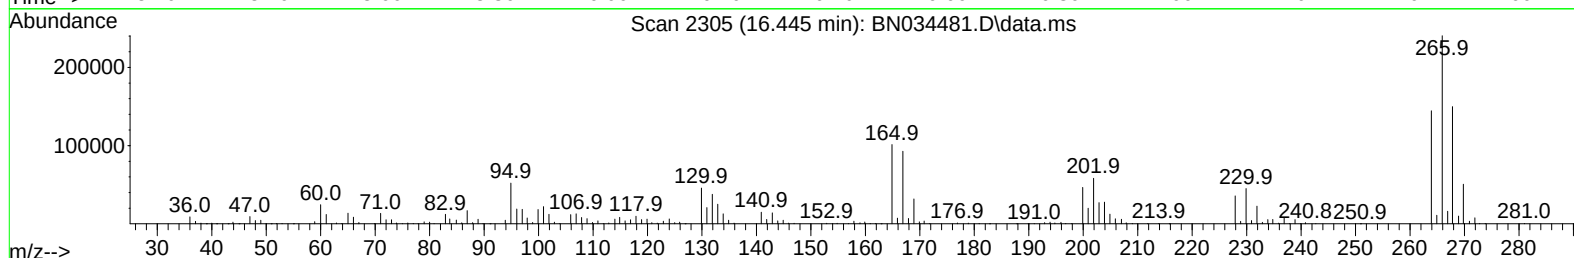


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034481.D
Acq On : 08 Oct 2024 21:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 52 Sample Multiplier: 1

Quant Time: Oct 09 05:44:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 05:44:40 2024
Response via : Initial Calibration

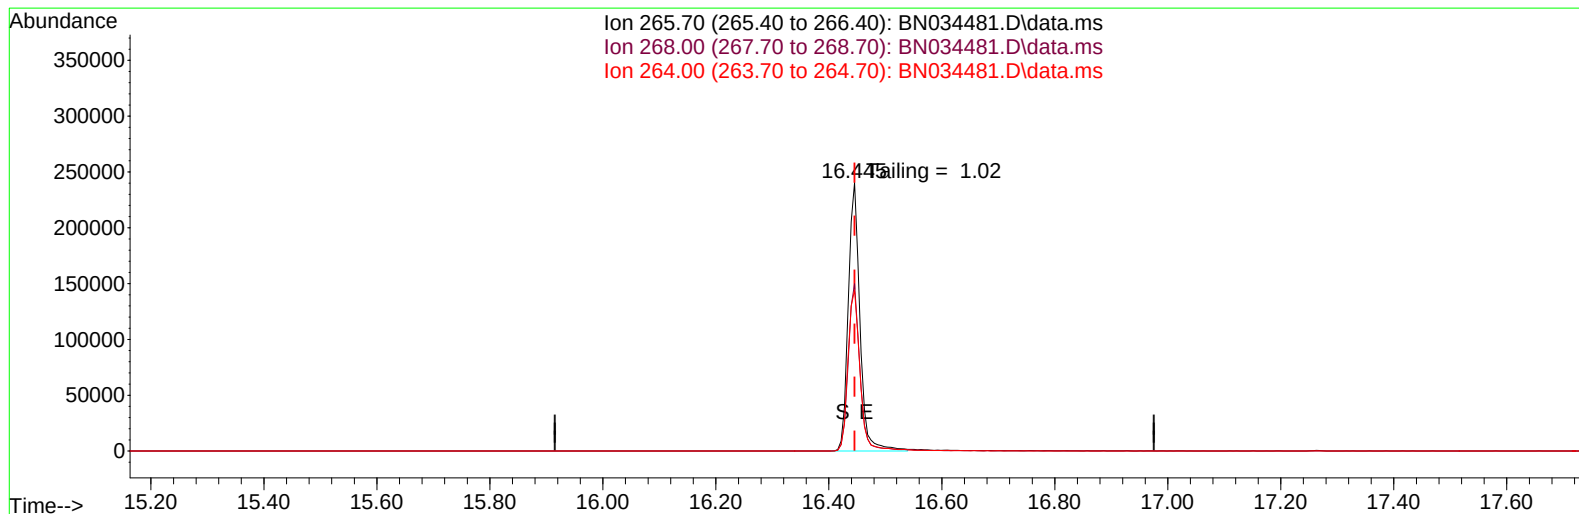

TIC: BN034481.D\data.ms

(70) Pentachlorophenol (C)




16.445min (0.000) 42804.03 ng

response 348680

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.31
264.00	61.60	60.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034481.D
Acq On : 08 Oct 2024 21:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 52 Sample Multiplier: 1

Quant Time: Oct 09 05:44:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 05:44:40 2024
Response via : Initial Calibration

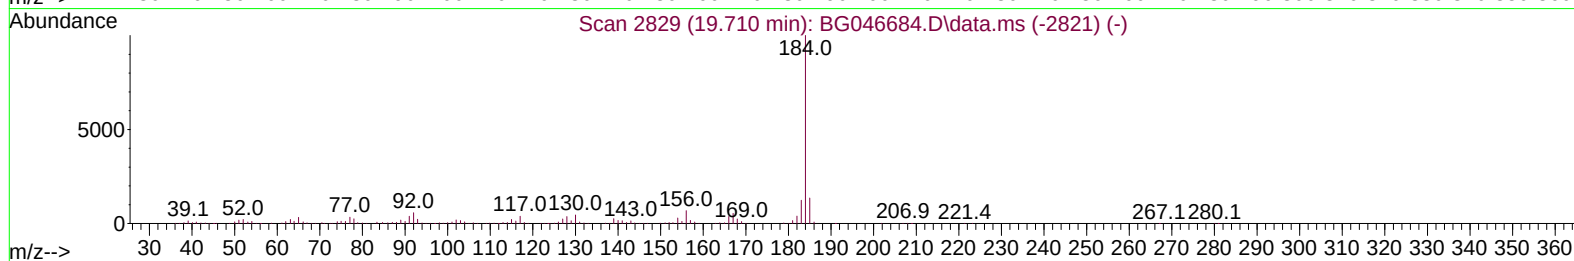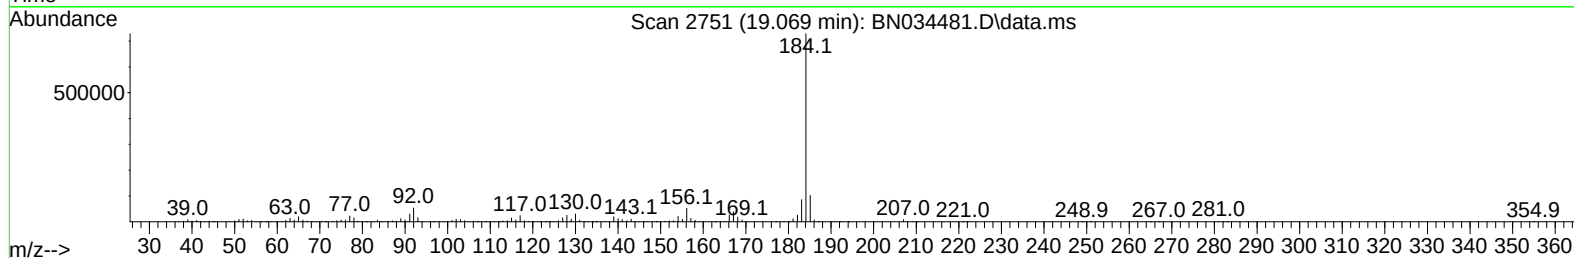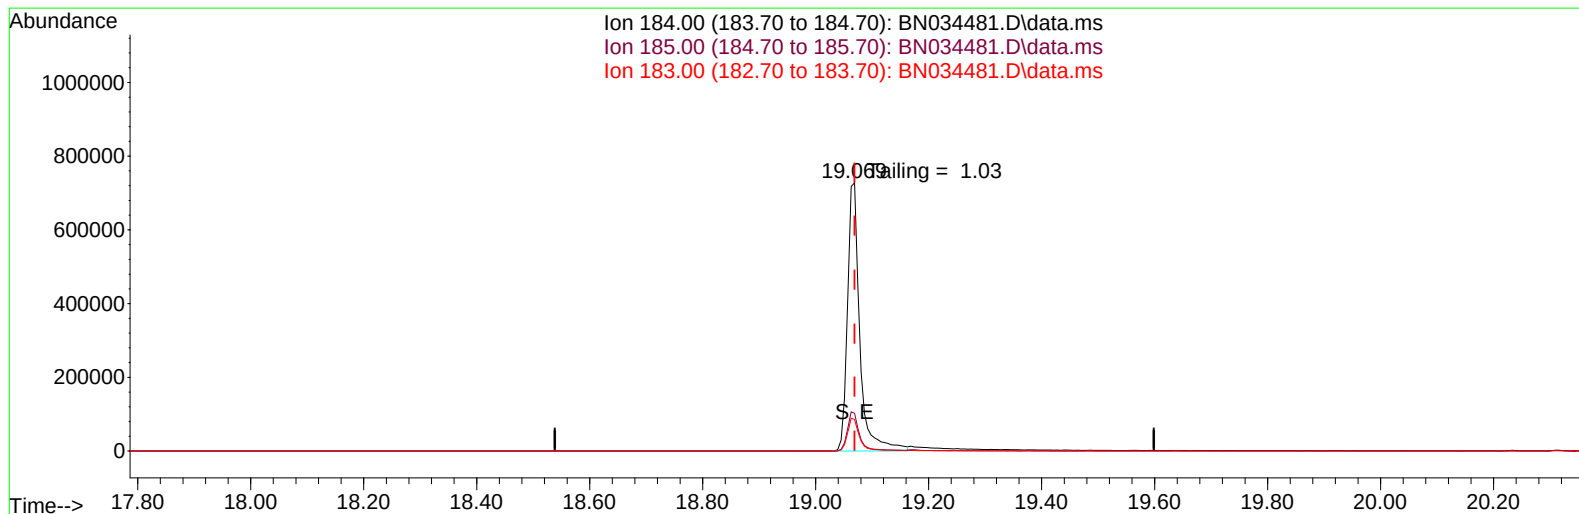

TIC: BN034481.D\data.ms

(77) Benzidine

19.069min (0.000) 0.00 ng

response 1175751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.74
0.00	0.00	0.00