
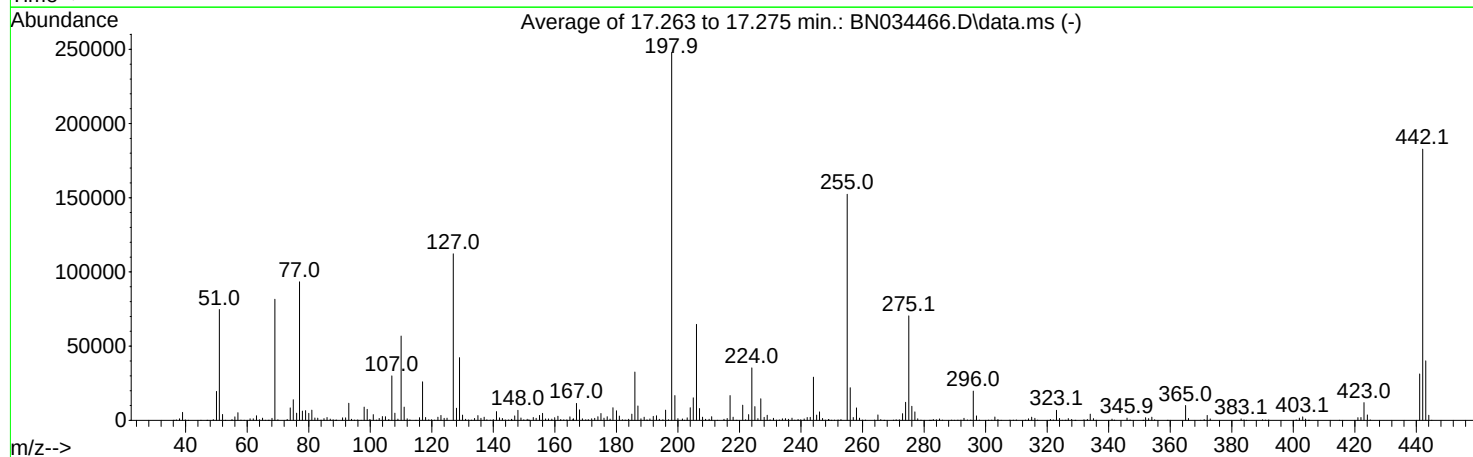


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034466.D
Acq On : 08 Oct 2024 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 14:44:02 2024

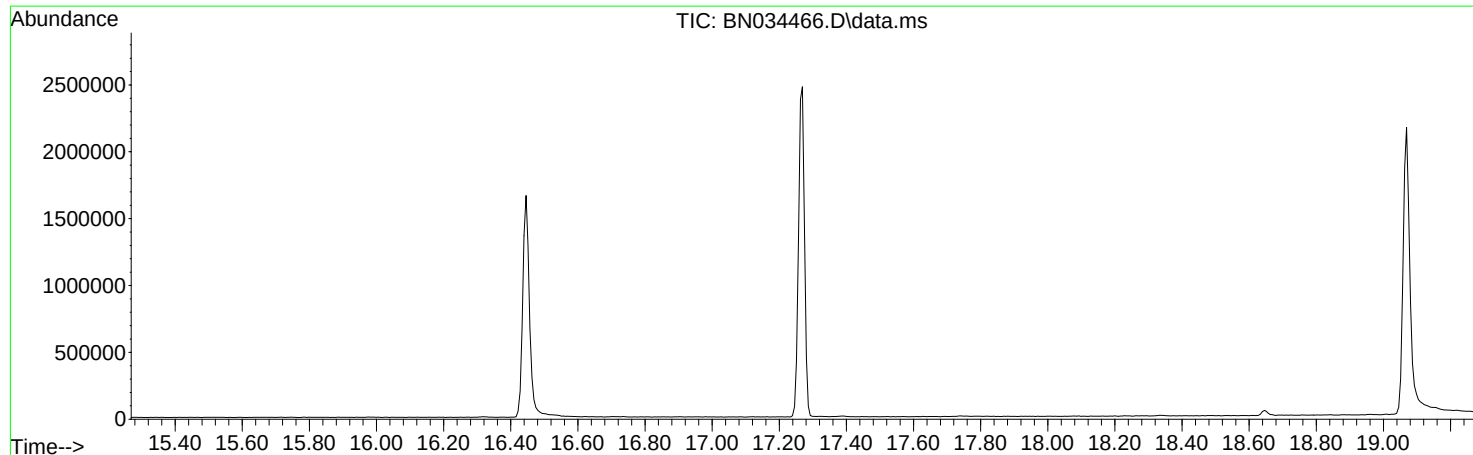




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	74689	PASS
68	69	0.00	2	1.8	1452	PASS
69	198	0.00	100	32.9	81608	PASS
70	69	0.00	2	0.5	438	PASS
127	198	10	80	45.3	112229	PASS
197	198	0.00	2	0.2	481	PASS
198	198	100	100	100.0	247851	PASS
199	198	5	9	6.8	16737	PASS
275	198	10	60	28.4	70443	PASS
365	198	1	100	4.0	10034	PASS
441	198	0.01	100	12.6	31291	PASS
442	442	50	100	100.0	182720	PASS
443	442	15	24	21.9	40101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034466.D
Acq On : 08 Oct 2024 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 08 16:07:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 27 02:40:30 2024
Response via : Initial Calibration

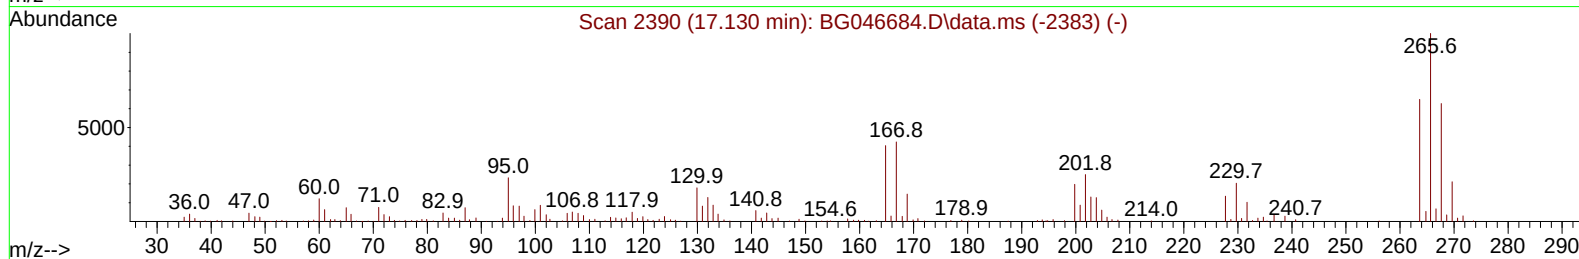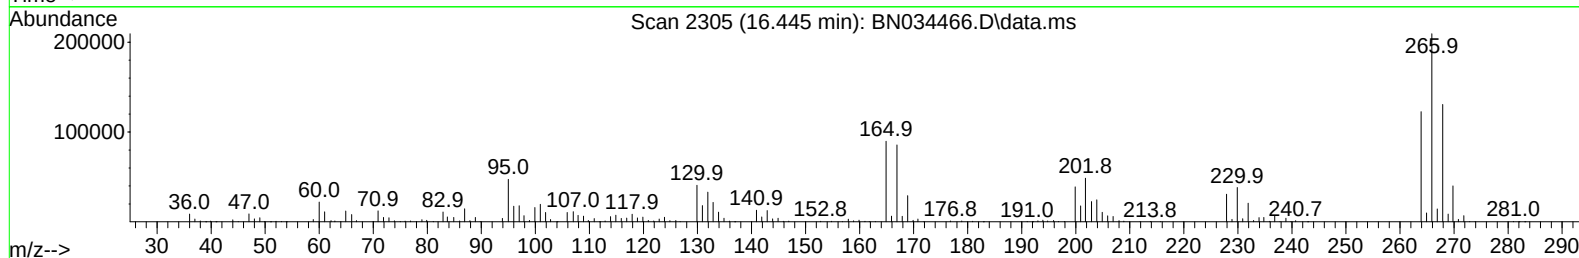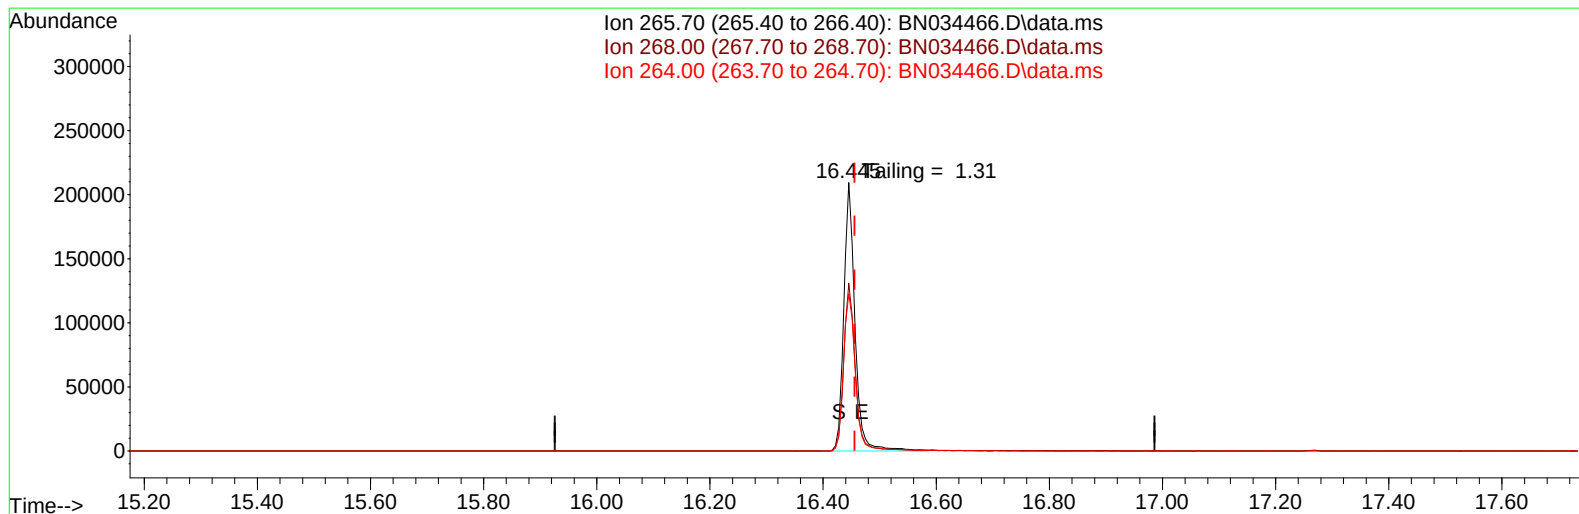

TIC: BN034466.D\data.ms

(70) Pentachlorophenol (C)

16.445min (-0.011) 23244.89 ng




response 286217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.44
264.00	61.60	58.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034466.D
Acq On : 08 Oct 2024 11:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 08 16:07:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 27 02:40:30 2024
Response via : Initial Calibration

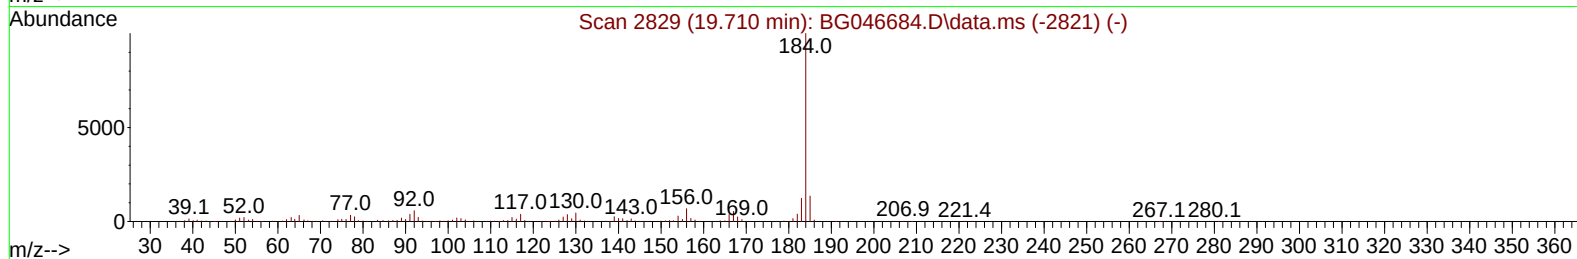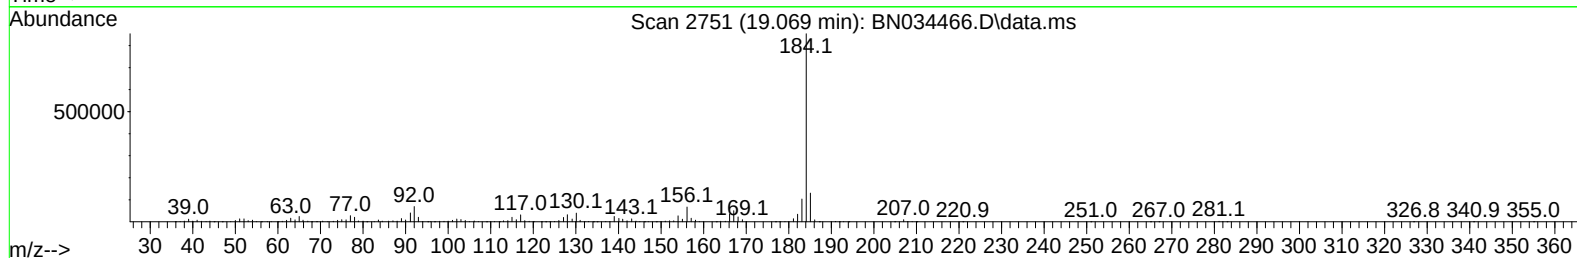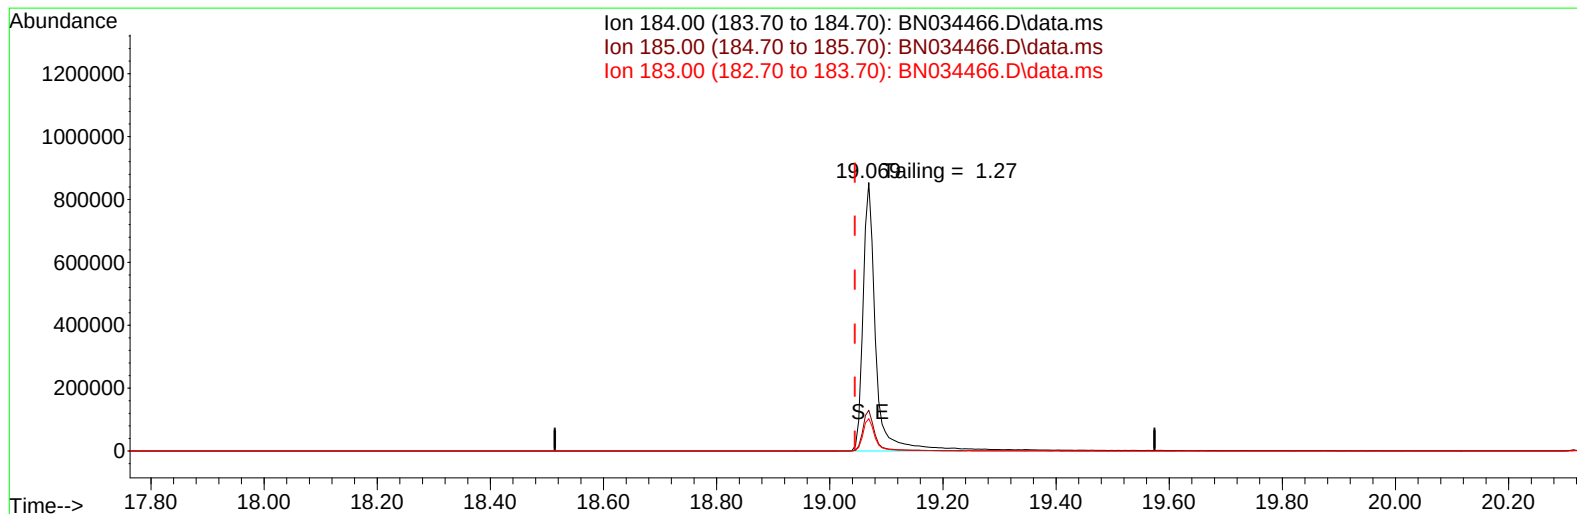

TIC: BN034466.D\data.ms

(77) Benzidine

19.069min (+ 0.025) 0.00 ng

response 1354534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.22
183.00	13.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2024	BNA_N	<u>BN034466.D</u>
Compound Name	Response	Retention Time
DDT	602450	20.316
DDD	134279	19.875
DDE	195	19.416
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
134474	736924	18.25

Instrument :
BNA_N
ClientSampleId :
DFTPP