
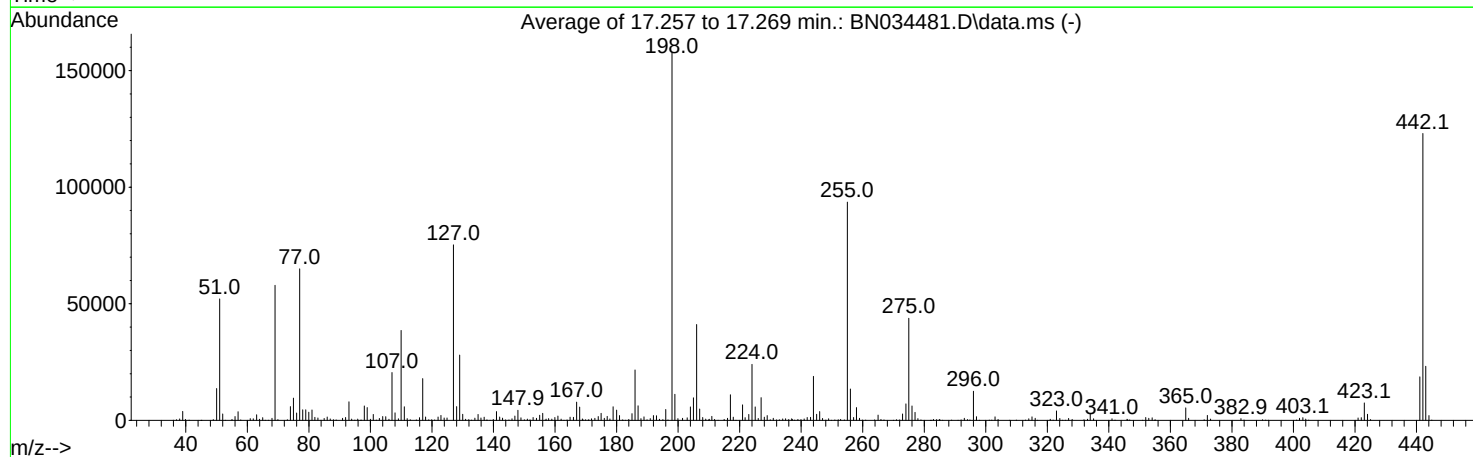


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034481.D
Acq On : 08 Oct 2024 21:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 26 14:44:02 2024

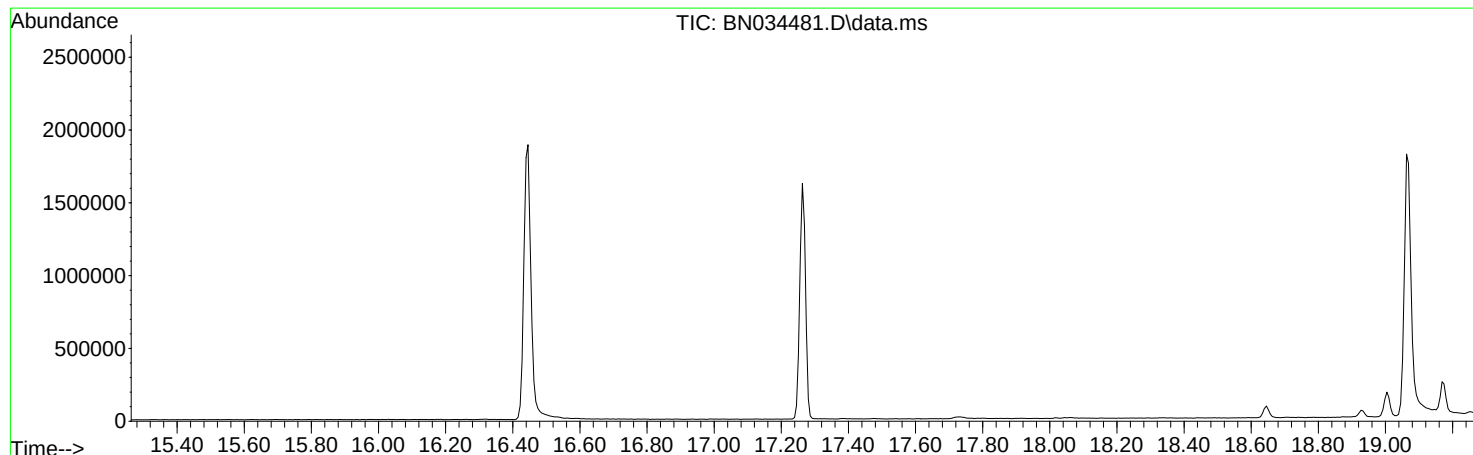




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	52075	PASS
68	69	0.00	2	1.5	864	PASS
69	198	0.00	100	36.7	57947	PASS
70	69	0.00	2	0.6	333	PASS
127	198	10	80	47.7	75280	PASS
197	198	0.00	2	0.2	240	PASS
198	198	100	100	100.0	157760	PASS
199	198	5	9	7.1	11193	PASS
275	198	10	60	27.8	43784	PASS
365	198	1	100	3.4	5360	PASS
441	198	0.01	100	11.8	18647	PASS
442	442	50	100	100.0	123021	PASS
443	442	15	24	18.8	23169	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034481.D
Acq On : 08 Oct 2024 21:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 09 05:44:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 05:44:40 2024
Response via : Initial Calibration

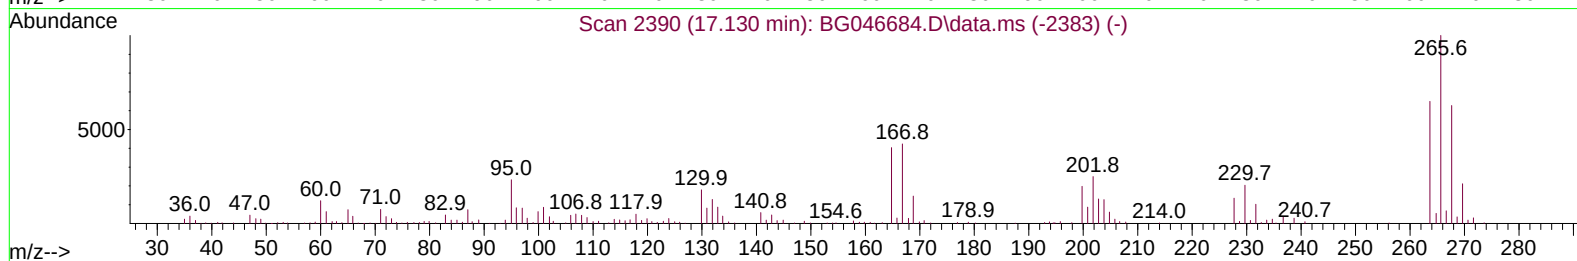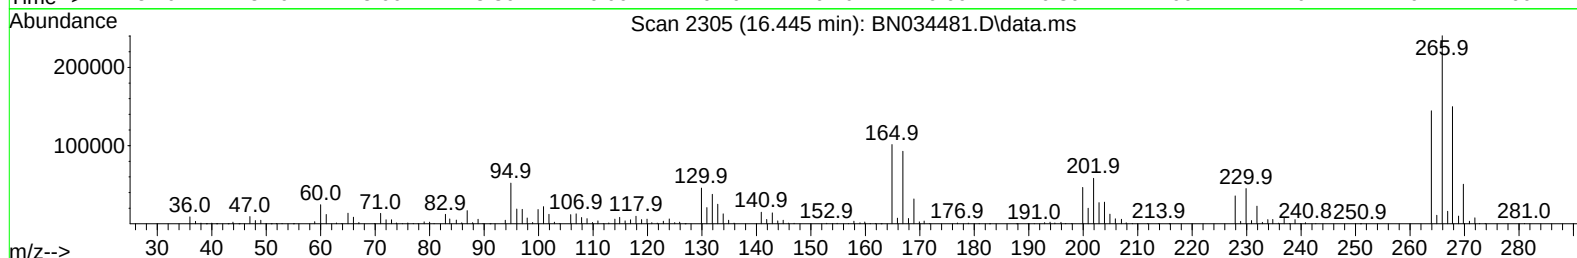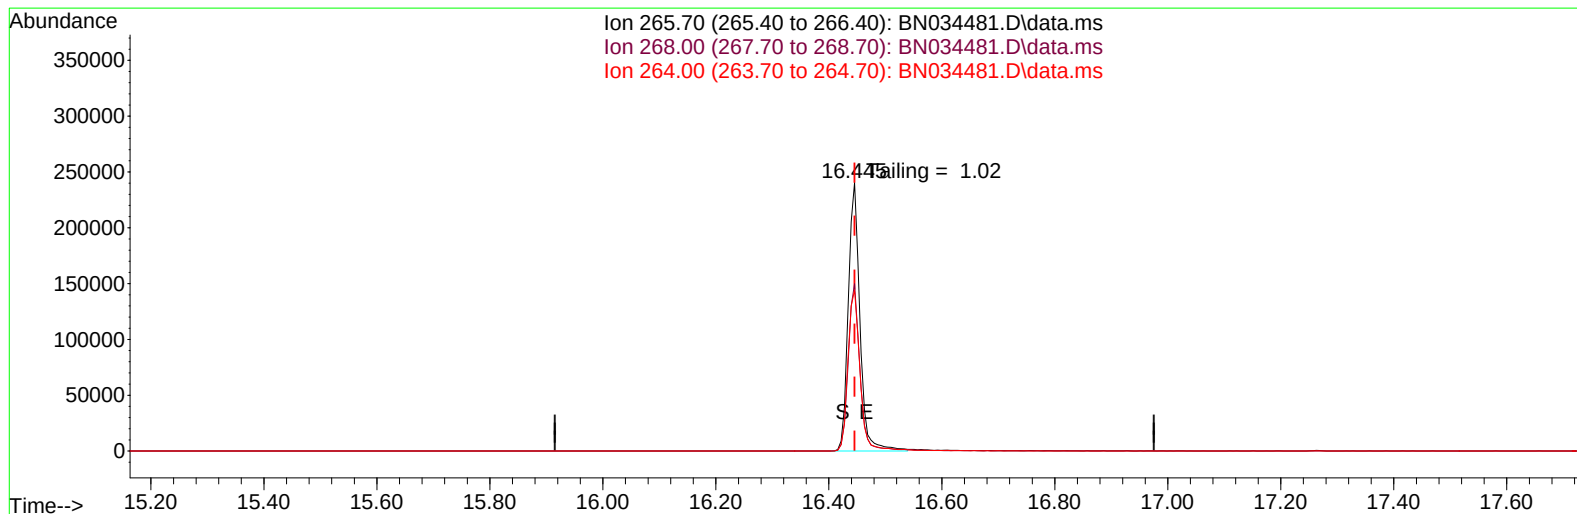

TIC: BN034481.D\data.ms

(70) Pentachlorophenol (C)

16.445min (0.000) 42804.03 ng




response 348680

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.31
264.00	61.60	60.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100824\
Data File : BN034481.D
Acq On : 08 Oct 2024 21:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 09 05:44:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 05:44:40 2024
Response via : Initial Calibration

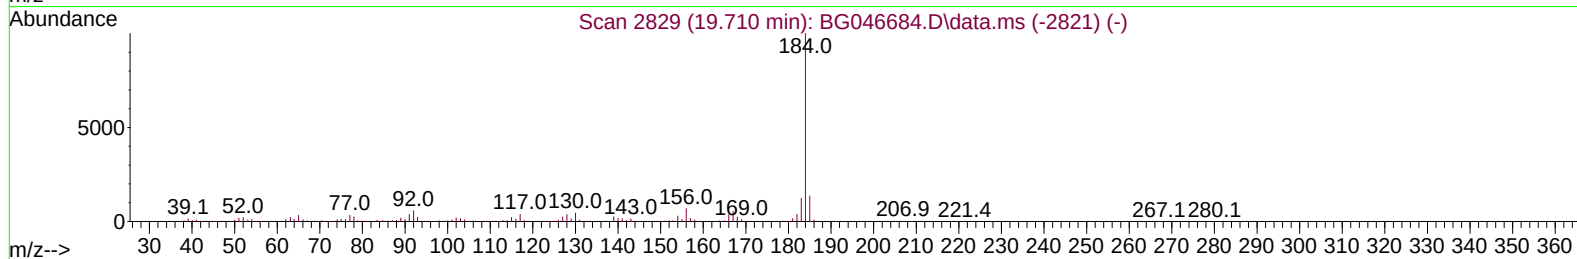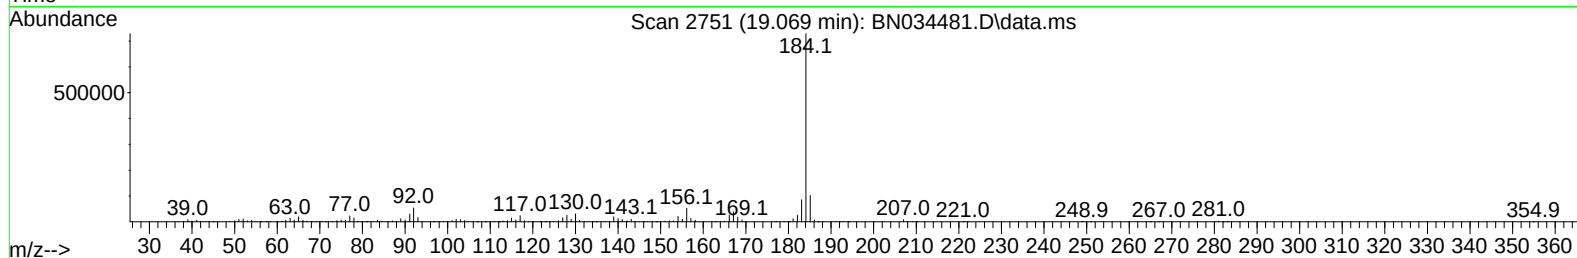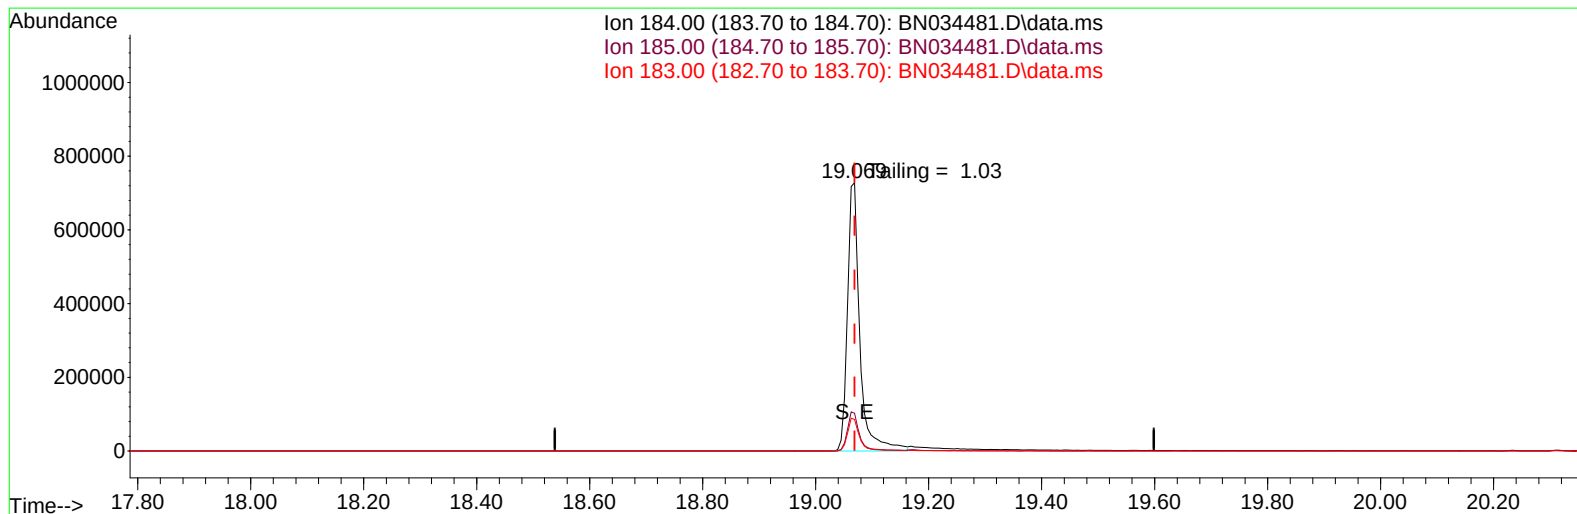

TIC: BN034481.D\data.ms

(77) Benzidine

19.069min (0.000) 0.00 ng

response 1175751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2024	BNA_N	<u>BN034481.D</u>
Compound Name	Response	Retention Time
DDT	591796	20.316
DDD	67424	19.874
DDE	1583	19.357
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
69007	660803	10.44

Instrument :
BNA_N
ClientSampleId :
DFTPP