

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:05:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

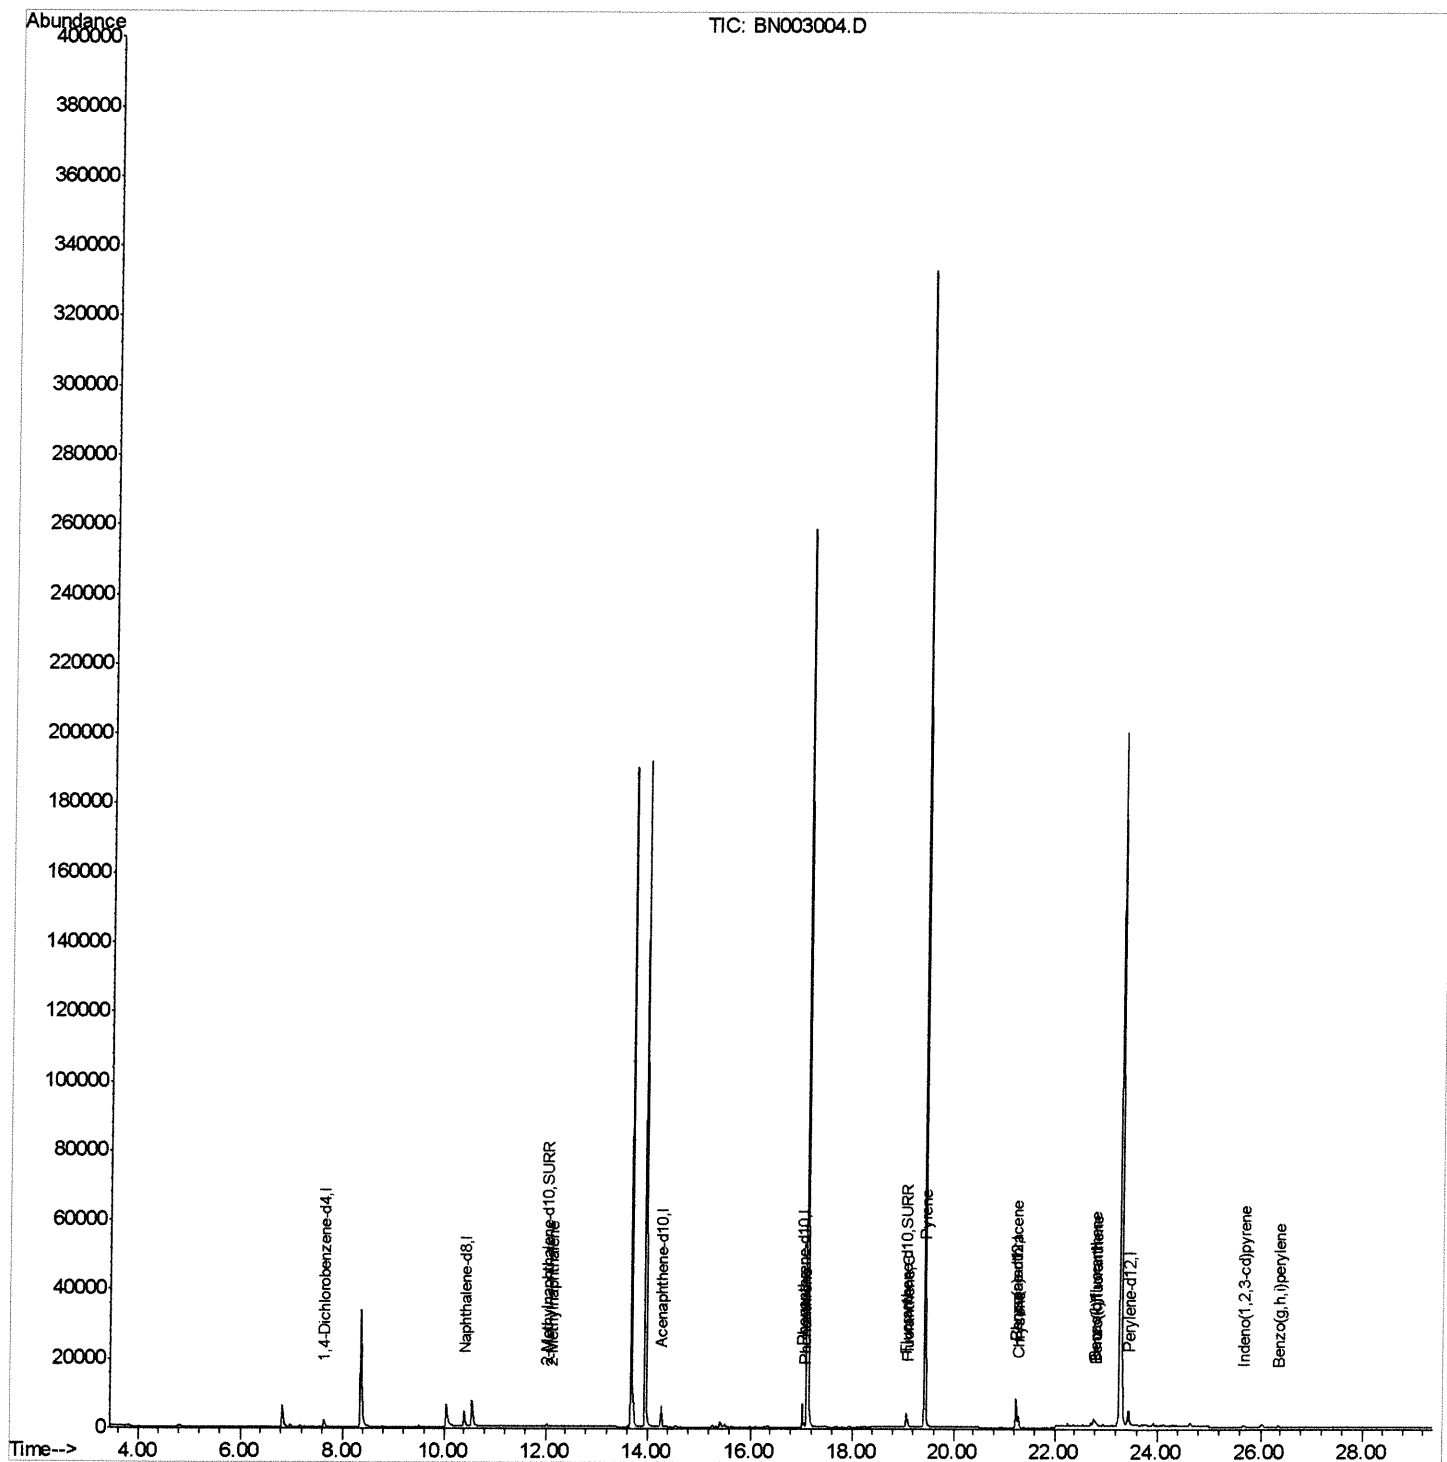

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:01:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

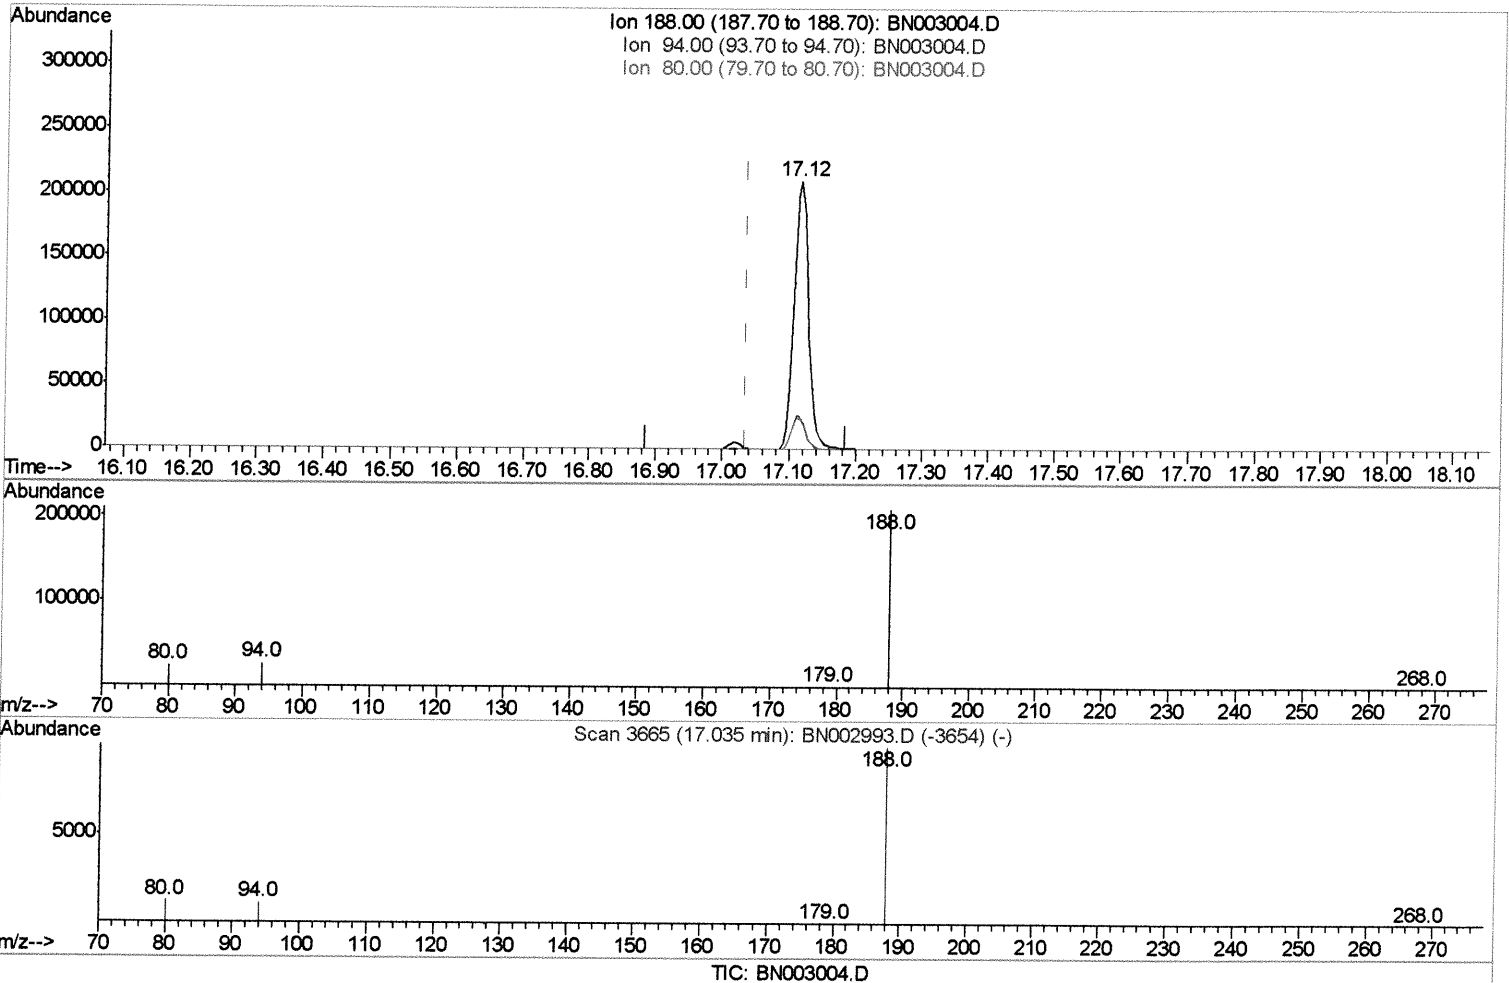

(10) Phenanthrene-d10 (I)
 17.116min (+0.080) 0.40ng/ul
 response 310928

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.39
80.00	12.70	11.20
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:01:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

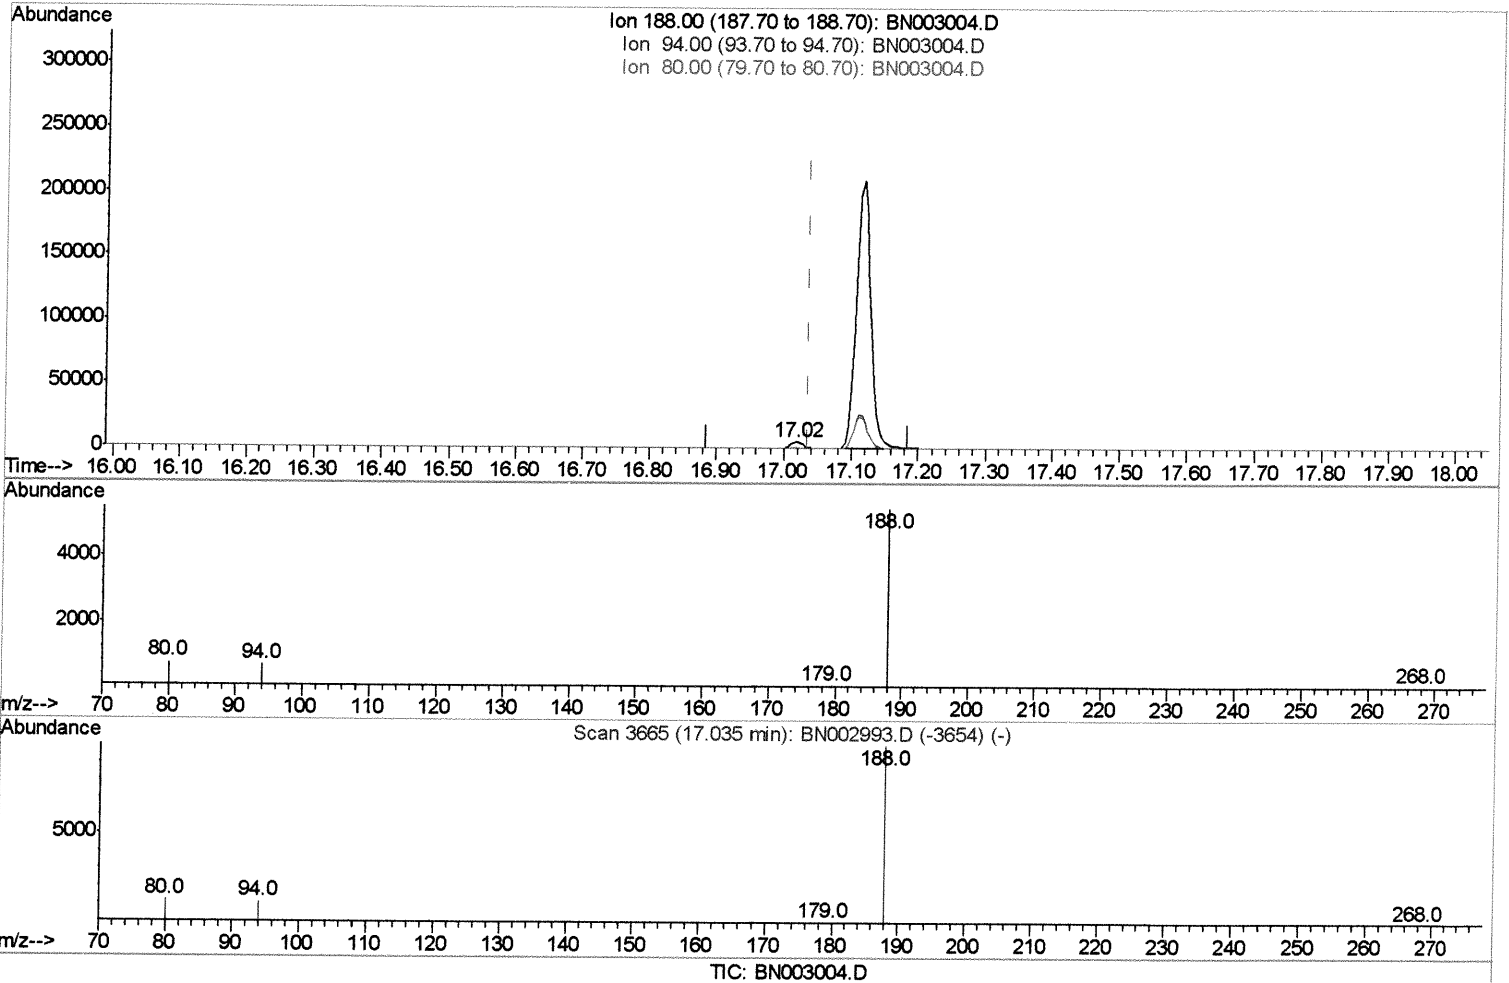

(10) Phenanthrene-d10 (I)

17.019min (-0.017) 0.40ng/ul m *SJ 10/10/18*

response 7965

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.08
80.00	12.70	13.22
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
Data File : BN003004.D
Acq On : 09 Oct 2018 01:12
Operator : MJ/SJ
Sample : J5115-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC15

Manual Integrations
APPROVED

Sohil
10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 09 01:14:49 2018
Response via : Initial Calibration

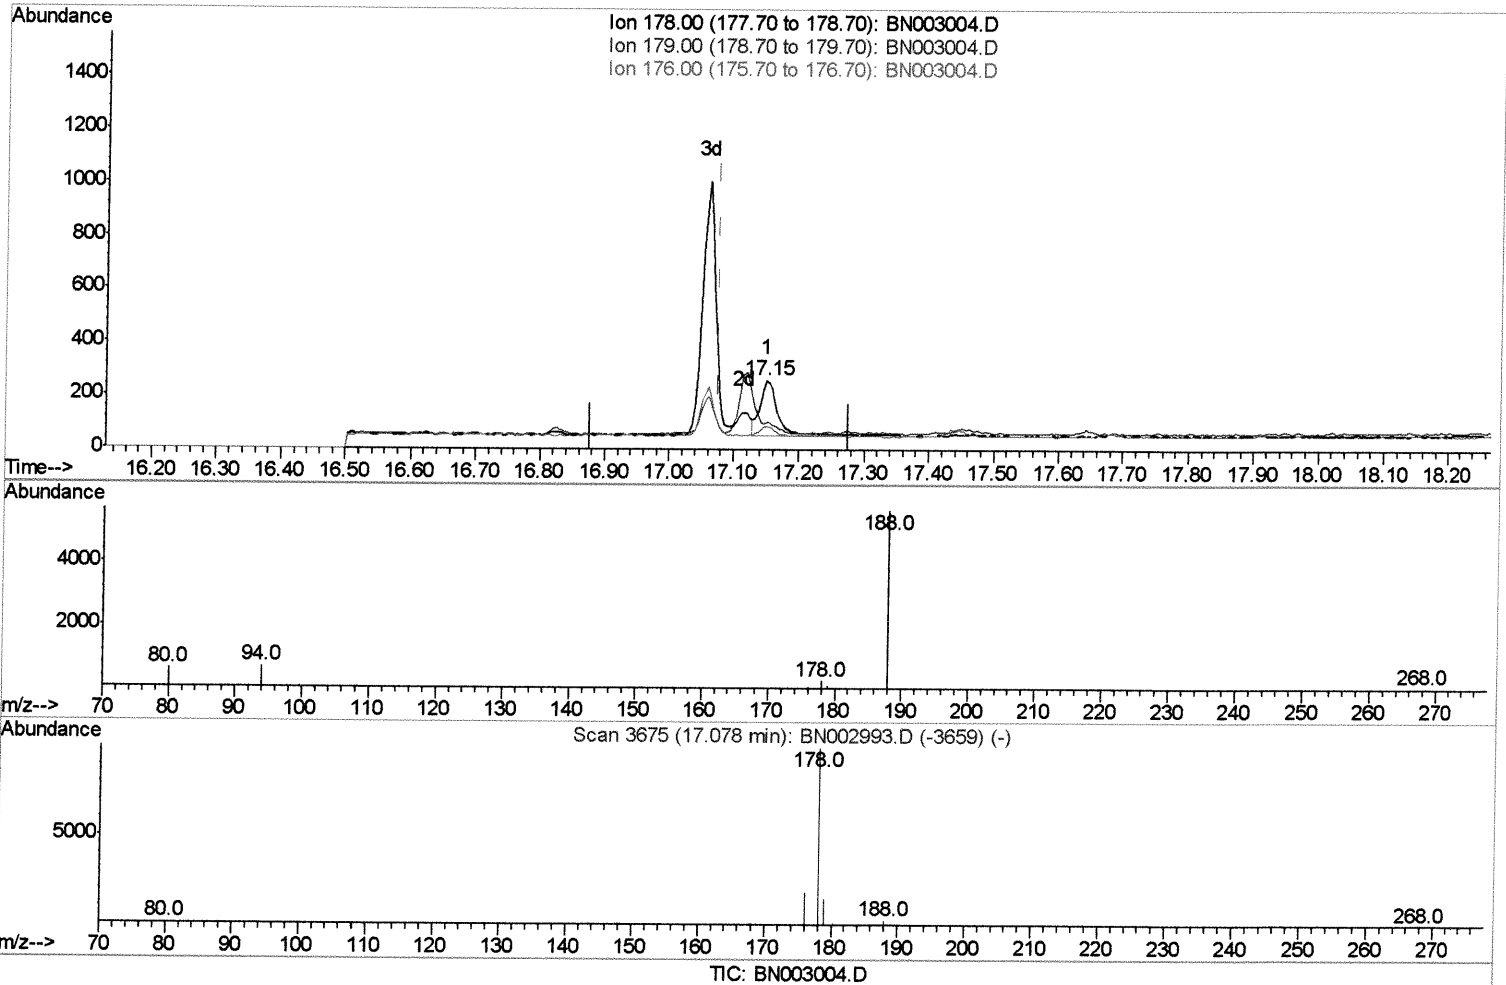

(12) Phenanthrene

17.149min (+0.072) 0.02ng/ul

response 371

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	40.46#
176.00	19.30	33.21#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

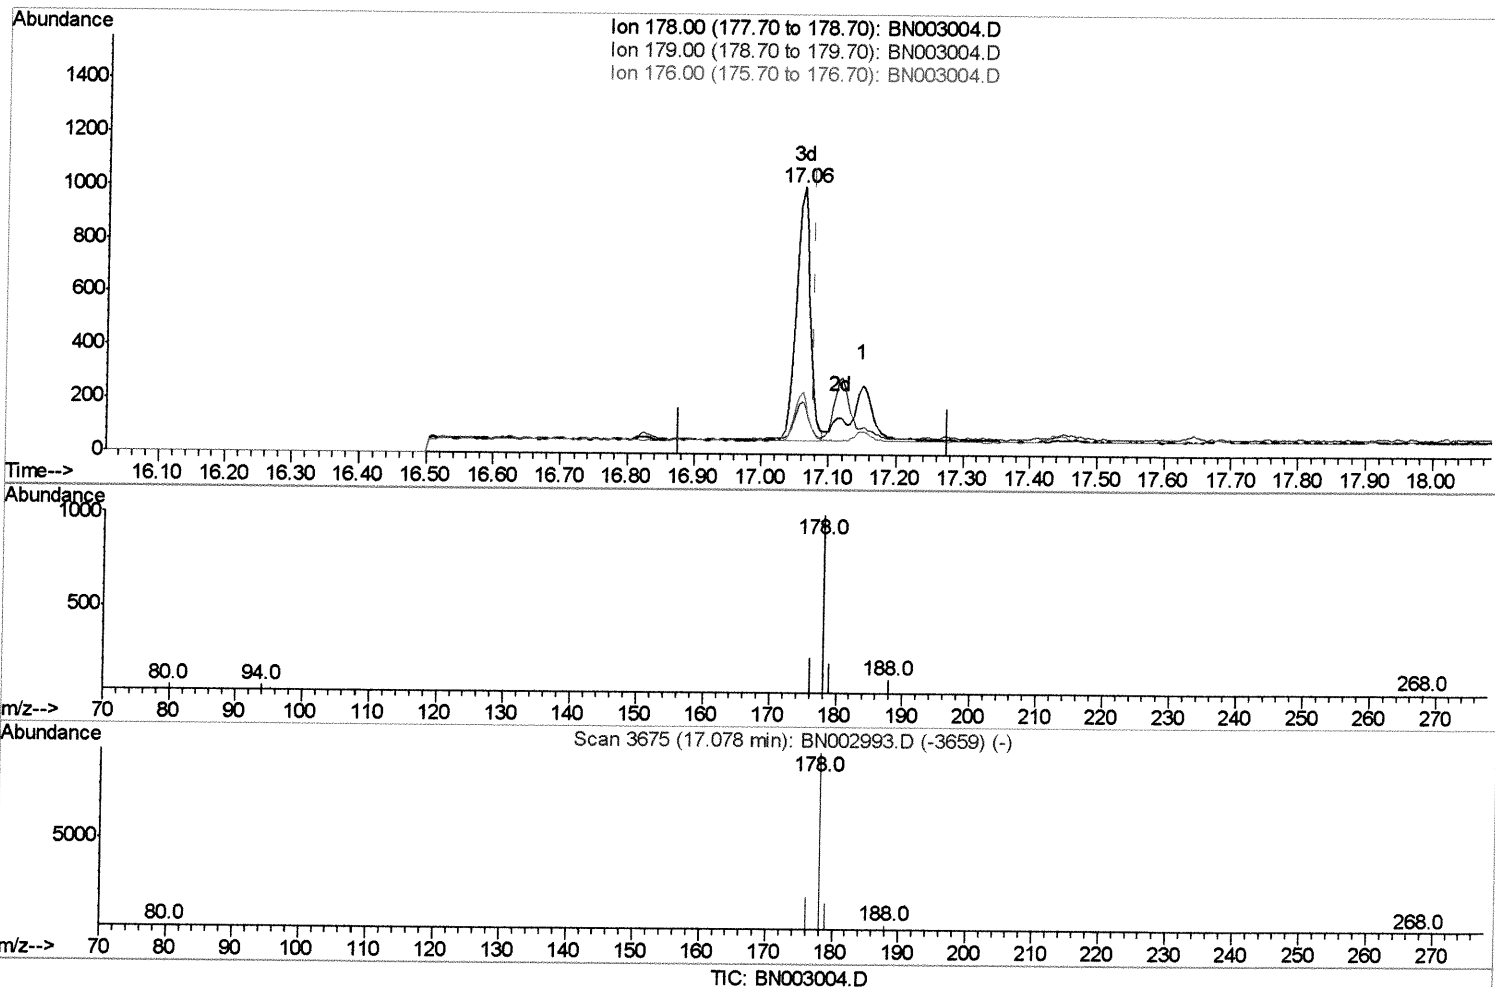

(12) Phenanthrene

17.061min (-0.017) 0.06ng/ul m

5310/10/18

response 1346

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	19.94#
176.00	19.30	23.43#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
Data File : BN003004.D
Acq On : 09 Oct 2018 01:12
Operator : MJ/SJ
Sample : J5115-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC15

Manual Integrations
APPROVED

Sohil
10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 09 01:14:49 2018
Response via : Initial Calibration

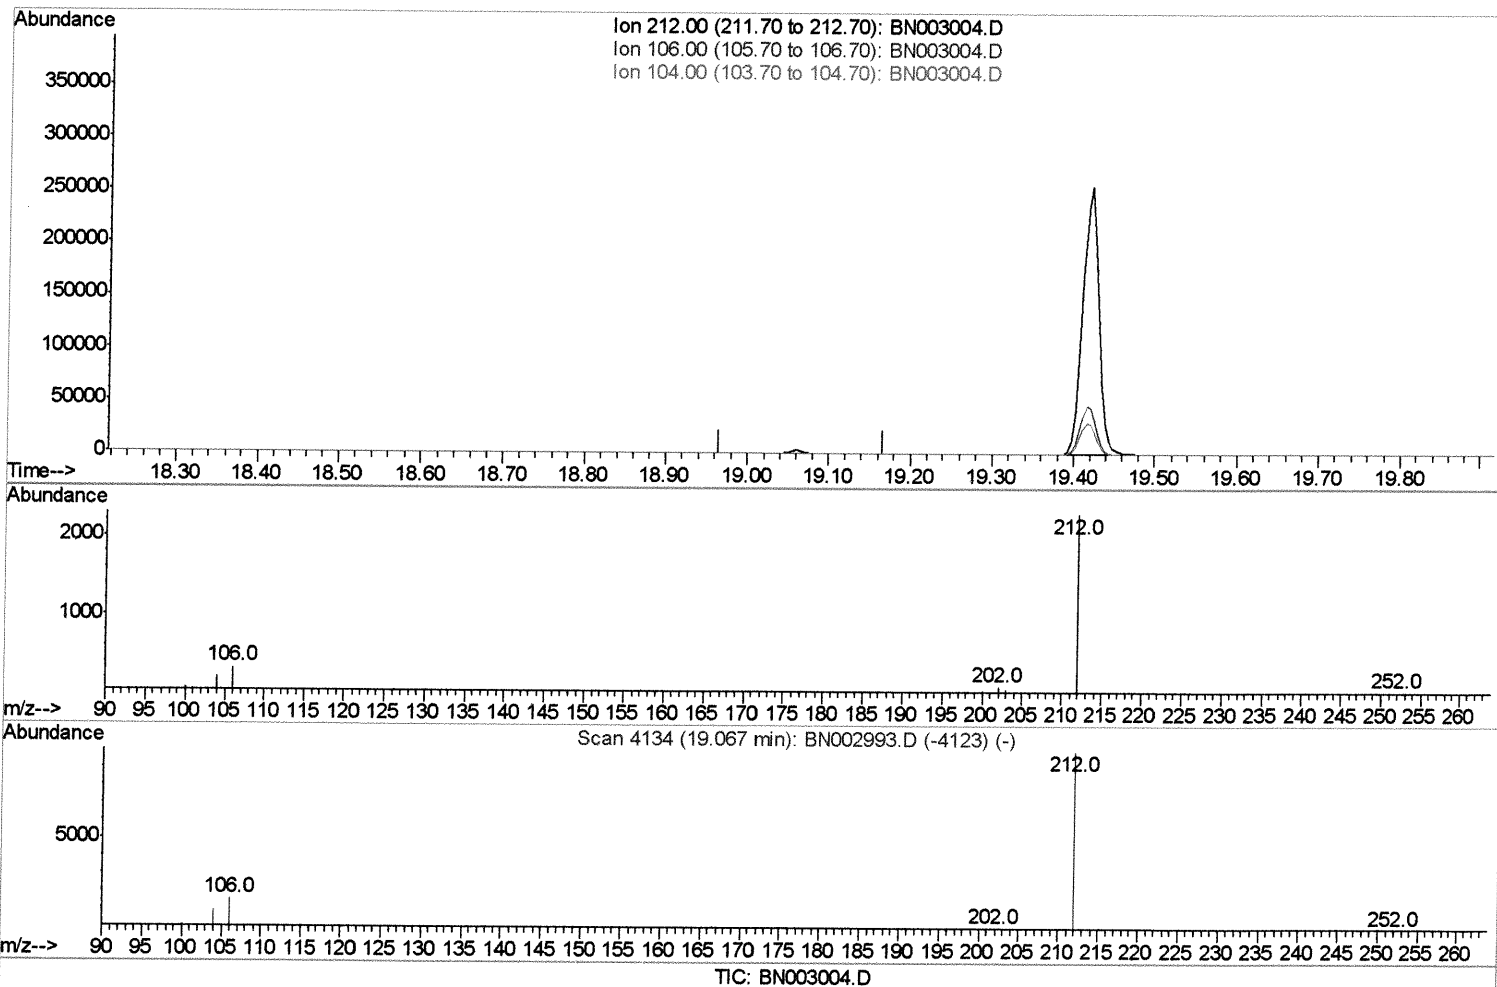

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

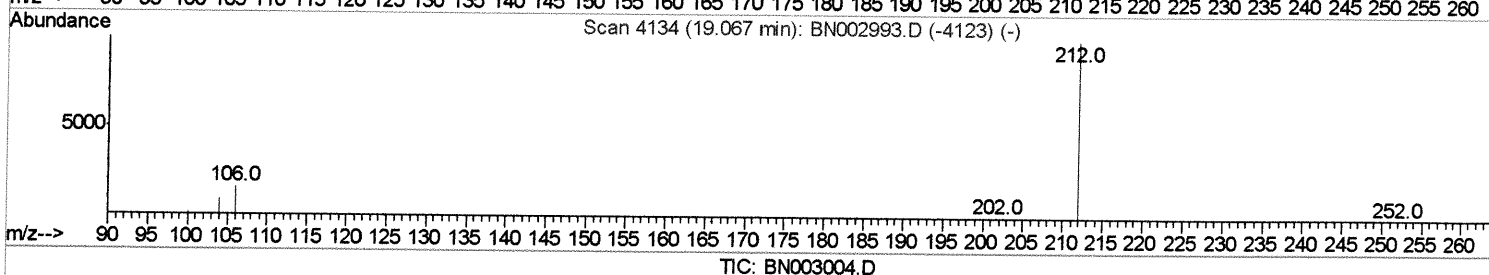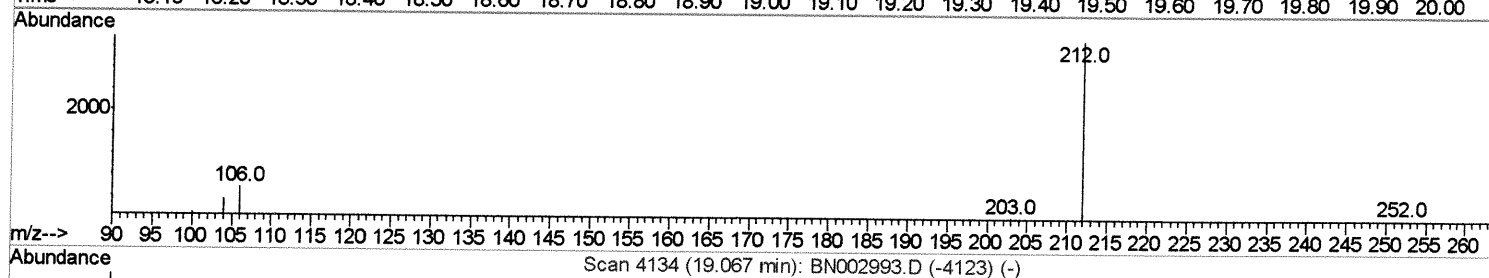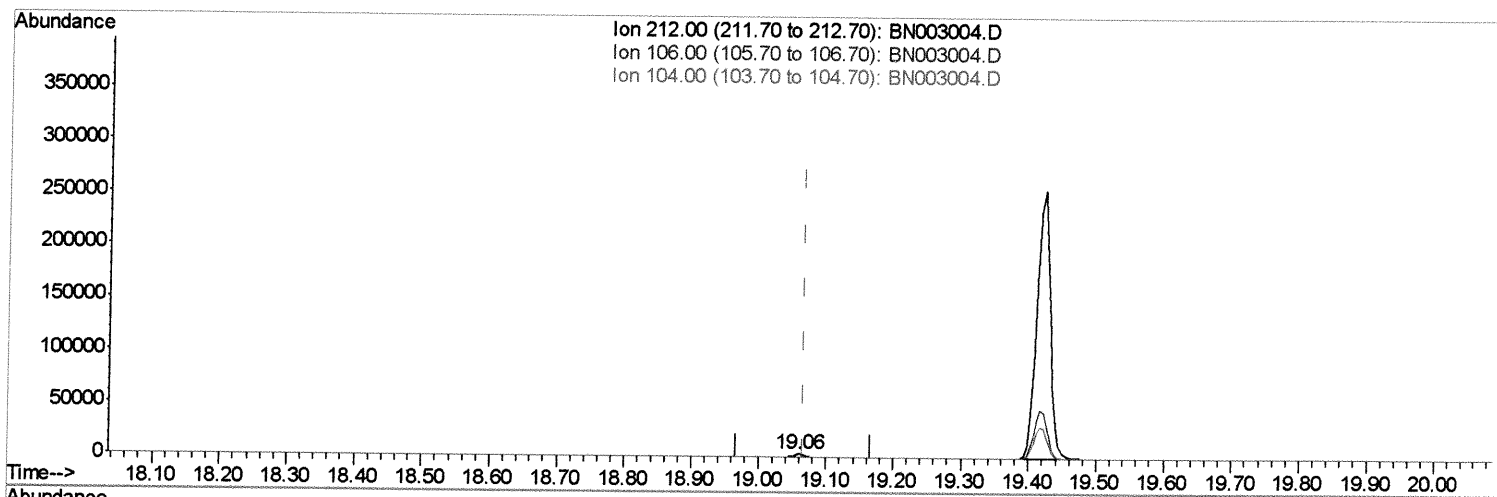

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.21ng/ul m

SS 10/10/18

response 4767

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

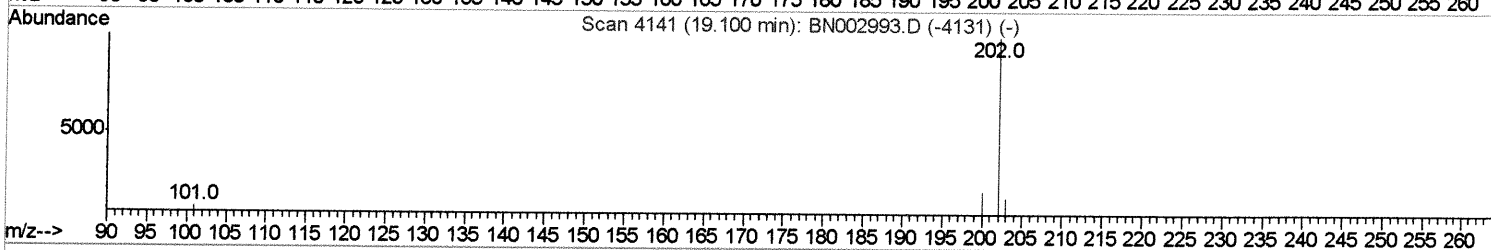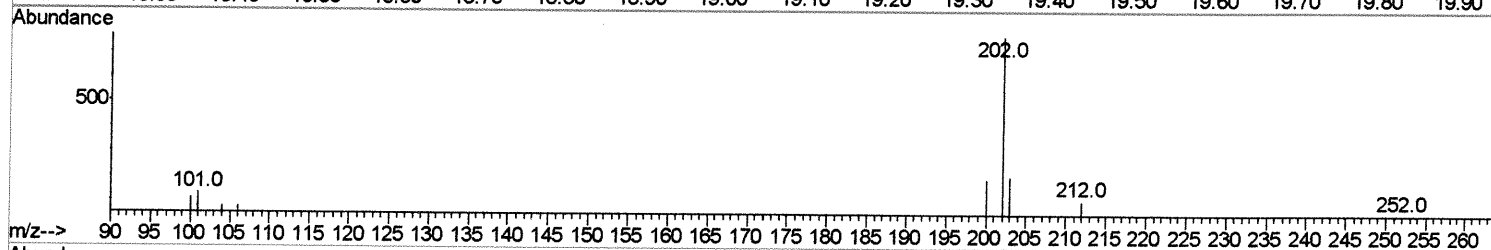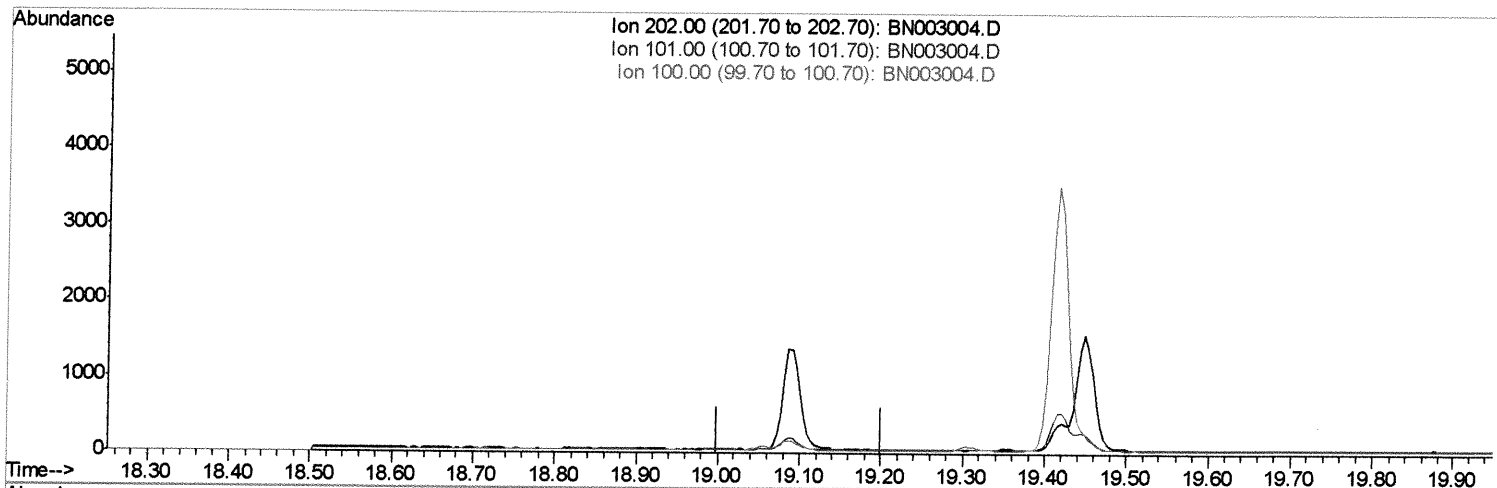

TIC: BN003004.D

(15) Fluoranthene (C)

19.100min (-19.100) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
Data File : BN003004.D
Acq On : 09 Oct 2018 01:12
Operator : MJ/SJ
Sample : J5115-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC15

Manual Integrations
APPROVED

Sohil
10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 09 01:14:49 2018
Response via : Initial Calibration

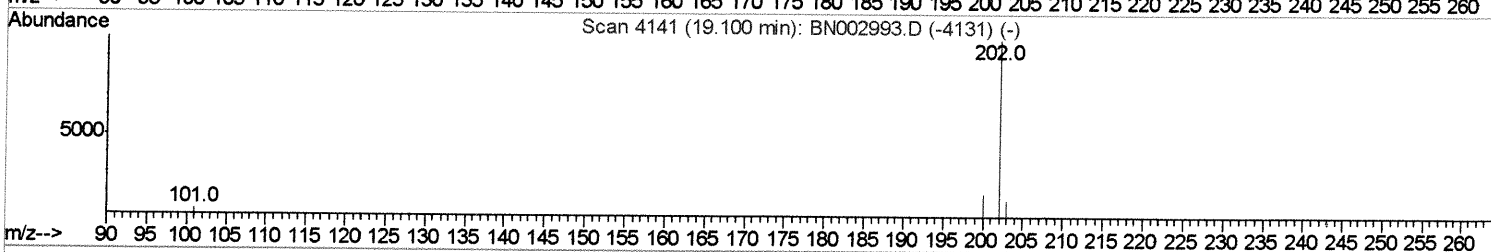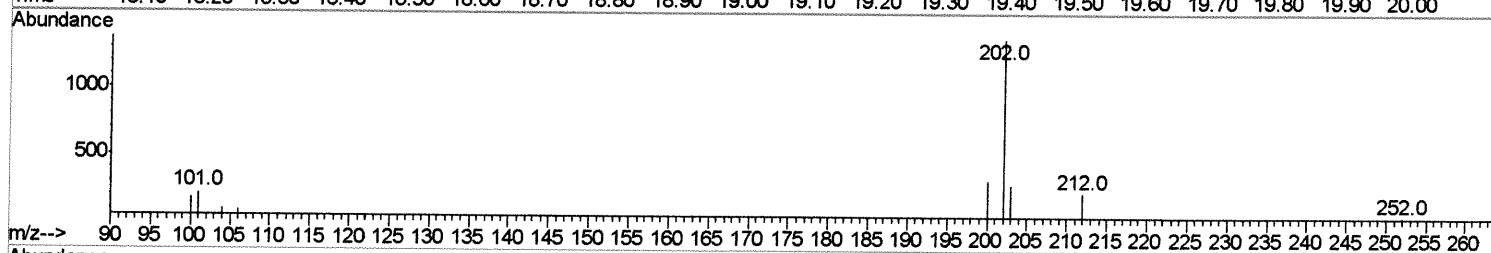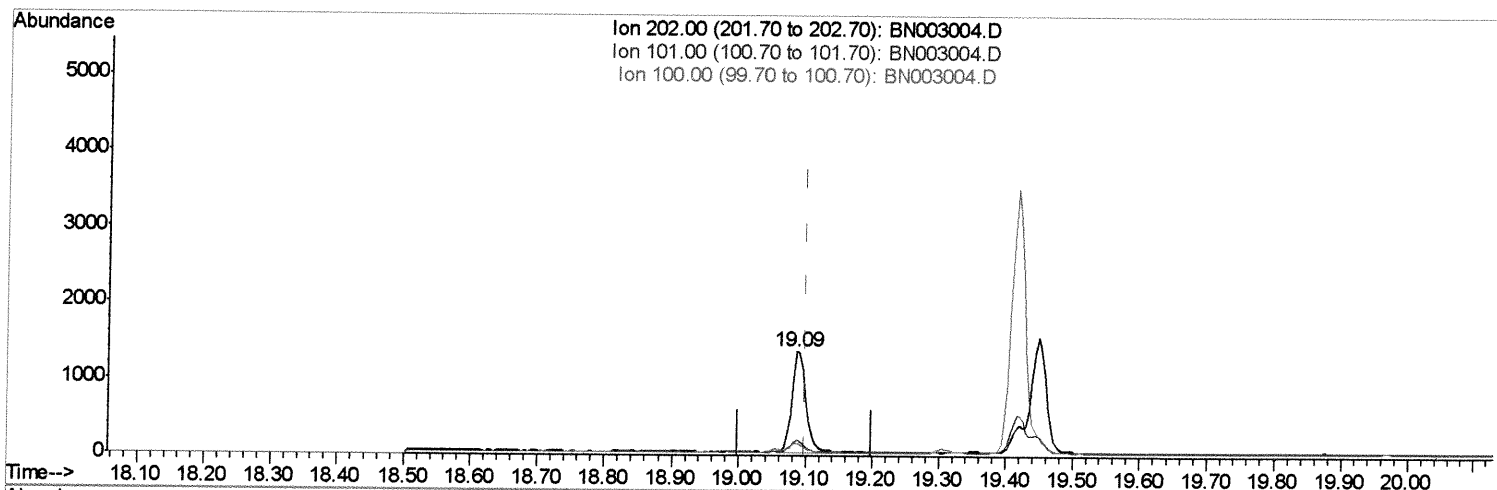

TIC: BN003004.D

(15) Fluoranthene (C)

19.086min (-0.014) 0.07ng/ul m

33 10/10/18

response 1944

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	15.54
100.00	9.10	12.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

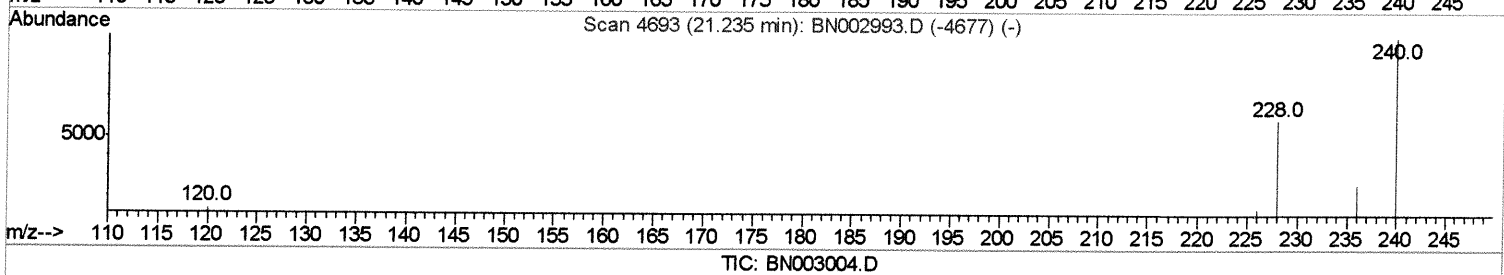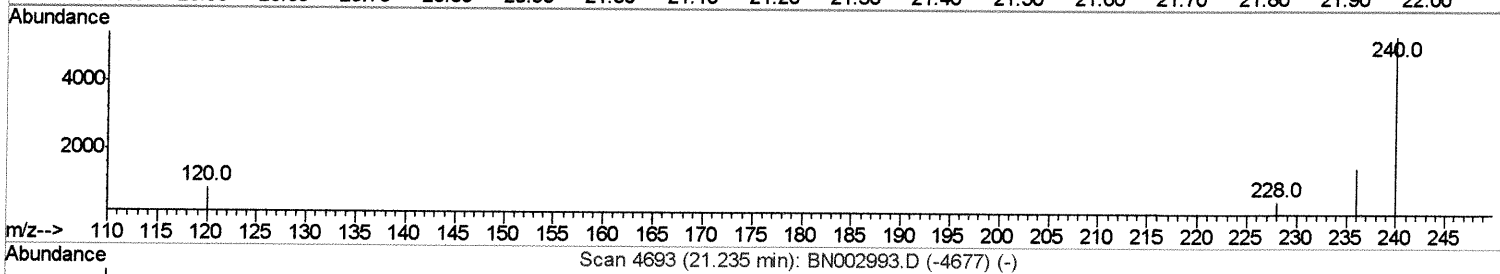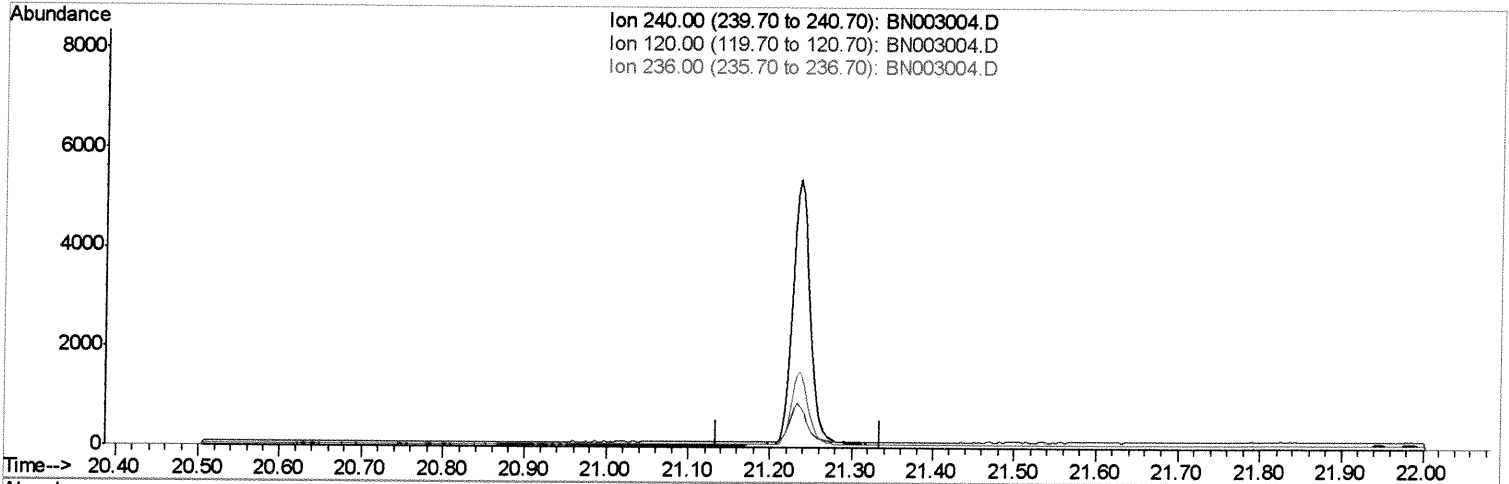

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ui

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

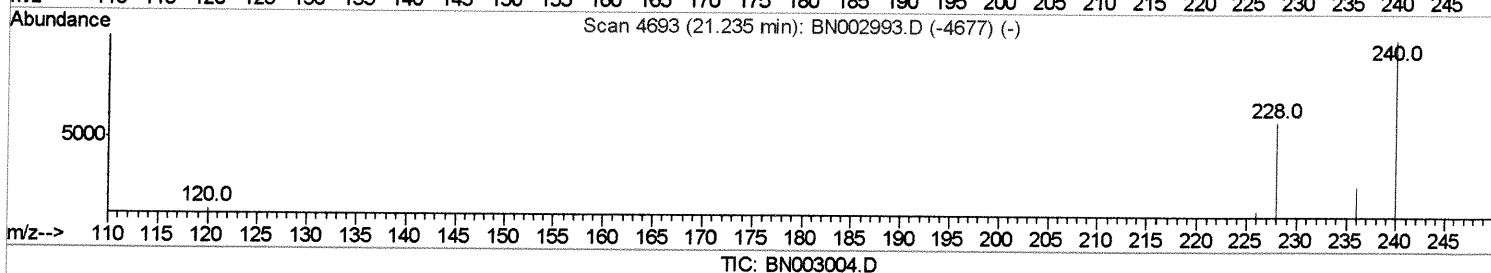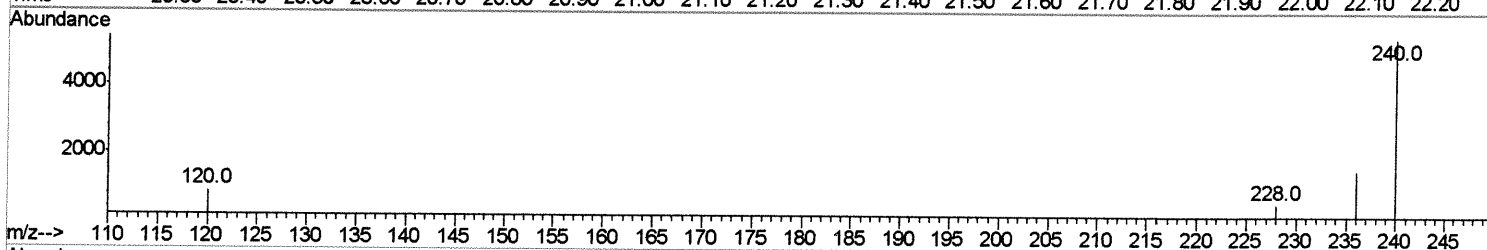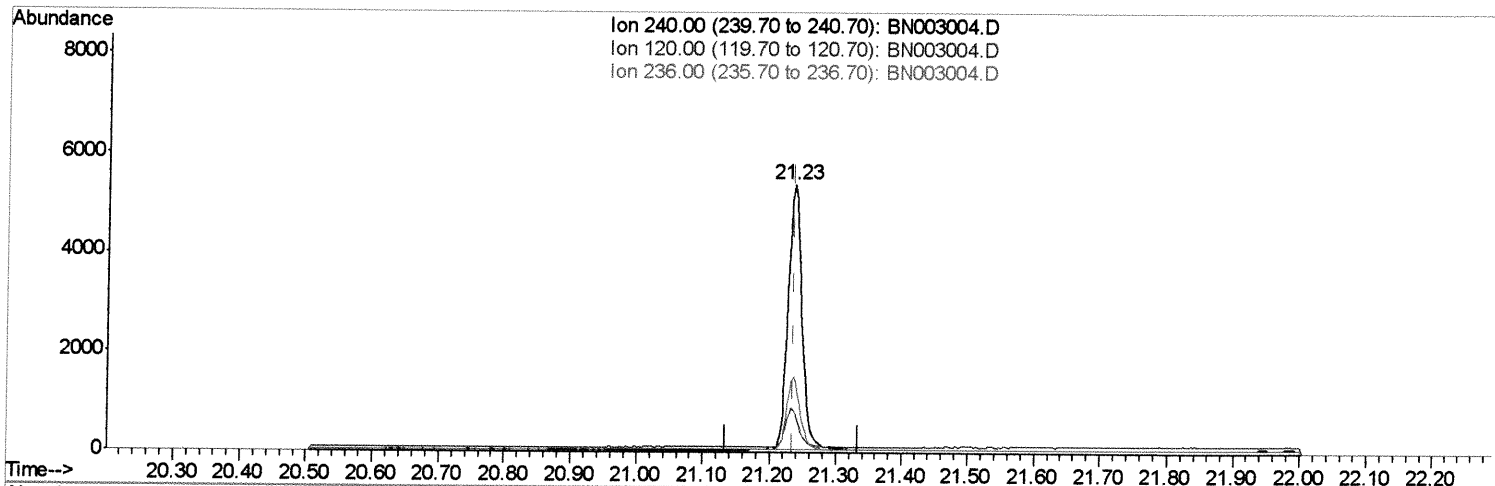

(16) Chrysene-d12 (I)

21.235min (0.000) 0.40ng/ul m

SJ 10/10/18

response 7813

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	16.07
236.00	28.10	28.61
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

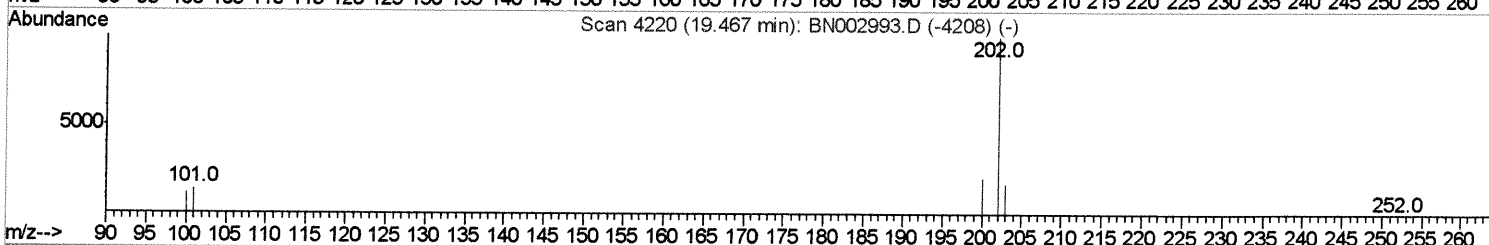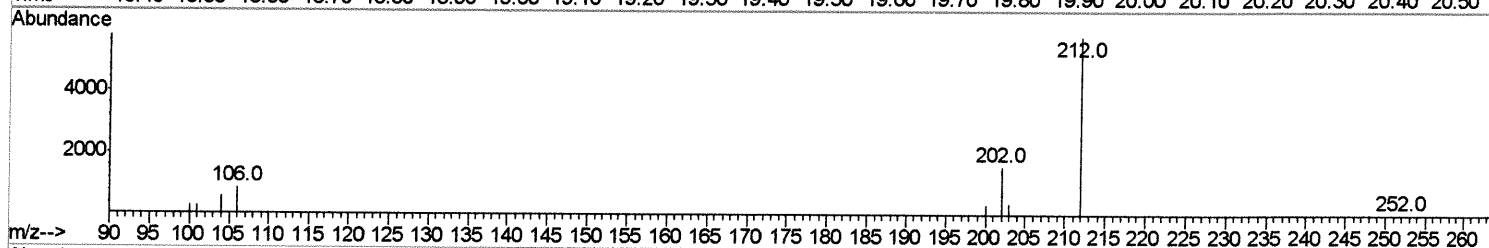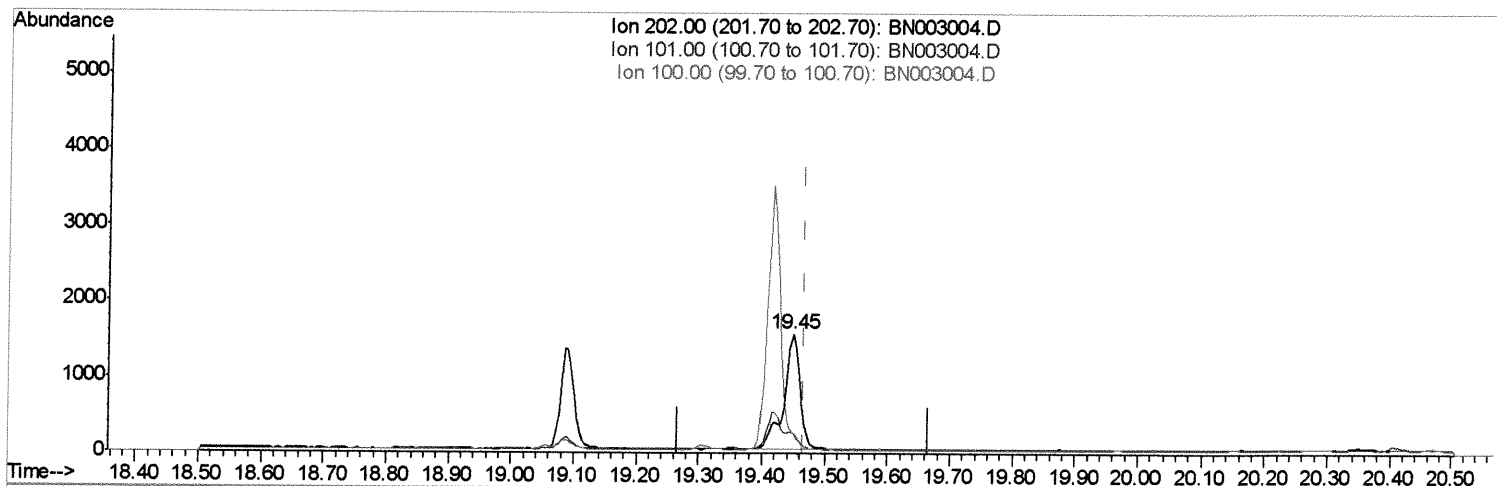

TIC: BN003004.D

(17) Pyrene

19.448min (-0.019) 0.09ng/ul

response 2744

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	17.50
100.00	12.40	17.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

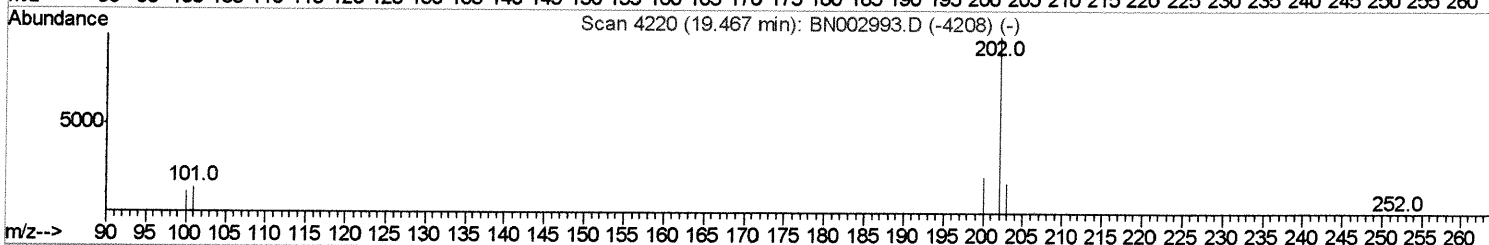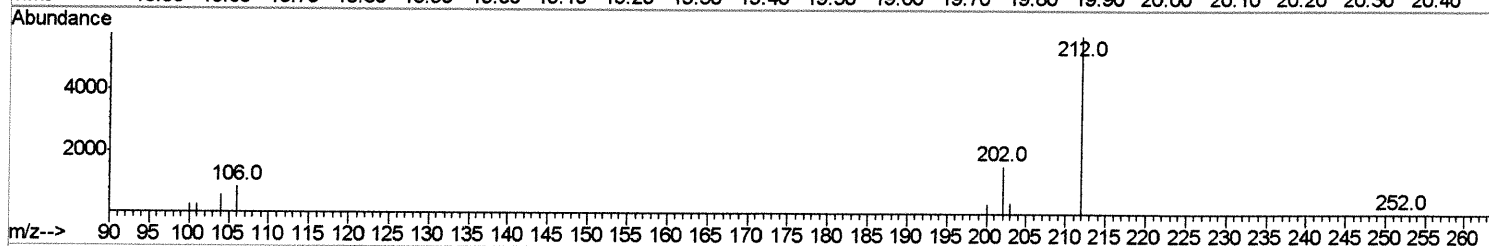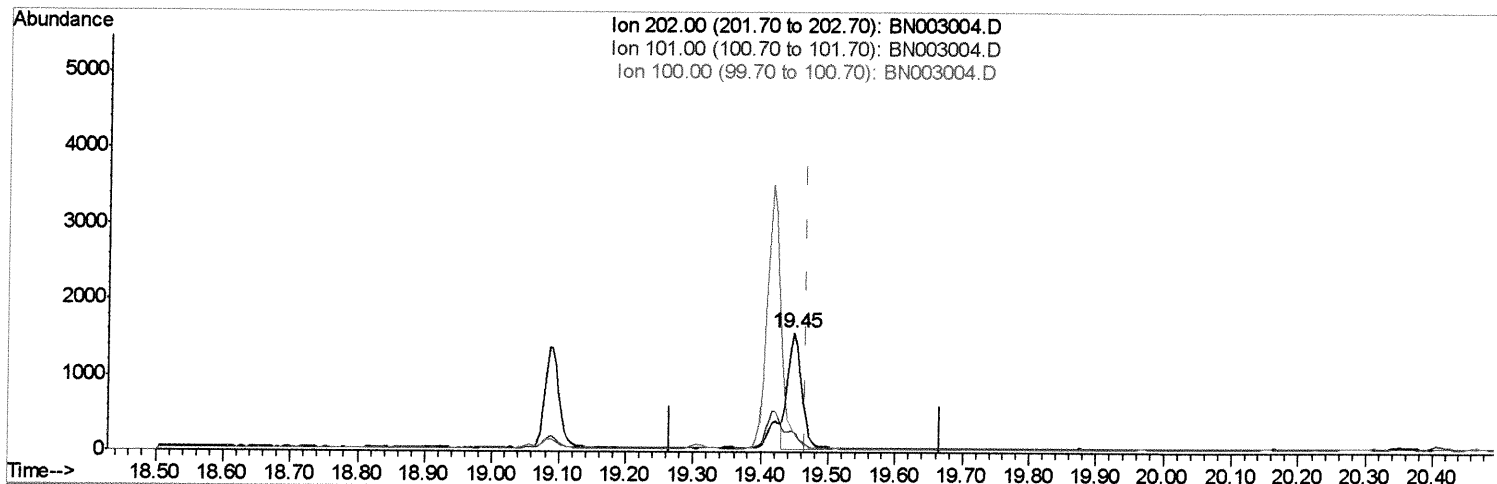

TIC: BN003004.D

(17) Pyrene

19.448min (-0.019) 0.07ng/ul m

5110/10/18

response 2211

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	17.50
100.00	12.40	17.44#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

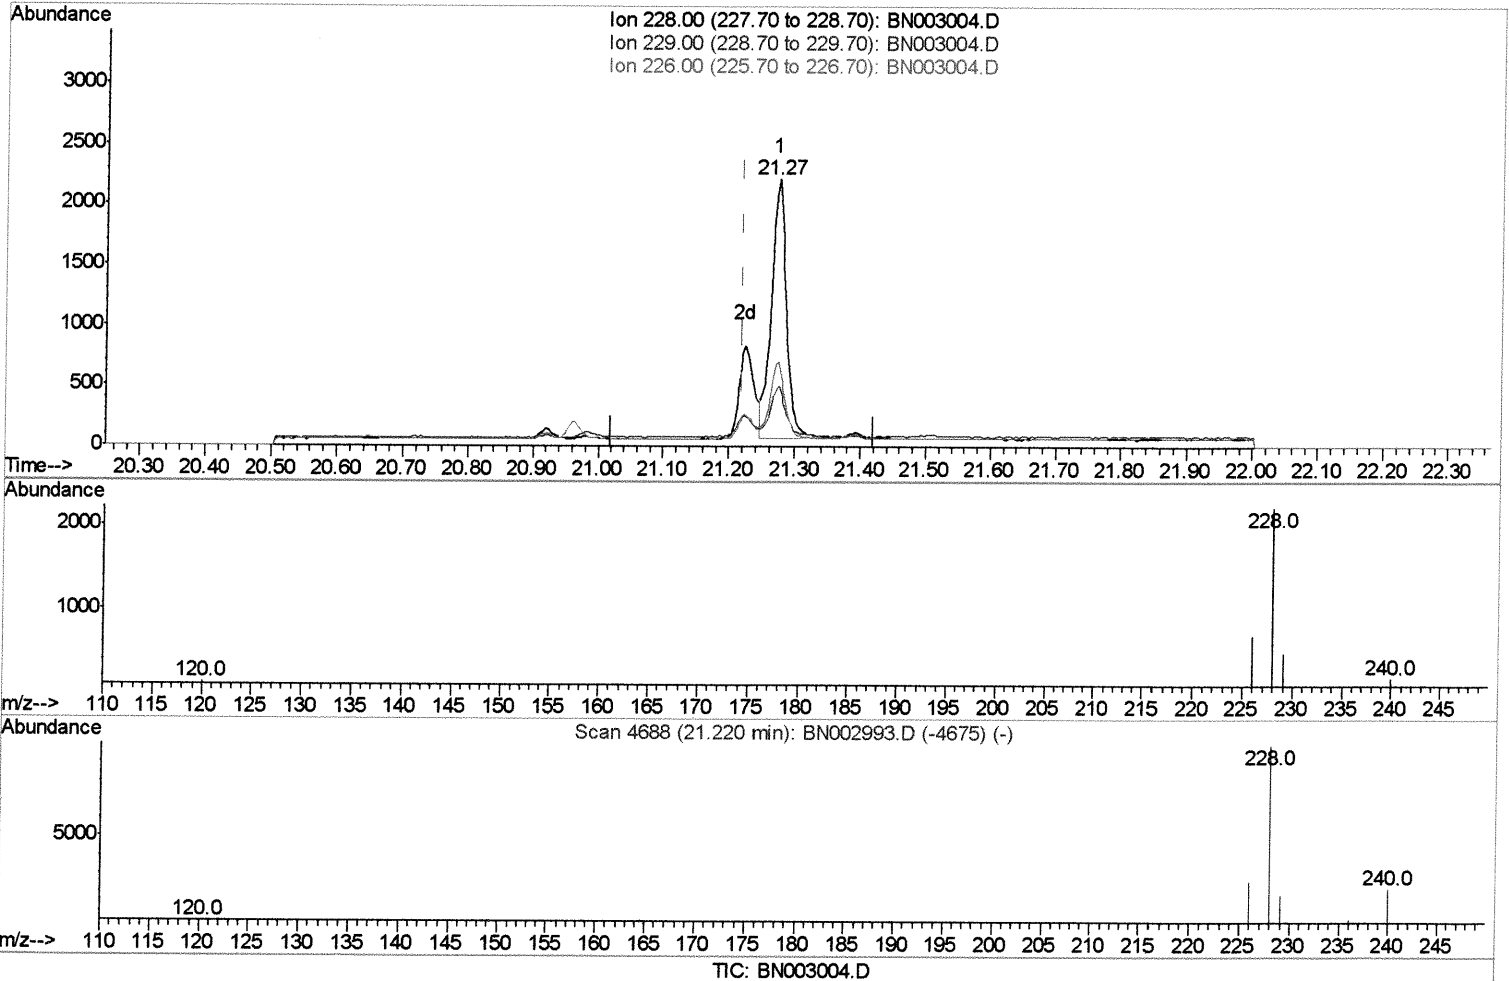

(18) Benzo(a)anthracene
 21.273min (+0.053) 0.14ng/ul
 response 3449

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	22.90
226.00	27.90	31.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

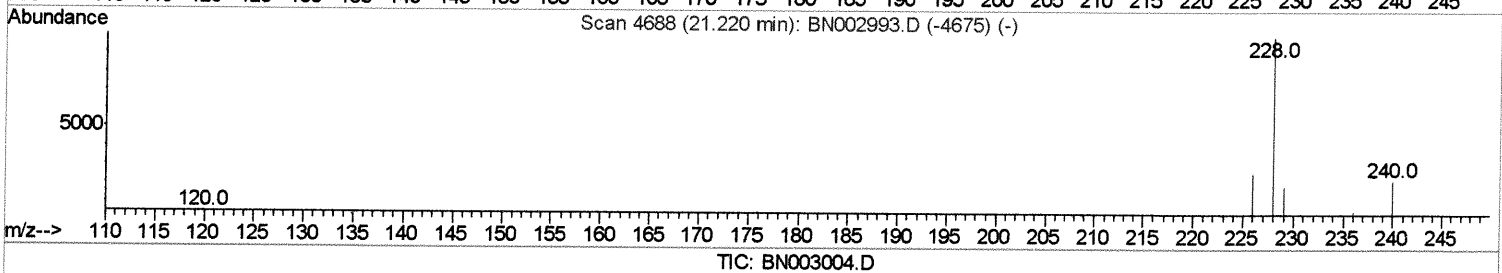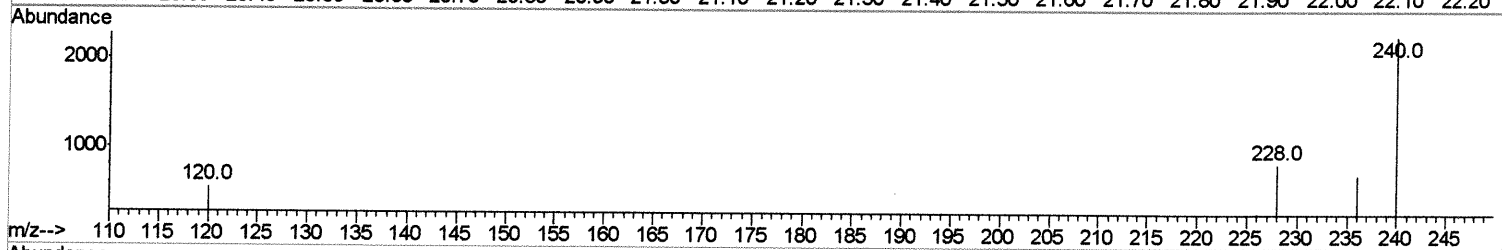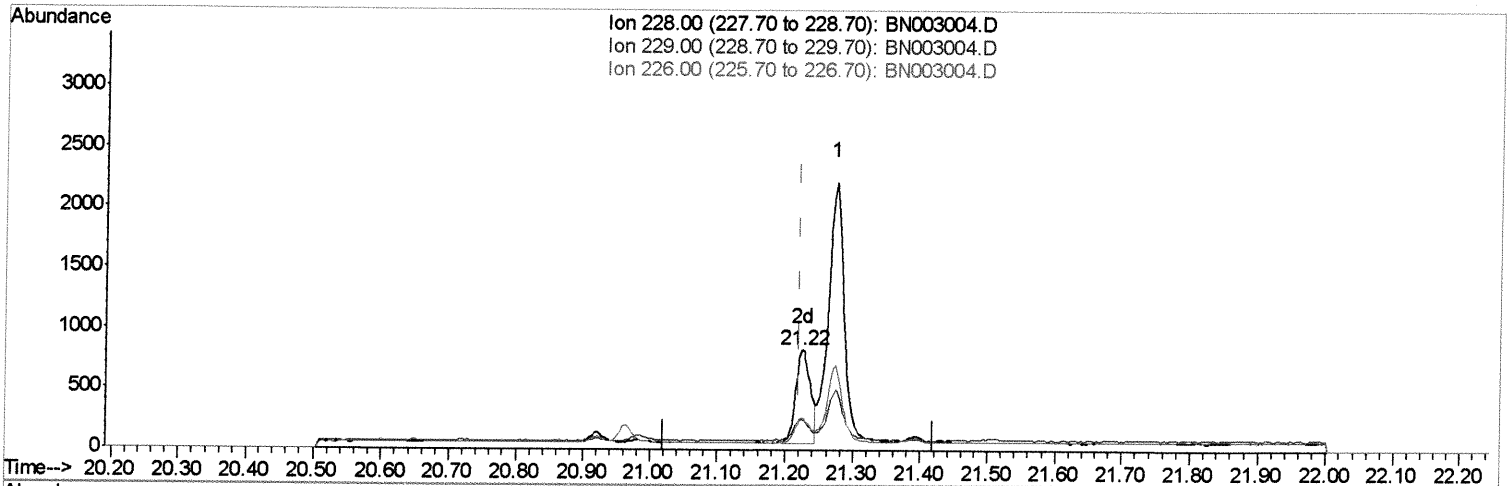

(18) Benzo(a)anthracene

21.223min (+0.003) 0.05ng/ul m

23 10/10/18

response 1181

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	31.53#
226.00	27.90	32.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

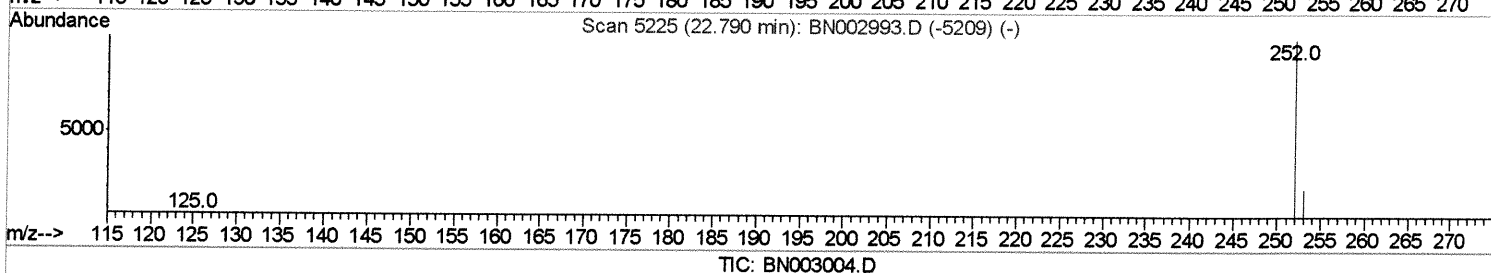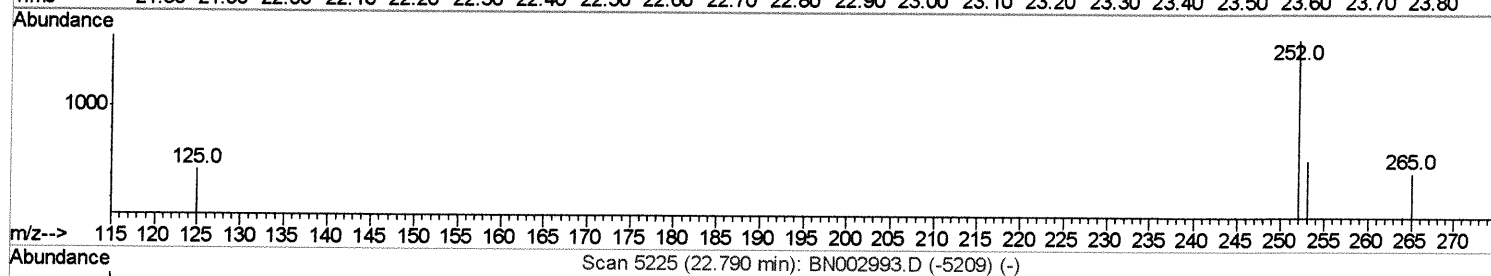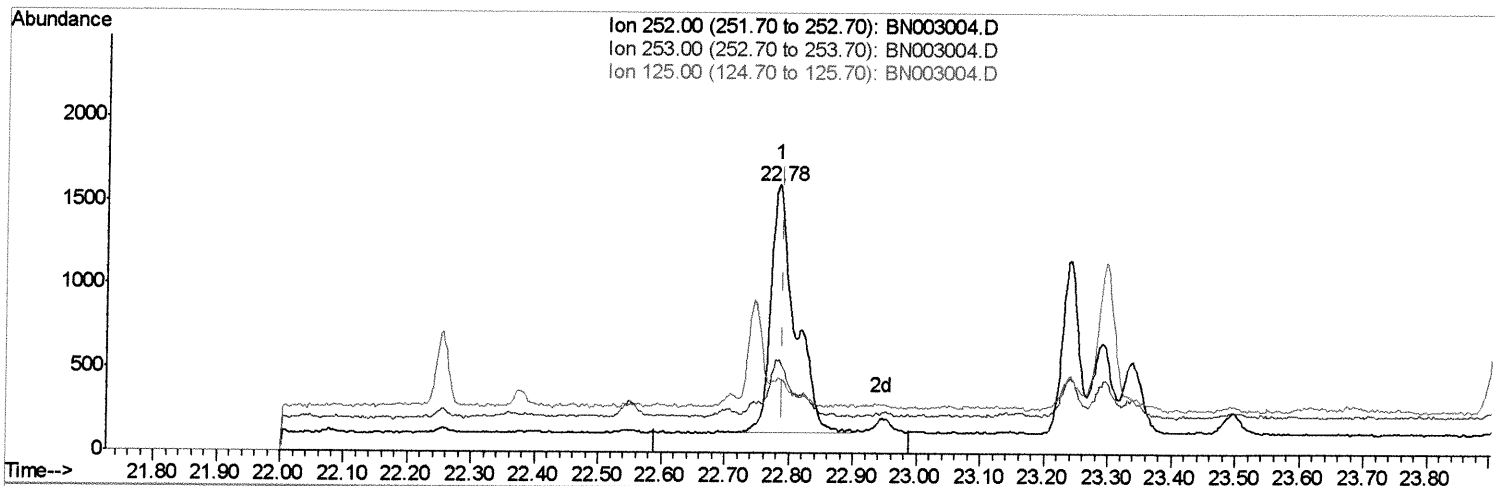

(21) Benzo(b)fluoranthene
 22.784min (-0.006) 0.16ng/ul
 response 4001

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	34.98
125.00	17.10	28.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

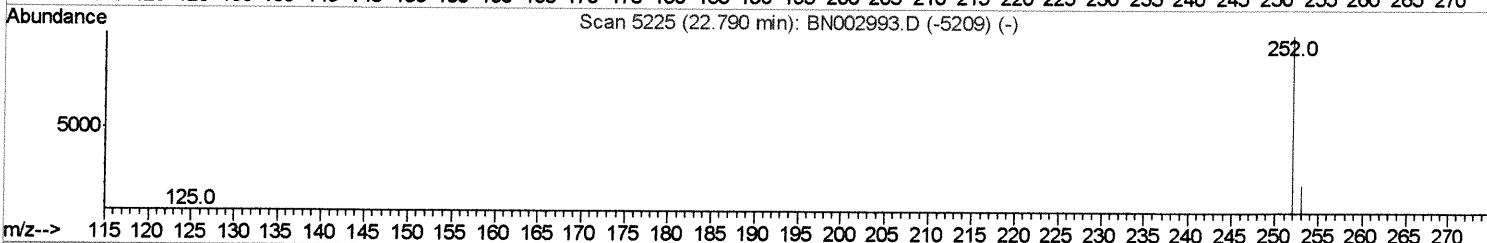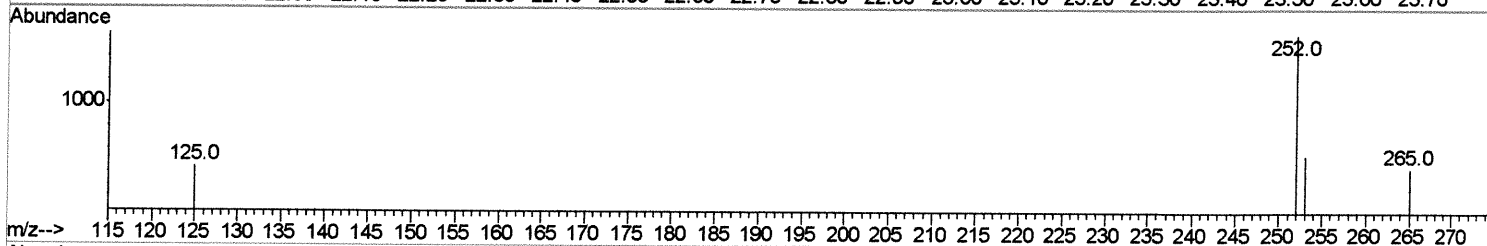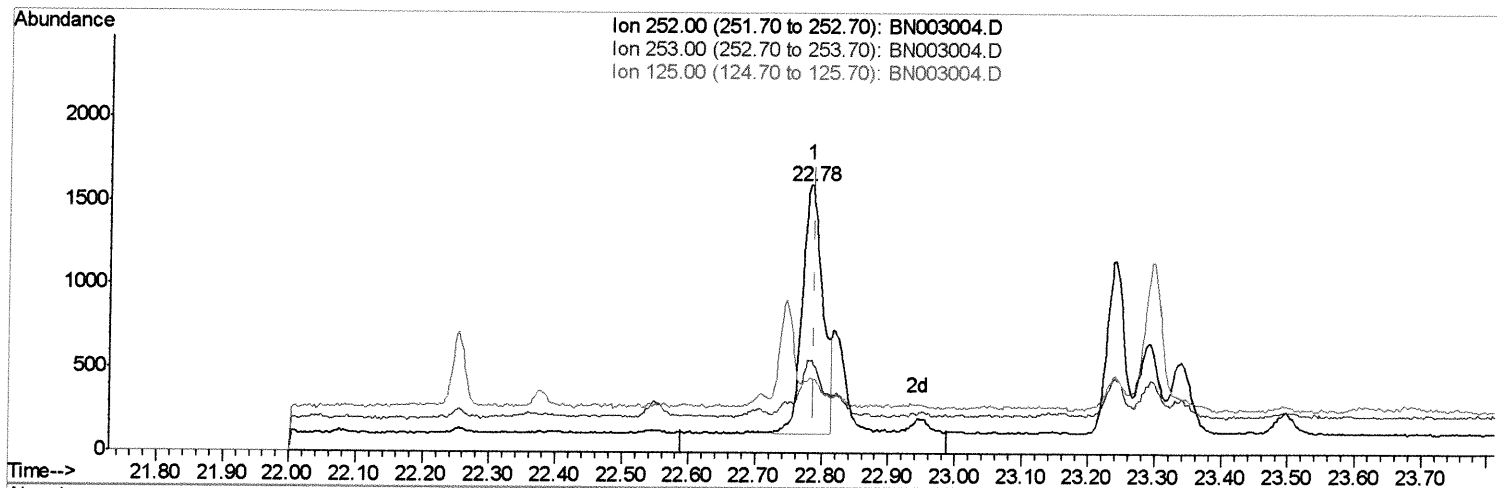

TIC: BN003004.D

(21) Benzo(b)fluoranthene

22.784min (-0.006) 0.13ng/ul m

SJ 10/10/18

response 3176

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	34.98
125.00	17.10	28.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

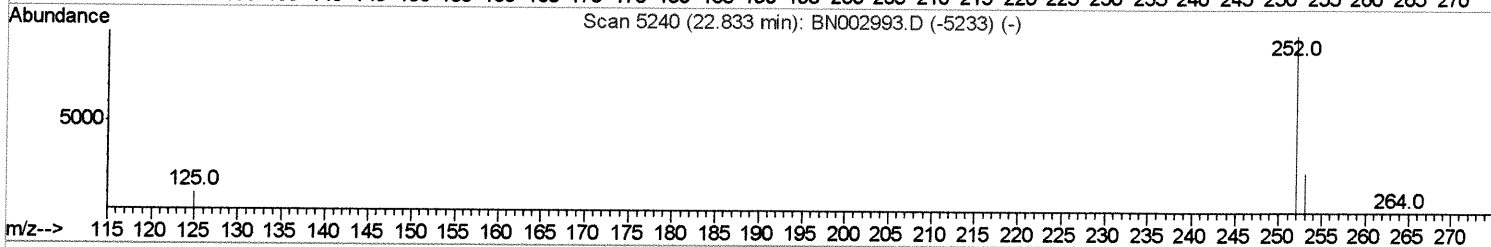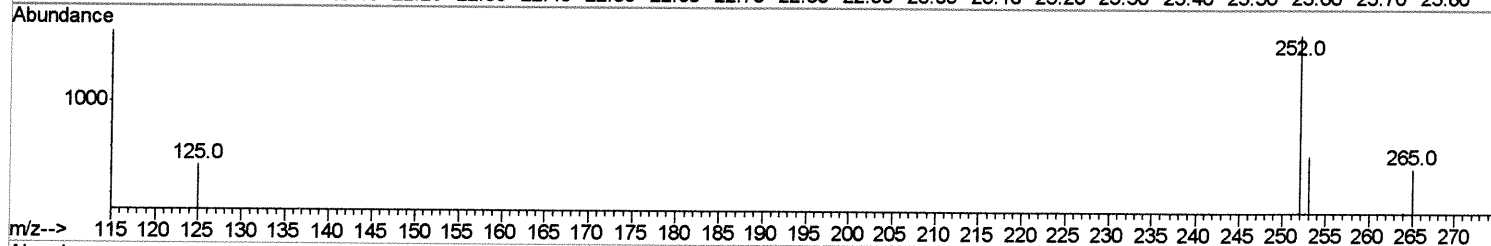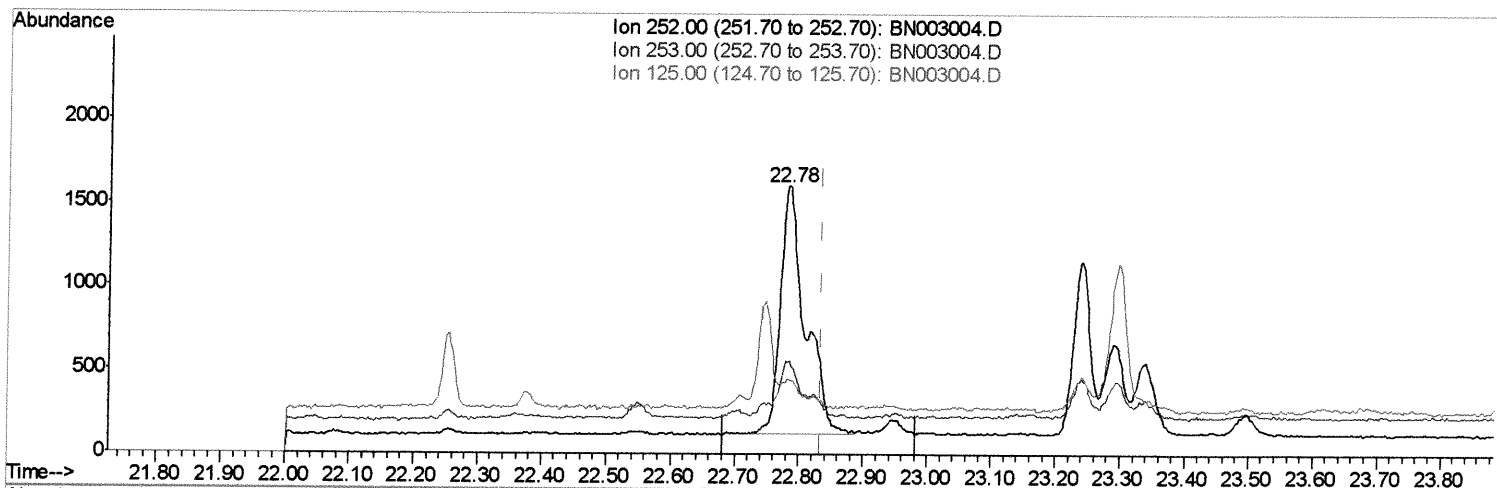

TIC: BN003004.D

(22) Benzo(k)fluoranthene

22.784min (-0.050) 0.15ng/ul

response 3989

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	34.98#
125.00	17.60	28.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:03:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

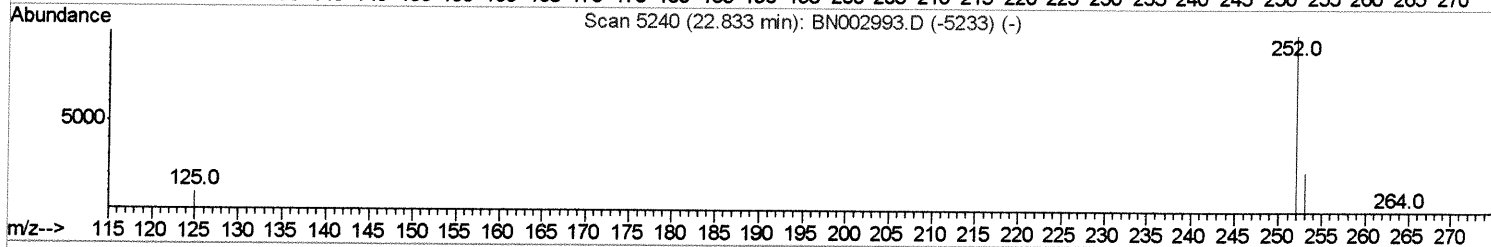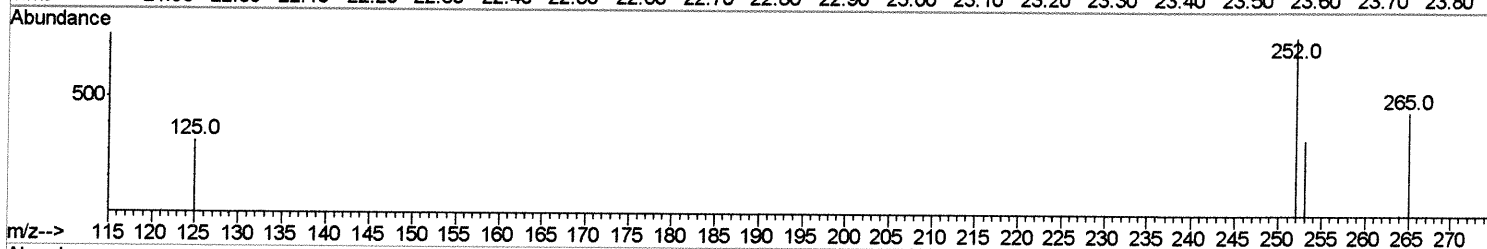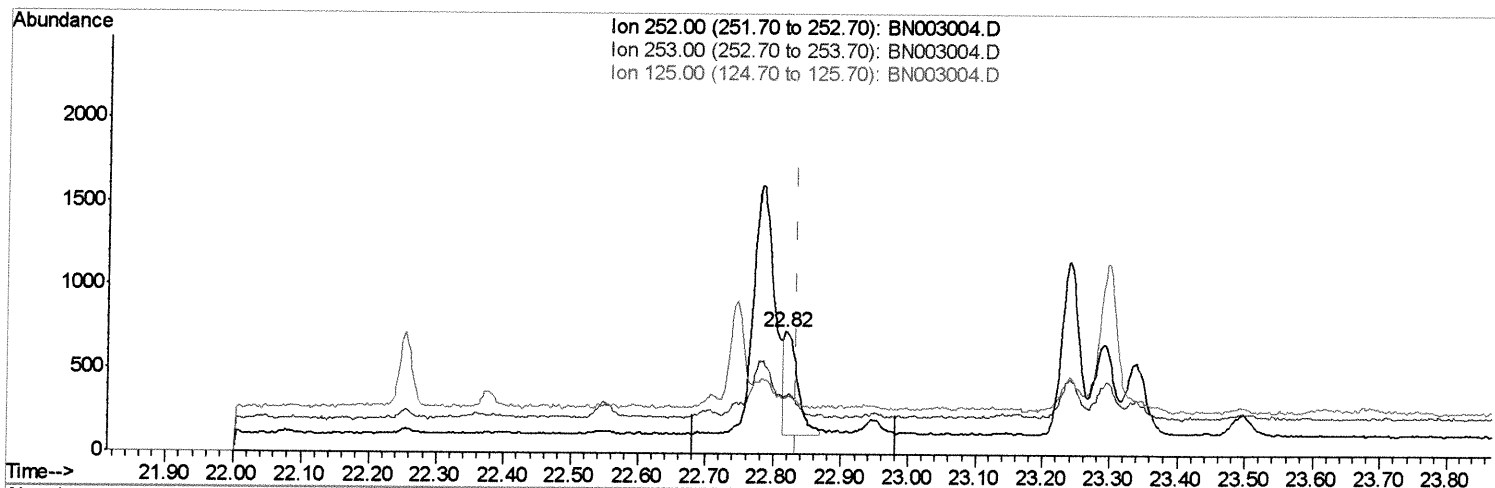

TIC: BN003004.D

(22) Benzo(k)fluoranthene

22.816min (-0.018) 0.03ng/ul m

210/10/18

response 840

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	47.74#
125.00	17.60	45.83#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003004.D
 Acq On : 09 Oct 2018 01:12
 Operator : MJ/SJ
 Sample : J5115-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC15

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:58 PM

Quant Time: Oct 09 02:05:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 01:14:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1367	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.40	136	5795	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3393	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	7965m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	7813m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6999	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.03	152	1761	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	4767m	0.21	ng/ul	0.00

Target Compounds

					Ovalue
5) 2-Methylnaphthalene	12.11	142	210	0.021	ng/ul 93
12) Phenanthrene	17.06	178	1346m	0.061	ng/ul
15) Fluoranthene	19.09	202	1944m	0.075	ng/ul
17) Pyrene	19.45	202	2211m	0.073	ng/ul
18) Benzo(a)anthracene	21.22	228	1181m	0.047	ng/ul
19) Chrysene	21.27	228	3453	0.135	ng/ul 96
21) Benzo(b)fluoranthene	22.78	252	3176m	0.126	ng/ul
22) Benzo(k)fluoranthene	22.82	252	840m	0.032	ng/ul
24) Indeno(1,2,3-cd)pyrene	25.68	276	1004	0.039	ng/ul 99
26) Benzo(g,h,i)perylene	26.37	276	1044	0.048	ng/ul# 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed