

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:40:49 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

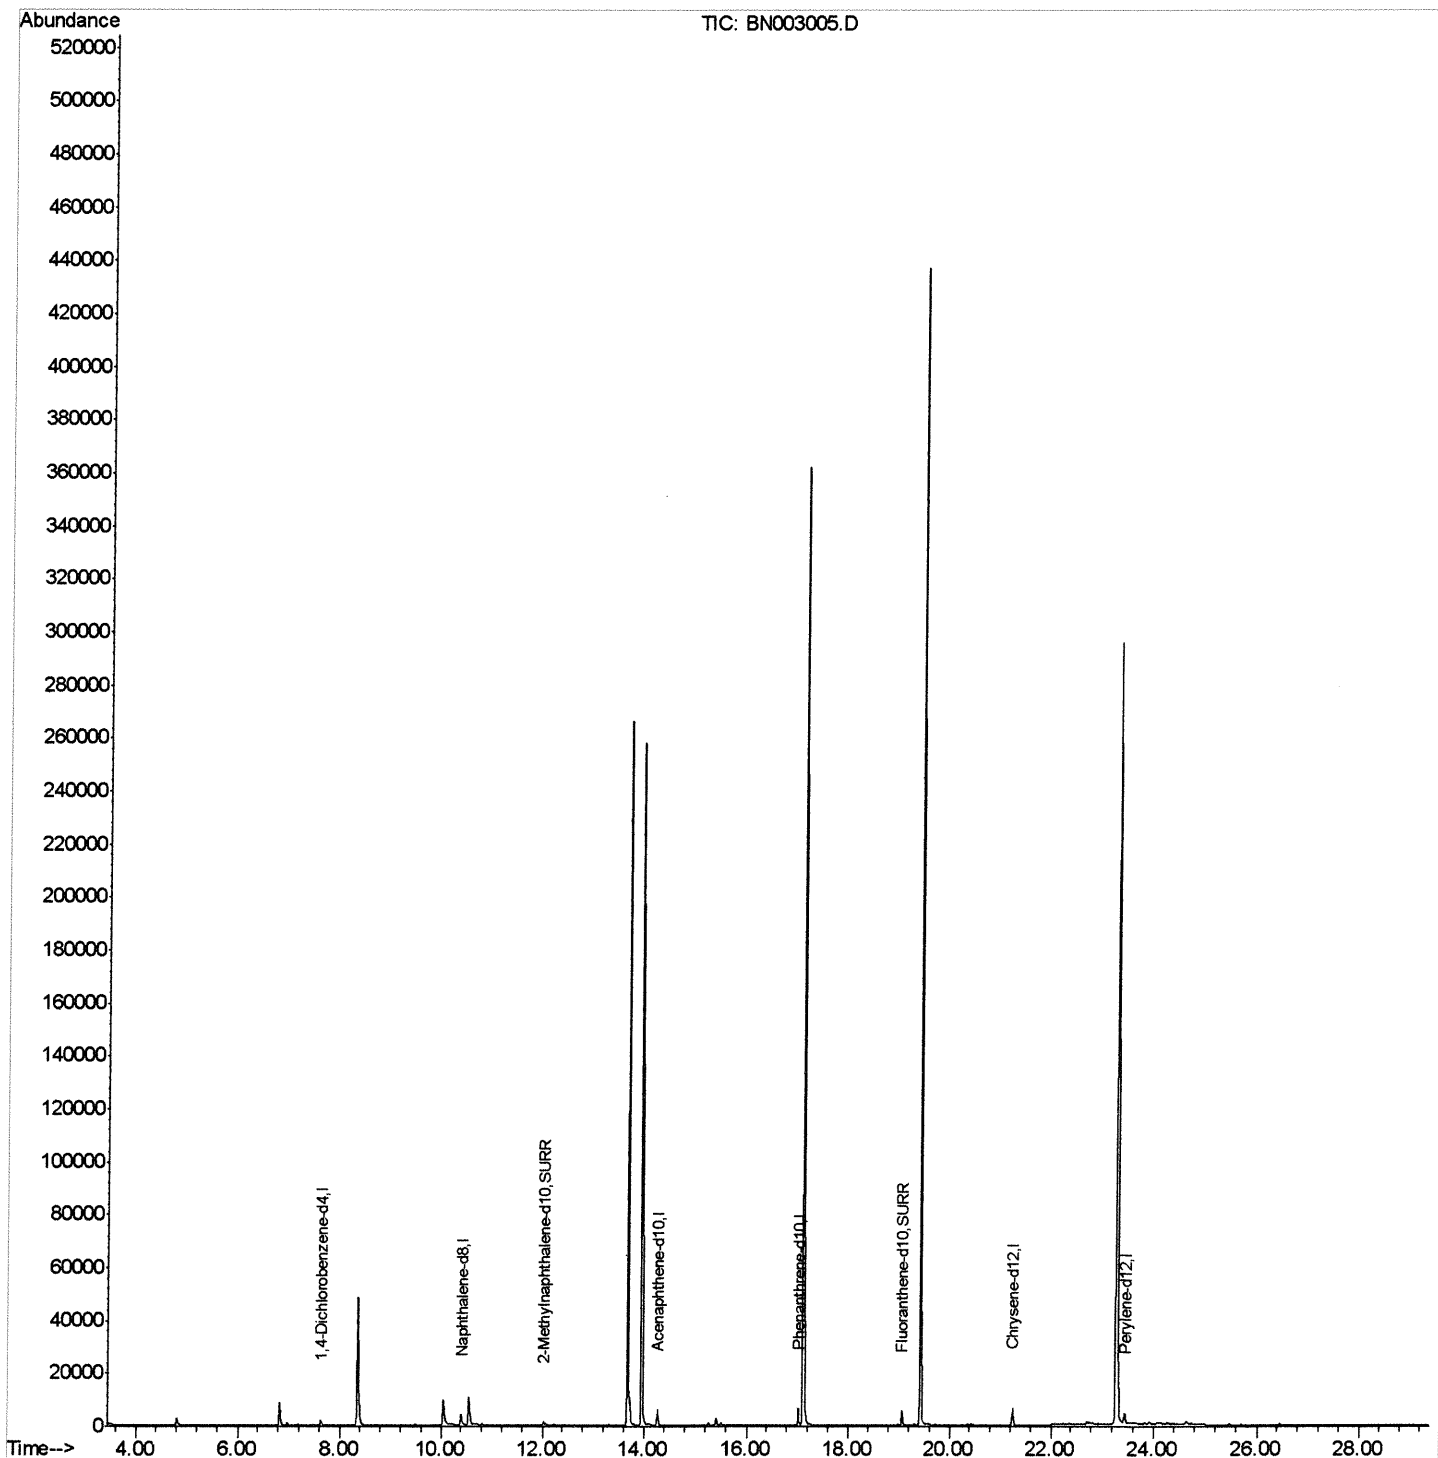

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:37:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

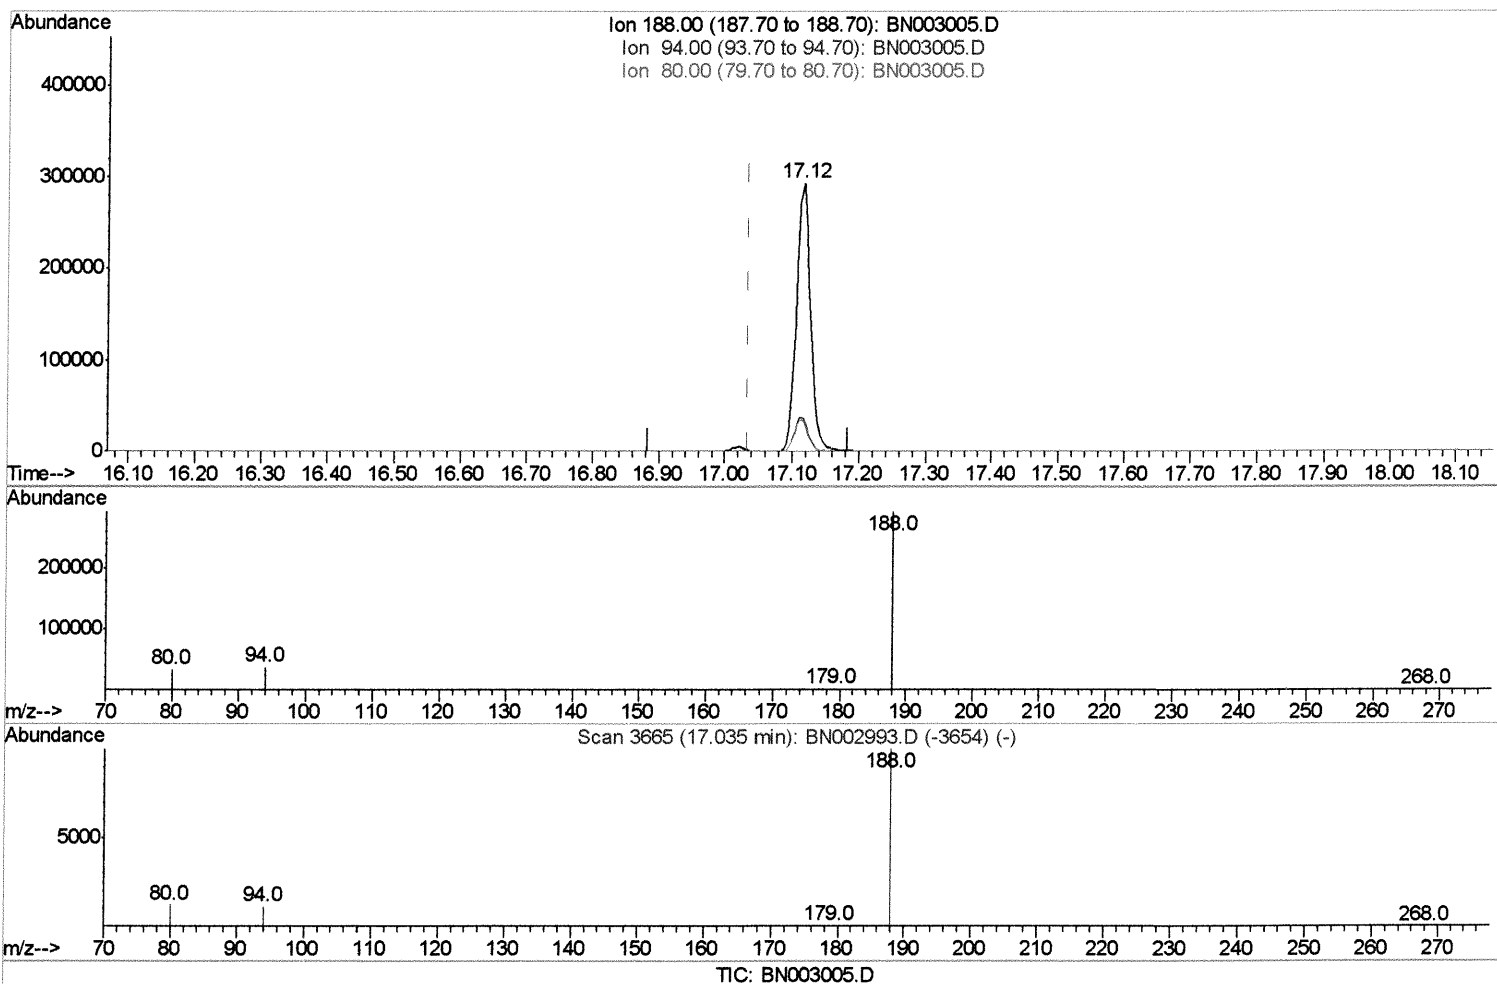

(10) Phenanthrene-d10 (I)
 17.116min (+0.080) 0.40ng/ul
 response 422997

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.48
80.00	12.70	11.31
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:37:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

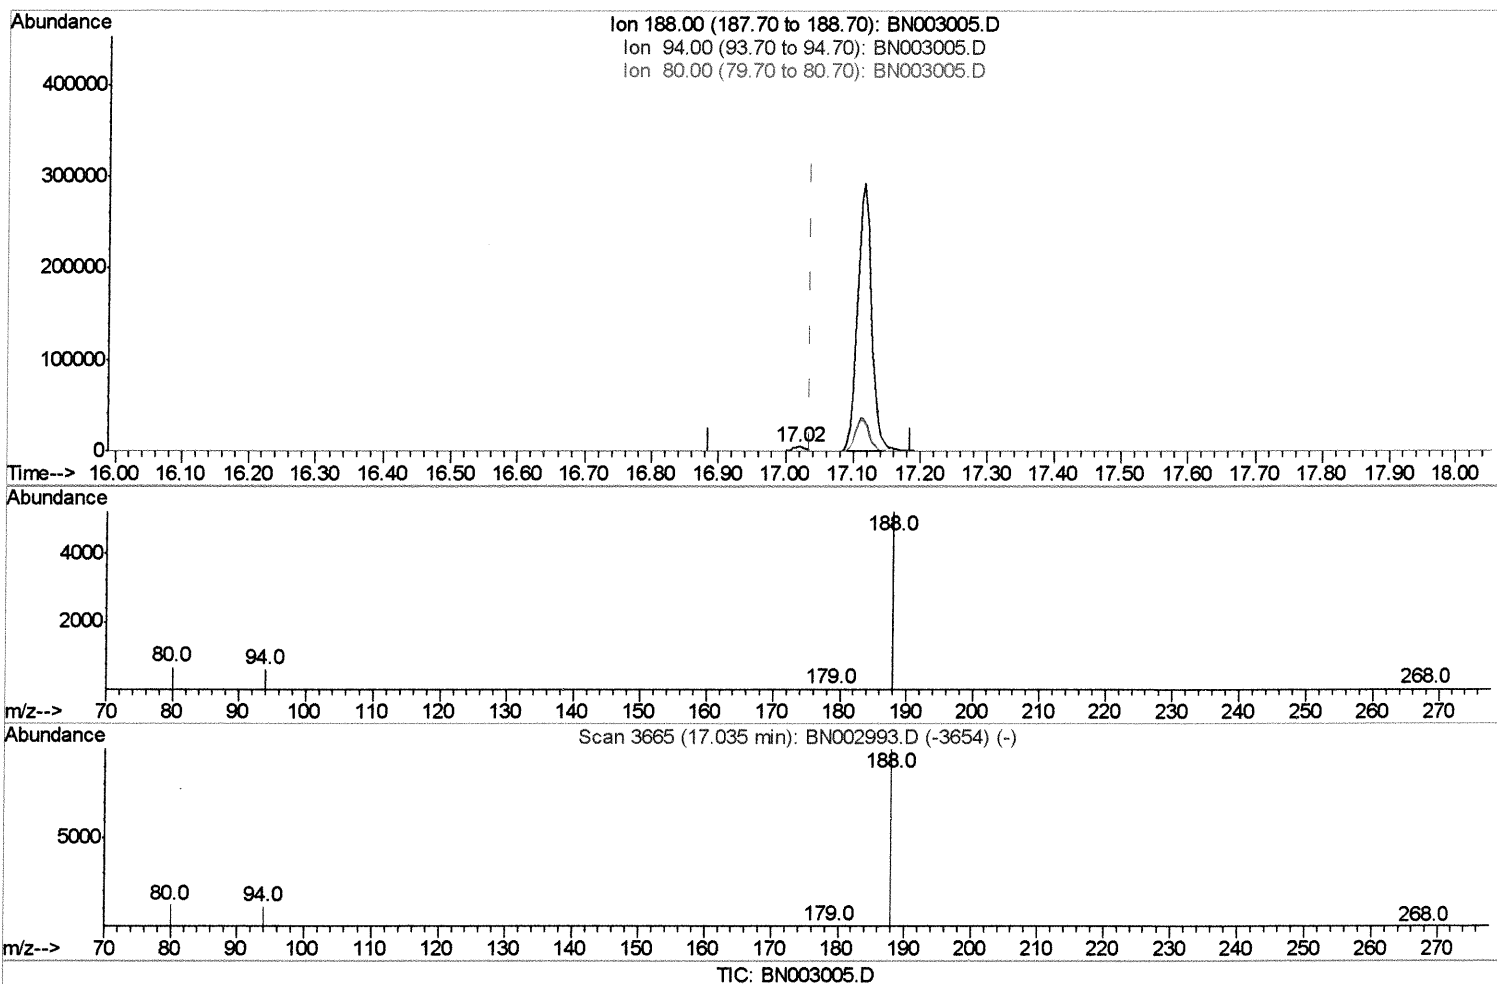

(10) Phenanthrene-d10 (I)

17.019min (-0.017) 0.40ng/ul m

5/10/10/18

response 7513

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.90
80.00	12.70	13.21
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:39:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

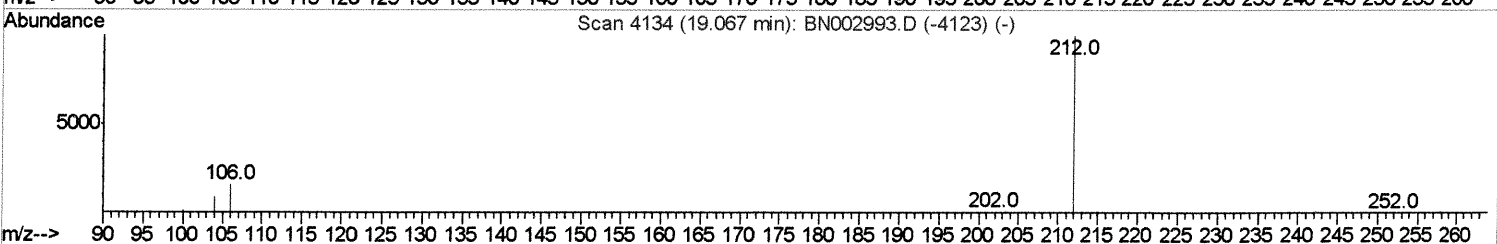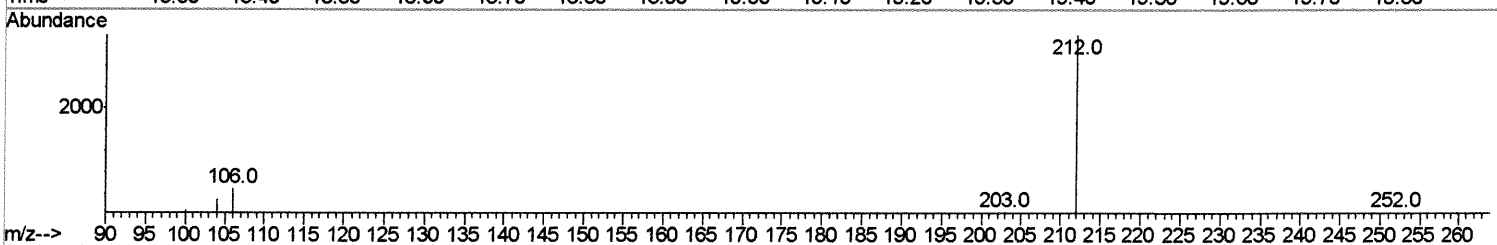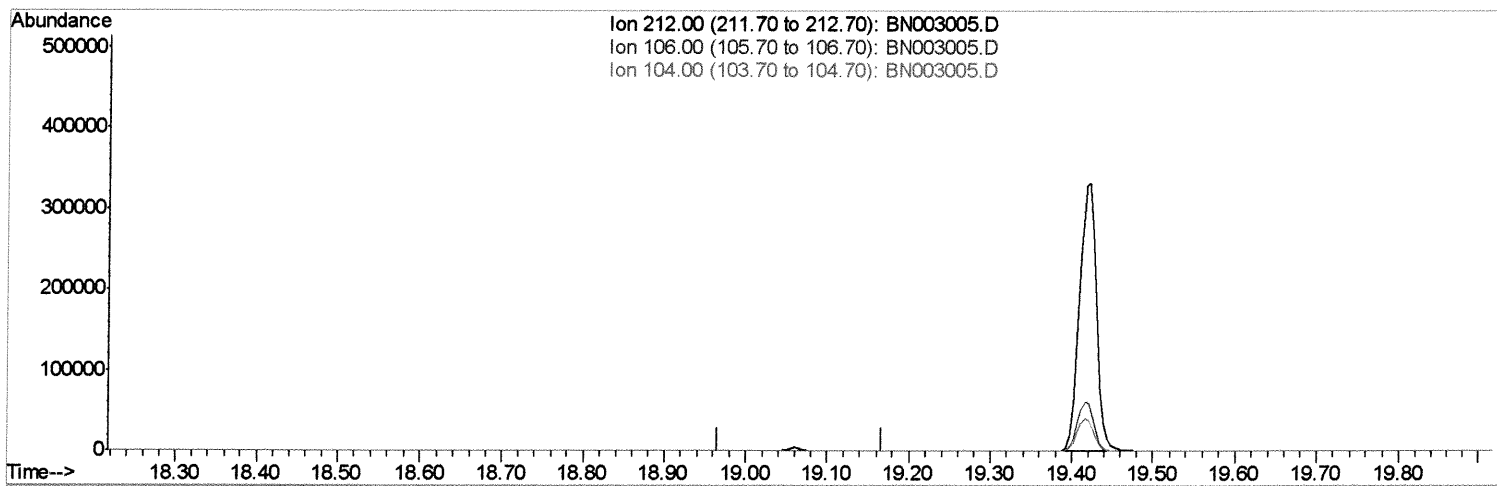

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:39:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

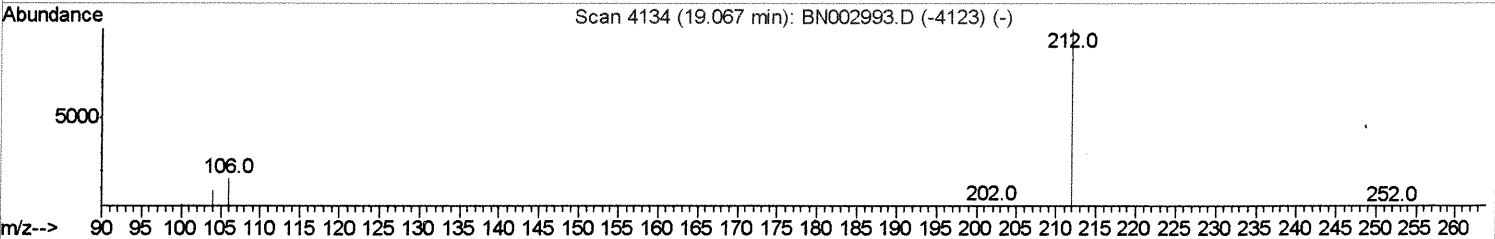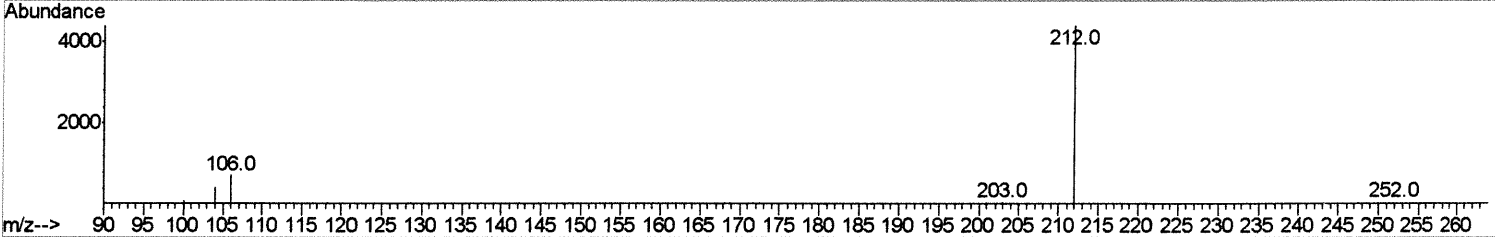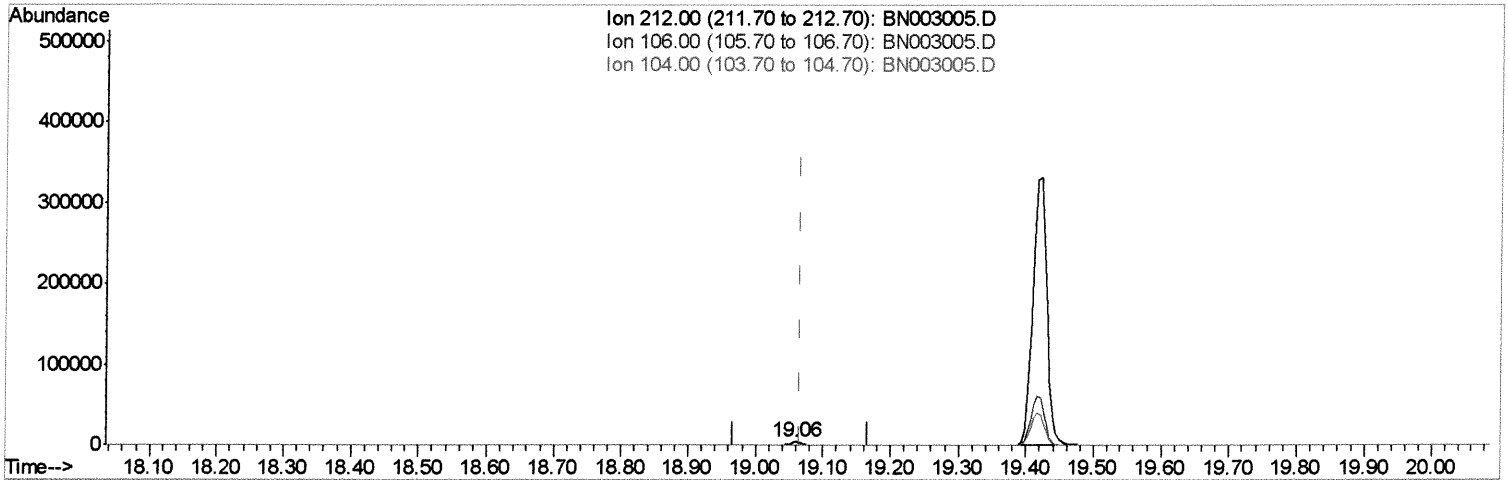

TIC: BN003005.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.30ng/ul m

response 6431

Ion Exp% Act%

212.00 100 100

106.00 15.40 0.00#

104.00 8.60 0.00#

0.00 0.00 0.00

51 10/10/18

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:39:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

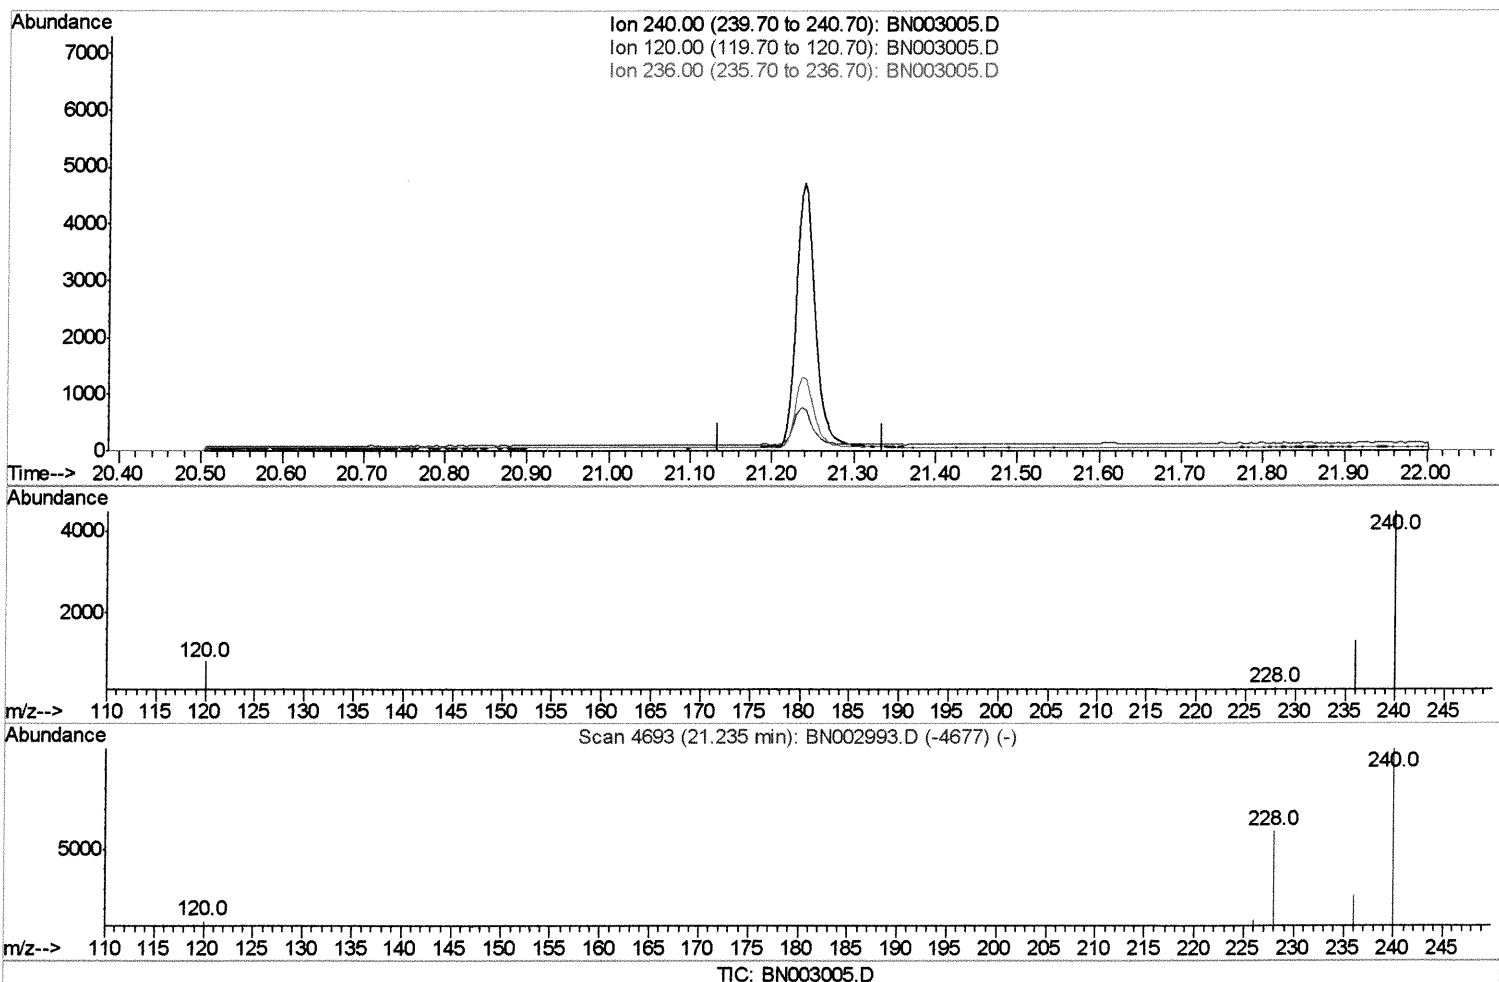

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
 Data File : BN003005.D
 Acq On : 09 Oct 2018 01:47
 Operator : MJ/SJ
 Sample : J5115-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC42

Manual Integrations
 APPROVED

Sohil
 10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:39:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 09 08:37:03 2018
 Response via : Initial Calibration

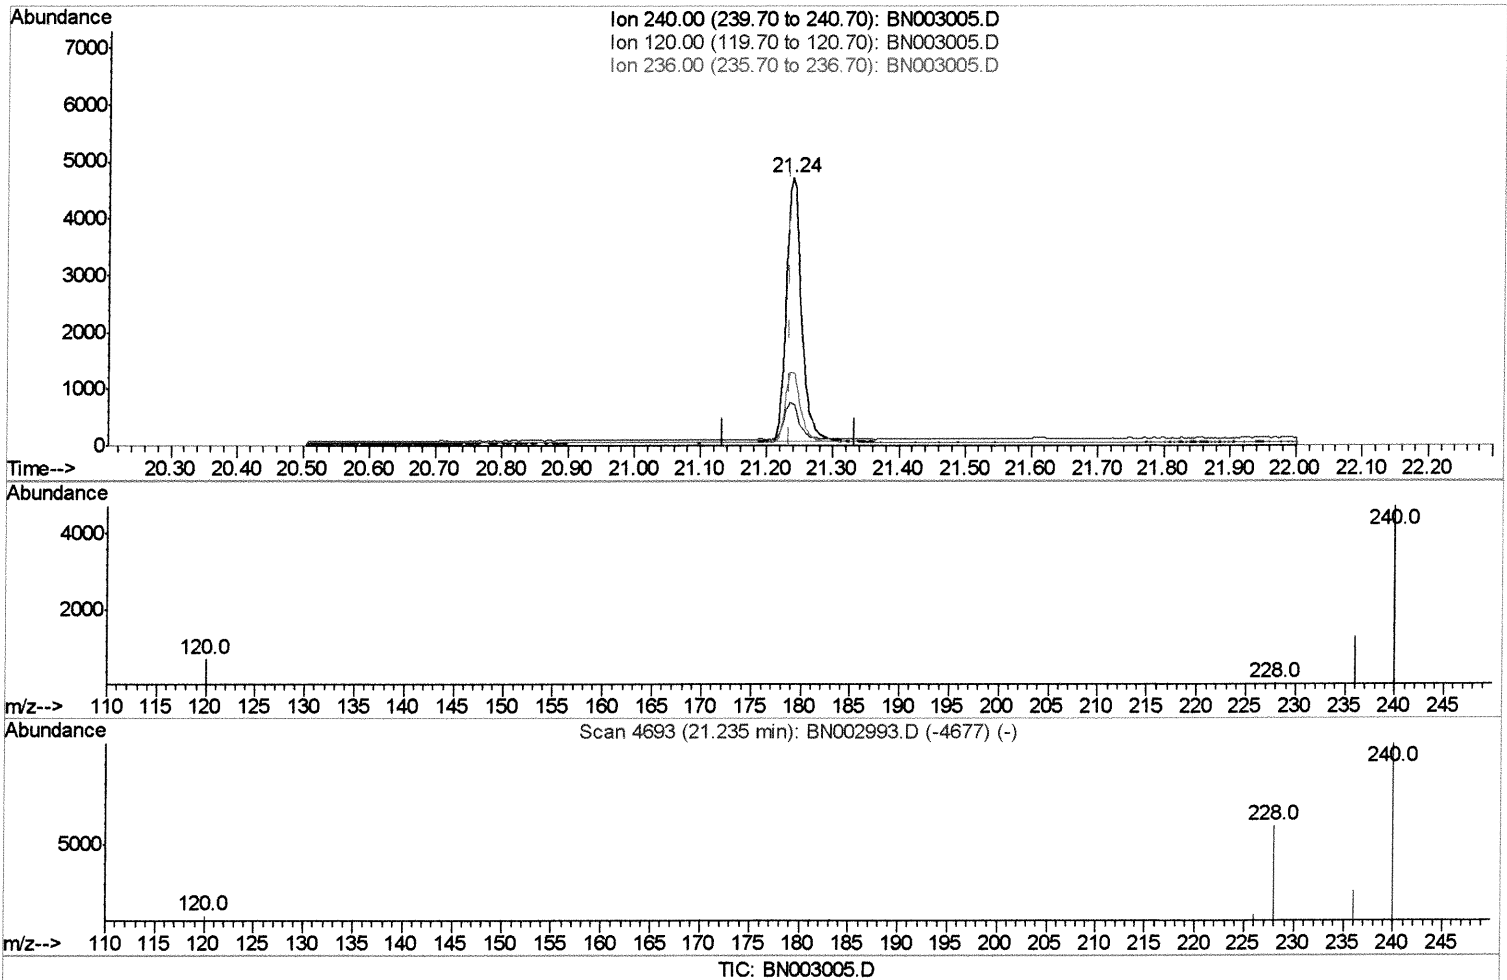

(16) Chrysene-d12 (I)

21.238min (+0.003) 0.40ng/ul m

51 10/10/18

response 7315

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	15.75
236.00	28.10	27.85
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100918\
Data File : BN003005.D
Acq On : 09 Oct 2018 01:47
Operator : MJ/SJ
Sample : J5115-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC42

Manual Integrations
APPROVED

Sohil
10/9/2018 5:37:59 PM

Quant Time: Oct 09 08:40:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 09 08:37:03 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1289	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.40	136	5467	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3213	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	7513m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	7315m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6874	0.40	ng/ul	-0.01

> SS 10/10/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	2328	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	6431m	0.30	ng/ul	0.00

SS 10/10/18

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed