
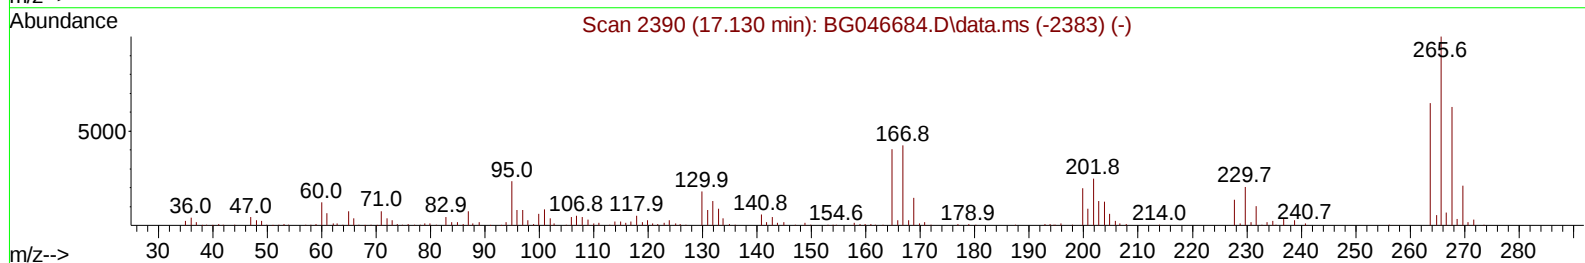
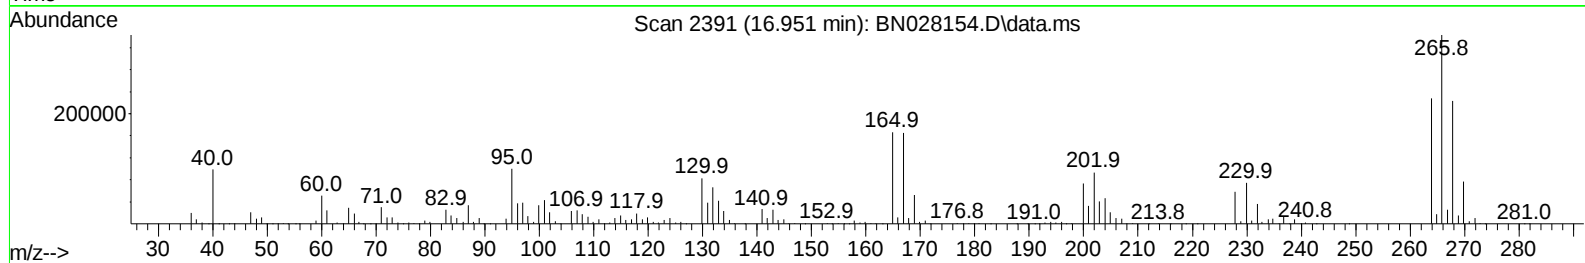


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028154.D
Acq On : 09 Oct 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 01:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

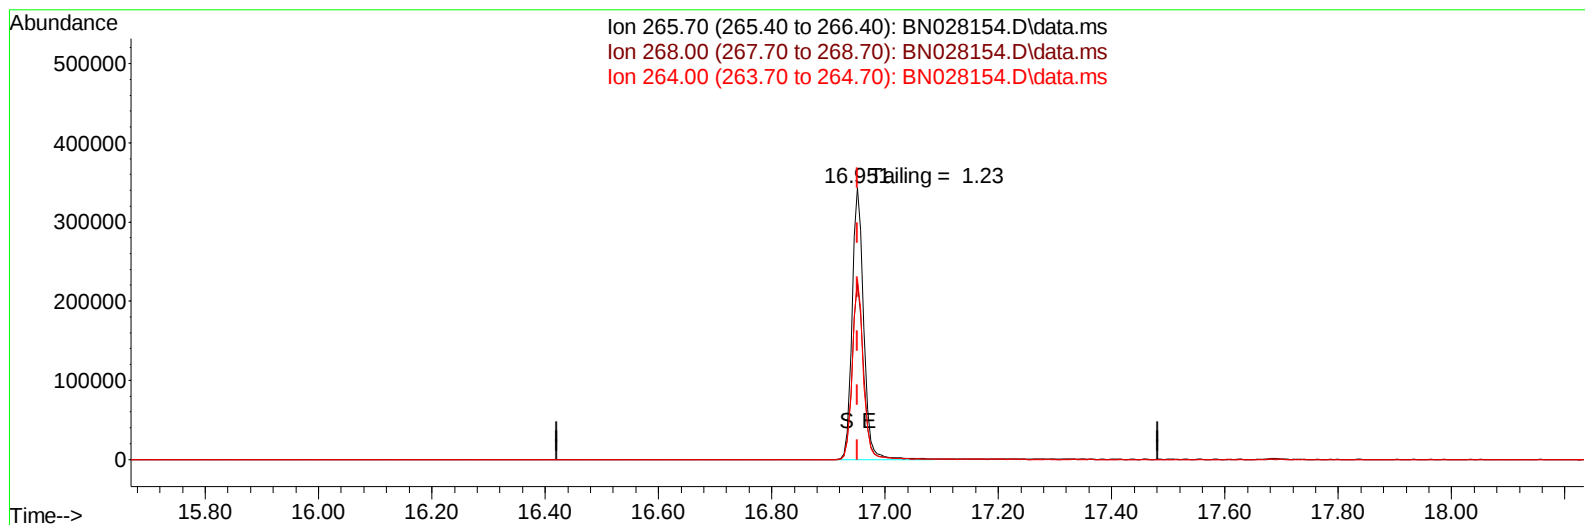

TIC: BN028154.D\data.ms

(70) Pentachlorophenol (C)




16.951min (0.000) 20965.11 ng

response 492435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.20
264.00	61.60	66.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028154.D
Acq On : 09 Oct 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 01:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

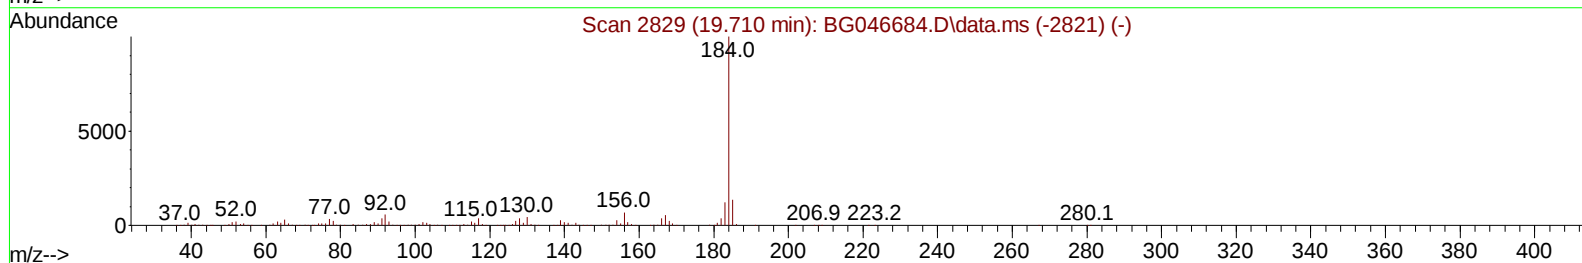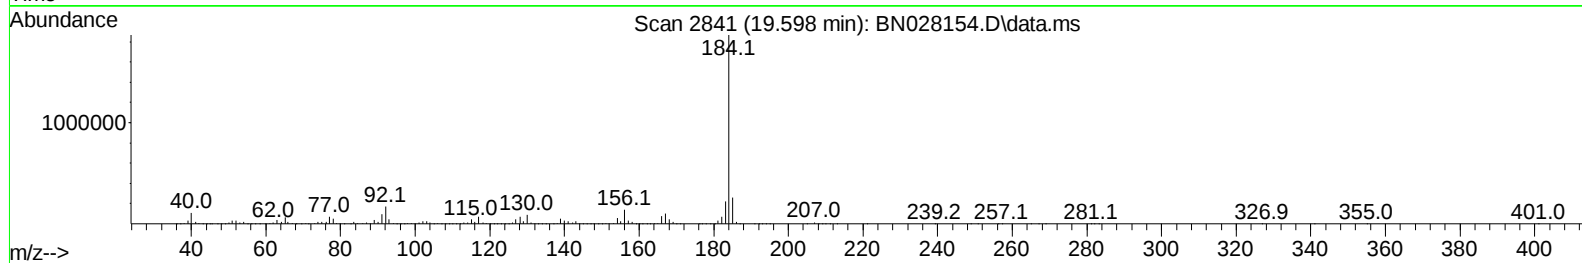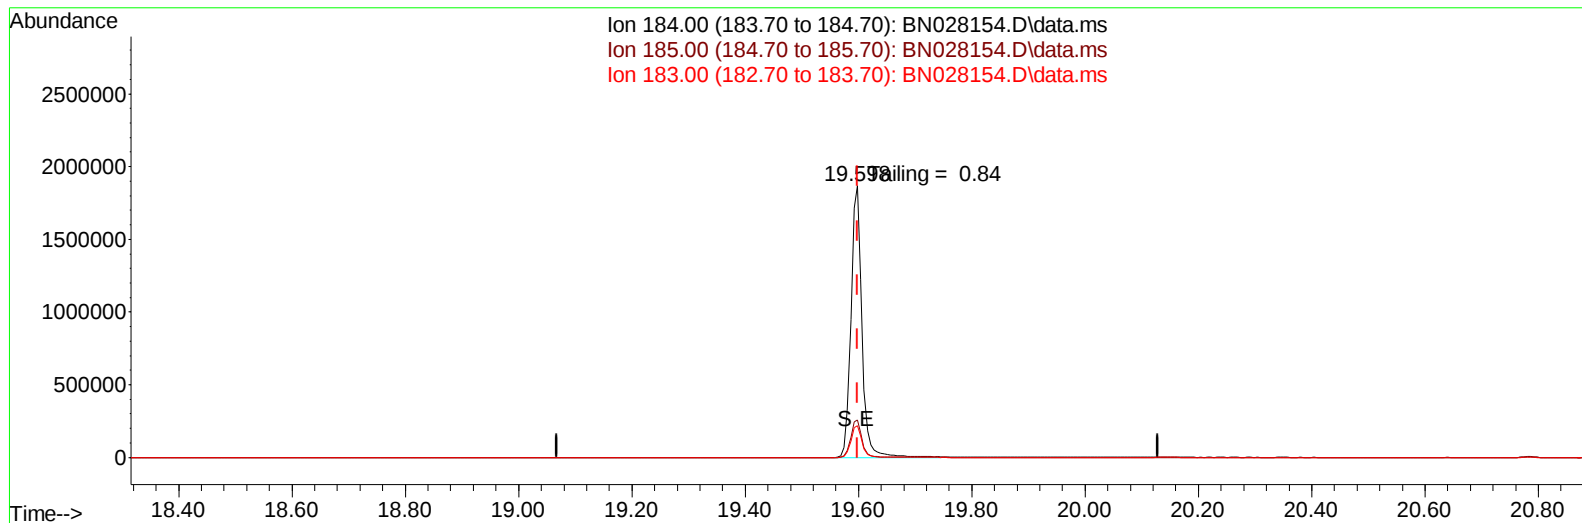

TIC: BN028154.D\data.ms

(77) Benzidine**19.598min (0.000) 1148845.30 ng****response 2549778**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	11.74
0.00	0.00	0.00