
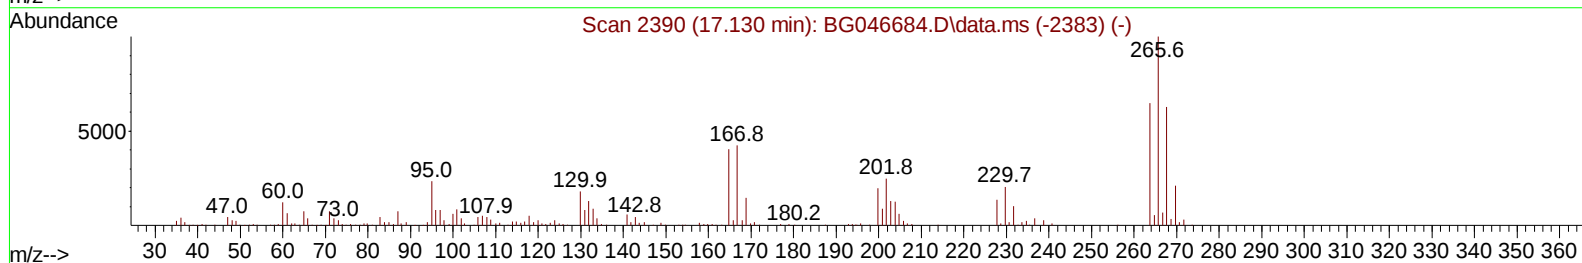
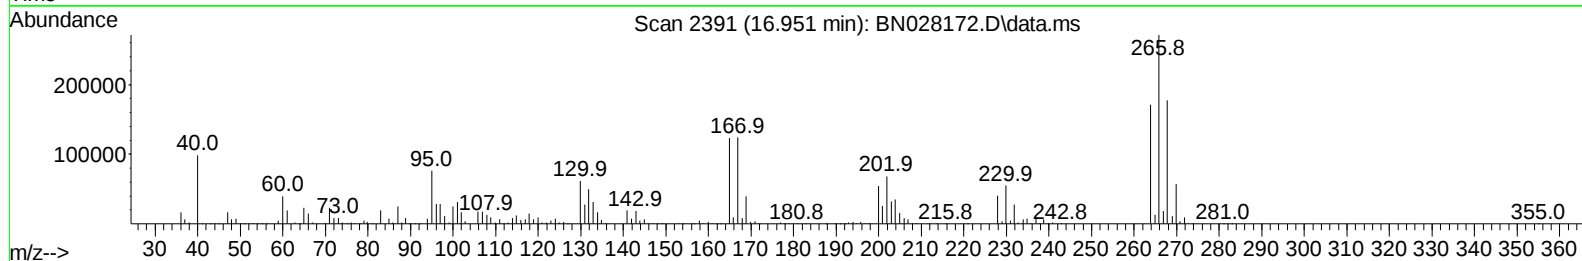


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028172.D
Acq On : 09 Oct 2023 23:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 01:48:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

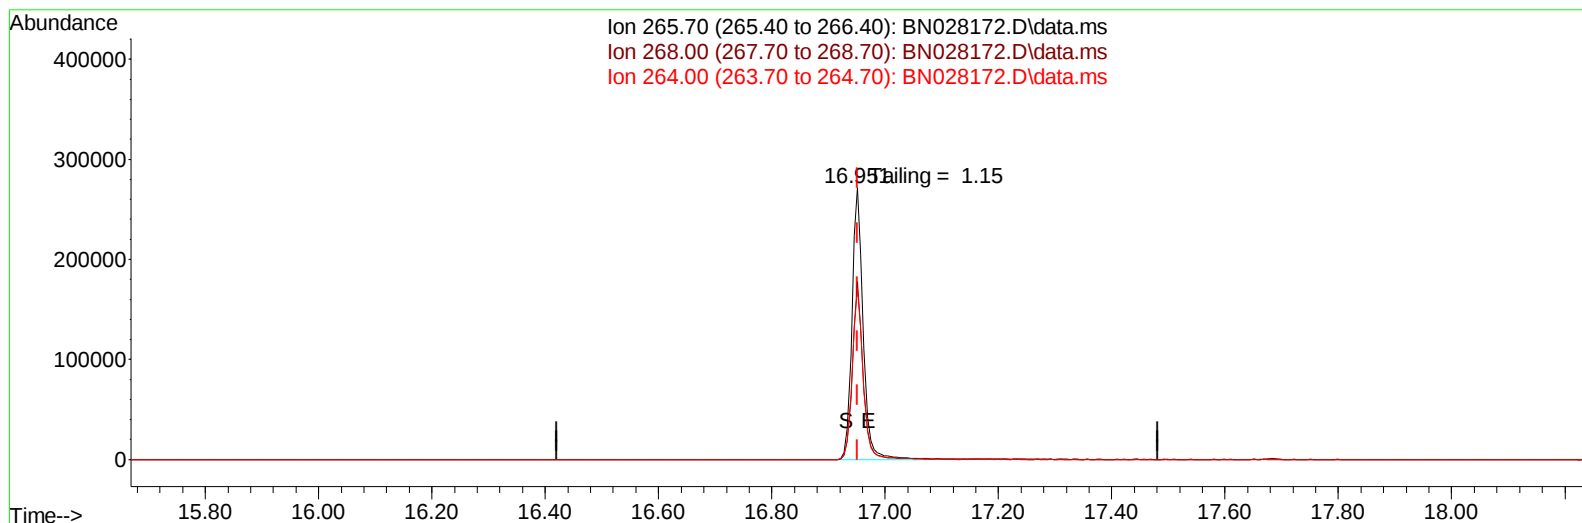



TIC: BN028172.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 24384.70 ng

response 374884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.50
264.00	61.60	63.15
0.00	0.00	0.00

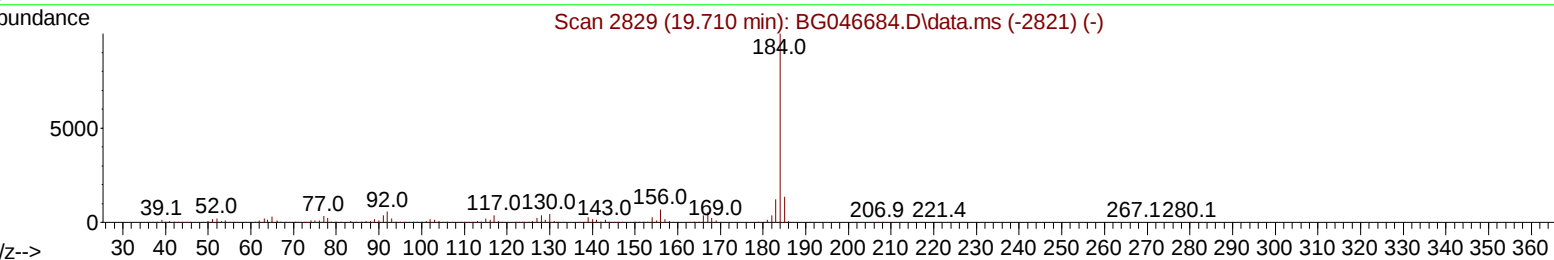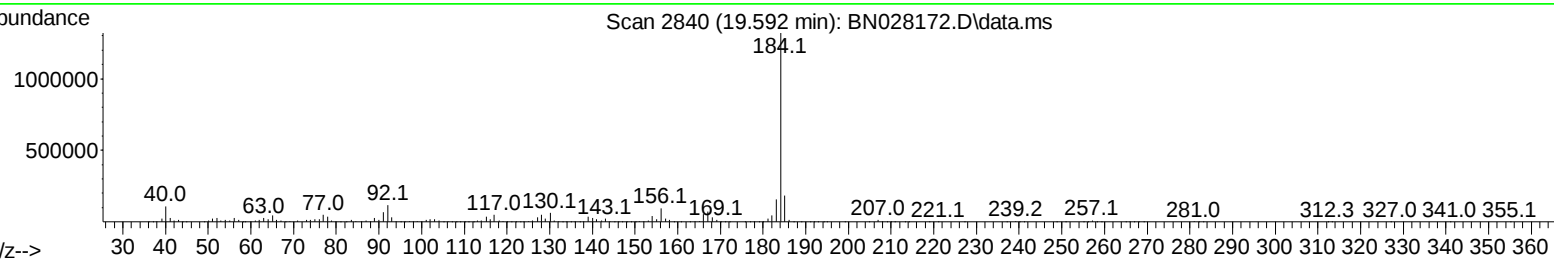

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	11.91
0.00	0.00	0.00