
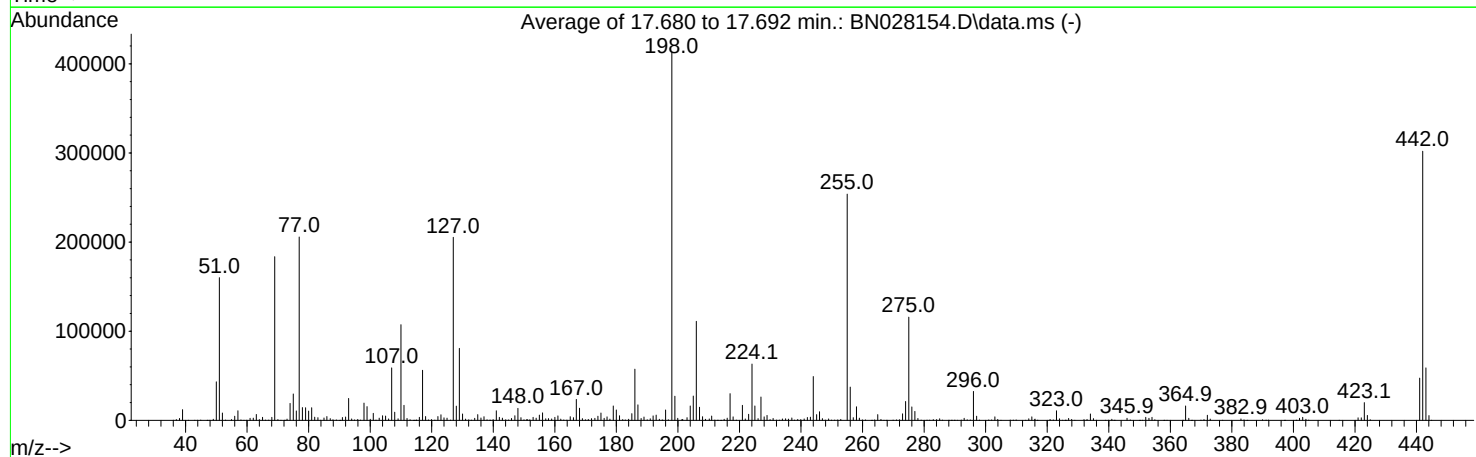


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028154.D
Acq On : 09 Oct 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 10 00:42:22 2023

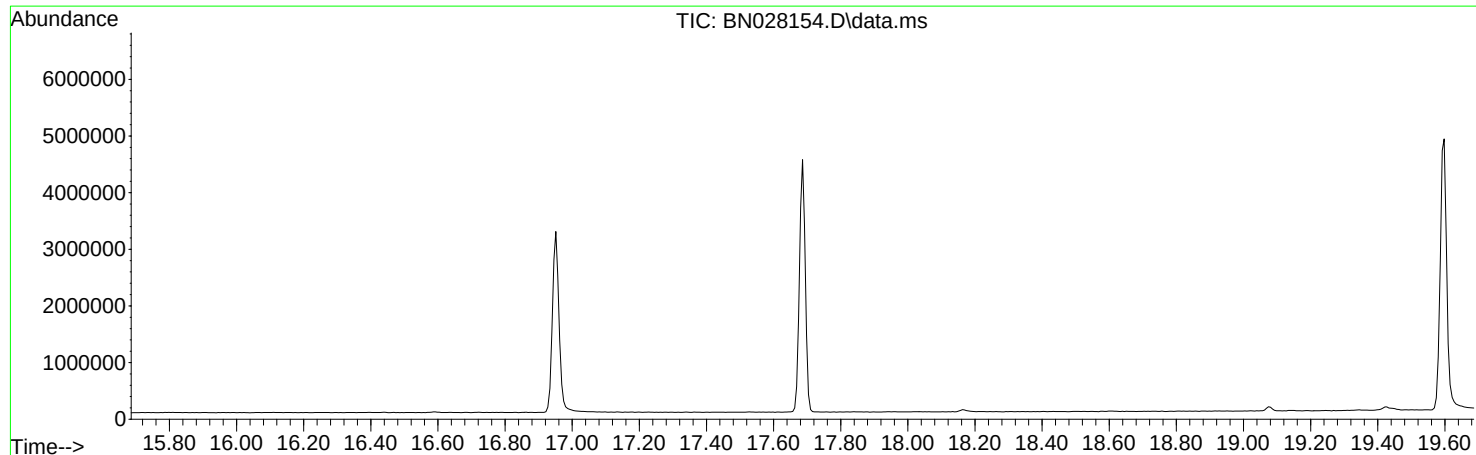




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	160107	PASS
68	69	0.00	2	1.9	3506	PASS
69	198	0.00	100	44.5	183701	PASS
70	69	0.00	2	0.5	987	PASS
127	198	10	80	49.7	205291	PASS
197	198	0.00	2	0.2	761	PASS
198	198	100	100	100.0	412693	PASS
199	198	5	9	6.6	27157	PASS
275	198	10	60	28.1	115765	PASS
365	198	1	100	3.9	16234	PASS
441	198	0.01	100	11.5	47344	PASS
442	442	50	100	100.0	301952	PASS
443	442	15	24	19.5	58904	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028154.D
Acq On : 09 Oct 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 01:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

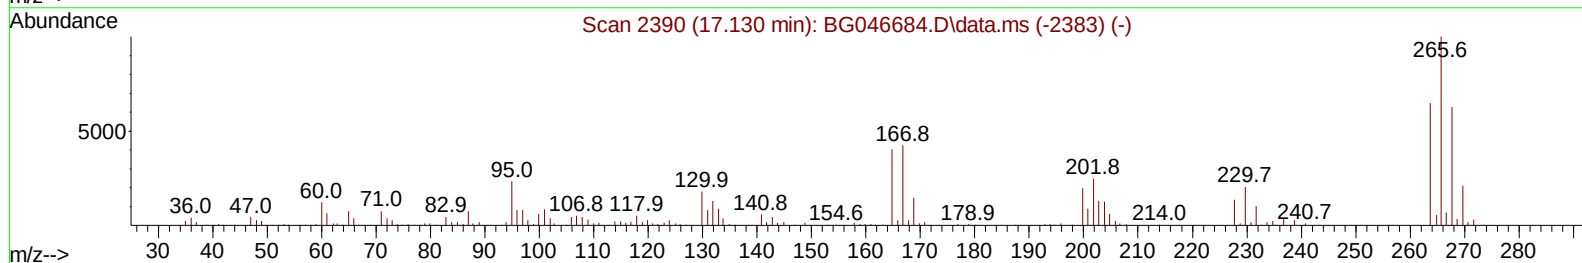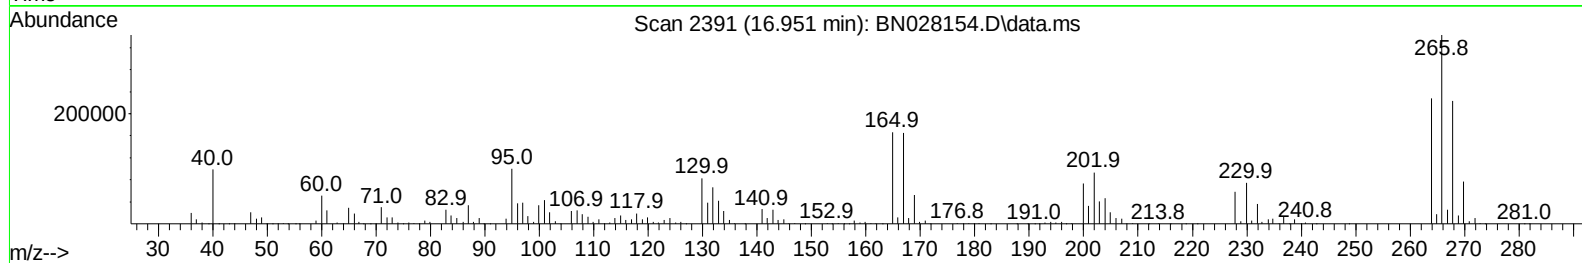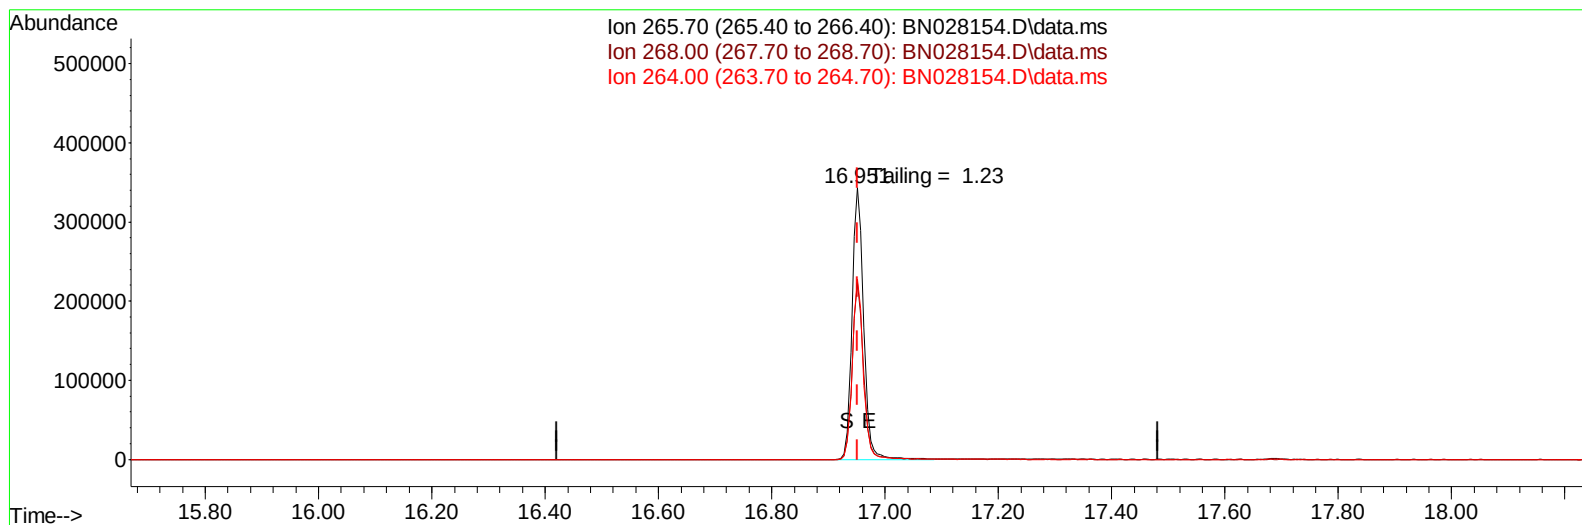

TIC: BN028154.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 20965.11 ng




response 492435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.20
264.00	61.60	66.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
 Data File : BN028154.D
 Acq On : 09 Oct 2023 10:10
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 10 01:47:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 01:46:56 2023
 Response via : Initial Calibration

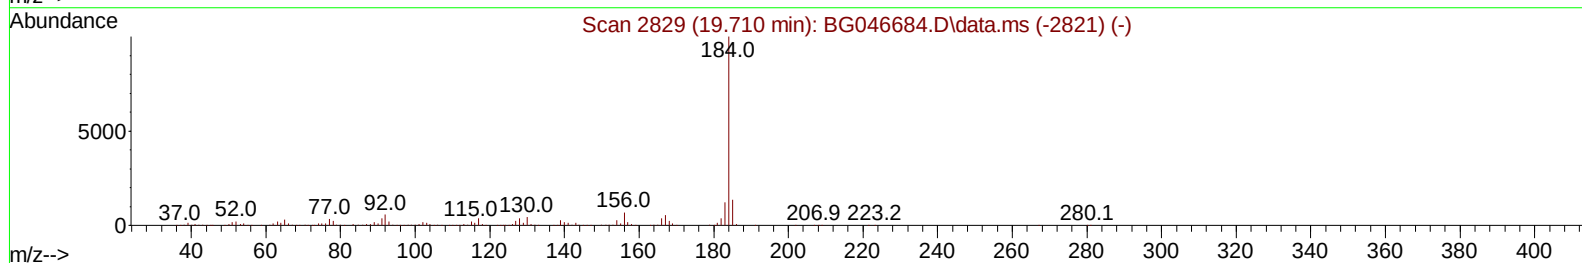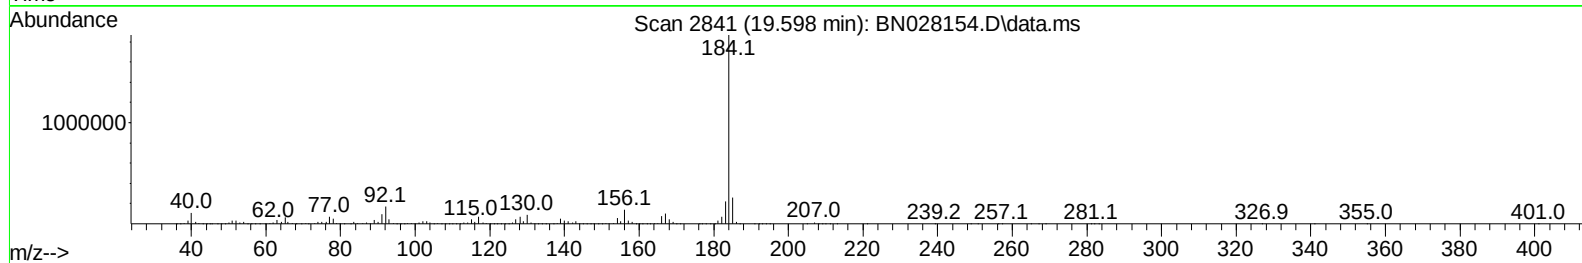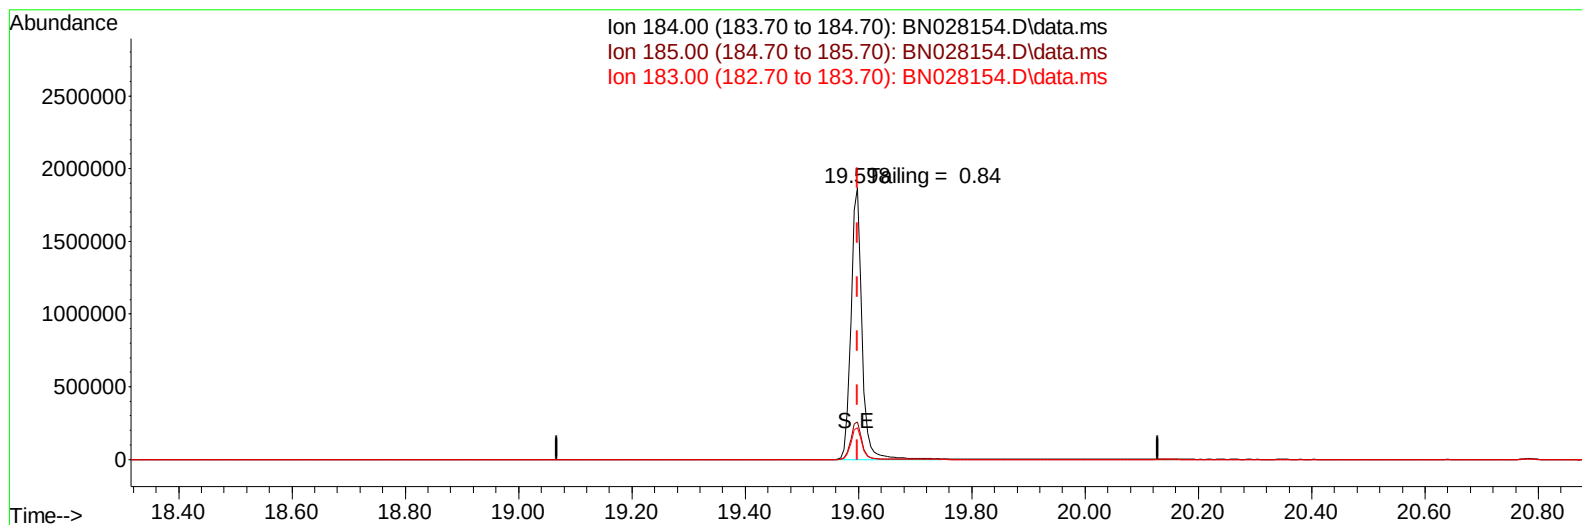

TIC: BN028154.D\data.ms

(77) Benzidine

19.598min (0.000) 1148845.30 ng

response 2549778

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2023	BNA_N	<u>BN028154.D</u>
Compound Name	Response	Retention Time
DDT	1319295	20.786
DDD	101245	20.351
DDE	4664	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
105909	1425204	7.43

Instrument :
BNA_N
ClientSampleId :
DFTPP