


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028172.D
Acq On : 09 Oct 2023 23:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 10 00:42:22 2023

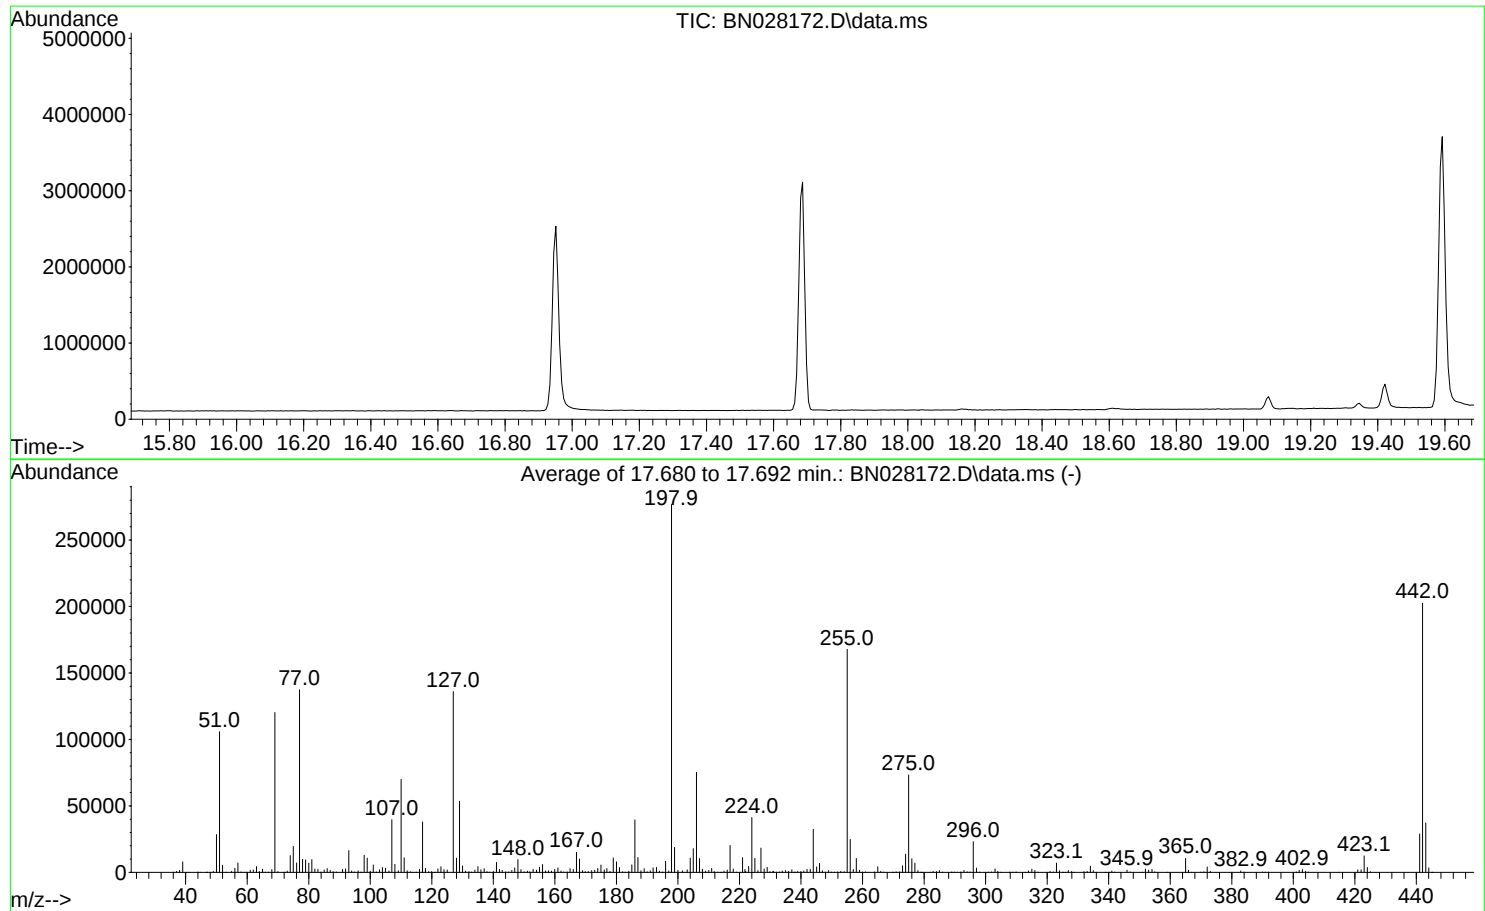




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	105836	PASS
68	69	0.00	2	1.8	2200	PASS
69	198	0.00	100	43.5	120285	PASS
70	69	0.00	2	0.5	631	PASS
127	198	10	80	49.1	135992	PASS
197	198	0.00	2	0.4	1138	PASS
198	198	100	100	100.0	276693	PASS
199	198	5	9	6.8	18790	PASS
275	198	10	60	26.5	73352	PASS
365	198	1	100	3.8	10503	PASS
441	198	0.01	100	10.4	28896	PASS
442	442	50	100	100.0	202475	PASS
443	442	15	24	18.4	37235	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028172.D
Acq On : 09 Oct 2023 23:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 01:48:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

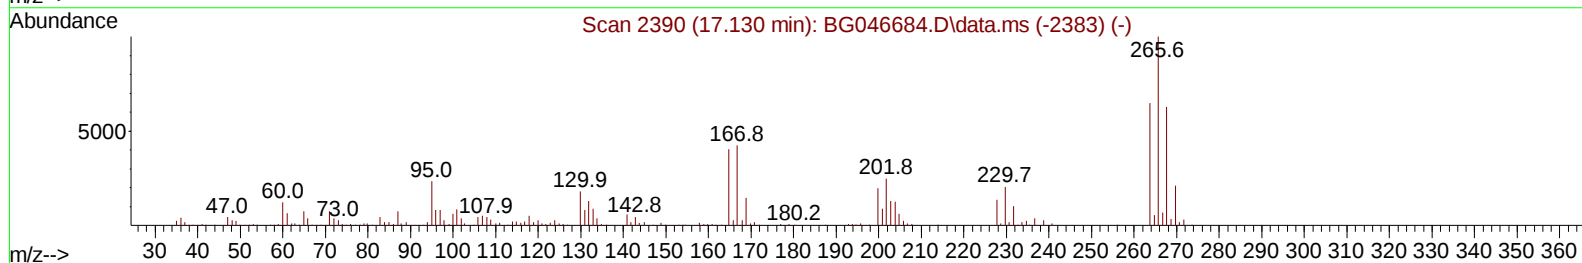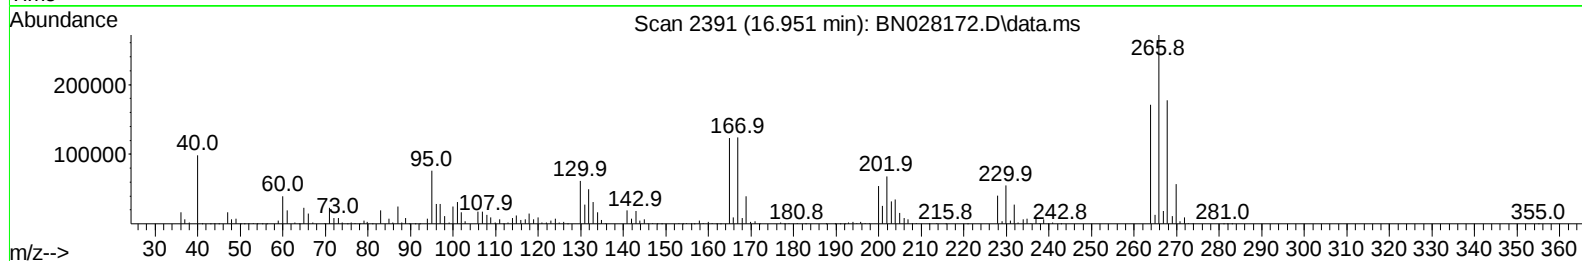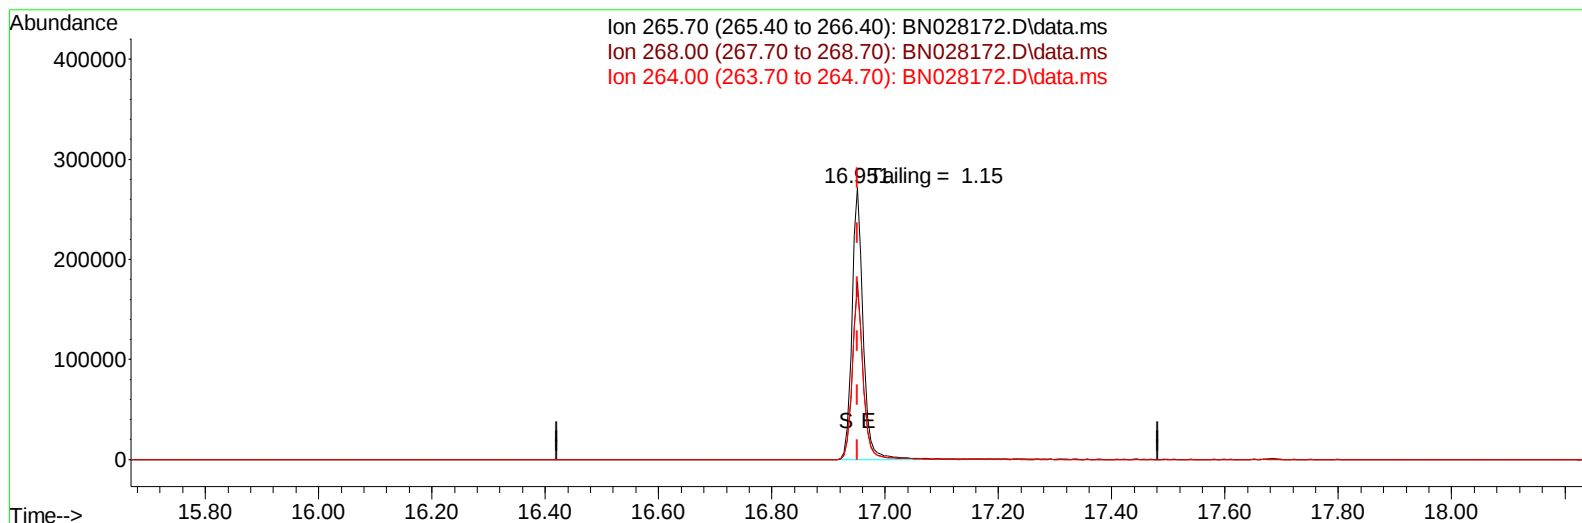

TIC: BN028172.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 24384.70 ng




response 374884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.50
264.00	61.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100923\
Data File : BN028172.D
Acq On : 09 Oct 2023 23:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 10 01:48:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 01:46:56 2023
Response via : Initial Calibration

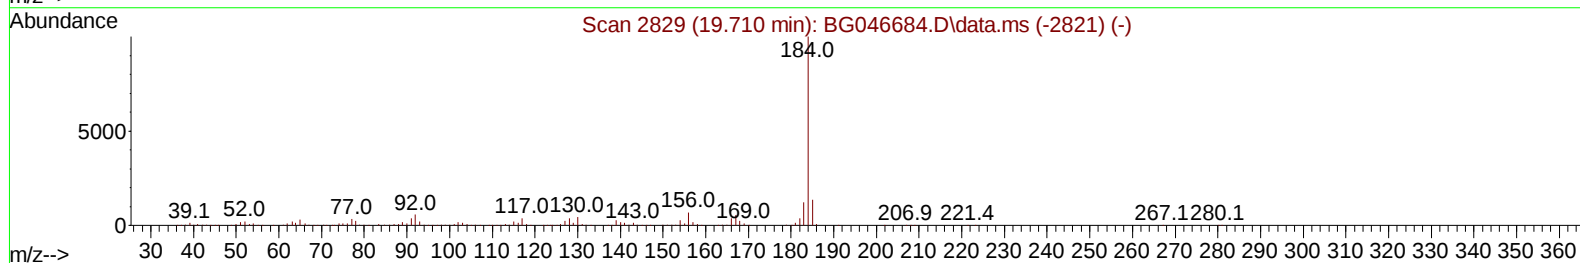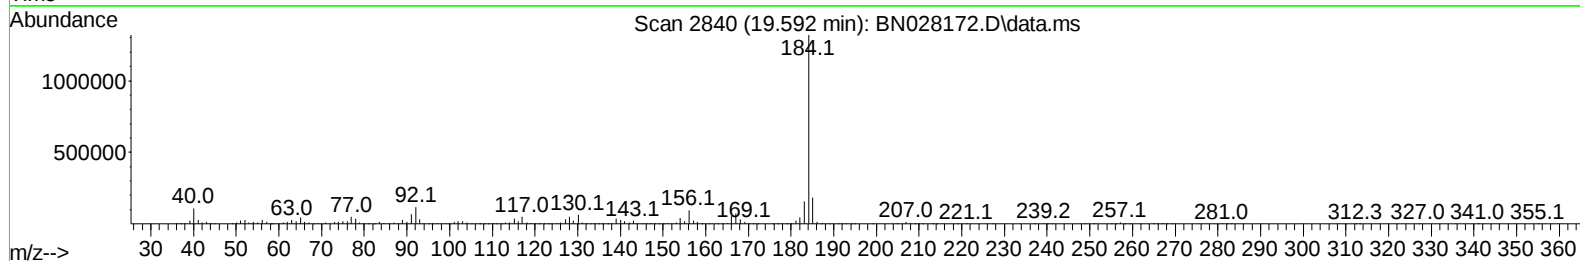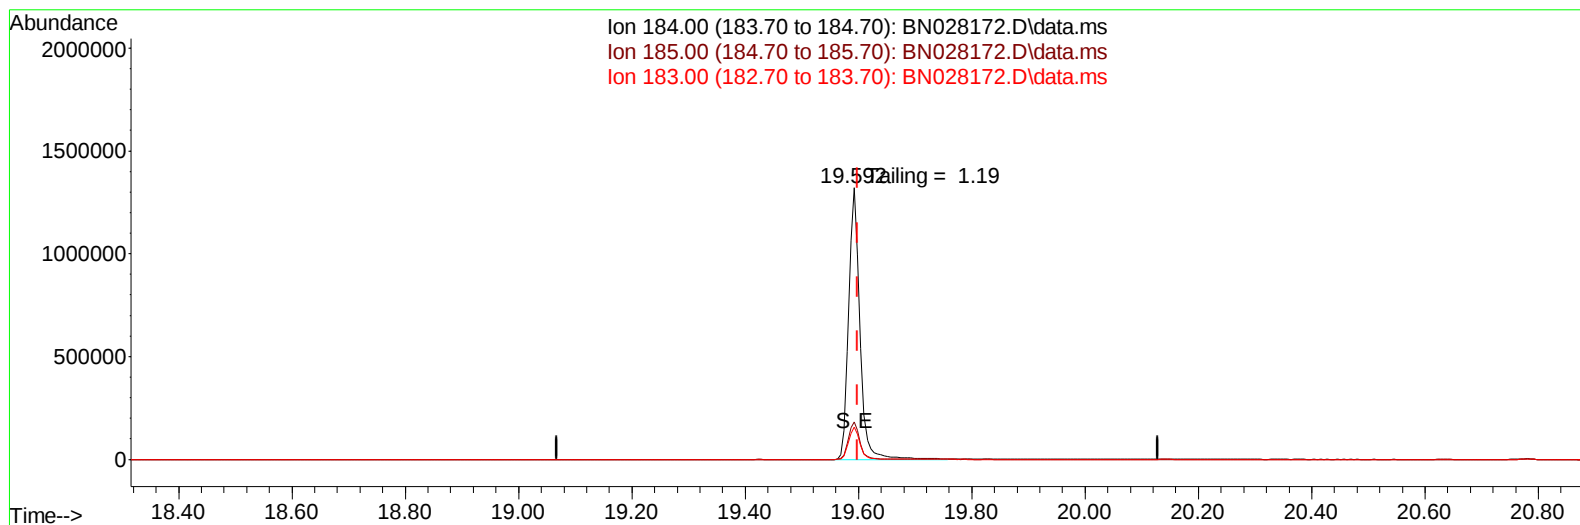

TIC: BN028172.D\data.ms

(77) Benzidine

19.592min (-0.006) 0.00 ng

response 1840705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2023	BNA_N	<u>BN028172.D</u>
Compound Name	Response	Retention Time
DDT	975504	20.78
DDD	110777	20.345
DDE	5295	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
116072	1091576	10.63

Instrument :
BNA_N
ClientSampleId :
DFTPP